

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041621\
 Data File : PL066229.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Apr 2021 13:51
 Operator : AR\AJ
 Sample : M2042-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FS-SB12A(55-56)

Manual Integrations
 APPROVED

Ankita
 4/20/2021 11:45:54 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 16 23:04:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 15:37:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.445	4.154	44643921	73007123	17.540	18.149
28)	SA Decachlor...	8.171	9.355	45937291	64492499	19.259	19.747
Target Compounds							
10)	B gamma-Chl...	5.361	6.321	8085502	8638998	2.184	1.893m
11)	B alpha-Chl...	5.427	6.393	5905971	8097419	1.595	1.791

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041621\
Data File : PL066229.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Apr 2021 13:51
Operator : AR\AJ
Sample : M2042-05
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
FS-SB12A(55-56)


Manual Integrations
APPROVED

Ankita
4/20/2021 11:45:54 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 23:04:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 15:37:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

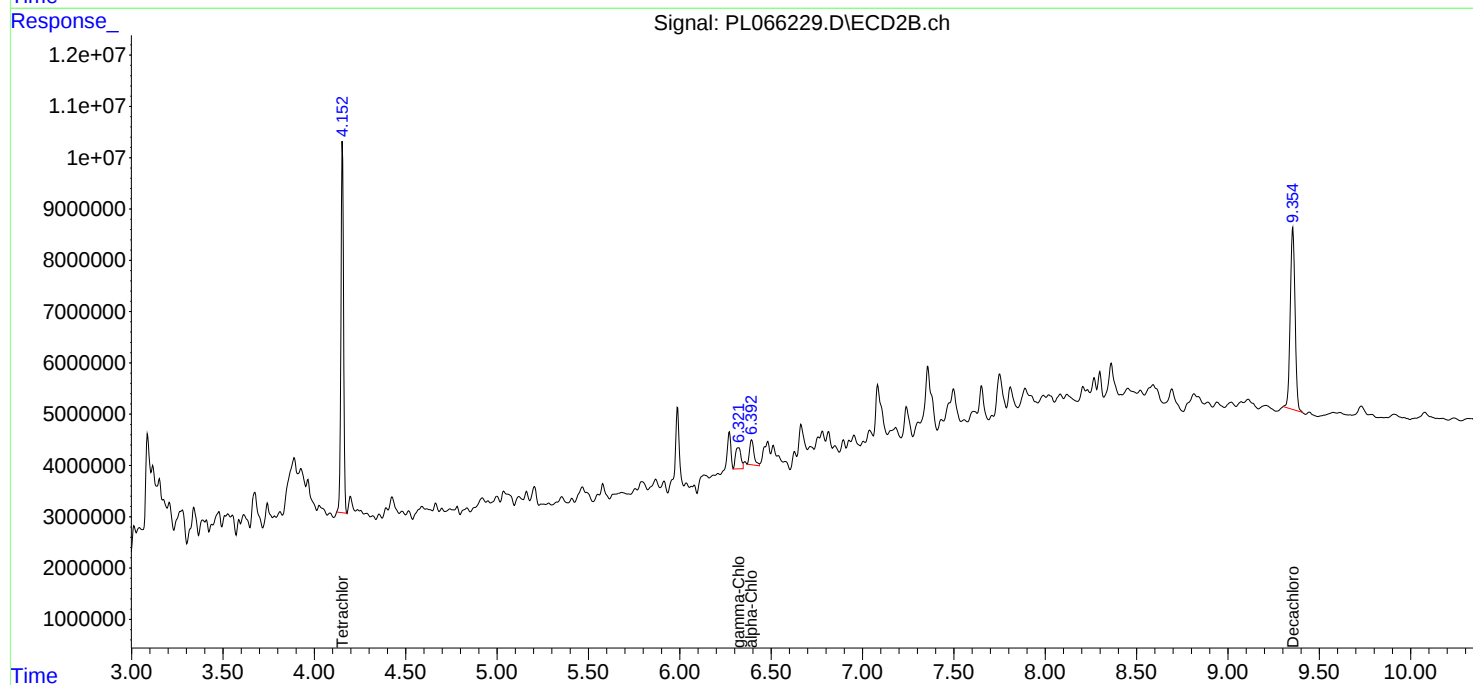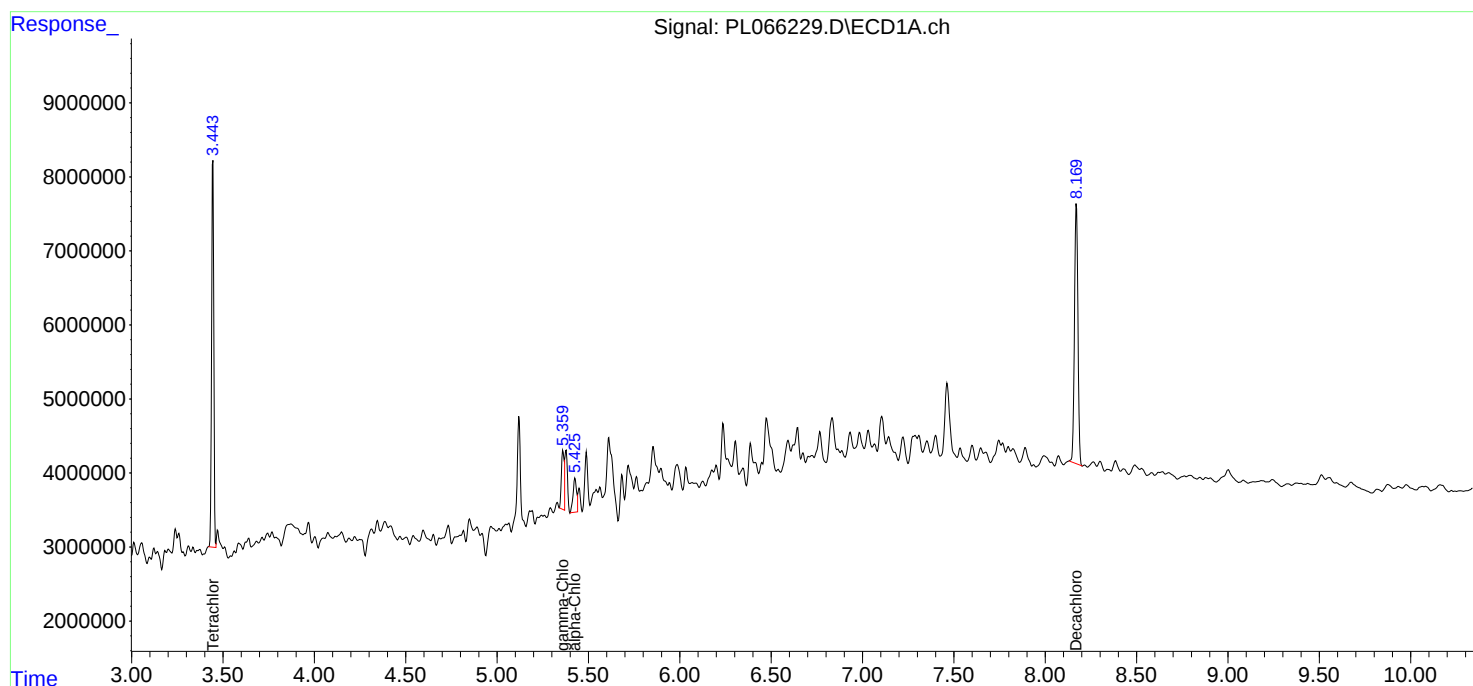

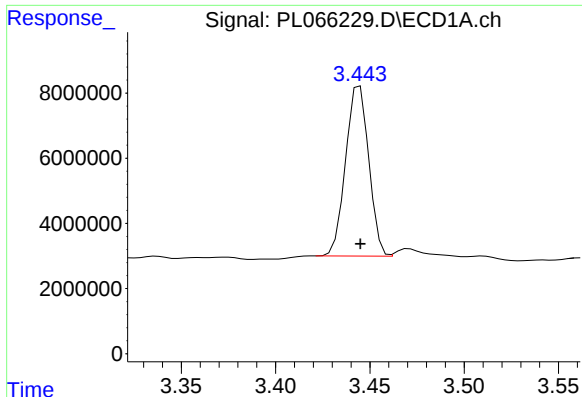


#1 Tetrachloro-m-xylene

R.T.: 3.445 min
Delta R.T.: 0.000 min
Response: 44643921
Conc: 17.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
FS-SB12A(55-56)


Manual Integrations
APPROVED

Ankita
4/20/2021 11:45:54 AM

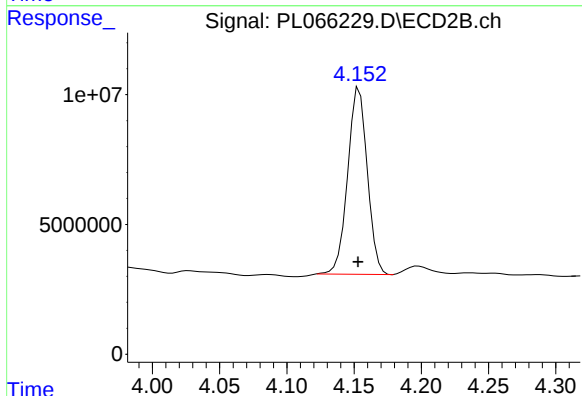


#1 Tetrachloro-m-xylene

R.T.: 4.154 min
Delta R.T.: 0.000 min
Response: 73007123
Conc: 18.15 ng/ml

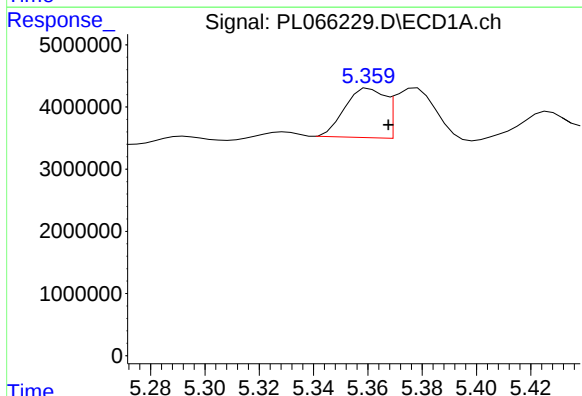


#10 gamma-Chlordane

R.T.: 5.361 min
Delta R.T.: -0.007 min
Response: 8085502
Conc: 2.18 ng/ml

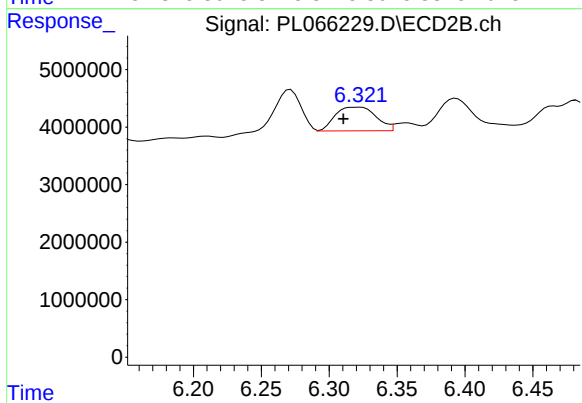

#10 gamma-Chlordane

R.T.: 6.321 min
Delta R.T.: 0.011 min
Response: 8638998
Conc: 1.89 ng/ml m

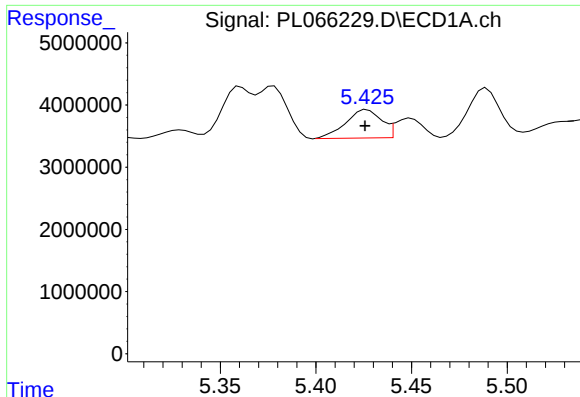


#11 alpha-Chlordane

R.T.: 5.427 min
Delta R.T.: 0.001 min
Response: 5905971
Conc: 1.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
FS-SB12A(55-56)


Manual Integrations
APPROVED

Ankita
4/20/2021 11:45:54 AM

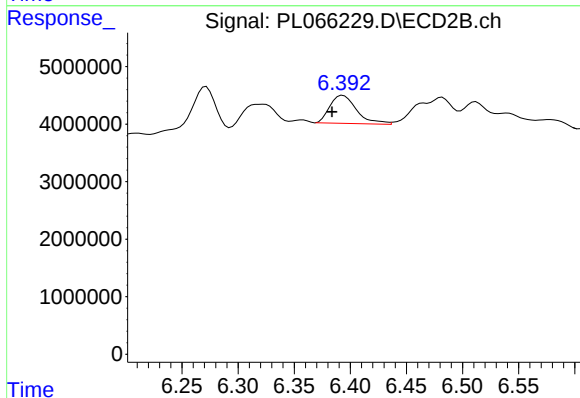


#11 alpha-Chlordane

R.T.: 6.393 min
Delta R.T.: 0.010 min
Response: 8097419
Conc: 1.79 ng/ml

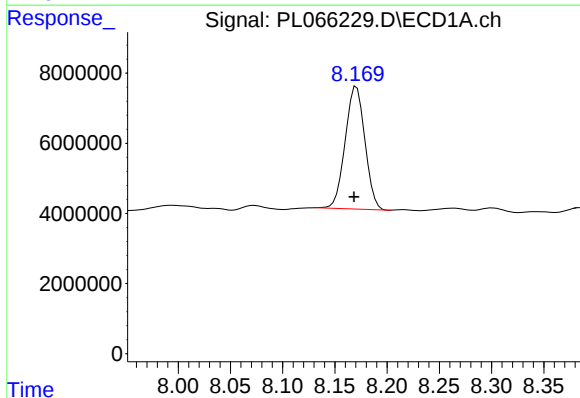

#28 Decachlorobiphenyl

R.T.: 8.171 min
Delta R.T.: 0.002 min
Response: 45937291
Conc: 19.26 ng/ml

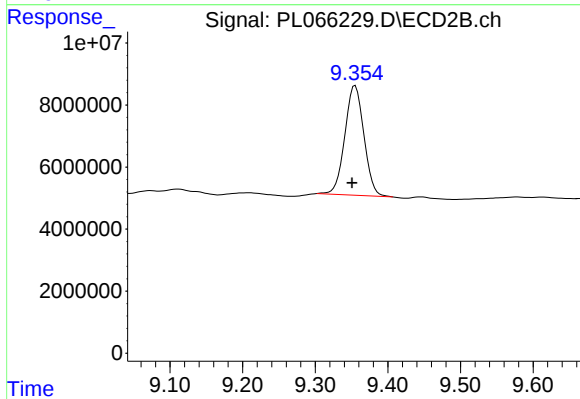

#28 Decachlorobiphenyl

R.T.: 9.355 min
Delta R.T.: 0.004 min
Response: 64492499
Conc: 19.75 ng/ml