

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041621\
 Data File : PL066237.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Apr 2021 15:57
 Operator : AR\AJ
 Sample : M2050-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-7

Manual Integrations
 APPROVED

Ankita
 4/20/2021 11:46:11 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 16 23:06:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 15:37:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.446	4.155	28685999	45980116	11.270	11.431
28) SA Decachlor...	8.171	9.356	25998539	36666072	10.900	11.227
Target Compounds						
12) B 4,4'-DDE	5.593	6.542	54397320	63659511	14.583	15.380
17) MA 4,4'-DDT	6.338	7.342	56499534	28337005	17.726m	8.353m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041621\
Data File : PL066237.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Apr 2021 15:57
Operator : AR\AJ
Sample : M2050-01
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
TP-7


Manual Integrations
APPROVED

Ankita
4/20/2021 11:46:11 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 23:06:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 15:37:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

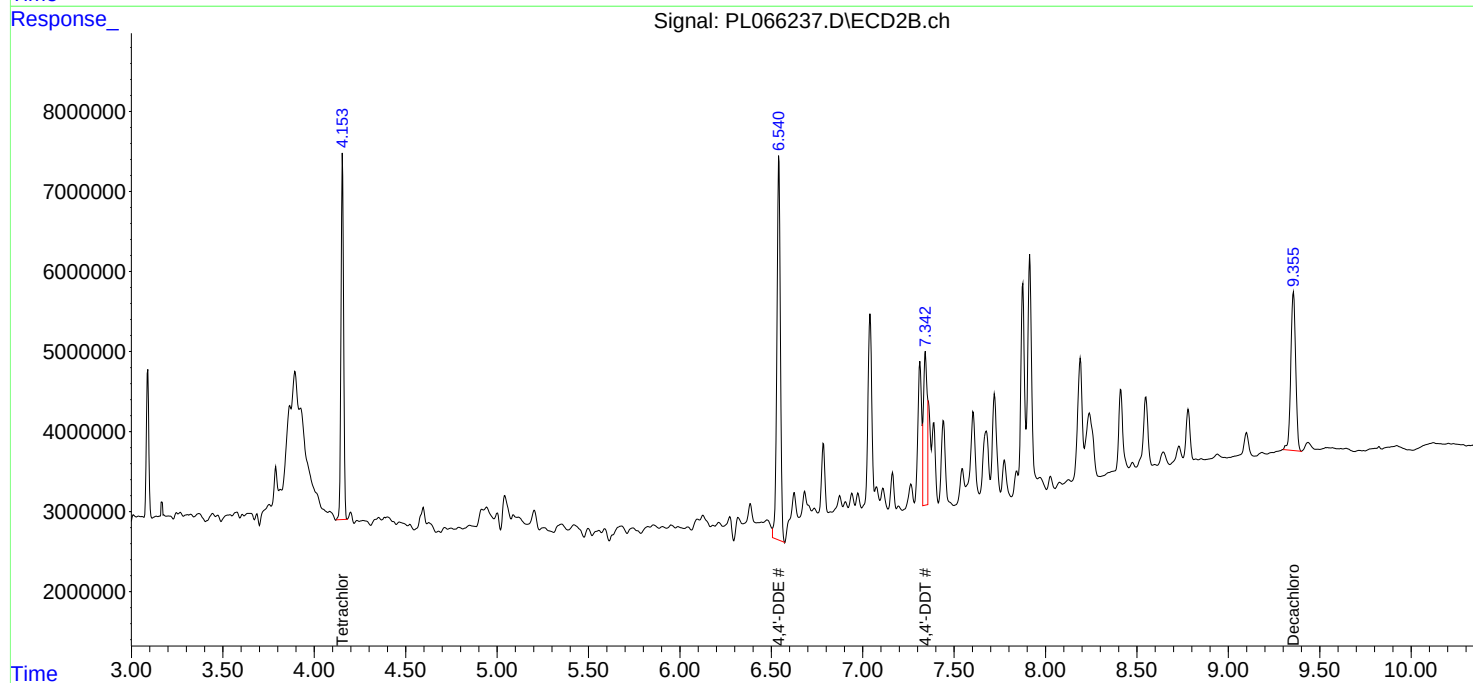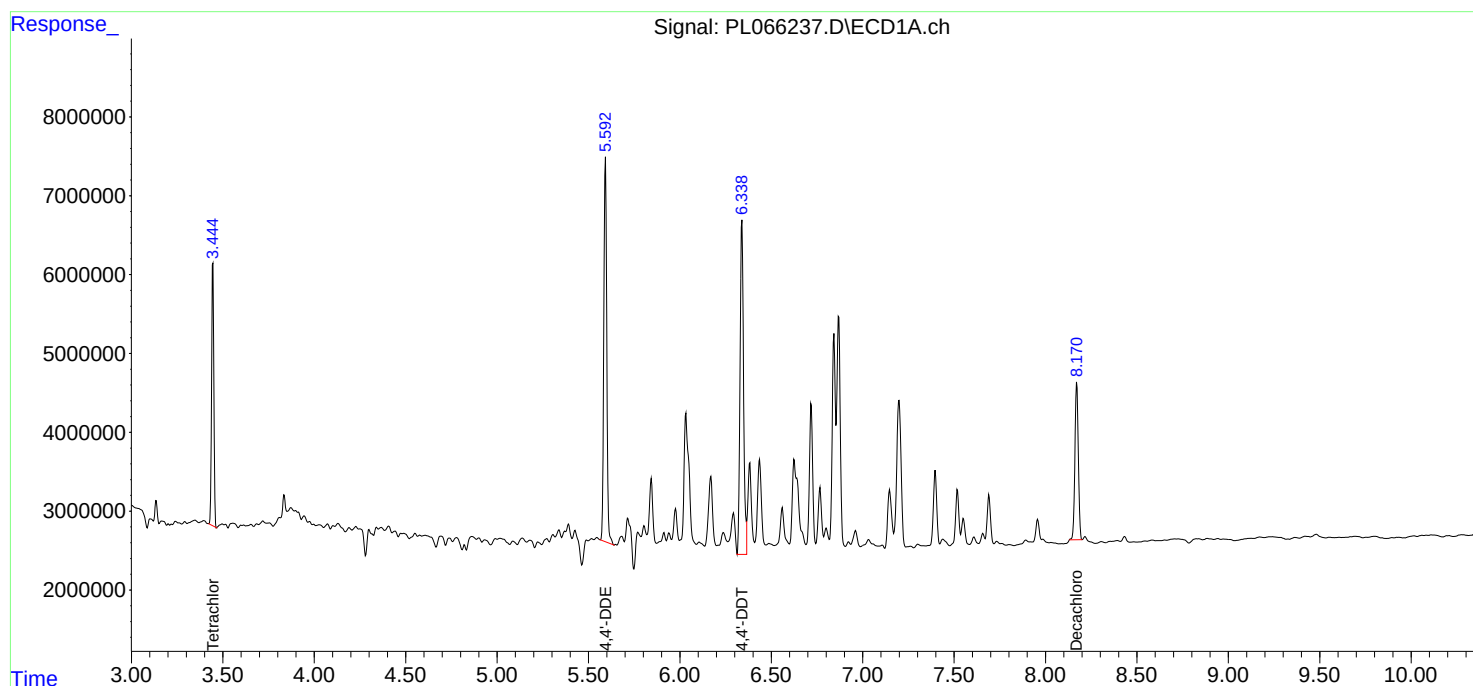

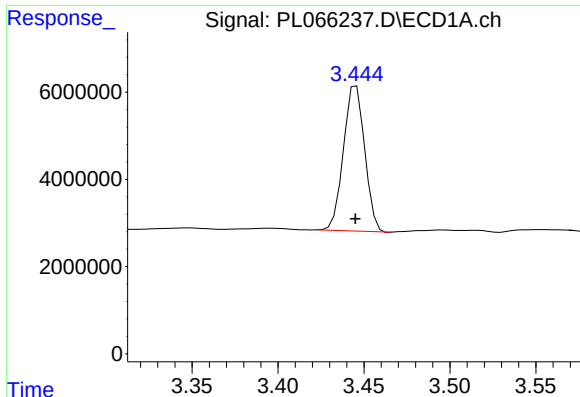


#1 Tetrachloro-m-xylene

R.T.: 3.446 min
Delta R.T.: 0.000 min
Response: 28685999
Conc: 11.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-7


Manual Integrations
APPROVED

Ankita
4/20/2021 11:46:11 AM

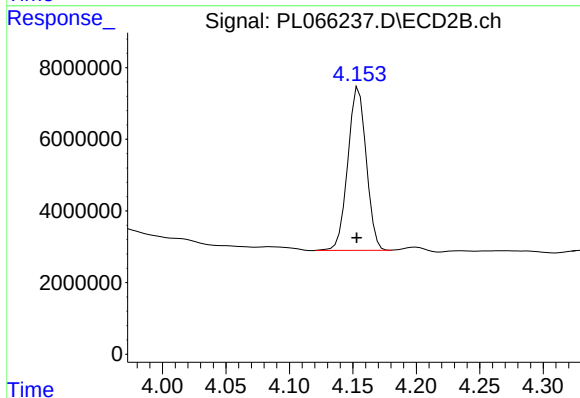


#1 Tetrachloro-m-xylene

R.T.: 4.155 min
Delta R.T.: 0.002 min
Response: 45980116
Conc: 11.43 ng/ml

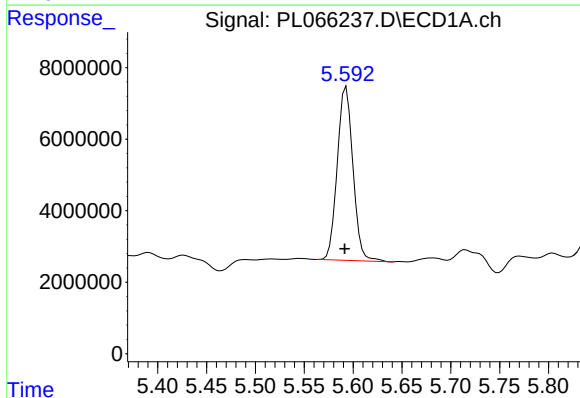


#12 4,4'-DDE

R.T.: 5.593 min
Delta R.T.: 0.002 min
Response: 54397320
Conc: 14.58 ng/ml

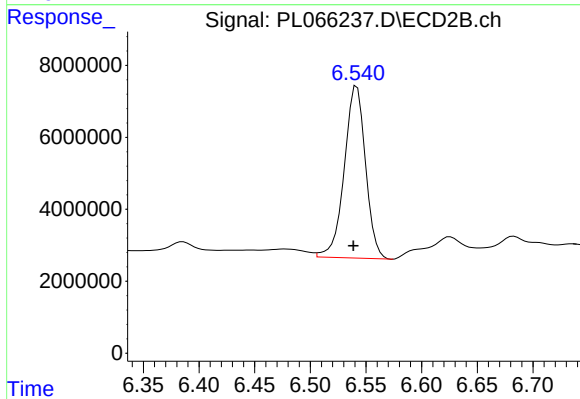

#12 4,4'-DDE

R.T.: 6.542 min
Delta R.T.: 0.003 min
Response: 63659511
Conc: 15.38 ng/ml

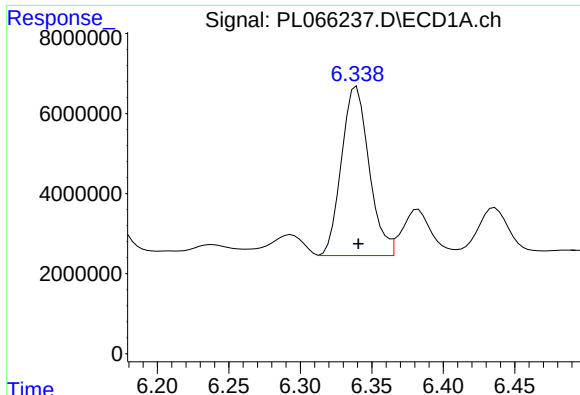


#17 4,4'-DDT

R.T.: 6.338 min
Delta R.T.: -0.003 min
Response: 56499534
Conc: 17.73 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TP-7


Manual Integrations
APPROVED

Ankita
4/20/2021 11:46:11 AM

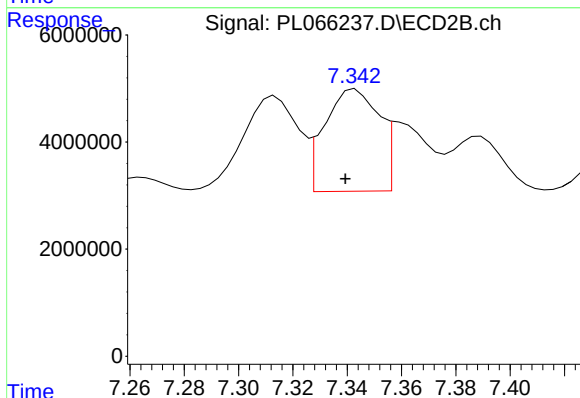


#17 4,4'-DDT

R.T.: 7.342 min
Delta R.T.: 0.002 min
Response: 28337005
Conc: 8.35 ng/ml m

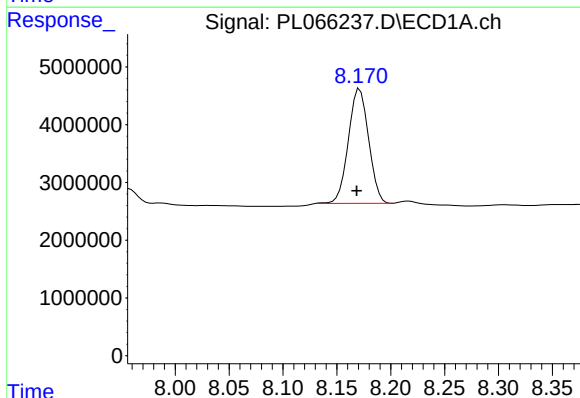

#28 Decachlorobiphenyl

R.T.: 8.171 min
Delta R.T.: 0.003 min
Response: 25998539
Conc: 10.90 ng/ml

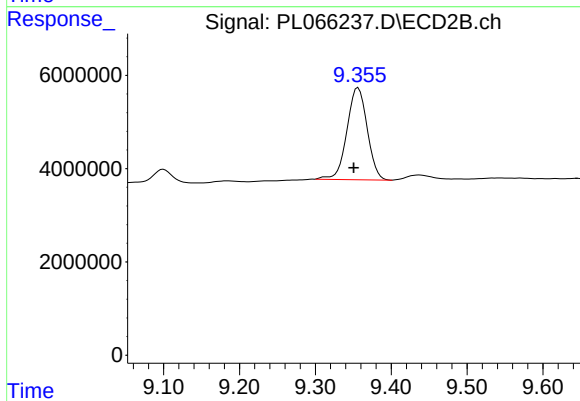

#28 Decachlorobiphenyl

R.T.: 9.356 min
Delta R.T.: 0.006 min
Response: 36666072
Conc: 11.23 ng/ml