

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041621\
 Data File : PL066242.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Apr 2021 17:09
 Operator : AR\AJ
 Sample : M2050-07
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-5

Manual Integrations
 APPROVED

Ankita
 4/20/2021 11:46:21 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 16 23:08:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 15:37:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.445	4.155	29058501	47168159	11.417	11.726
28) SA Decachlor...	8.171	9.357	29254511	52997584	12.265	16.228 #
Target Compounds						
12) B 4,4'-DDE	5.591	6.541	7155113	8879147	1.918m	2.145m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041621\
Data File : PL066242.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Apr 2021 17:09
Operator : AR\AJ
Sample : M2050-07
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
TP-5


Manual Integrations
APPROVED

Ankita
4/20/2021 11:46:21 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 23:08:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 15:37:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

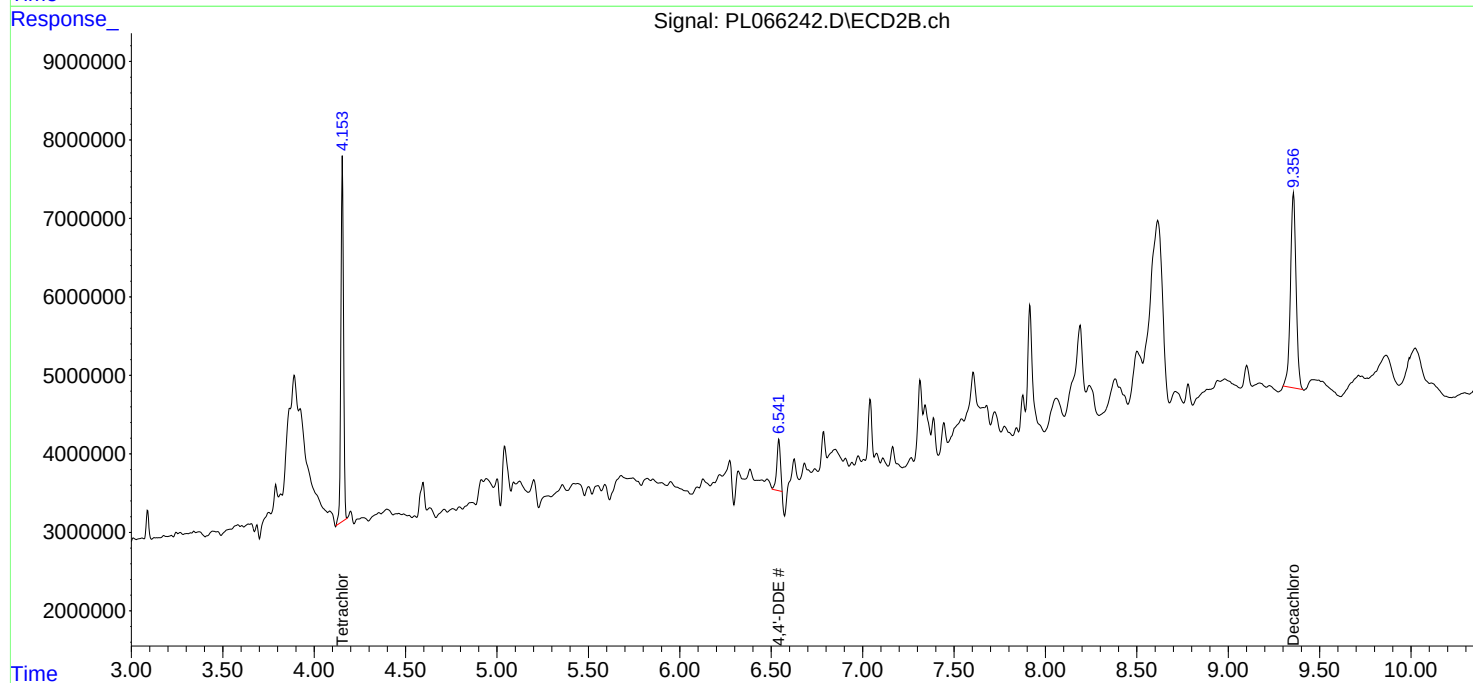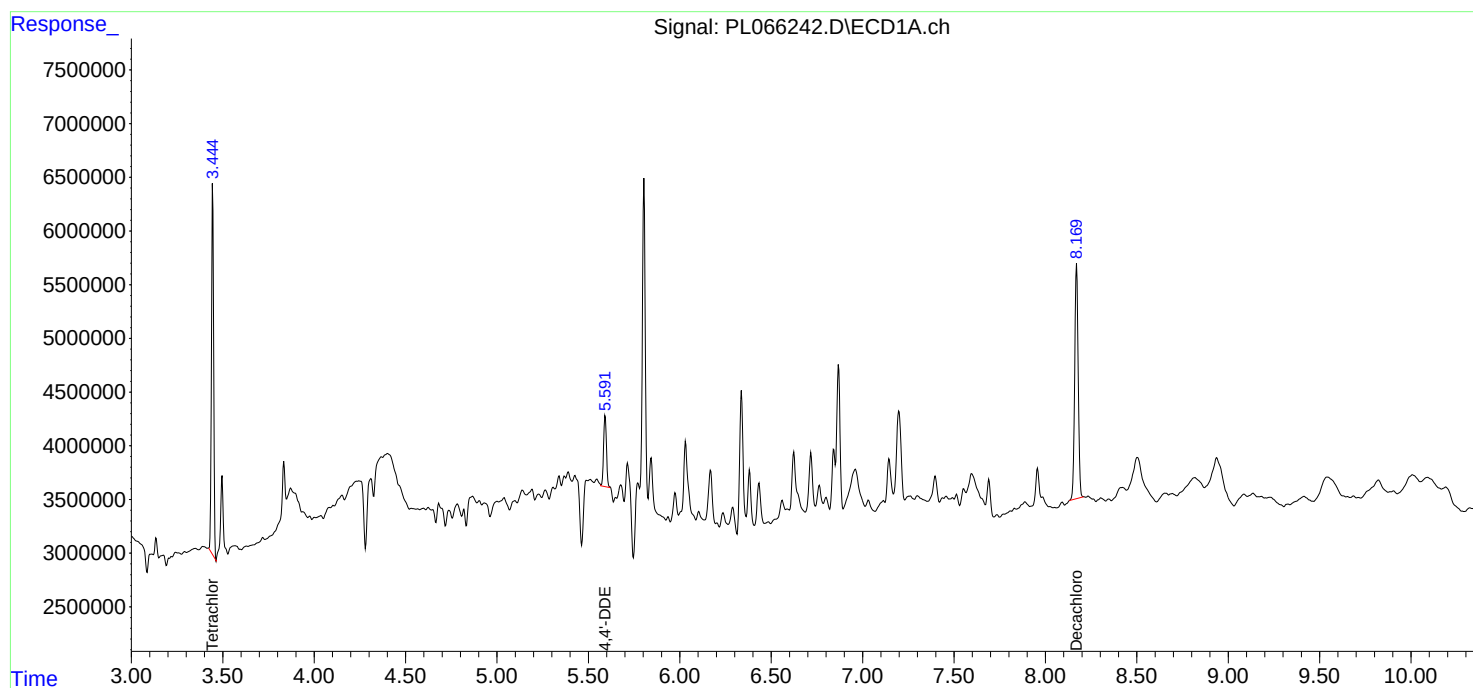

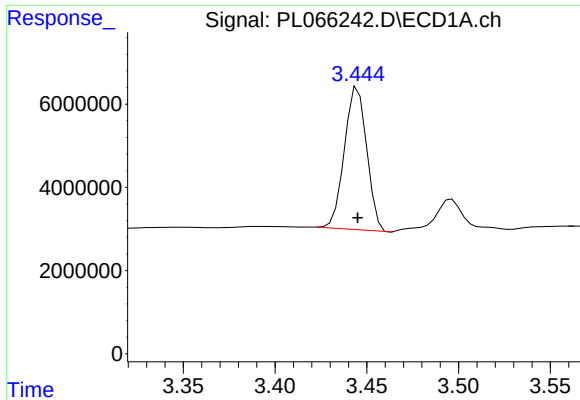


#1 Tetrachloro-m-xylene

R.T.: 3.445 min
Delta R.T.: 0.000 min
Response: 29058501
Conc: 11.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-5


Manual Integrations
APPROVED

Ankita
4/20/2021 11:46:21 AM

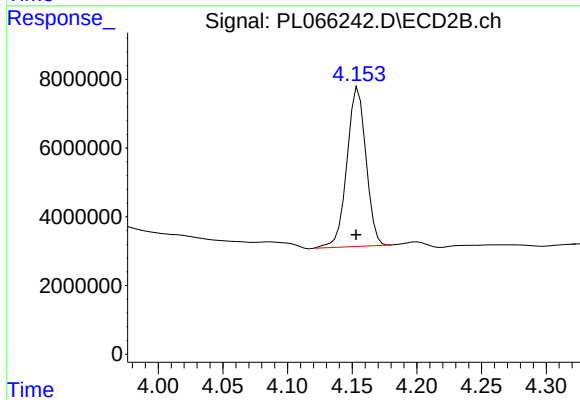


#1 Tetrachloro-m-xylene

R.T.: 4.155 min
Delta R.T.: 0.002 min
Response: 47168159
Conc: 11.73 ng/ml

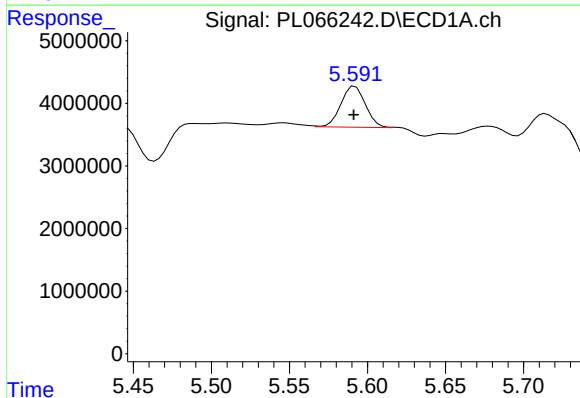


#12 4,4'-DDE

R.T.: 5.591 min
Delta R.T.: 0.000 min
Response: 7155113
Conc: 1.92 ng/ml m

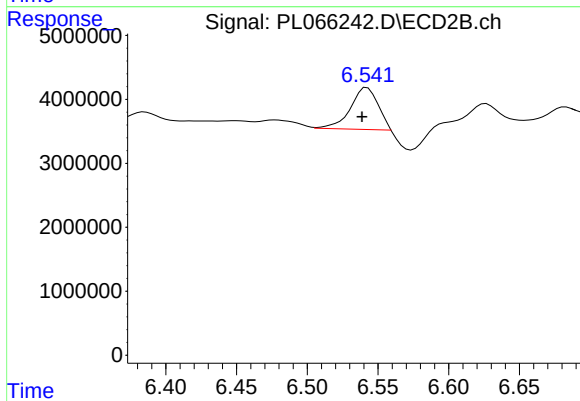

#12 4,4'-DDE

R.T.: 6.541 min
Delta R.T.: 0.002 min
Response: 8879147
Conc: 2.15 ng/ml m

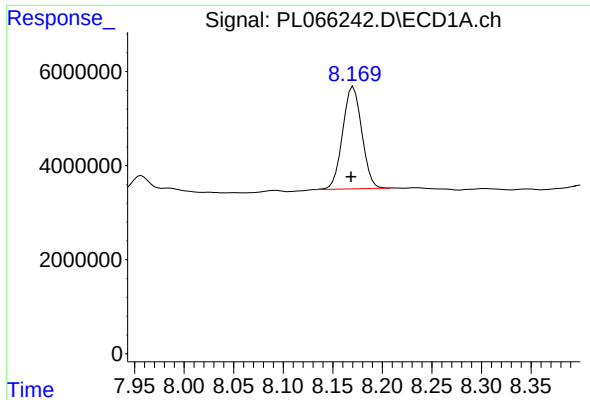


#28 Decachlorobiphenyl

R.T.: 8.171 min
Delta R.T.: 0.002 min
Response: 29254511
Conc: 12.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-5

Manual Integrations
APPROVED

Ankita
4/20/2021 11:46:21 AM

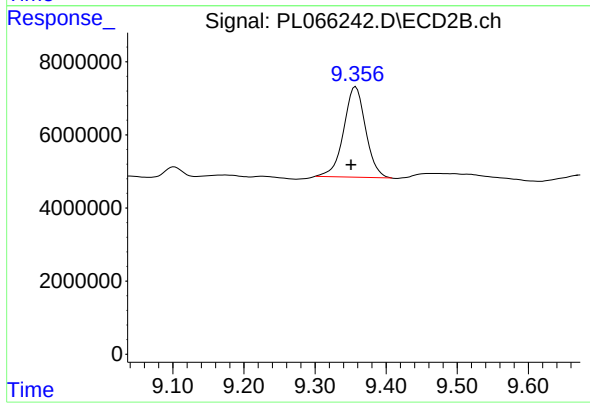

#28 Decachlorobiphenyl

R.T.: 9.357 min
Delta R.T.: 0.006 min
Response: 52997584
Conc: 16.23 ng/ml