

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041621\
 Data File : PL066244.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Apr 2021 17:38
 Operator : AR\AJ
 Sample : M2050-11
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-3

Manual Integrations
 APPROVED

Ankita
 4/20/2021 11:46:24 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 16 23:09:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 15:37:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.445	4.155	24372277	39443176	9.575	9.805
28)	SA Decachlor...	8.170	9.356	22735784	32289443	9.532m	9.887
Target Compounds							
5)	MB Aldrin	4.703	5.679	2432525	7185613	0.621m	1.440m#
12)	B 4,4'-DDE	5.592	6.541	10318817	10658526	2.766	2.575m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041621\
Data File : PL066244.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Apr 2021 17:38
Operator : AR\AJ
Sample : M2050-11
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-3


Manual Integrations
APPROVED

Ankita
4/20/2021 11:46:24 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 23:09:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 15:37:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

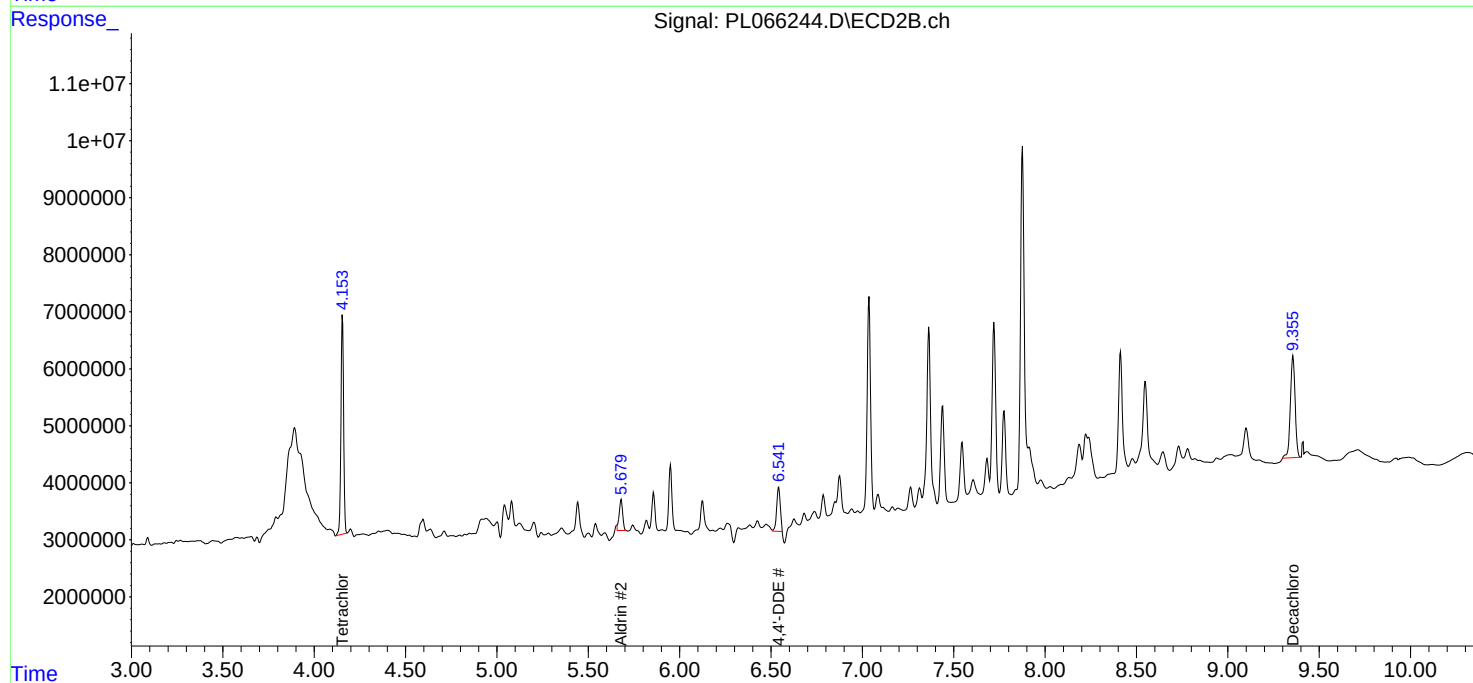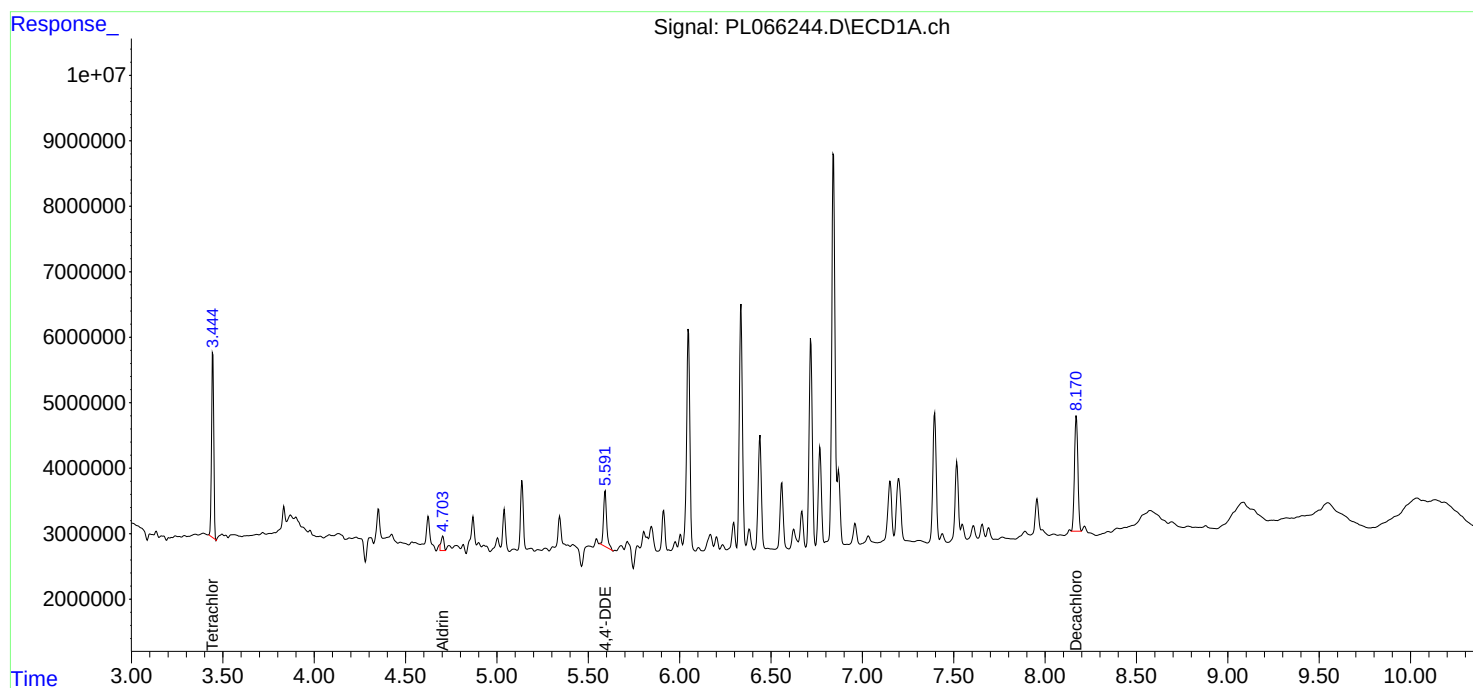

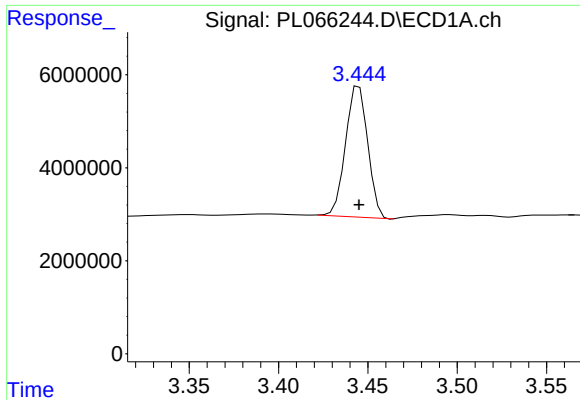


#1 Tetrachloro-m-xylene

R.T.: 3.445 min
Delta R.T.: 0.000 min
Response: 24372277
Conc: 9.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3


Manual Integrations
APPROVED

Ankita
4/20/2021 11:46:24 AM

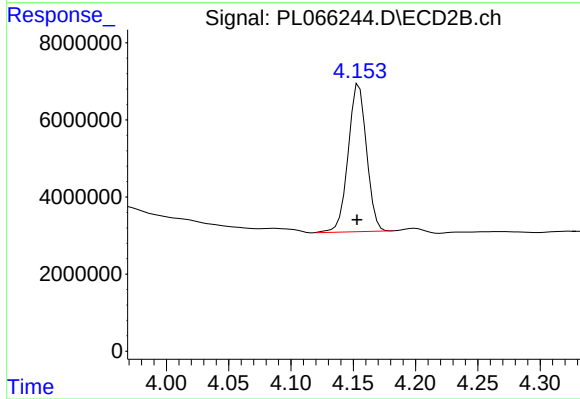


#1 Tetrachloro-m-xylene

R.T.: 4.155 min
Delta R.T.: 0.002 min
Response: 39443176
Conc: 9.81 ng/ml

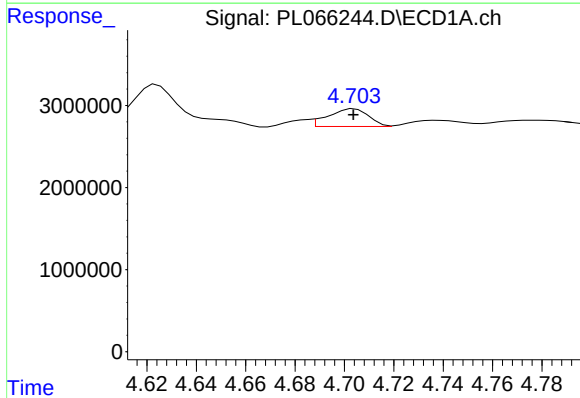


#5 Aldrin

R.T.: 4.703 min
Delta R.T.: 0.000 min
Response: 2432525
Conc: 0.62 ng/ml m

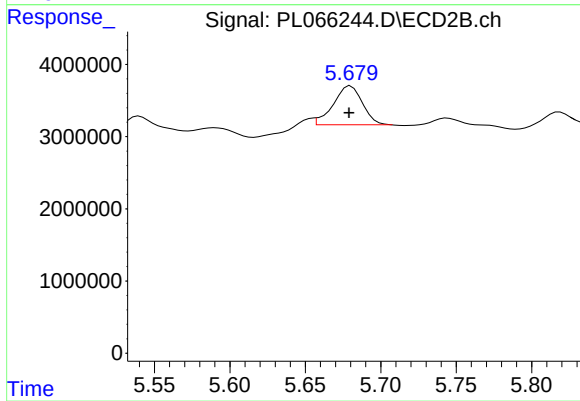

#5 Aldrin

R.T.: 5.679 min
Delta R.T.: 0.000 min
Response: 7185613
Conc: 1.44 ng/ml m

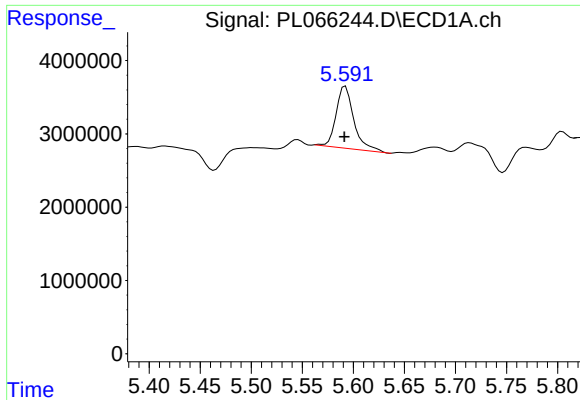


#12 4,4'-DDE

R.T.: 5.592 min
Delta R.T.: 0.000 min
Response: 10318817
Conc: 2.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3


Manual Integrations
APPROVED

Ankita
4/20/2021 11:46:24 AM

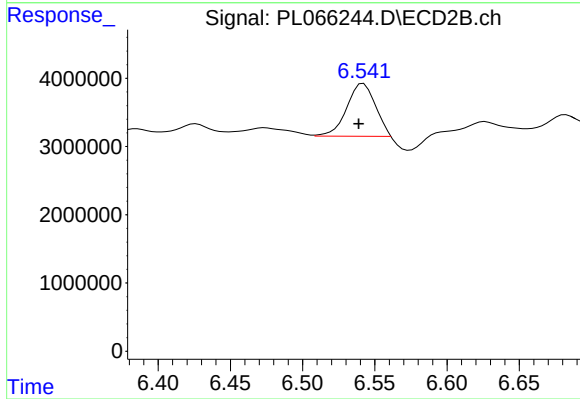


#12 4,4'-DDE

R.T.: 6.541 min
Delta R.T.: 0.002 min
Response: 10658526
Conc: 2.58 ng/ml m

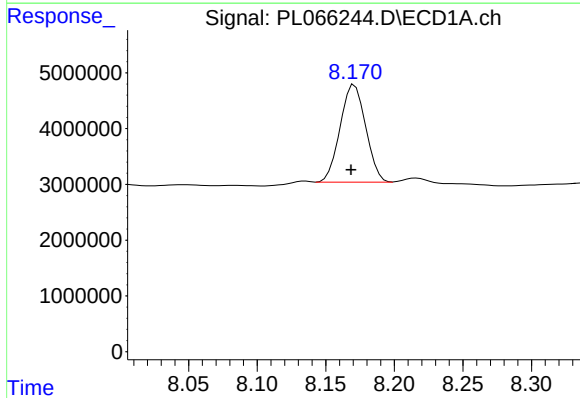

#28 Decachlorobiphenyl

R.T.: 8.170 min
Delta R.T.: 0.001 min
Response: 22735784
Conc: 9.53 ng/ml m

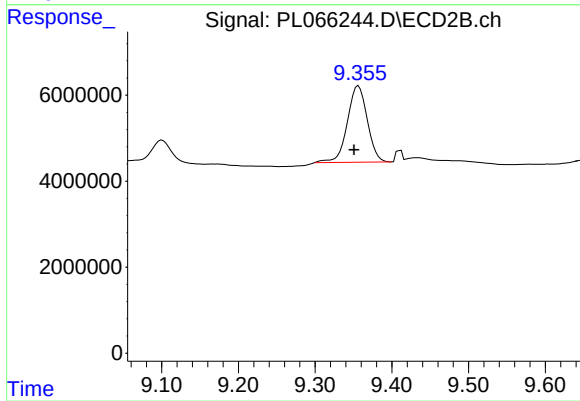

#28 Decachlorobiphenyl

R.T.: 9.356 min
Delta R.T.: 0.006 min
Response: 32289443
Conc: 9.89 ng/ml