

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041621\
 Data File : PL066246.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Apr 2021 18:06
 Operator : AR\AJ
 Sample : M2050-15
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-1

Manual Integrations
 APPROVED

Ankita
 4/20/2021 11:46:30 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 16 23:10:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 15:37:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.445	4.155	24739962	39598213	9.720	9.844
28)	SA Decachlor...	8.172	9.356	20612188	25320694	8.641	7.753
Target Compounds							
11)	B alpha-Chl...	5.424	6.384	1941699	4219182	0.524m	0.933m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041621\
Data File : PL066246.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Apr 2021 18:06
Operator : AR\AJ
Sample : M2050-15
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
TP-1


Manual Integrations
APPROVED

Ankita
4/20/2021 11:46:30 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 23:10:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 15:37:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

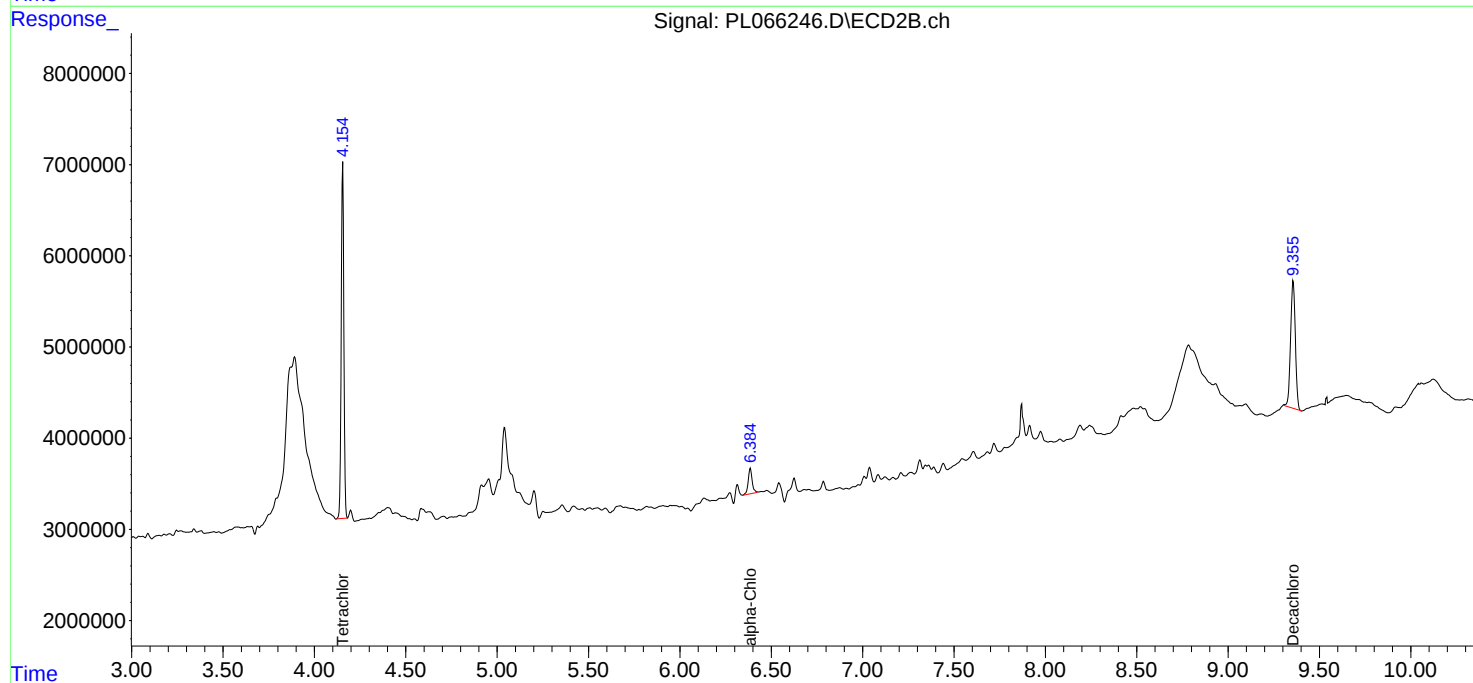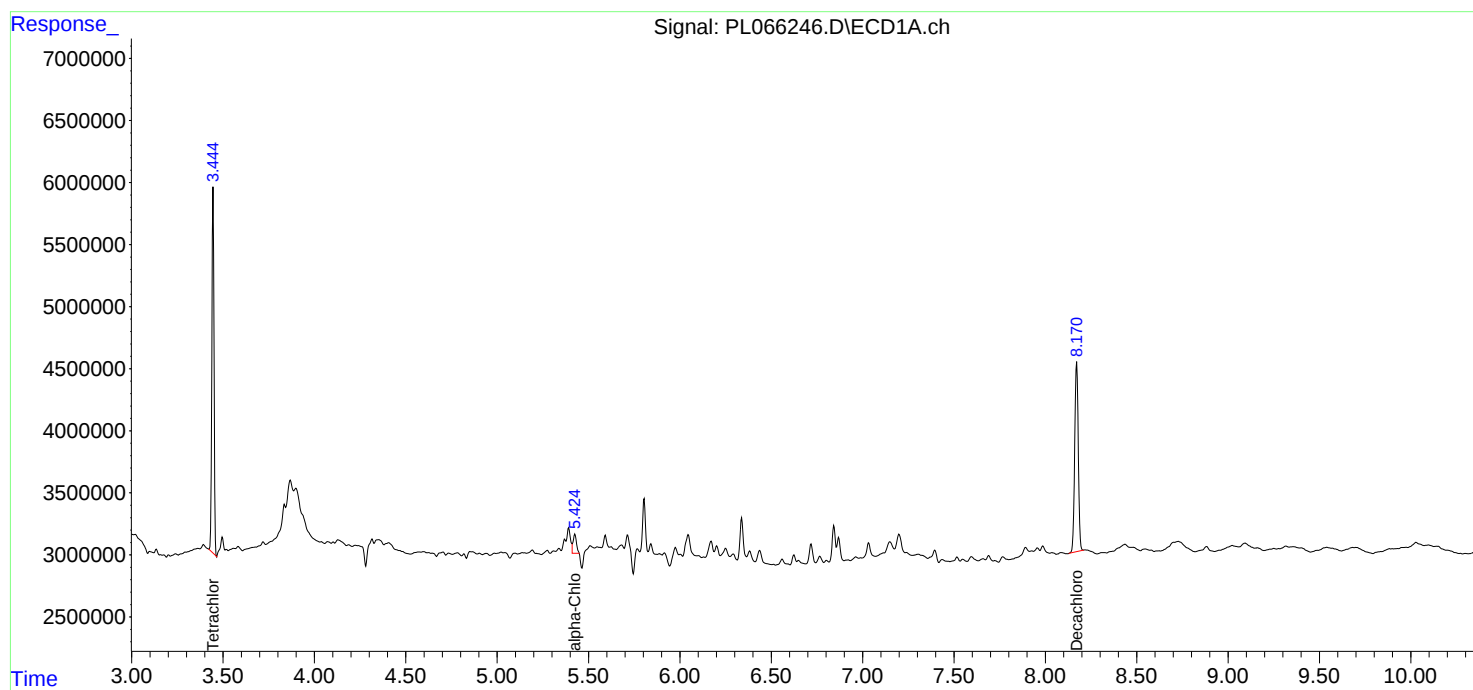

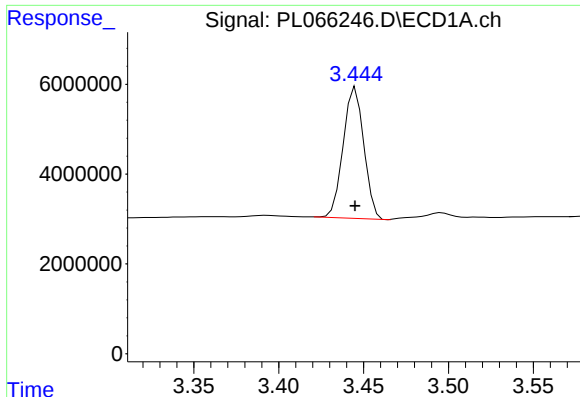


#1 Tetrachloro-m-xylene

R.T.: 3.445 min
Delta R.T.: 0.000 min
Response: 24739962
Conc: 9.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1


Manual Integrations
APPROVED

Ankita
4/20/2021 11:46:30 AM

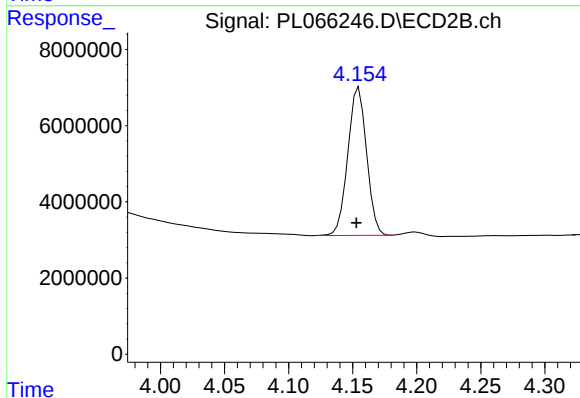


#1 Tetrachloro-m-xylene

R.T.: 4.155 min
Delta R.T.: 0.002 min
Response: 39598213
Conc: 9.84 ng/ml

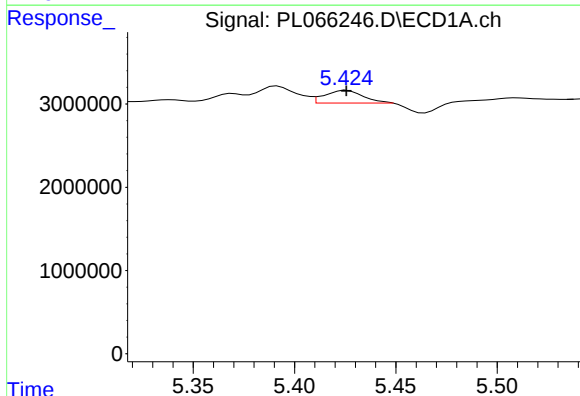


#11 alpha-Chlordane

R.T.: 5.424 min
Delta R.T.: -0.001 min
Response: 1941699
Conc: 0.52 ng/ml m

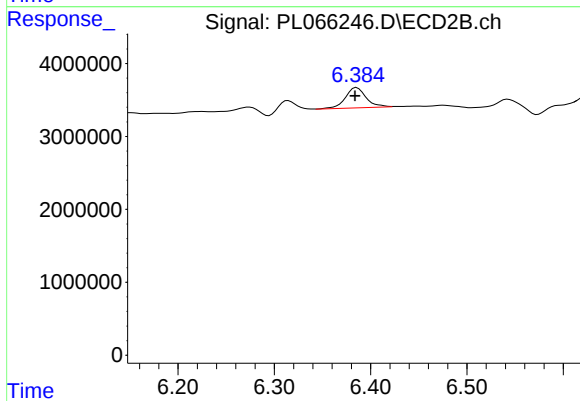

#11 alpha-Chlordane

R.T.: 6.384 min
Delta R.T.: 0.000 min
Response: 4219182
Conc: 0.93 ng/ml m

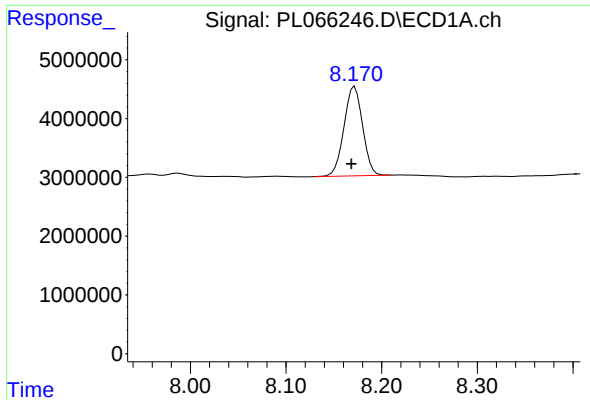


#28 Decachlorobiphenyl

R.T.: 8.172 min
Delta R.T.: 0.003 min
Response: 20612188
Conc: 8.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1

Manual Integrations
APPROVED

Ankita
4/20/2021 11:46:30 AM

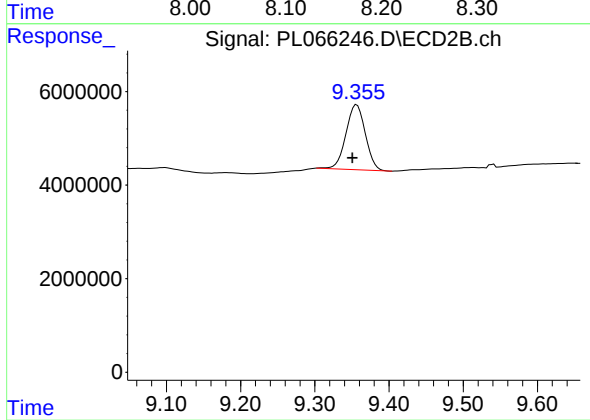

#28 Decachlorobiphenyl

R.T.: 9.356 min
Delta R.T.: 0.006 min
Response: 25320694
Conc: 7.75 ng/ml