

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041719\
 Data File : PL047493.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Apr 2019 12:21
 Operator : AJ\SJ
 Sample : K2423-17
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP5-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 18 01:09:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.356	3.975	132.0E6	43720365	18.148	19.095
28)	SA Decachlor...	8.031	9.026	144.5E6	42579674	17.176	18.365
Target Compounds							
10)	B gamma-Chl...	5.267	6.077	6137861	2360987	0.597	0.832 #
11)	B alpha-Chl...	0.000	6.151	0	3807660	N.D.	1.342 #
25)	Chlordane-3	5.267	6.077	6137861	2360987	5.511	6.192
26)	Chlordane-4	0.000	6.151	0	3807660	N.D.	8.252 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041719\
Data File : PL047493.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Apr 2019 12:21
Operator : AJ\SJ
Sample : K2423-17
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP5-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 18 01:09:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

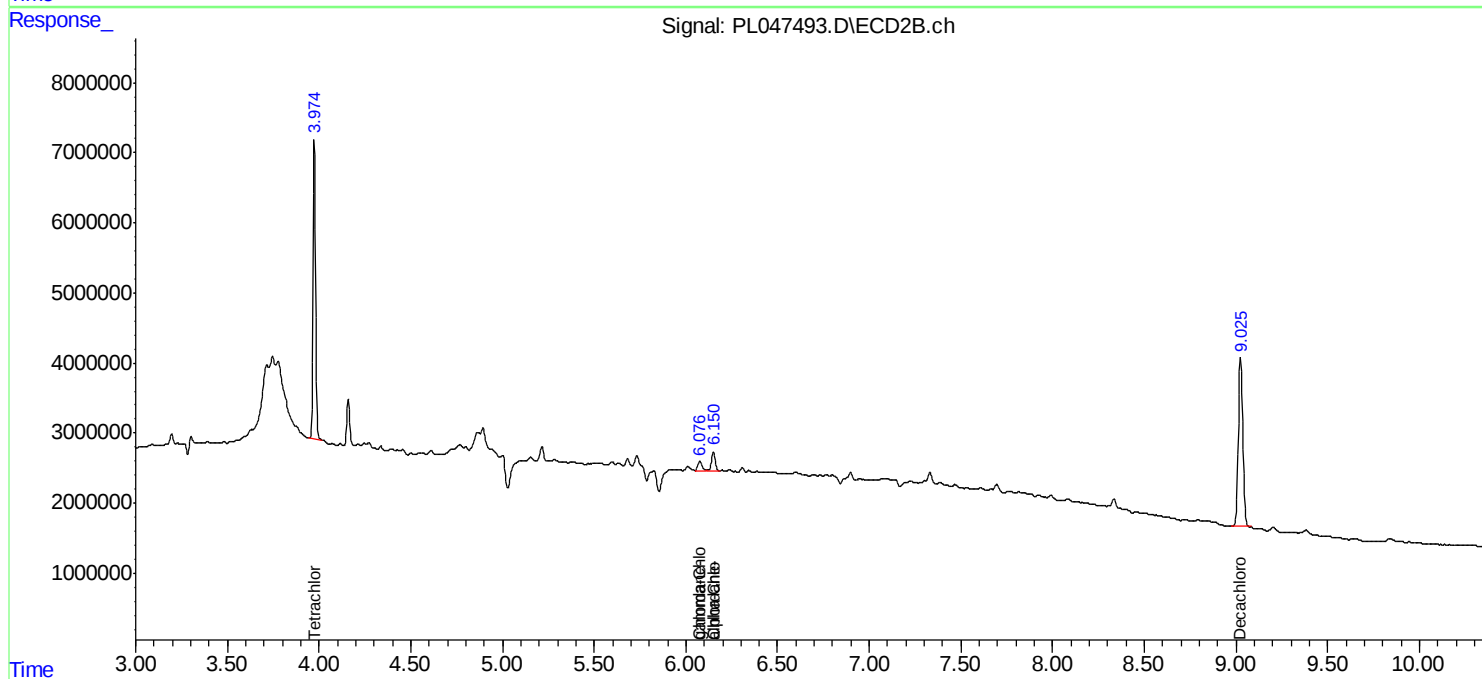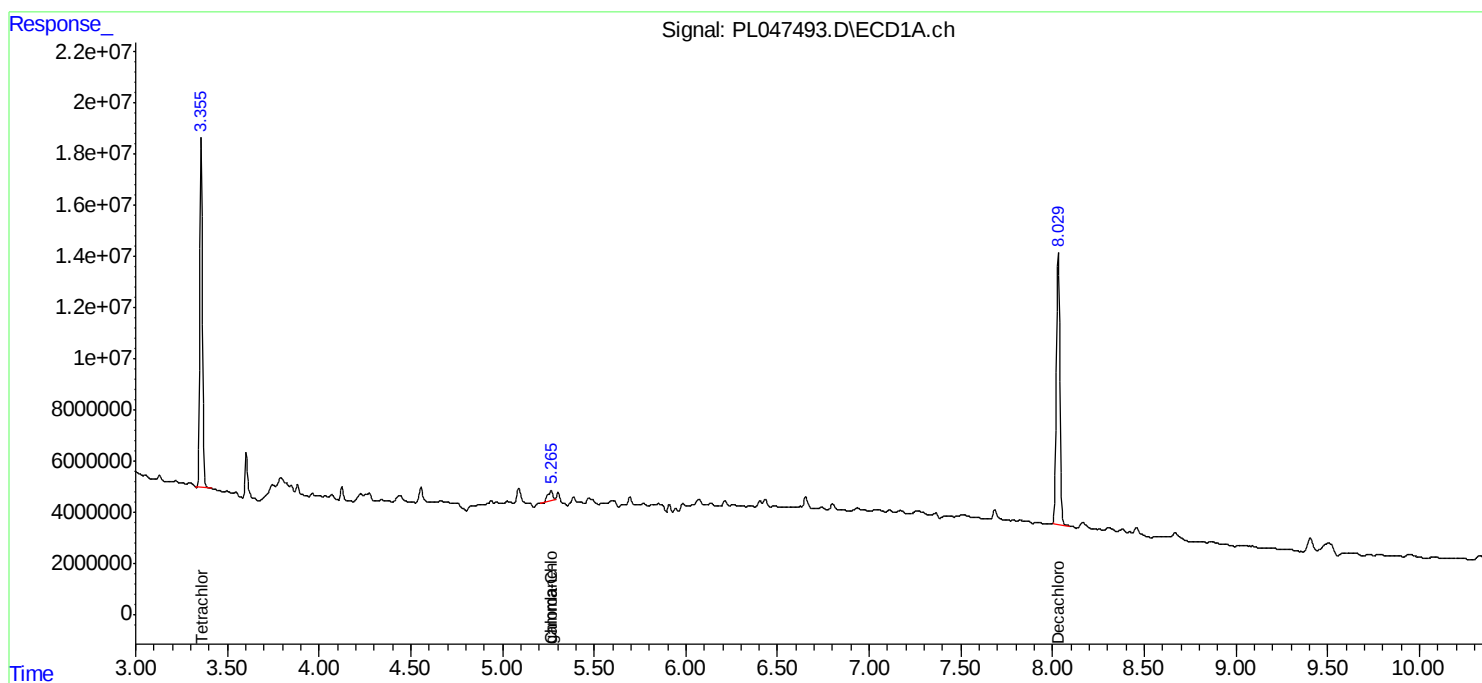


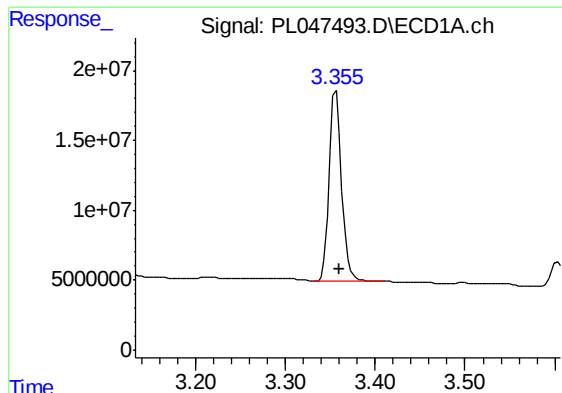

#1 Tetrachloro-m-xylene


R.T.: 3.356 min
Delta R.T.: -0.005 min
Response: 132018360
Conc: 18.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP5-A

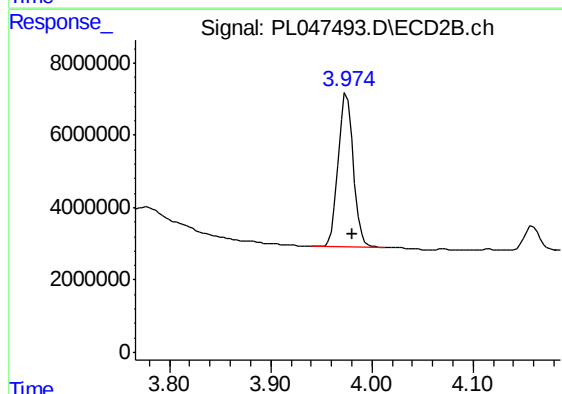


#1 Tetrachloro-m-xylene

R.T.: 3.975 min
Delta R.T.: -0.005 min
Response: 43720365
Conc: 19.10 ng/ml

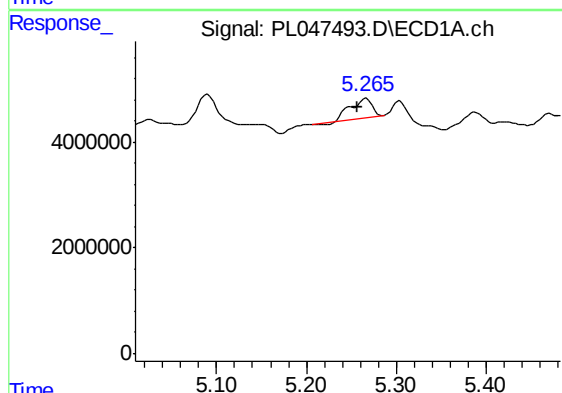


#10 gamma-Chlordane

R.T.: 5.267 min
Delta R.T.: 0.010 min
Response: 6137861
Conc: 0.60 ng/ml

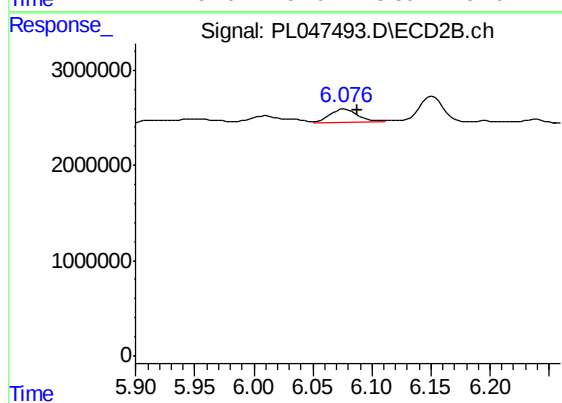

#10 gamma-Chlordane


R.T.: 6.077 min
Delta R.T.: -0.010 min
Response: 2360987
Conc: 0.83 ng/ml

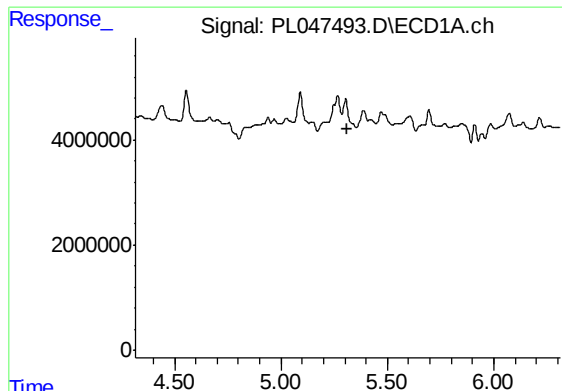

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.314 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP5-A

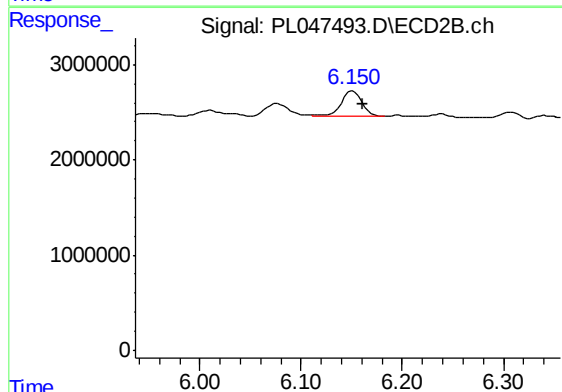


#11 alpha-Chlordane

R.T.: 6.151 min
Delta R.T.: -0.009 min
Response: 3807660
Conc: 1.34 ng/ml

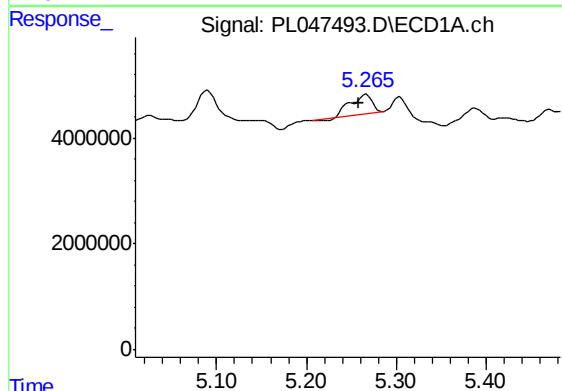


#25 Chlordane-3

R.T.: 5.267 min
Delta R.T.: 0.009 min
Response: 6137861
Conc: 5.51 ng/ml

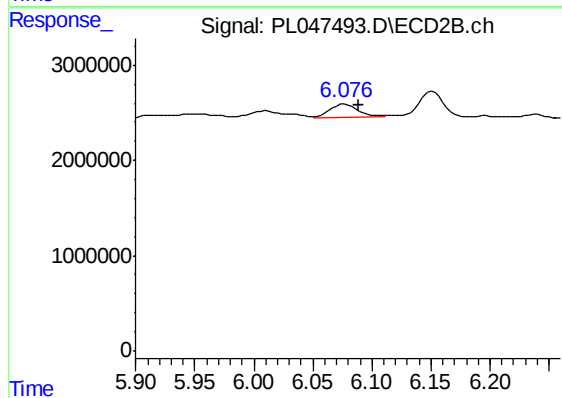

#25 Chlordane-3


R.T.: 6.077 min
Delta R.T.: -0.012 min
Response: 2360987
Conc: 6.19 ng/ml

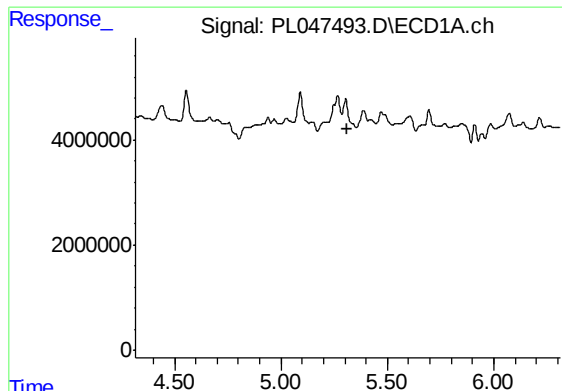

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.314 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP5-A

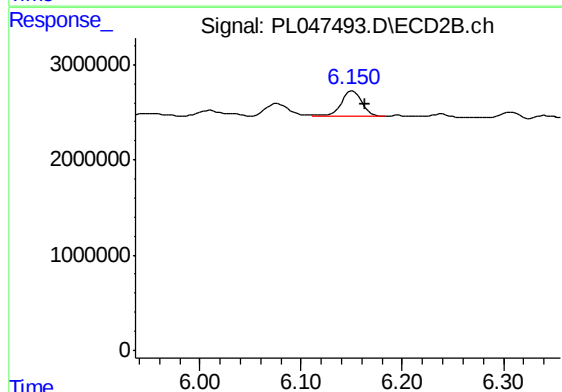


#26 Chlordane-4

R.T.: 6.151 min
Delta R.T.: -0.012 min
Response: 3807660
Conc: 8.25 ng/ml

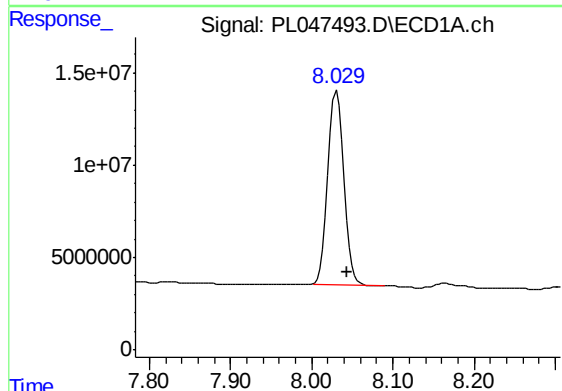

#28 Decachlorobiphenyl

R.T.: 8.031 min
Delta R.T.: -0.013 min
Response: 144469775
Conc: 17.18 ng/ml

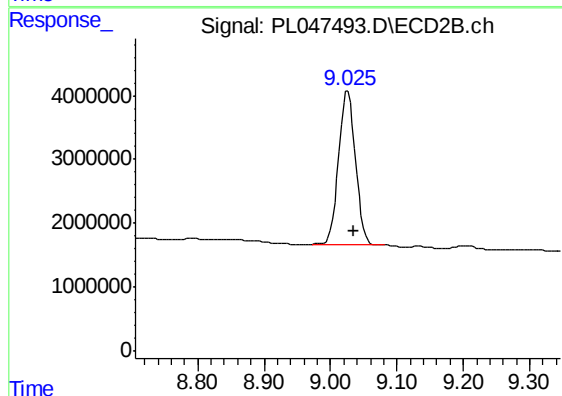

#28 Decachlorobiphenyl

R.T.: 9.026 min
Delta R.T.: -0.009 min
Response: 42579674
Conc: 18.37 ng/ml