

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041719\
 Data File : PL047545.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Apr 2019 02:20
 Operator : AJ\SJ
 Sample : K2442-12
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-21-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 18 05:27:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.357	3.975	137.7E6	45120699	18.925	19.707
28) SA Decachlor...	8.031	9.026	167.0E6	53964574	19.861	23.276
Target Compounds						
2) A alpha-BHC	3.789	0.000	8961877	0	0.768	N.D. #
23) Chlordane-1	4.236f	0.000	10754705	0	31.980	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041719\
Data File : PL047545.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Apr 2019 02:20
Operator : AJ\SJ
Sample : K2442-12
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-21-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 18 05:27:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

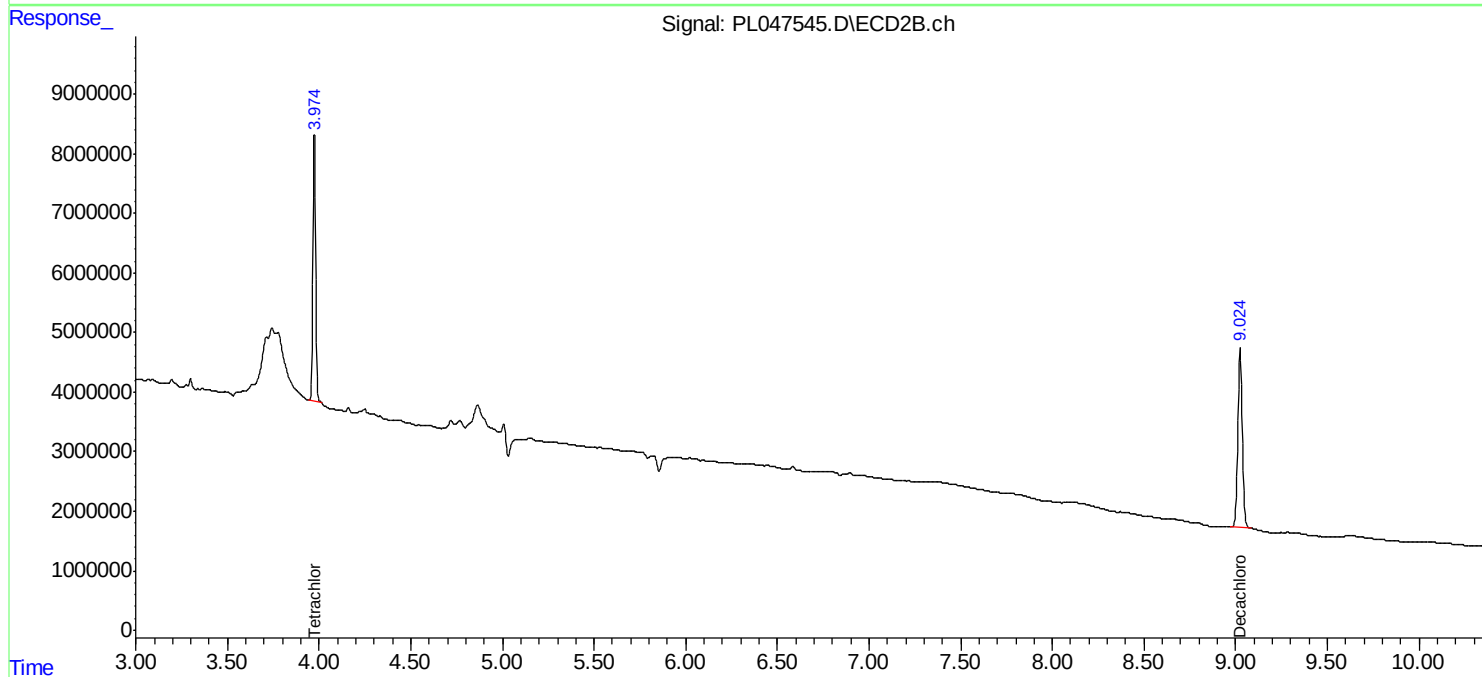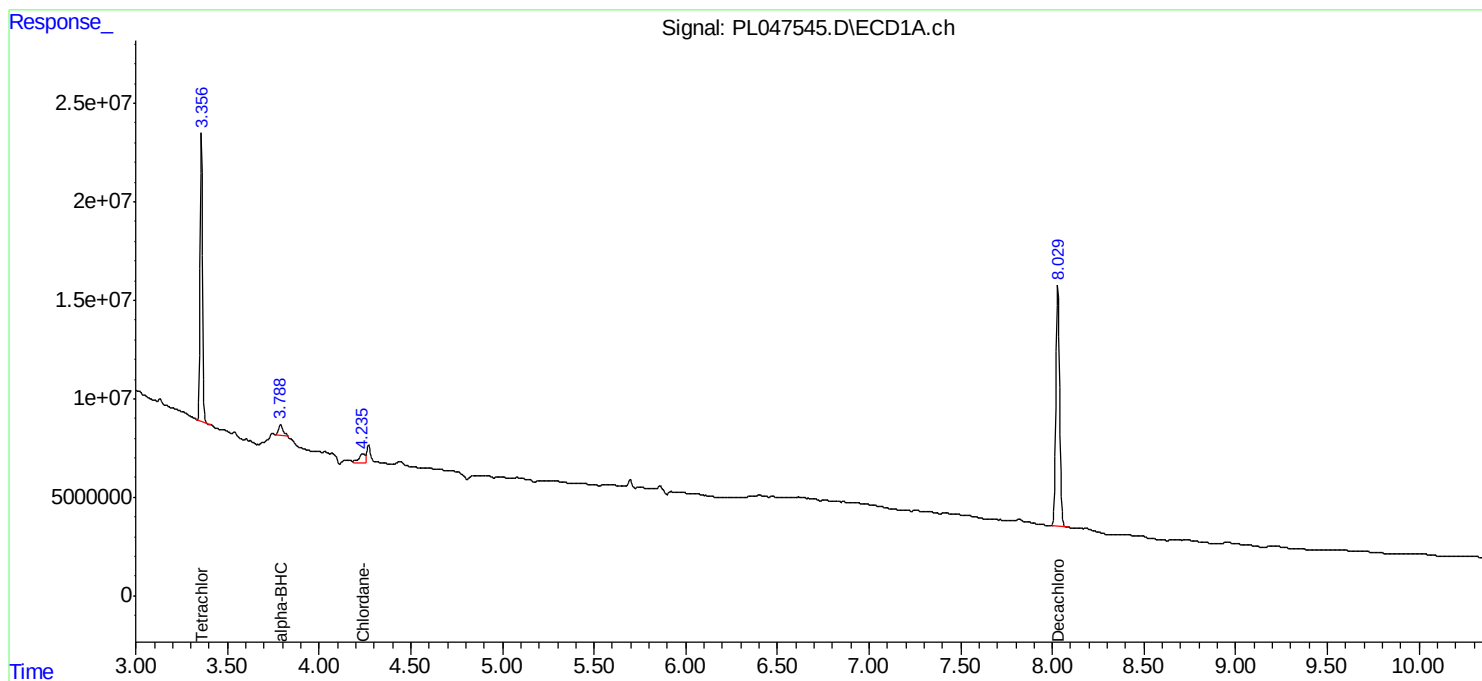


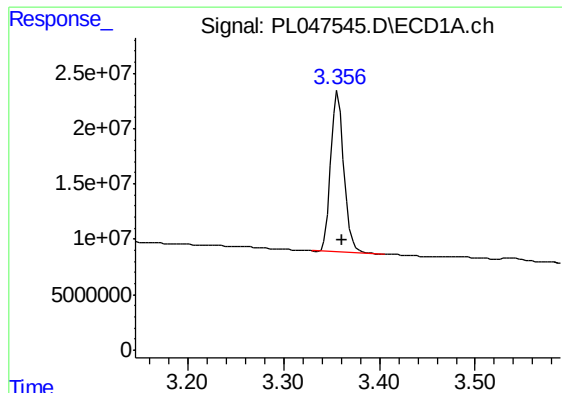

#1 Tetrachloro-m-xylene


R.T.: 3.357 min
Delta R.T.: -0.004 min
Response: 137671440
Conc: 18.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-21-S

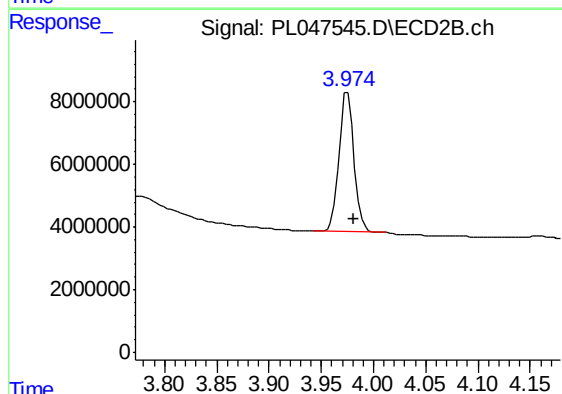


#1 Tetrachloro-m-xylene

R.T.: 3.975 min
Delta R.T.: -0.005 min
Response: 45120699
Conc: 19.71 ng/ml

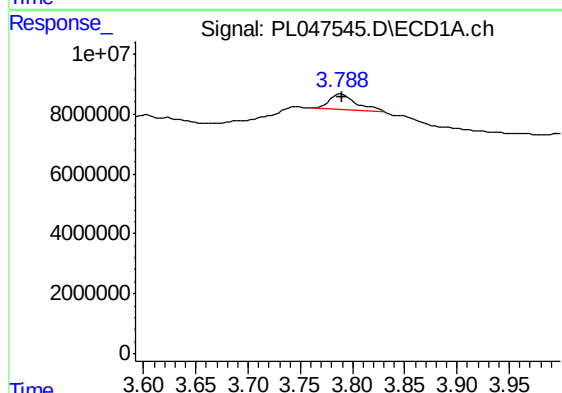


#2 alpha-BHC

R.T.: 3.789 min
Delta R.T.: -0.001 min
Response: 8961877
Conc: 0.77 ng/ml

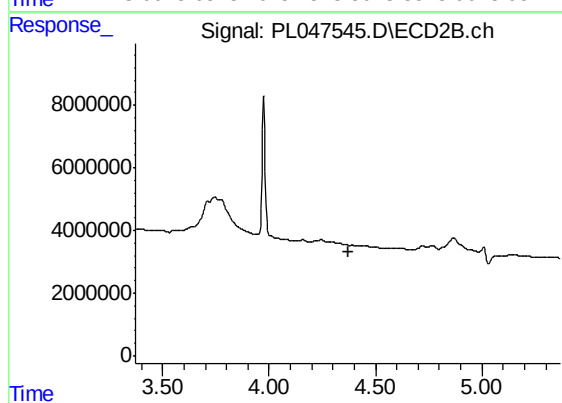

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.371 min
Response: 0
Conc: N.D.

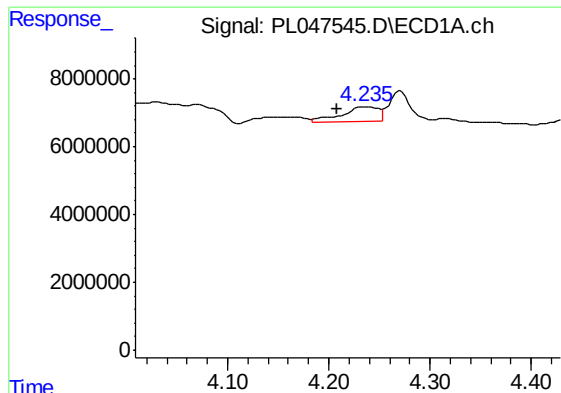

#23 Chlordane-1


R.T.: 4.236 min
Delta R.T.: 0.028 min
Response: 10754705
Conc: 31.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-21-S

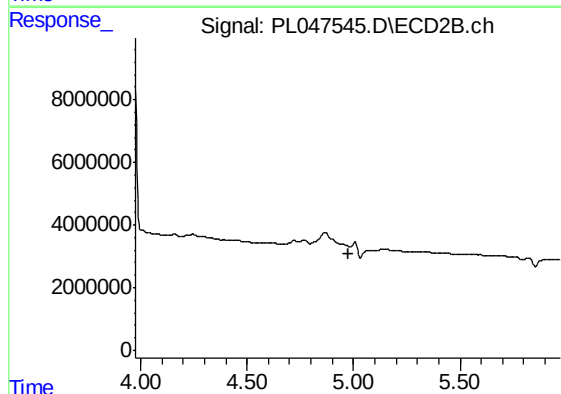


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.975 min
Response: 0
Conc: N.D.

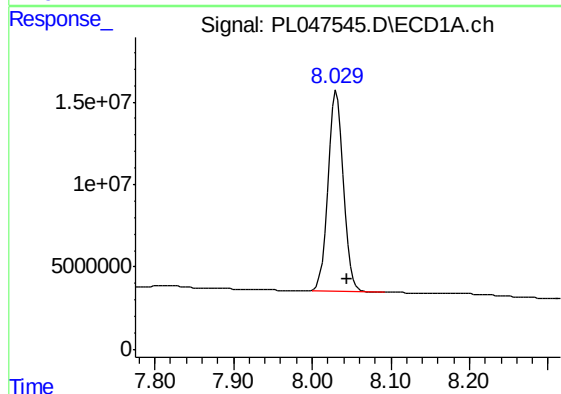

#28 Decachlorobiphenyl

R.T.: 8.031 min
Delta R.T.: -0.013 min
Response: 167047759
Conc: 19.86 ng/ml

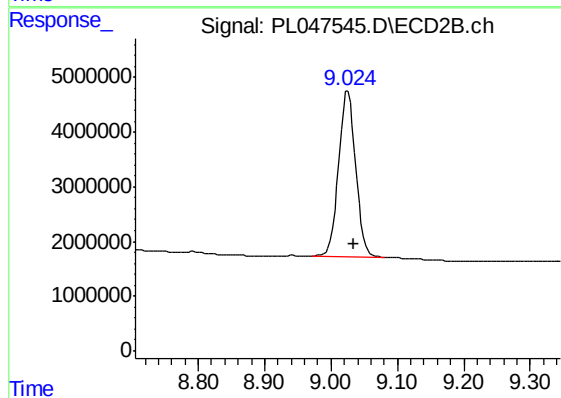

#28 Decachlorobiphenyl

R.T.: 9.026 min
Delta R.T.: -0.009 min
Response: 53964574
Conc: 23.28 ng/ml