

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041719\
 Data File : PL047518.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Apr 2019 19:38
 Operator : AJ\SJ
 Sample : K2437-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-PS-01-046

Manual Integrations
 APPROVED

Sohil
 4/18/2019 10:45:17 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 18 01:17:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.357	3.976	66265796	23208176	9.109	10.136
28)	SA Decachlor...	8.031	9.026	83210511	25777817	9.893	11.118
Target Compounds							
12)	B 4,4'-DDE	5.470	6.307	3075819	1062905	0.334m	0.428m#
17)	MA 4,4'-DDT	6.215	7.096	2917870	1153655	0.385m	0.550m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL0471719\
Data File : PL047518.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Apr 2019 19:38
Operator : AJ\SJ
Sample : K2437-01
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
FK-PS-01-046


Manual Integrations
APPROVED

Sohil
4/18/2019 10:45:17 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 18 01:17:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

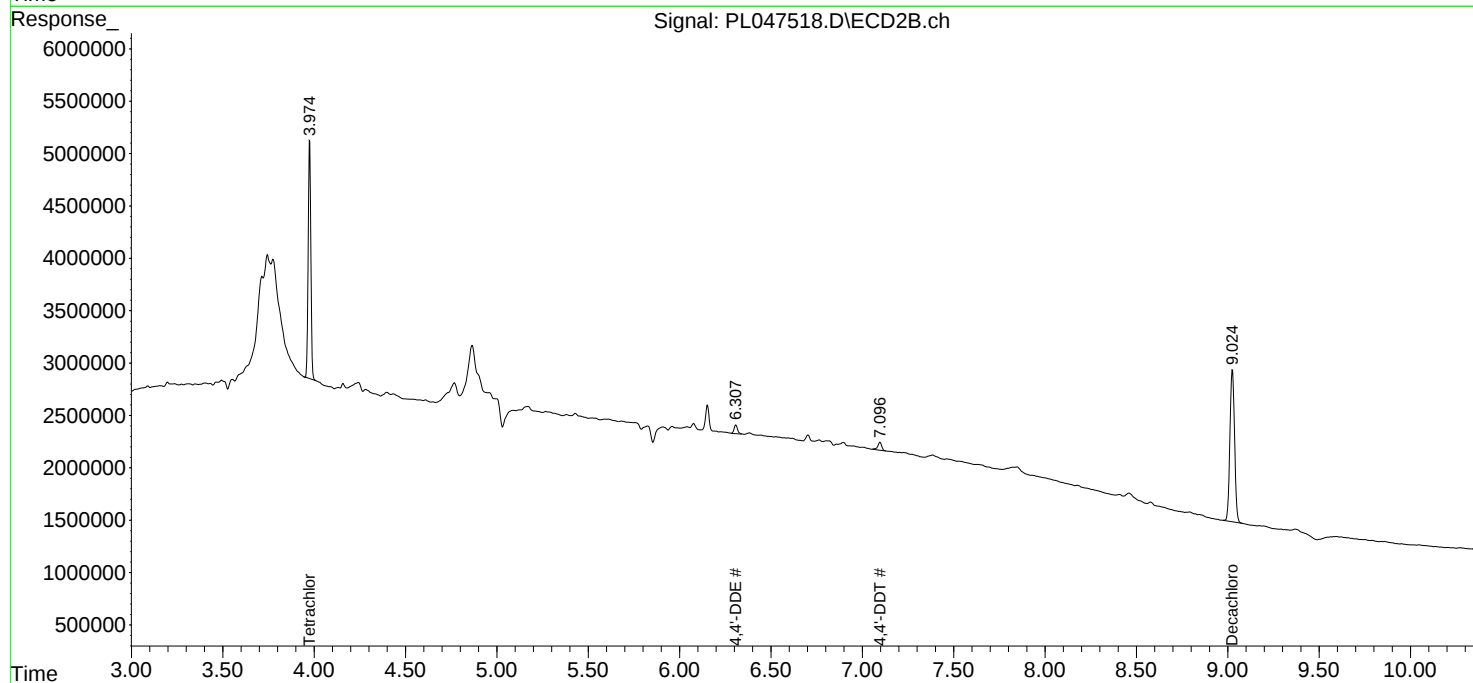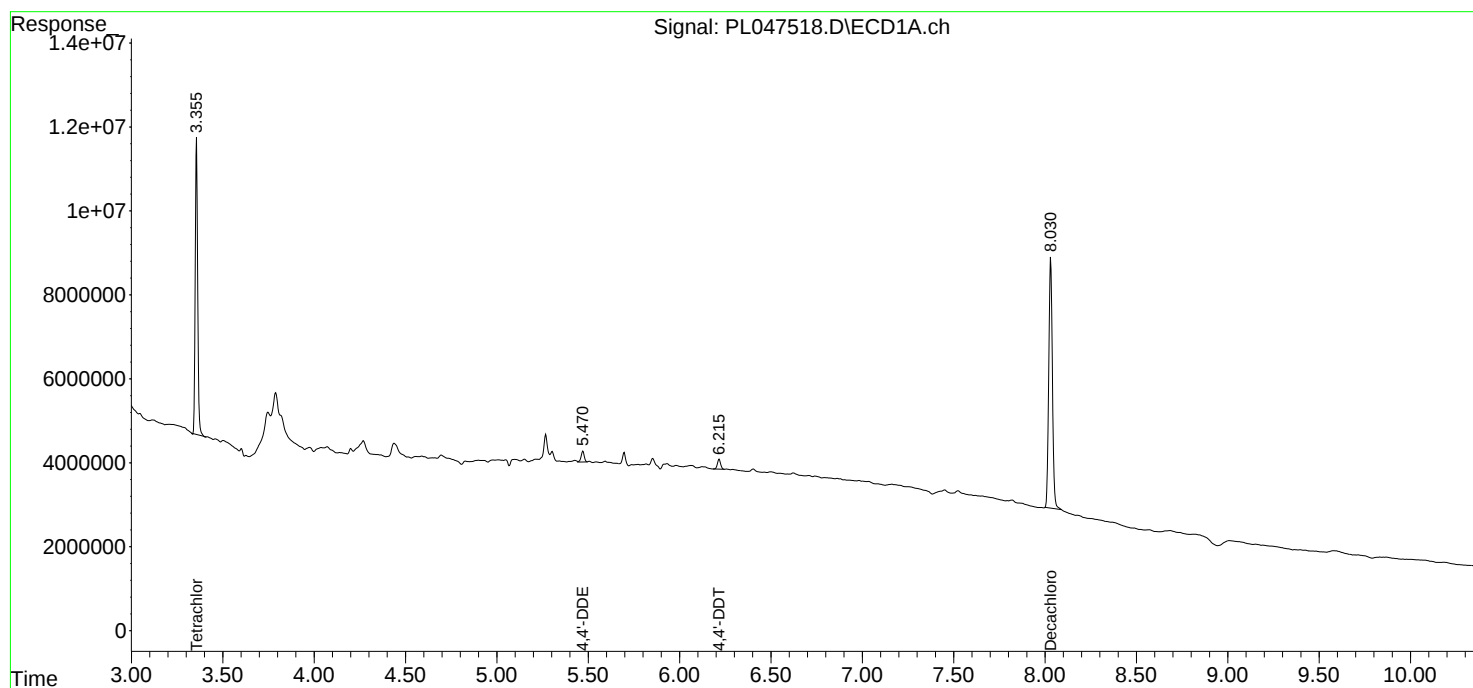

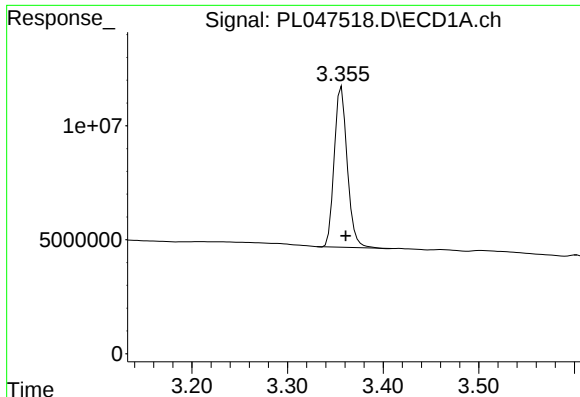


#1 Tetrachloro-m-xylene

R.T.: 3.357 min
Delta R.T.: -0.004 min
Response: 66265796
Conc: 9.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-046


Manual Integrations
APPROVED

Sohil
4/18/2019 10:45:17 AM

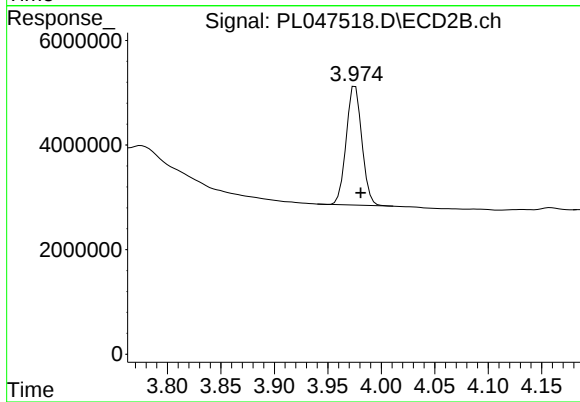


#1 Tetrachloro-m-xylene

R.T.: 3.976 min
Delta R.T.: -0.005 min
Response: 23208176
Conc: 10.14 ng/ml

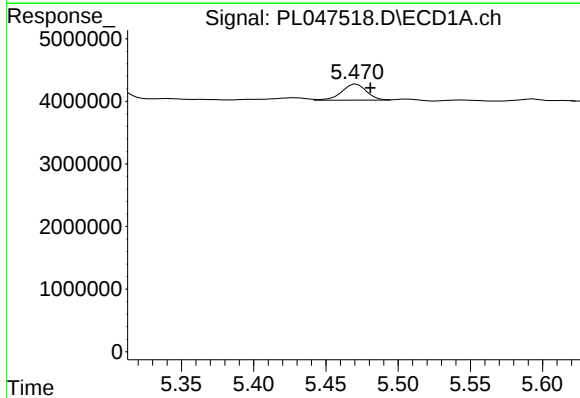


#12 4,4'-DDE

R.T.: 5.470 min
Delta R.T.: -0.011 min
Response: 3075819
Conc: 0.33 ng/ml m

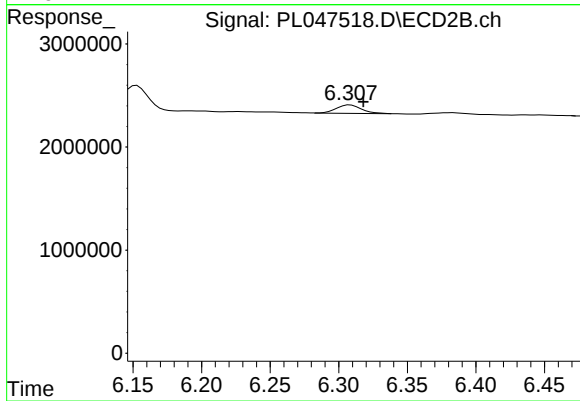

#12 4,4'-DDE

R.T.: 6.307 min
Delta R.T.: -0.011 min
Response: 1062905
Conc: 0.43 ng/ml m

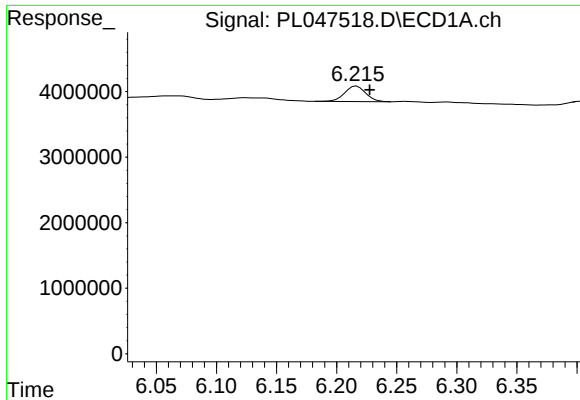


#17 4,4'-DDT

R.T.: 6.215 min
Delta R.T.: -0.012 min
Response: 2917870
Conc: 0.39 ng/ml m

Instrument :
ECD_L
ClientSampleId :
FK-PS-01-046


Manual Integrations
APPROVED

Sohil
4/18/2019 10:45:17 AM

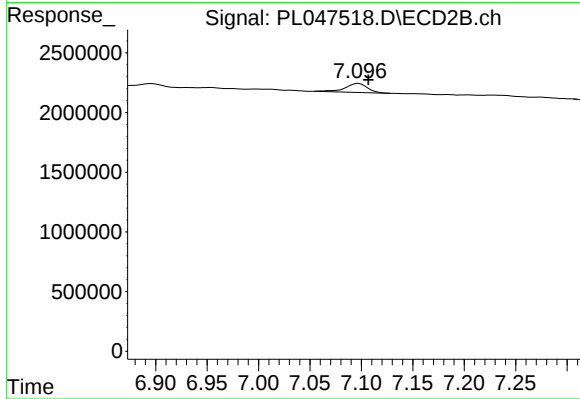


#17 4,4'-DDT

R.T.: 7.096 min
Delta R.T.: -0.011 min
Response: 1153655
Conc: 0.55 ng/ml m

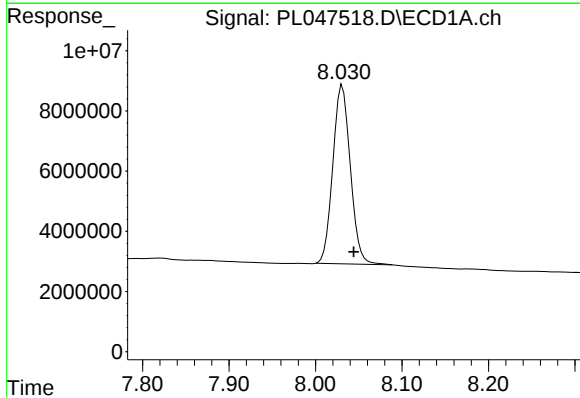

#28 Decachlorobiphenyl

R.T.: 8.031 min
Delta R.T.: -0.013 min
Response: 83210511
Conc: 9.89 ng/ml

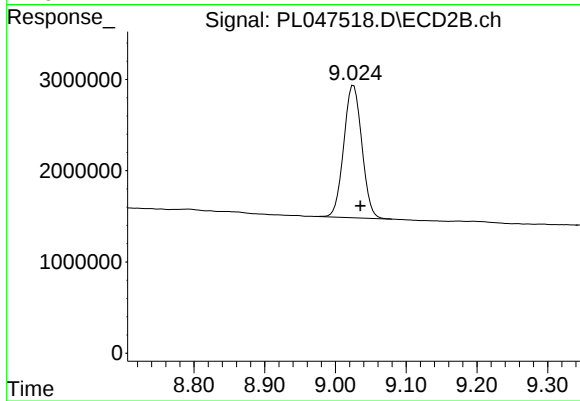

#28 Decachlorobiphenyl

R.T.: 9.026 min
Delta R.T.: -0.009 min
Response: 25777817
Conc: 11.12 ng/ml