

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041720\
 Data File : PL058132.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Apr 2020 13:26
 Operator : AJ\MA
 Sample : PB128300BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB128300BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 18 00:31:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.461	3.954	208.5E6	42249792	20.683	19.469
28)	SA Decachlor...	8.208	8.976	202.3E6	43360247	19.628	19.411
Target Compounds							
4)	MA Heptachlor	0.000	5.130	0	8529195	N.D.	2.541 #
5)	MB Aldrin	4.726	0.000	1413586	0	0.096	N.D. #
6)	B beta-BHC	0.000	4.817f	0	1632125	N.D.	1.175 #
10)	B gamma-Chl...	0.000	6.044	0	798206	N.D.	0.246 #
11)	B alpha-Chl...	0.000	6.097f	0	551488	N.D.	0.169 #
15)	B Endosulfa...	0.000	6.866	0	1192718	N.D.	0.460 #
23)	Chlordane-1	4.331	0.000	18672330	0	50.486	N.D. #
25)	Chlordane-3	0.000	6.044	0	798206	N.D.	1.845 #
26)	Chlordane-4	0.000	6.097f	0	551488	N.D.	1.051 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041720\
Data File : PL058132.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Apr 2020 13:26
Operator : AJ\MA
Sample : PB128300BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB128300BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 18 00:31:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

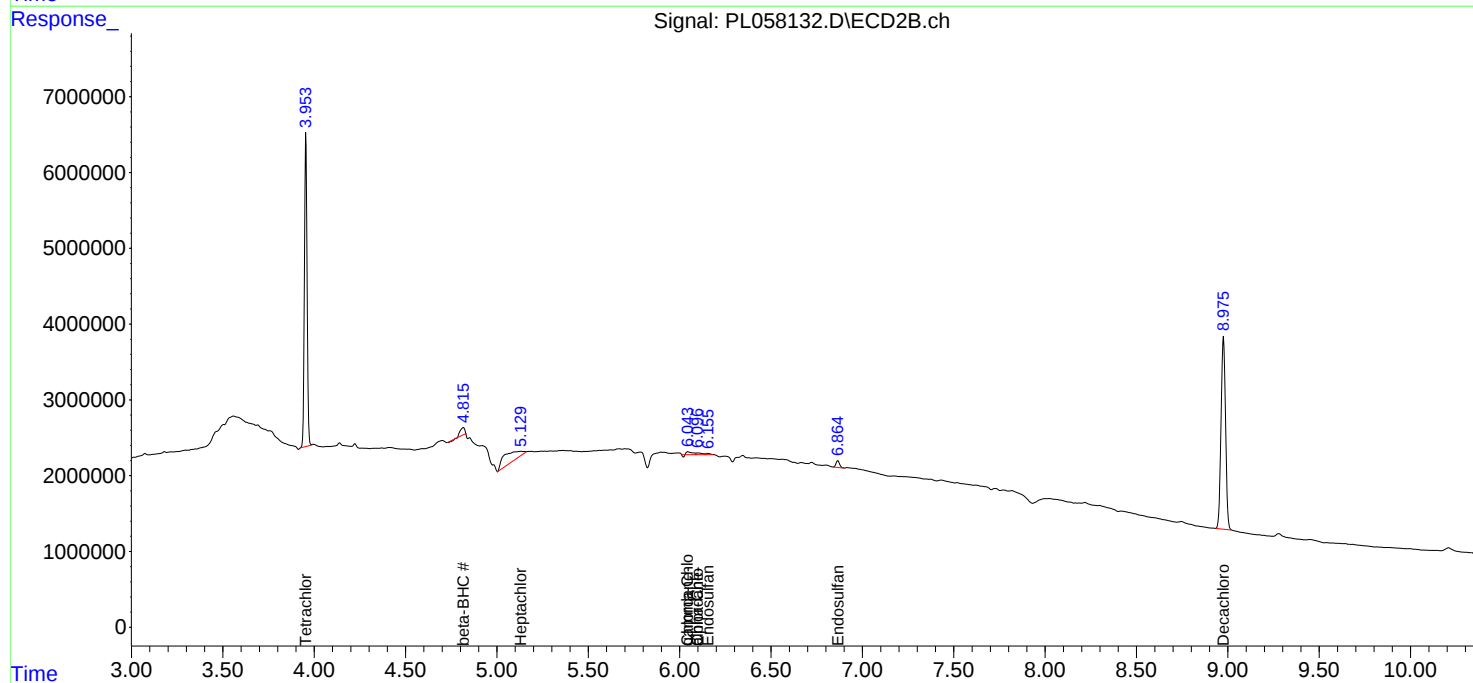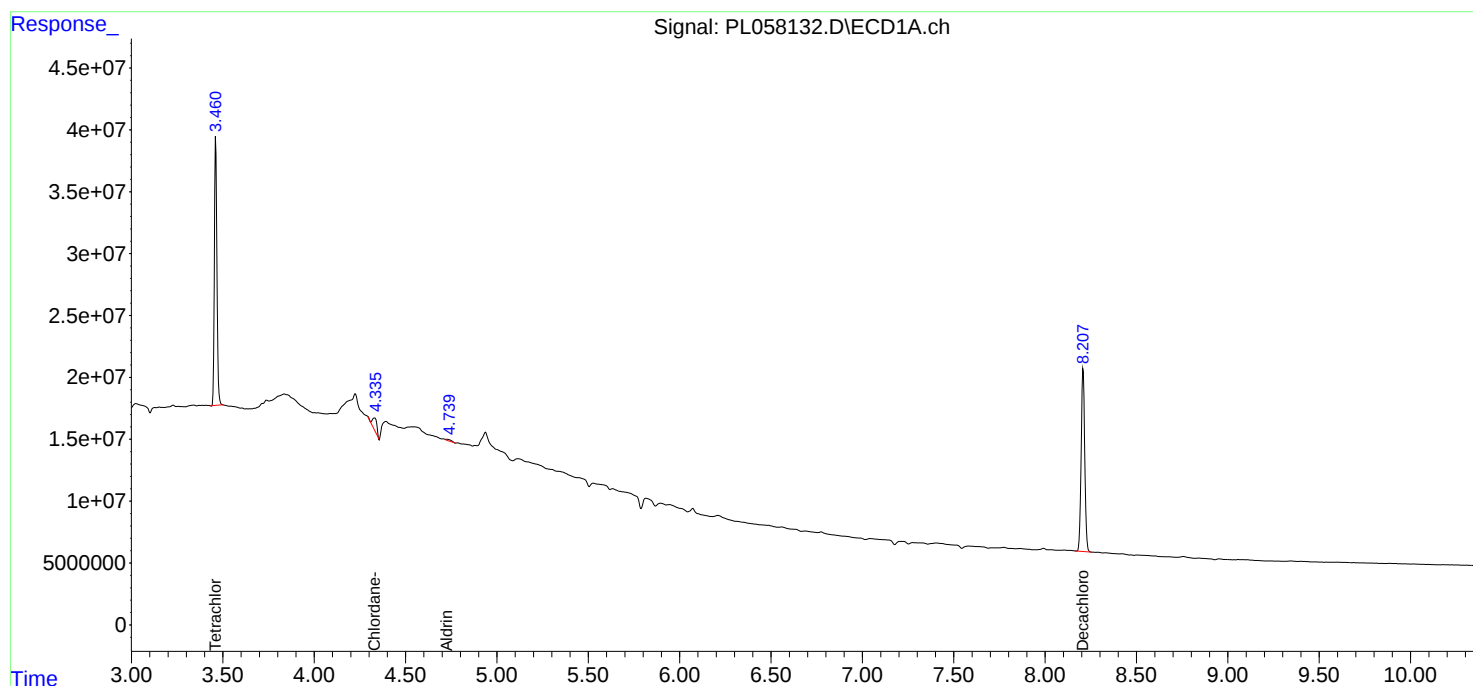


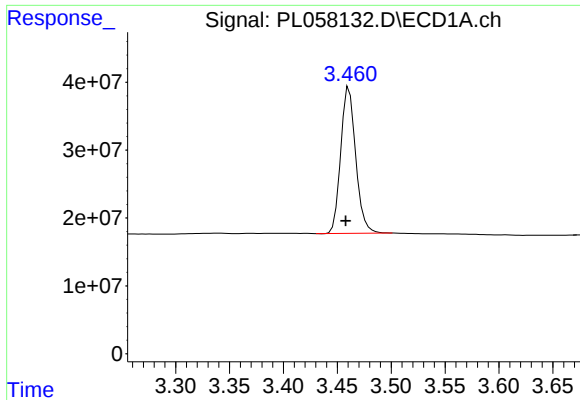

#1 Tetrachloro-m-xylene


R.T.: 3.461 min
Delta R.T.: 0.003 min
Response: 208506429
Conc: 20.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB128300BL

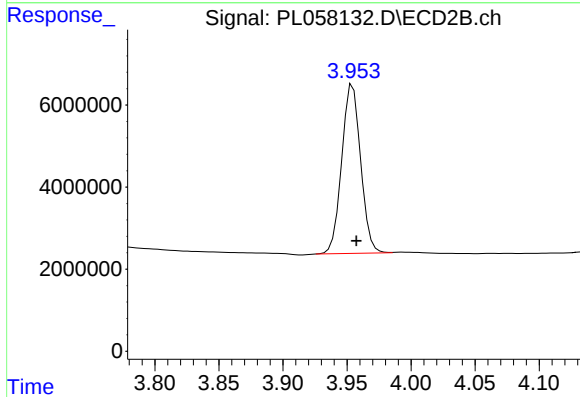


#1 Tetrachloro-m-xylene

R.T.: 3.954 min
Delta R.T.: -0.003 min
Response: 42249792
Conc: 19.47 ng/ml

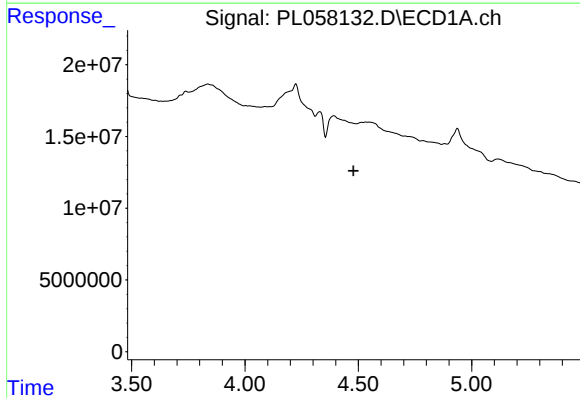


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.479 min
Response: 0
Conc: N.D.

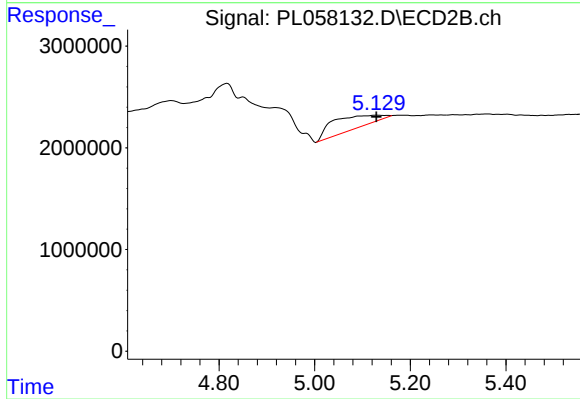

#4 Heptachlor


R.T.: 5.130 min
Delta R.T.: 0.002 min
Response: 8529195
Conc: 2.54 ng/ml

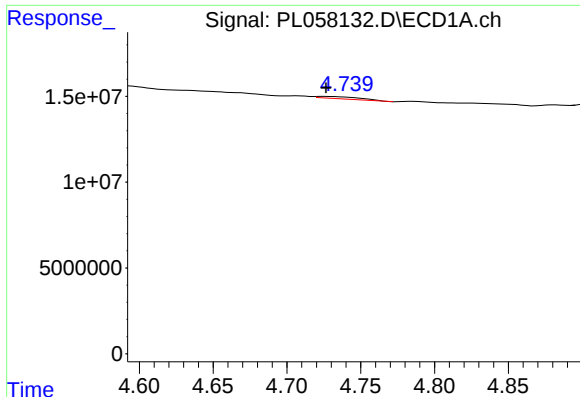

#5 Aldrin


R.T.: 4.726 min
Delta R.T.: 0.000 min
Response: 1413586
Conc: 0.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB128300BL

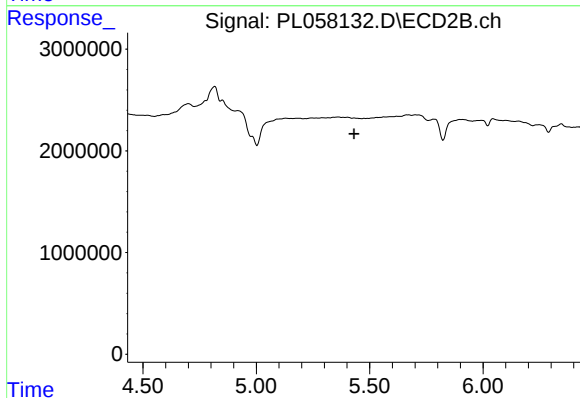


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.431 min
Response: 0
Conc: N.D.

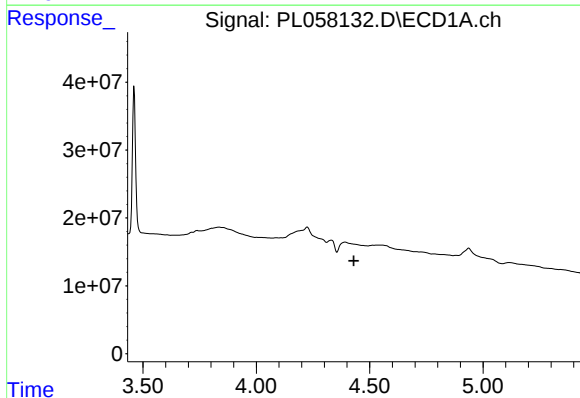


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.430 min
Response: 0
Conc: N.D.

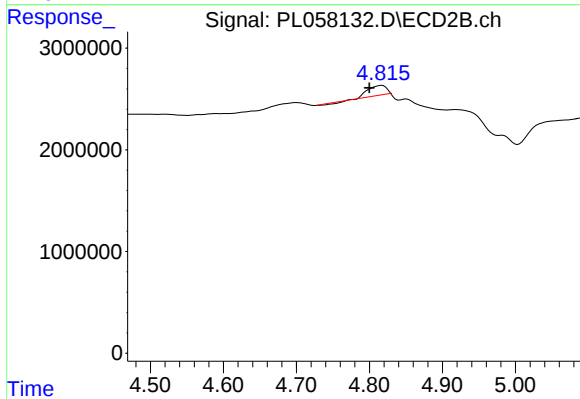

#6 beta-BHC


R.T.: 4.817 min
Delta R.T.: 0.017 min
Response: 1632125
Conc: 1.18 ng/ml

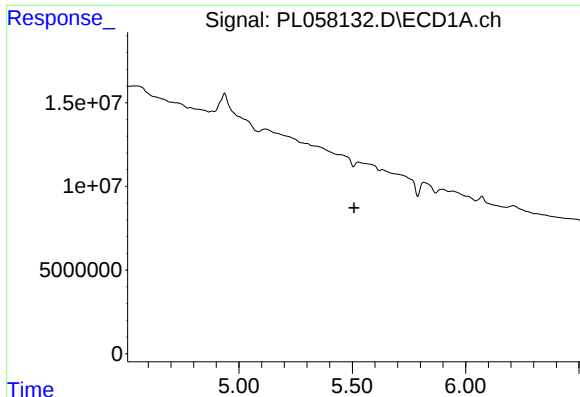

#9 Endosulfan I


R.T.: 5.528 min
Delta R.T.: 0.019 min
Response: -5845679
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB128300BL

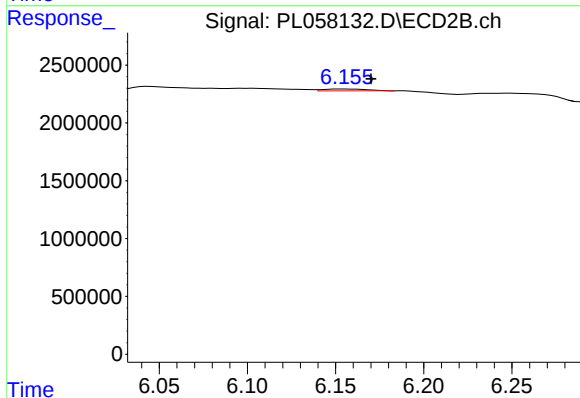


#9 Endosulfan I

R.T.: 6.156 min
Delta R.T.: -0.014 min
Response: 275408
Conc: 0.09 ng/ml

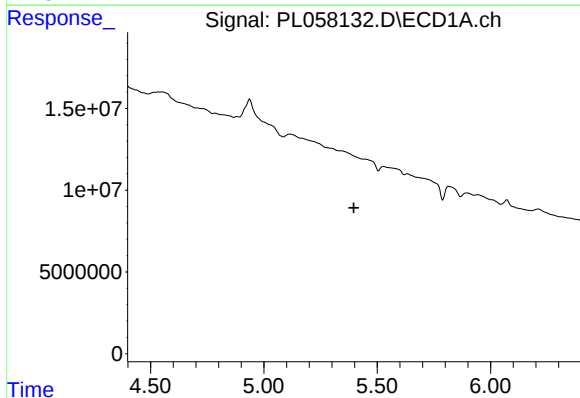


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.397 min
Response: 0
Conc: N.D.

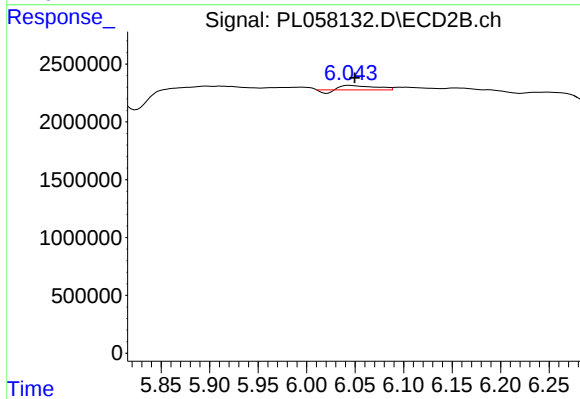

#10 gamma-Chlordane


R.T.: 6.044 min
Delta R.T.: -0.005 min
Response: 798206
Conc: 0.25 ng/ml

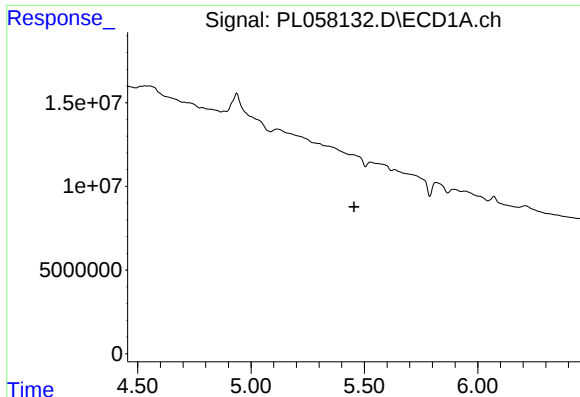

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB128300BL

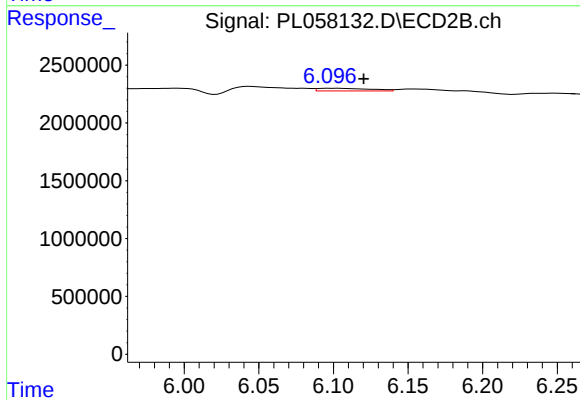


#11 alpha-Chlordane

R.T.: 6.097 min
Delta R.T.: -0.023 min
Response: 551488
Conc: 0.17 ng/ml

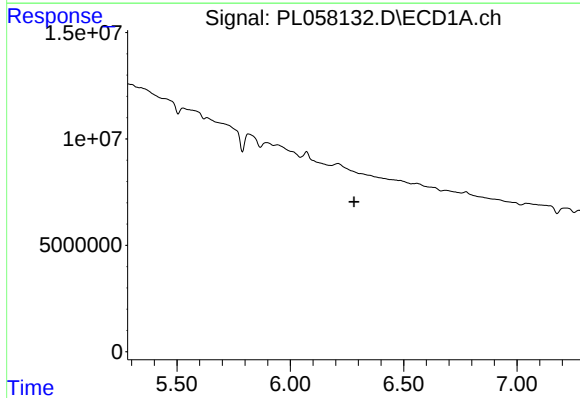


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.282 min
Response: 0
Conc: N.D.

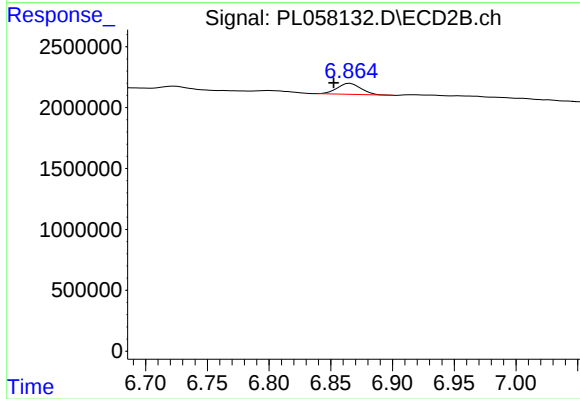

#15 Endosulfan II


R.T.: 6.866 min
Delta R.T.: 0.013 min
Response: 1192718
Conc: 0.46 ng/ml

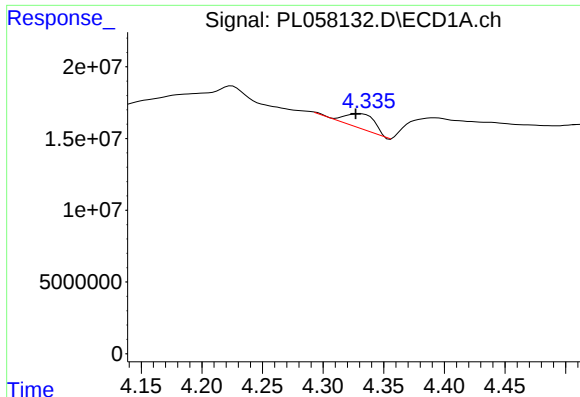

#23 Chlordane-1


R.T.: 4.331 min
Delta R.T.: 0.004 min
Response: 18672330
Conc: 50.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB128300BL

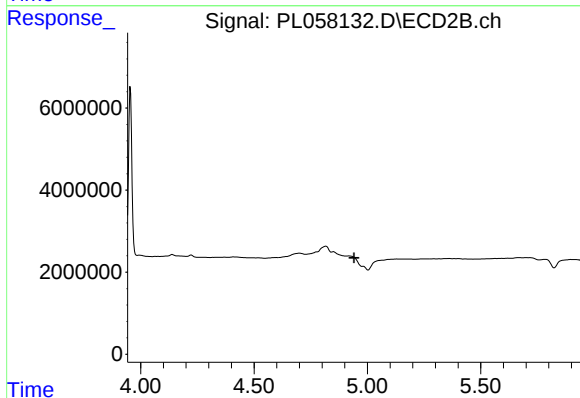


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

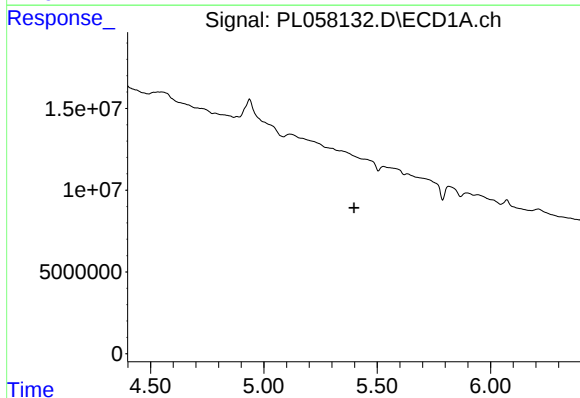


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.398 min
Response: 0
Conc: N.D.

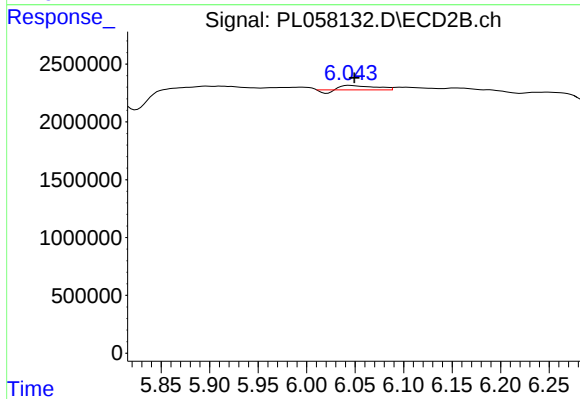

#25 Chlordane-3


R.T.: 6.044 min
Delta R.T.: -0.005 min
Response: 798206
Conc: 1.84 ng/ml

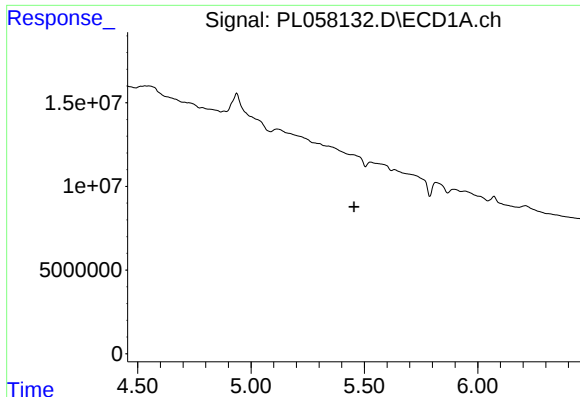

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.454 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB128300BL

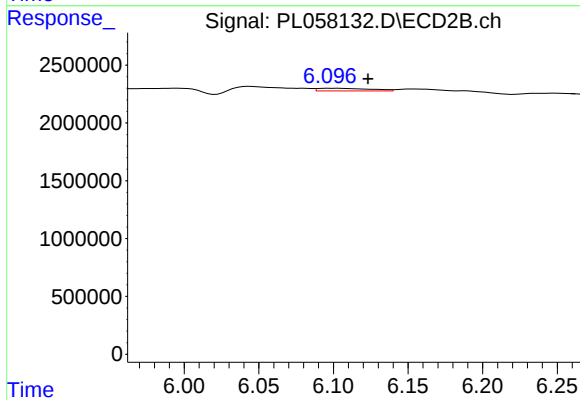


#26 Chlordane-4

R.T.: 6.097 min
Delta R.T.: -0.026 min
Response: 551488
Conc: 1.05 ng/ml

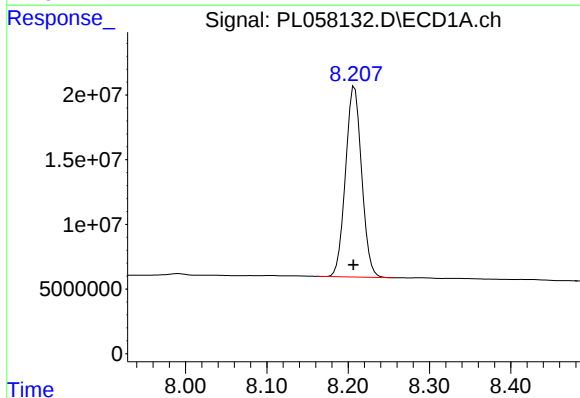

#28 Decachlorobiphenyl

R.T.: 8.208 min
Delta R.T.: 0.001 min
Response: 202336434
Conc: 19.63 ng/ml

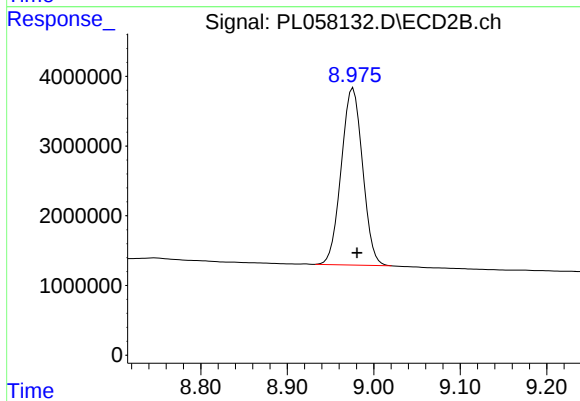

#28 Decachlorobiphenyl

R.T.: 8.976 min
Delta R.T.: -0.005 min
Response: 43360247
Conc: 19.41 ng/ml