

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041720\
 Data File : PL058166.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Apr 2020 21:53
 Operator : AJ\MA
 Sample : L2249-03
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WC-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 18 00:42:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.457	3.955	222.7E6	47701443	22.094	21.981
28)	SA Decachlor...	8.202	8.976	185.3E6	41799491	17.971	18.713
Target Compounds							
3)	MA gamma-BHC...	0.000	4.626	0	139708	N.D.	0.043 #
4)	MA Heptachlor	0.000	5.122	0	5234124	N.D.	1.560 #
5)	MB Aldrin	4.722	5.455f	-119639	164084	N.D.	0.051
15)	B Endosulfa...	0.000	6.866	0	640196	N.D.	0.247 #
16)	A 4,4'-DDD	6.136	0.000	2524144	0	0.253	N.D. #
19)	B Endosulfa...	0.000	7.204	0	317023	N.D.	0.134 #
21)	B Endrin ke...	7.182f	7.664	259829	587664	0.023	0.238 #
22)	Mirex	7.316f	0.000	921693	0	0.112	N.D. #
23)	Chlordane-1	4.312f	0.000	1869459	0	5.055	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041720\
Data File : PL058166.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Apr 2020 21:53
Operator : AJ\MA
Sample : L2249-03
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
WC-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 18 00:42:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

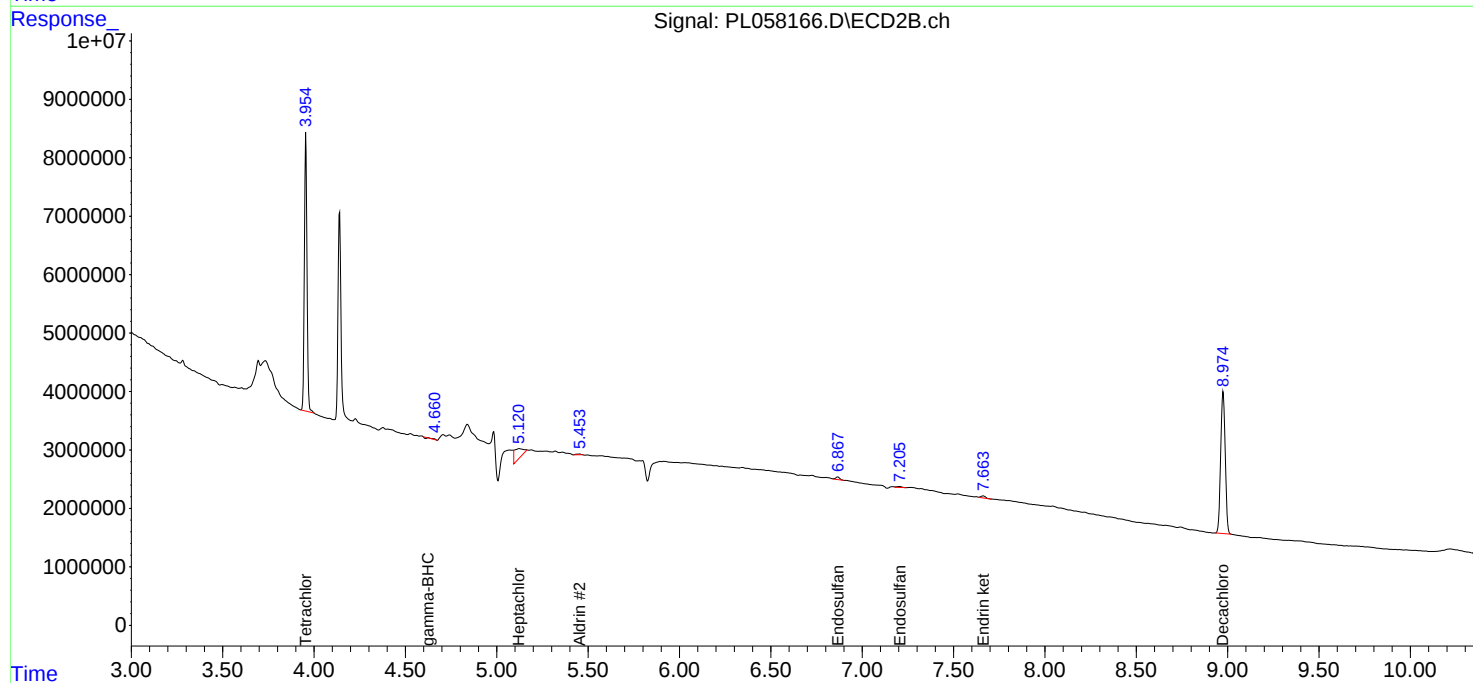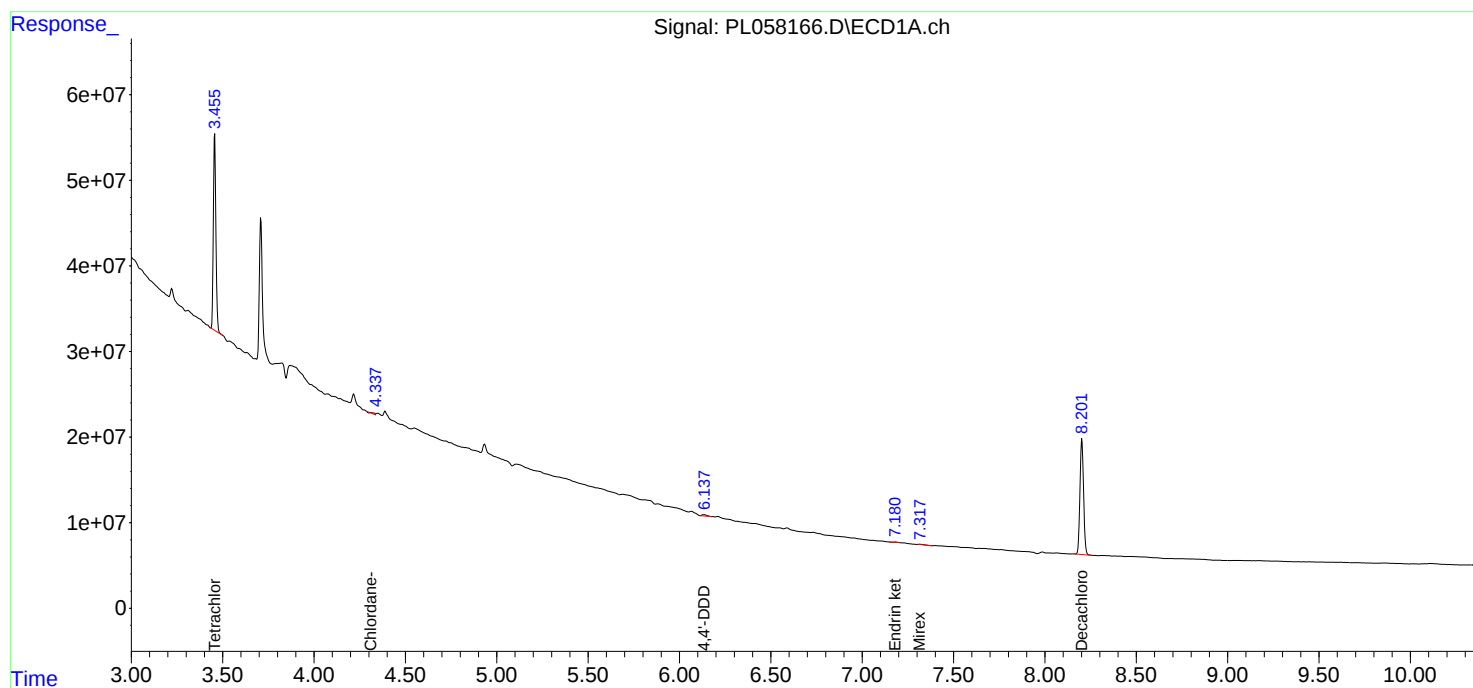


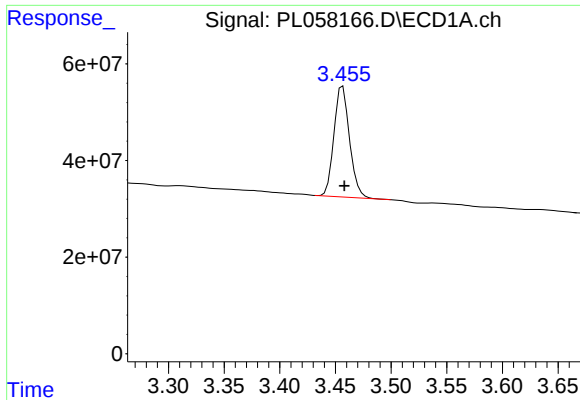

#1 Tetrachloro-m-xylene


R.T.: 3.457 min
Delta R.T.: -0.001 min
Response: 222731486
Conc: 22.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-3

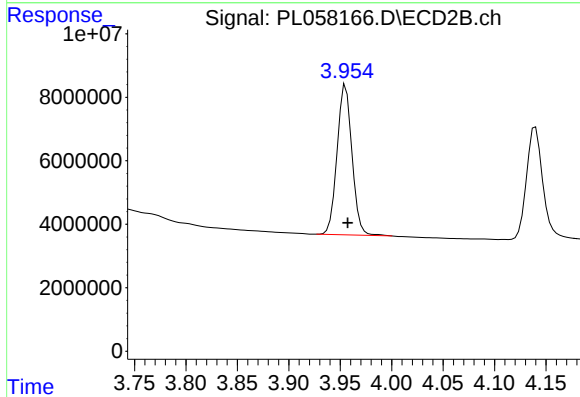


#1 Tetrachloro-m-xylene

R.T.: 3.955 min
Delta R.T.: -0.002 min
Response: 47701443
Conc: 21.98 ng/ml

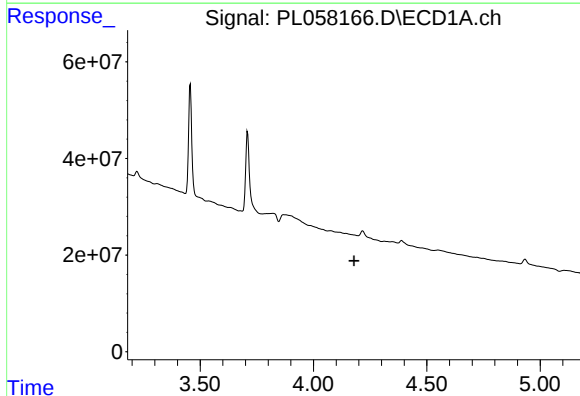


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.179 min
Response: 0
Conc: N.D.

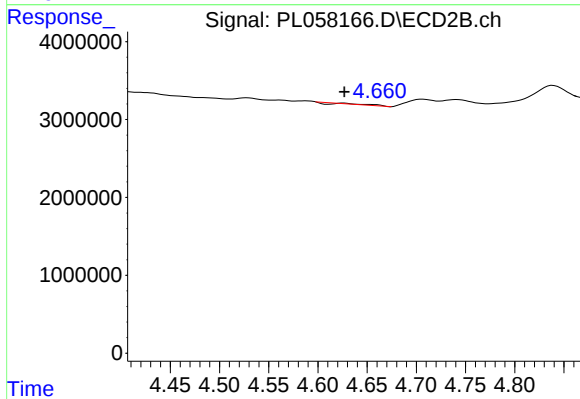

#3 gamma-BHC (Lindane)


R.T.: 4.626 min
Delta R.T.: 0.000 min
Response: 139708
Conc: 0.04 ng/ml

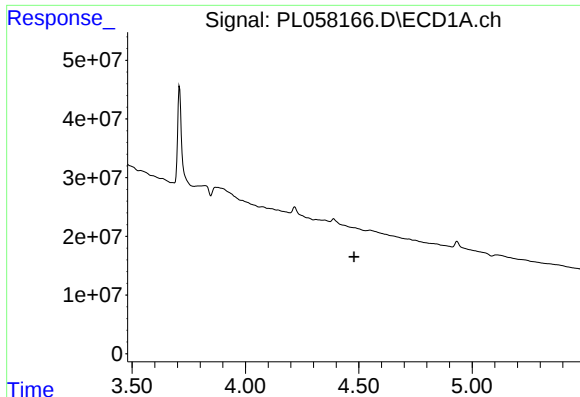

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
WC-3

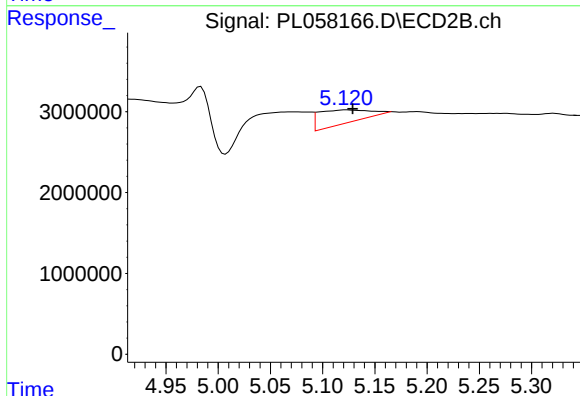


#4 Heptachlor

R.T.: 5.122 min
Delta R.T.: -0.006 min
Response: 5234124
Conc: 1.56 ng/ml

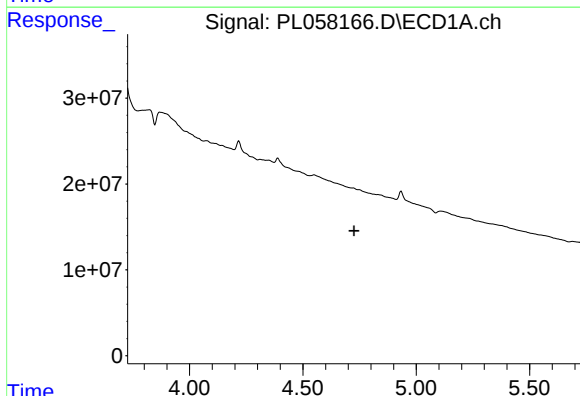


#5 Aldrin

R.T.: 4.722 min
Delta R.T.: -0.004 min
Response: -119639
Conc: N.D.

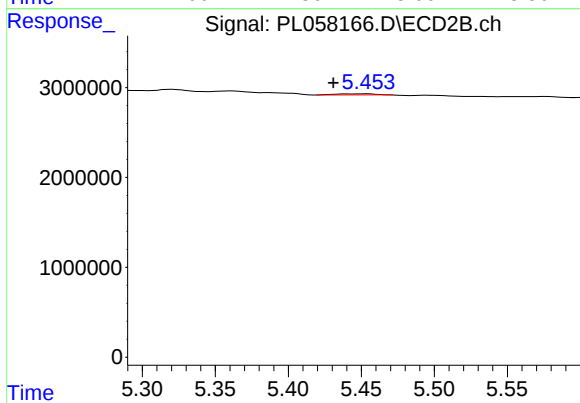

#5 Aldrin


R.T.: 5.455 min
Delta R.T.: 0.024 min
Response: 164084
Conc: 0.05 ng/ml

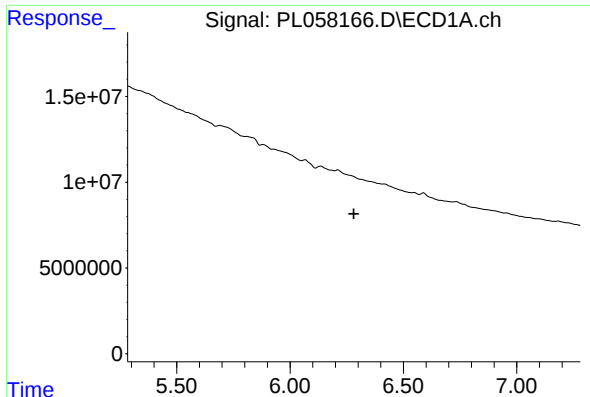

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.282 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
WC-3

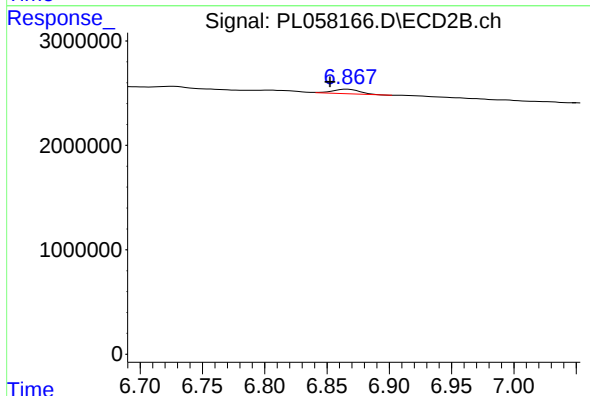


#15 Endosulfan II

R.T.: 6.866 min
Delta R.T.: 0.014 min
Response: 640196
Conc: 0.25 ng/ml

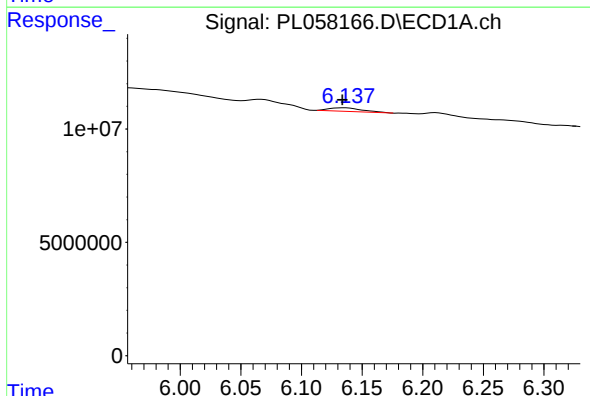


#16 4,4'-DDD

R.T.: 6.136 min
Delta R.T.: 0.002 min
Response: 2524144
Conc: 0.25 ng/ml

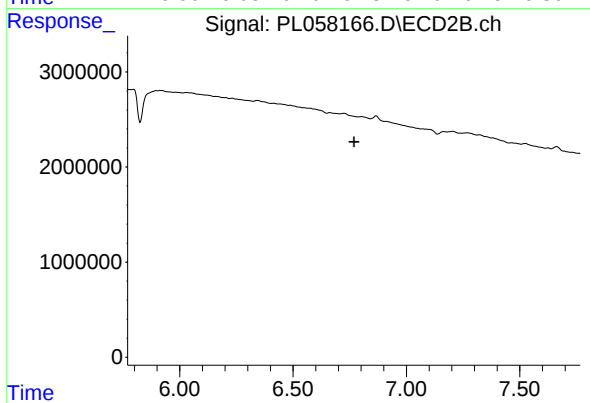

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.769 min
Response: 0
Conc: N.D.

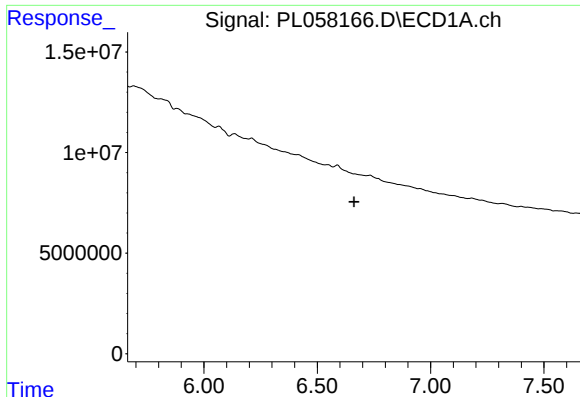

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 6.663 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
WC-3

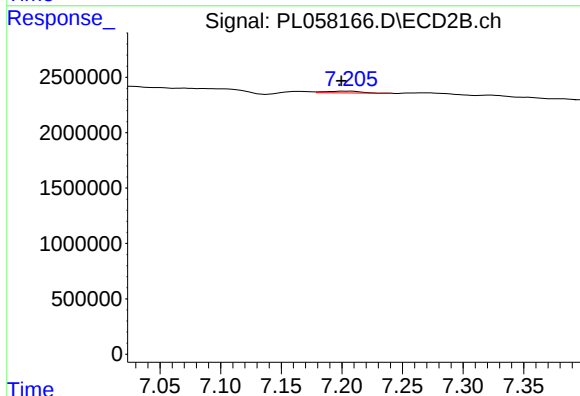


#19 Endosulfan Sulfate

R.T.: 7.204 min
Delta R.T.: 0.005 min
Response: 317023
Conc: 0.13 ng/ml

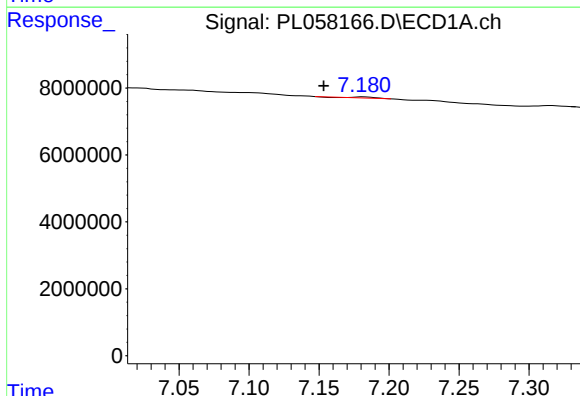


#21 Endrin ketone

R.T.: 7.182 min
Delta R.T.: 0.028 min
Response: 259829
Conc: 0.02 ng/ml

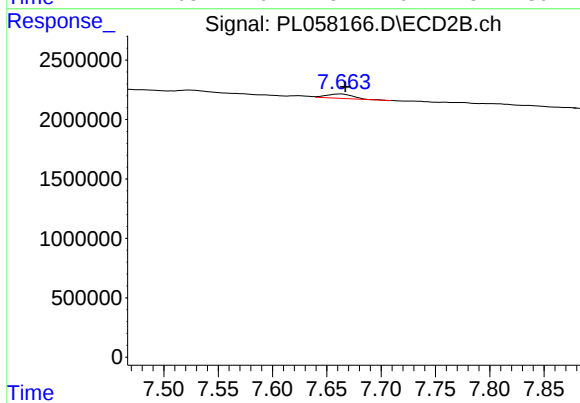

#21 Endrin ketone


R.T.: 7.664 min
Delta R.T.: -0.003 min
Response: 587664
Conc: 0.24 ng/ml

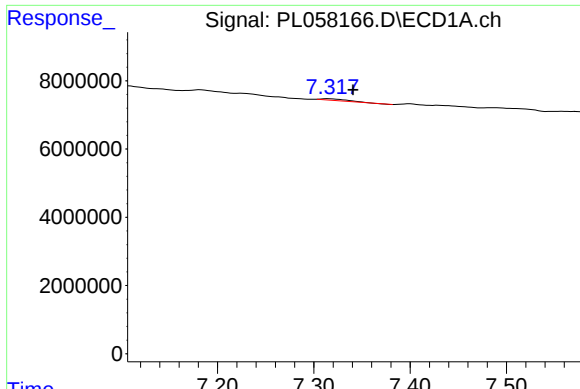

#22 Mirex


R.T.: 7.316 min
Delta R.T.: -0.025 min
Response: 921693
Conc: 0.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-3

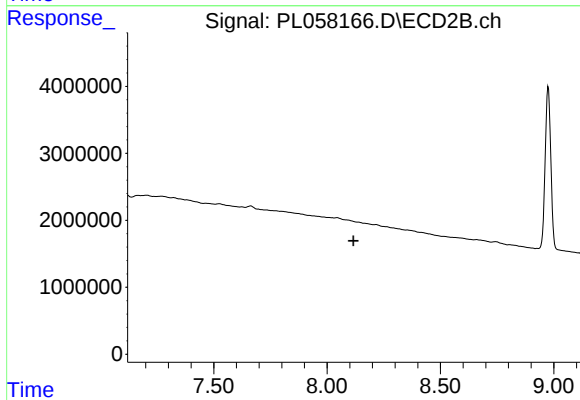


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 8.117 min
Response: 0
Conc: N.D.

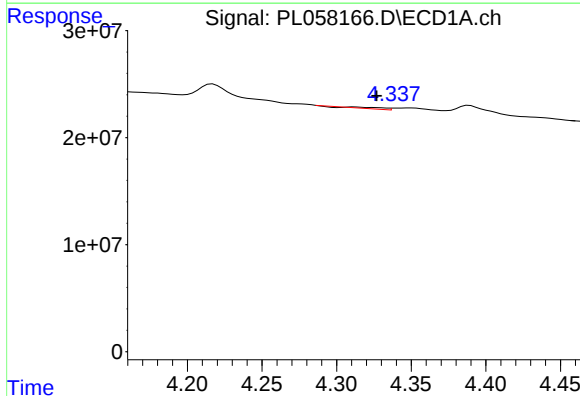


#23 Chlordane-1

R.T.: 4.312 min
Delta R.T.: -0.015 min
Response: 1869459
Conc: 5.05 ng/ml

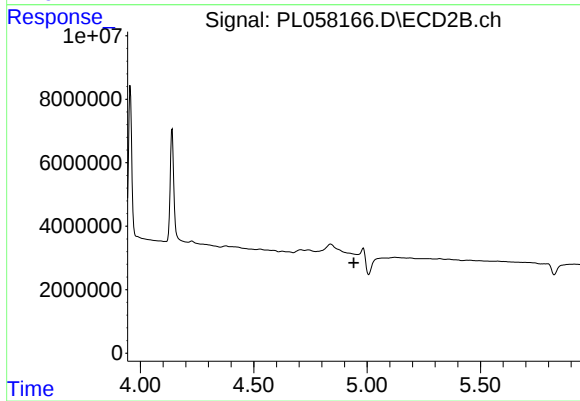

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

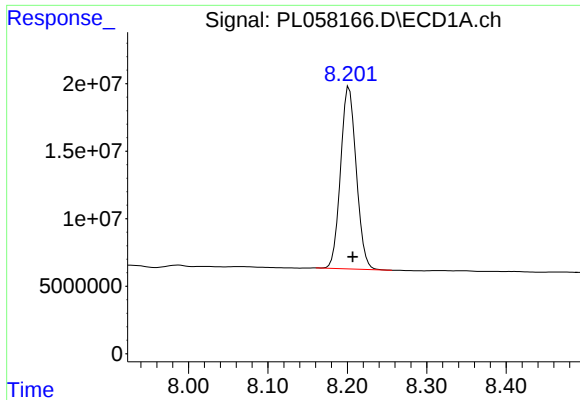

#28 Decachlorobiphenyl

R.T.: 8.202 min
Delta R.T.: -0.004 min
Response: 185255034
Conc: 17.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-3

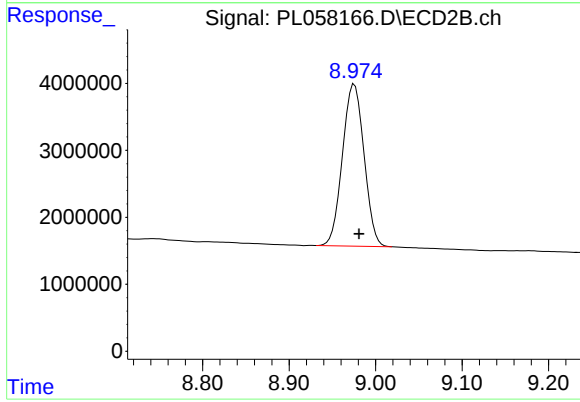

#28 Decachlorobiphenyl

R.T.: 8.976 min
Delta R.T.: -0.005 min
Response: 41799491
Conc: 18.71 ng/ml