

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041720\
 Data File : PL058170.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Apr 2020 22:50
 Operator : AJ\MA
 Sample : L2249-07
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WC-7

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 18 00:42:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.457	3.956	222.5E6	46167258	22.071	21.274
28)	SA Decachlor...	8.203	8.977	193.7E6	43770561	18.792	19.595
Target Compounds							
2)	A alpha-BHC	3.901	0.000	6778154	0	0.390	N.D. #
4)	MA Heptachlor	0.000	5.142	0	799365	N.D.	0.238 #
6)	B beta-BHC	4.436	0.000	10899949	0	1.726	N.D. #
7)	B delta-BHC	4.624	4.984f	18880281	11694901	1.244	6.514 #
8)	B Heptachlo...	0.000	5.798f	0	5013262	N.D.	1.857 #
15)	B Endosulfa...	0.000	6.868f	0	759266	N.D.	0.293 #
16)	A 4,4'-DDD	6.122	0.000	850046	0	0.085	N.D. #
21)	B Endrin ke...	7.180f	0.000	800509	0	0.072	N.D. #
23)	Chlordane-1	4.308f	0.000	869708	0	2.352	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041720\
Data File : PL058170.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Apr 2020 22:50
Operator : AJ\MA
Sample : L2249-07
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
WC-7

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 18 00:42:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

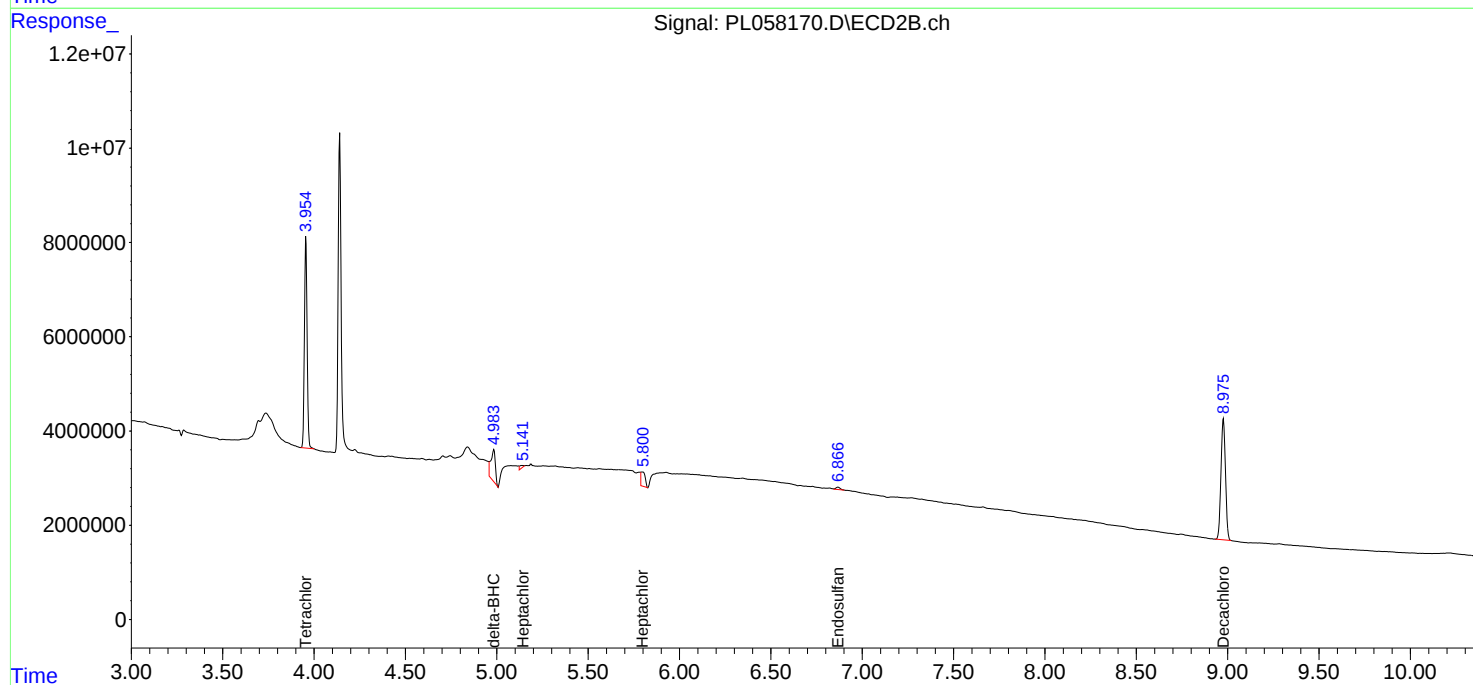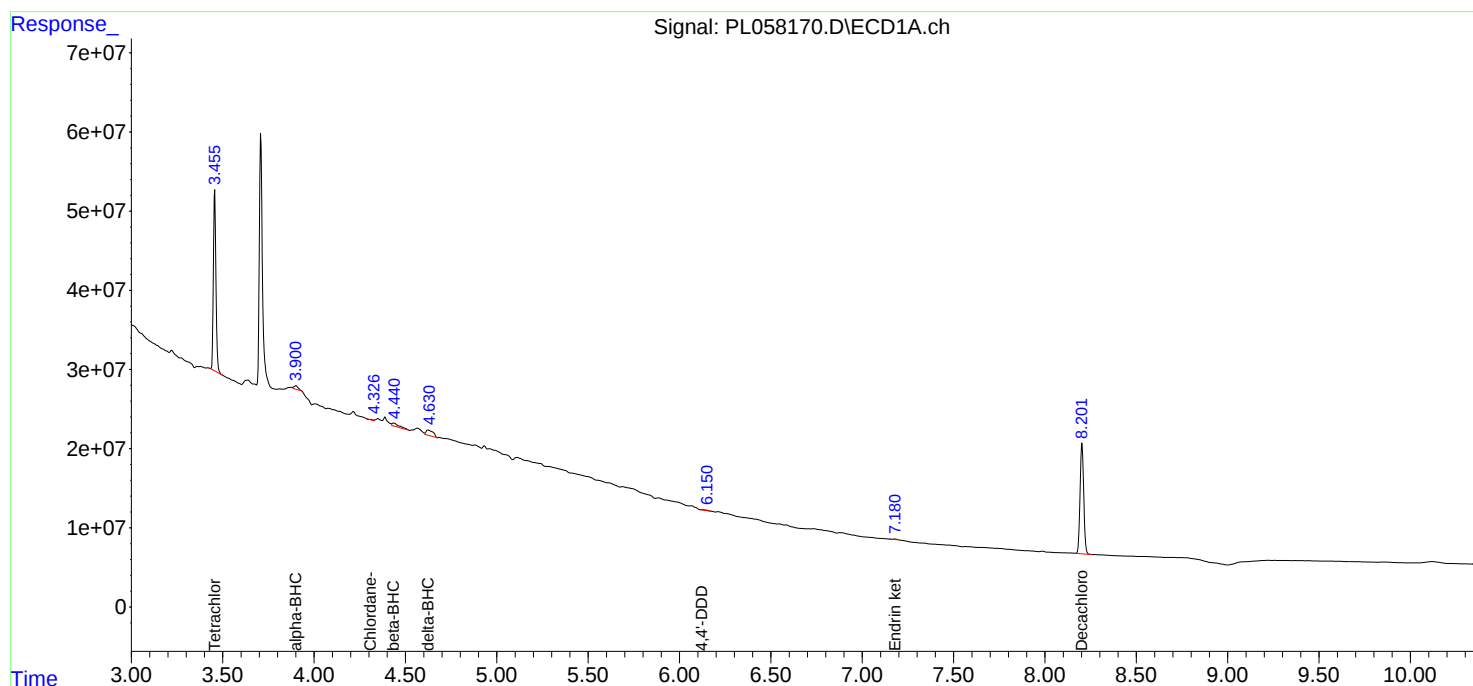


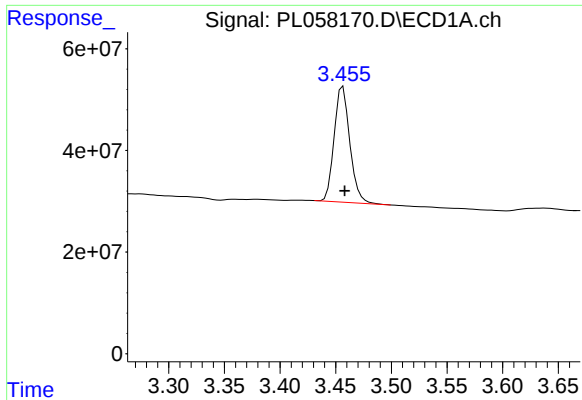

#1 Tetrachloro-m-xylene


R.T.: 3.457 min
Delta R.T.: -0.001 min
Response: 222501434
Conc: 22.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-7

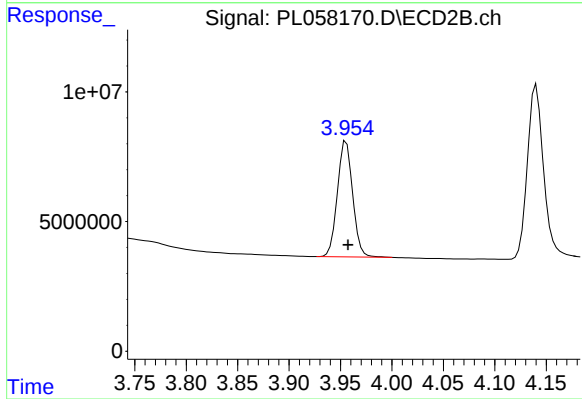


#1 Tetrachloro-m-xylene

R.T.: 3.956 min
Delta R.T.: -0.002 min
Response: 46167258
Conc: 21.27 ng/ml

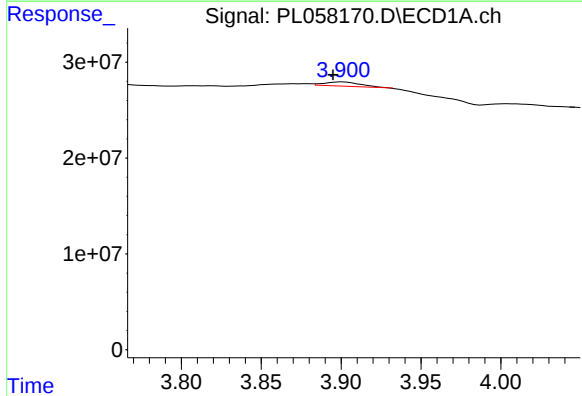


#2 alpha-BHC

R.T.: 3.901 min
Delta R.T.: 0.006 min
Response: 6778154
Conc: 0.39 ng/ml

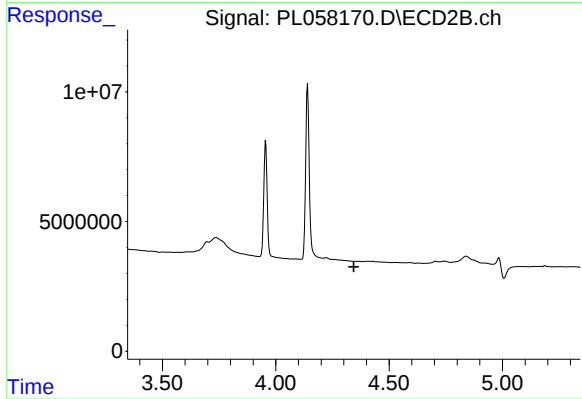

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.345 min
Response: 0
Conc: N.D.

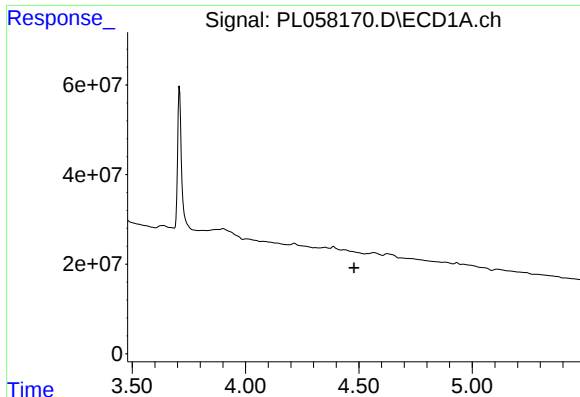

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
WC-7

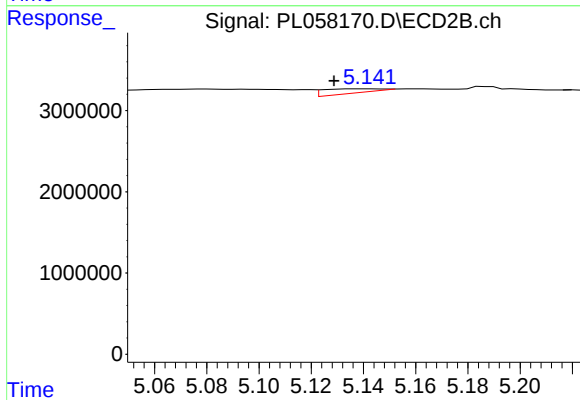


#4 Heptachlor

R.T.: 5.142 min
Delta R.T.: 0.013 min
Response: 799365
Conc: 0.24 ng/ml

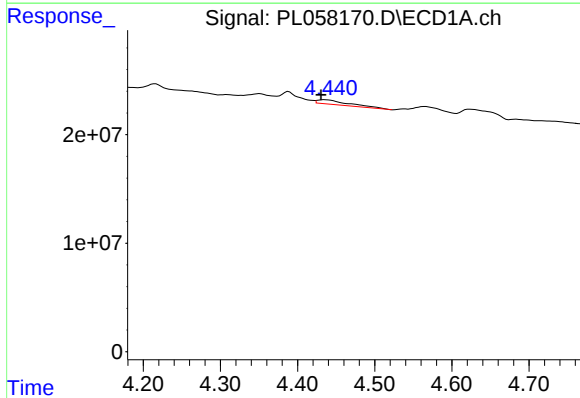


#6 beta-BHC

R.T.: 4.436 min
Delta R.T.: 0.005 min
Response: 10899949
Conc: 1.73 ng/ml

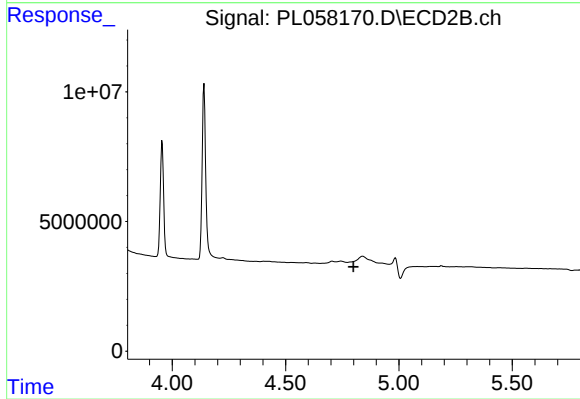

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.800 min
Response: 0
Conc: N.D.

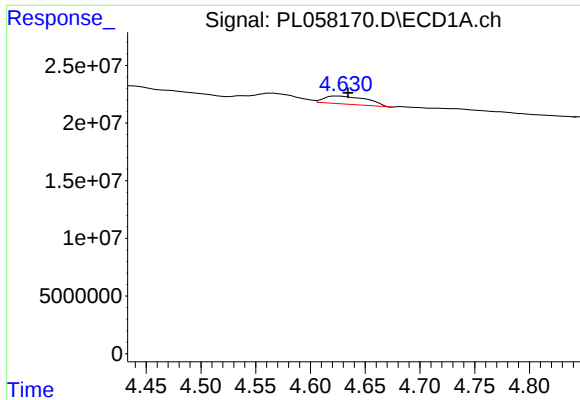

#7 delta-BHC


R.T.: 4.624 min
Delta R.T.: -0.010 min
Response: 18880281
Conc: 1.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-7

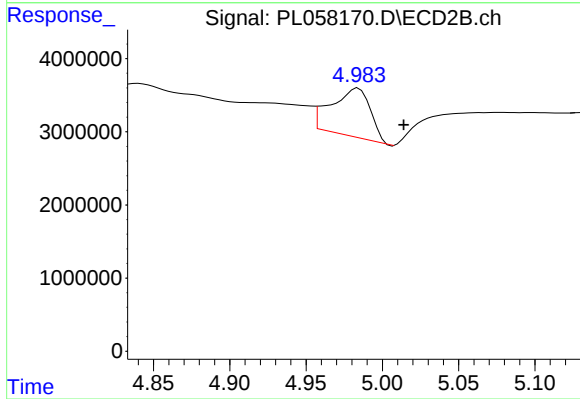


#7 delta-BHC

R.T.: 4.984 min
Delta R.T.: -0.030 min
Response: 11694901
Conc: 6.51 ng/ml

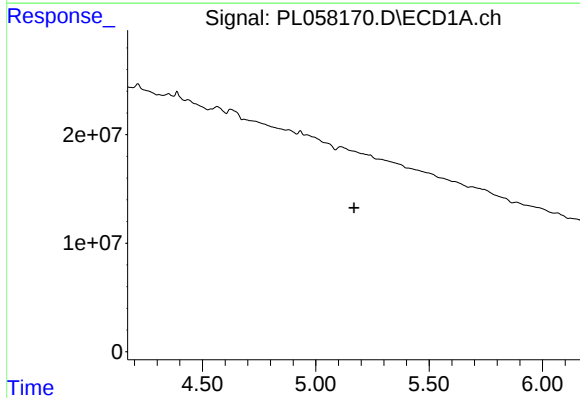


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.169 min
Response: 0
Conc: N.D.

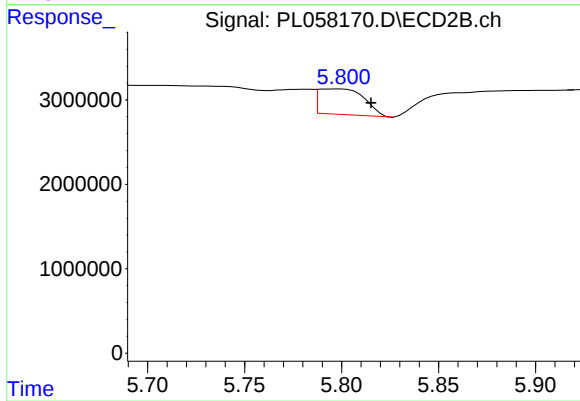

#8 Heptachlor epoxide


R.T.: 5.798 min
Delta R.T.: -0.017 min
Response: 5013262
Conc: 1.86 ng/ml

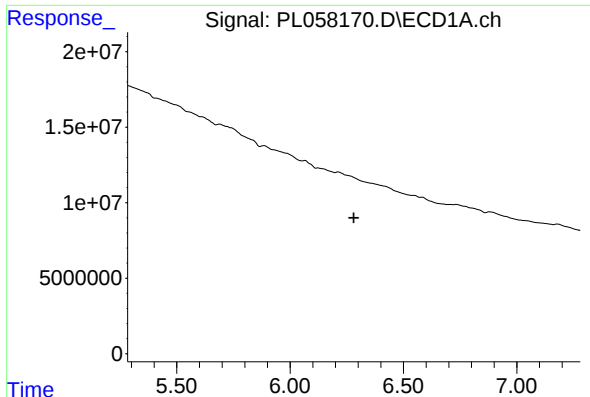

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.282 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
WC-7

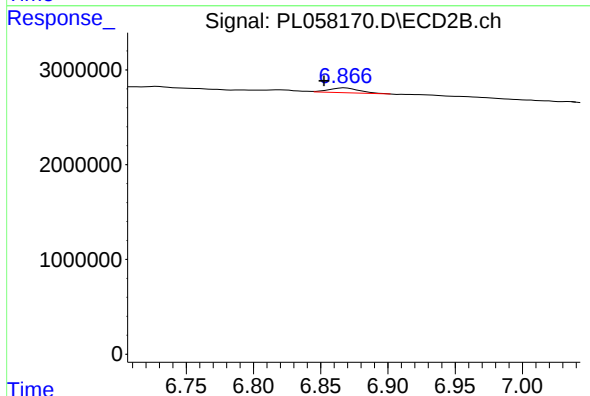


#15 Endosulfan II

R.T.: 6.868 min
Delta R.T.: 0.015 min
Response: 759266
Conc: 0.29 ng/ml

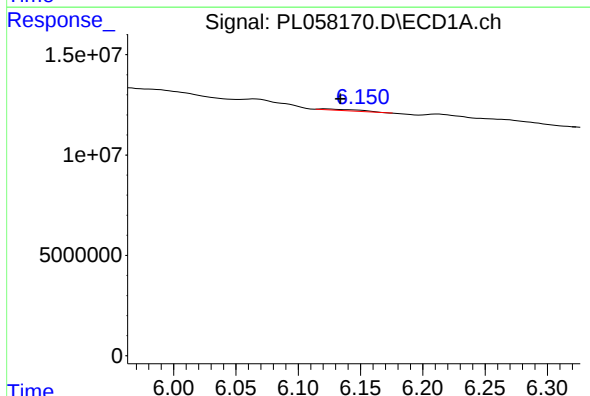


#16 4,4'-DDD

R.T.: 6.122 min
Delta R.T.: -0.012 min
Response: 850046
Conc: 0.09 ng/ml

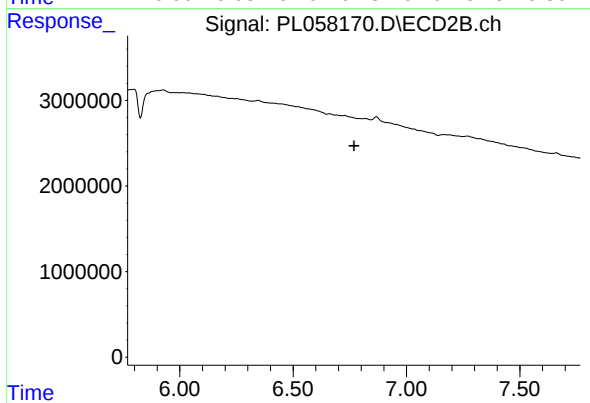

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.769 min
Response: 0
Conc: N.D.

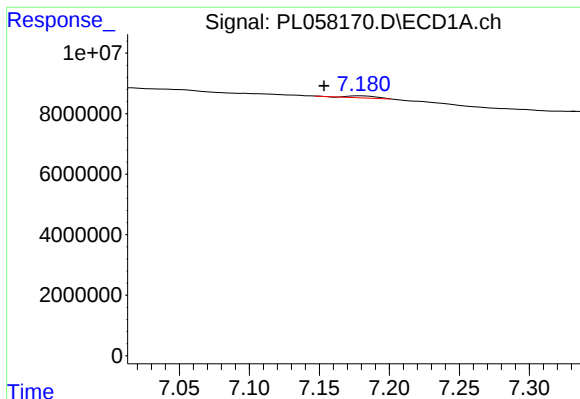

#21 Endrin ketone


R.T.: 7.180 min
Delta R.T.: 0.027 min
Response: 800509
Conc: 0.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-7

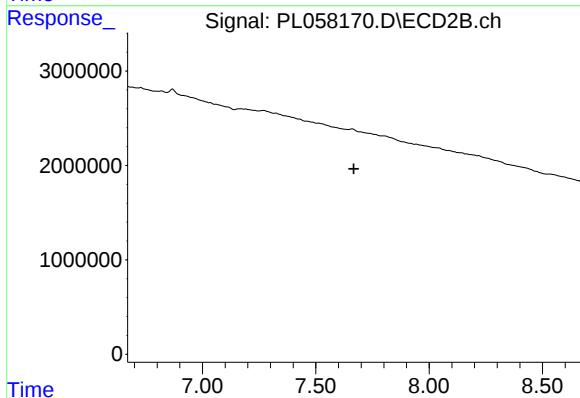


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.667 min
Response: 0
Conc: N.D.

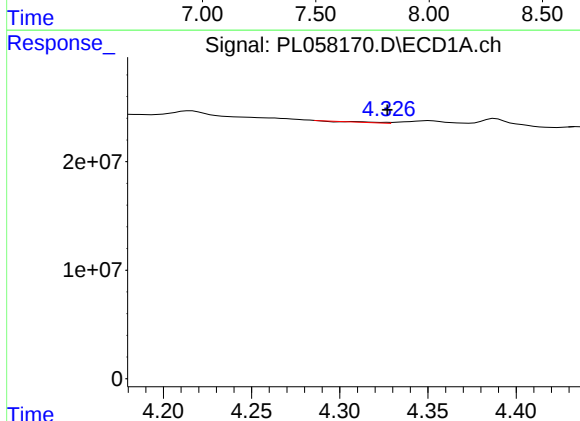


#23 Chlordane-1

R.T.: 4.308 min
Delta R.T.: -0.019 min
Response: 869708
Conc: 2.35 ng/ml

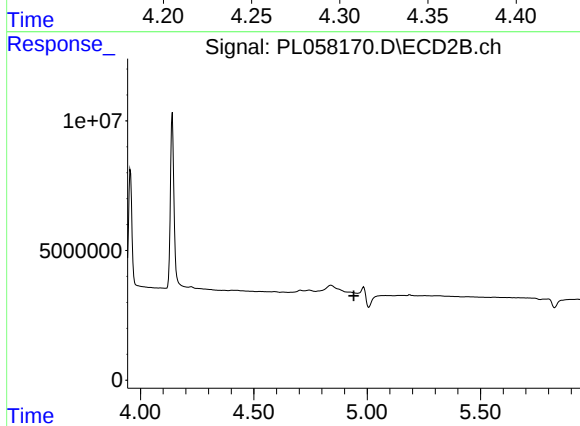

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

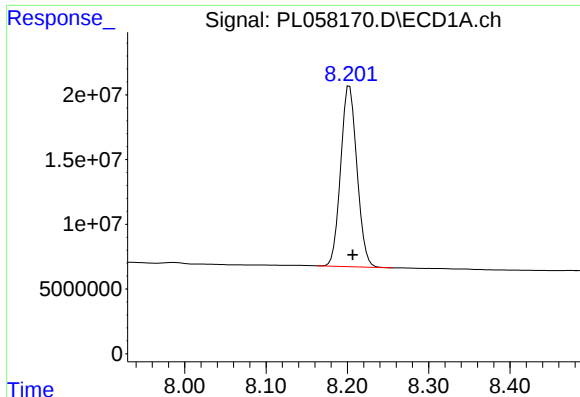

#28 Decachlorobiphenyl

R.T.: 8.203 min
Delta R.T.: -0.004 min
Response: 193712392
Conc: 18.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-7

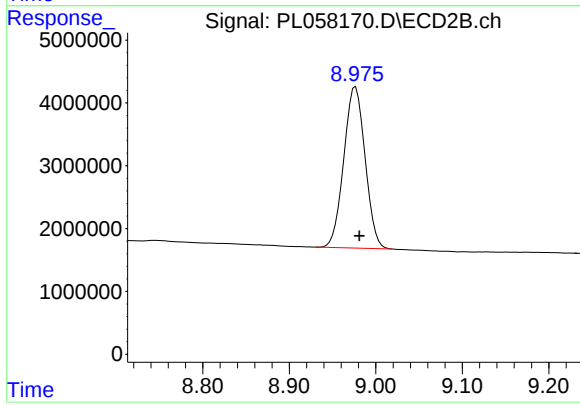

#28 Decachlorobiphenyl

R.T.: 8.977 min
Delta R.T.: -0.004 min
Response: 43770561
Conc: 19.59 ng/ml