

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041720\
 Data File : PL058150.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Apr 2020 17:51
 Operator : AJ\MA
 Sample : L2323-05
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-20-COMP

Manual Integrations
 APPROVED

mohammad
 4/21/2020 8:24:56 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 18 00:37:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.466	3.954	252.5E6	15930294	25.043m	7.341 #
28) SA Decachlor...	8.201	8.974	95282540	23676638	9.243	10.599

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041720\
Data File : PL058150.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Apr 2020 17:51
Operator : AJ\MA
Sample : L2323-05
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-20-COMP


Manual Integrations
APPROVED

mohammad
4/21/2020 8:24:56 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 18 00:37:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

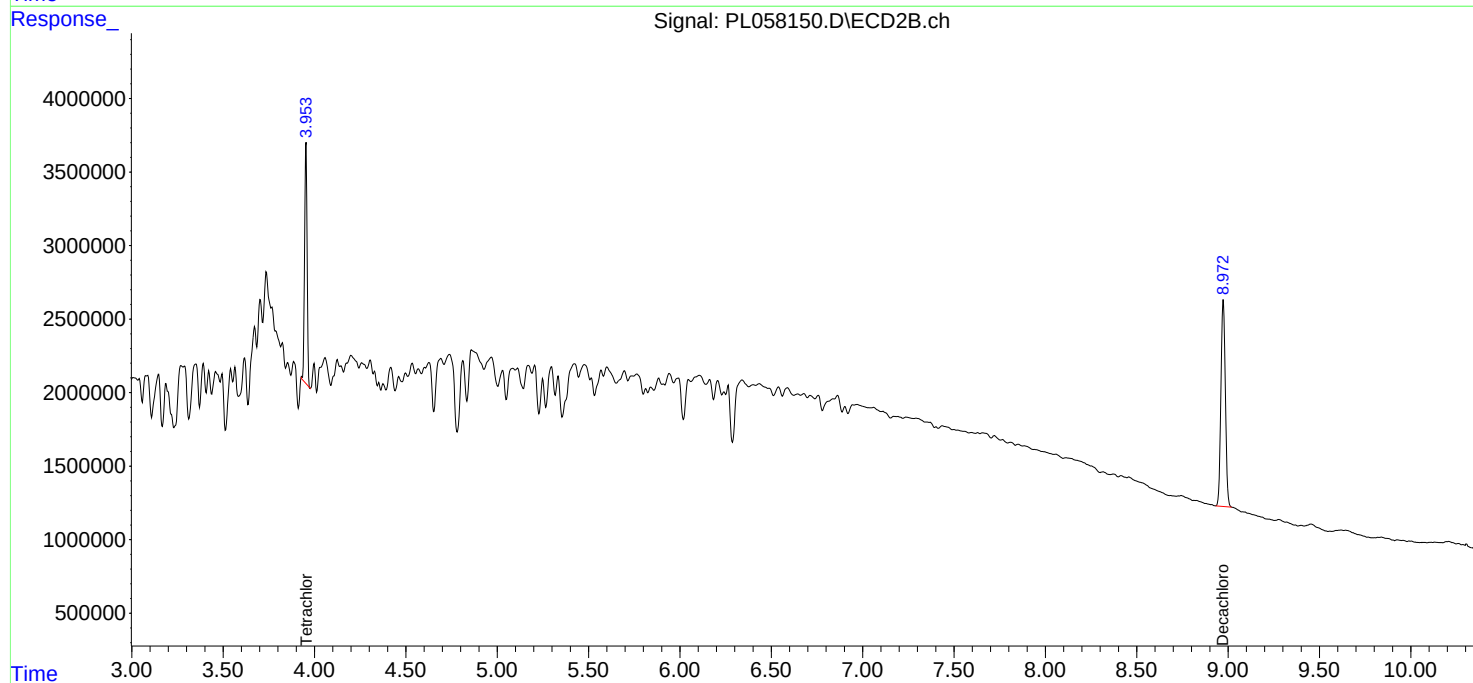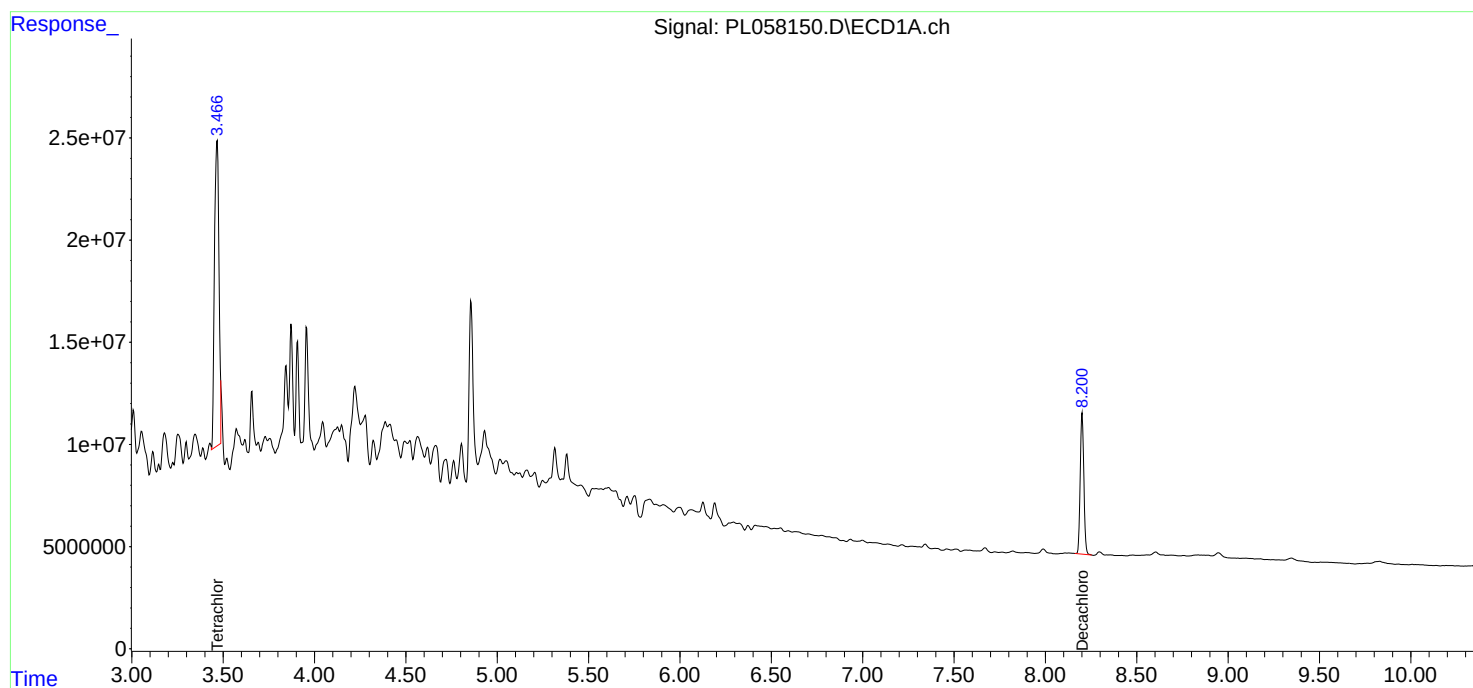

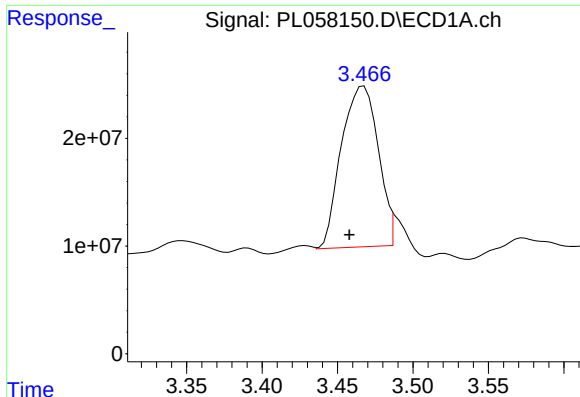


#1 Tetrachloro-m-xylene

R.T.: 3.466 min
Delta R.T.: 0.008 min
Response: 252462632
Conc: 25.04 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TP-20-COMP


Manual Integrations
APPROVED

mohammad
4/21/2020 8:24:56 AM

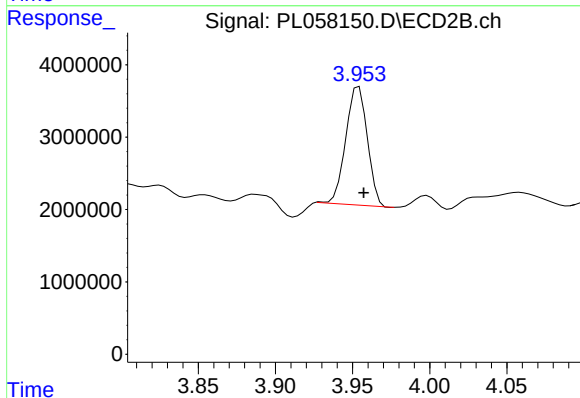


#1 Tetrachloro-m-xylene

R.T.: 3.954 min
Delta R.T.: -0.003 min
Response: 15930294
Conc: 7.34 ng/ml

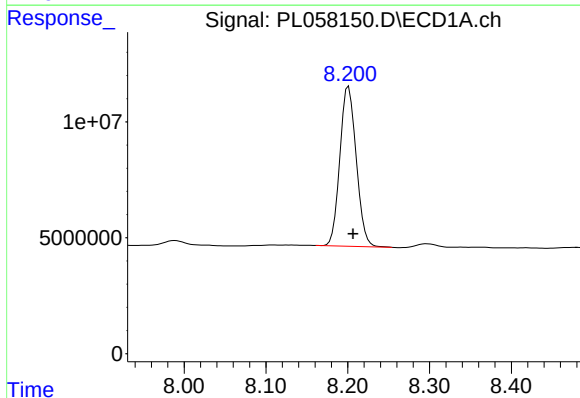

#28 Decachlorobiphenyl

R.T.: 8.201 min
Delta R.T.: -0.006 min
Response: 95282540
Conc: 9.24 ng/ml

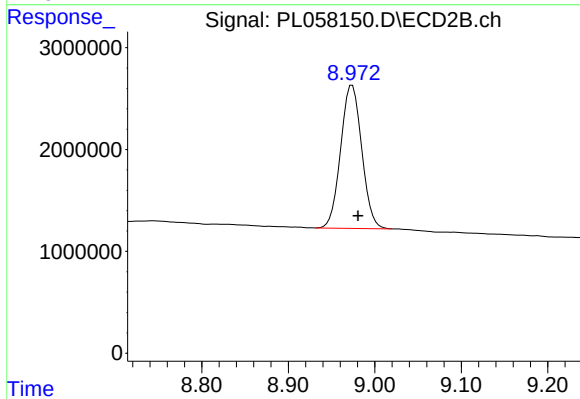

#28 Decachlorobiphenyl

R.T.: 8.974 min
Delta R.T.: -0.007 min
Response: 23676638
Conc: 10.60 ng/ml