

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041723\
 Data File : PL082153.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Apr 2023 22:22
 Operator : AR\AJ
 Sample : 02314-01
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 QUARTERLY-OUTFALL-002

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 04/18/2023
 Supervised By :Ankita Jodhani 04/18/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 18 04:55:28 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032223.M
 Quant Title : GC Extractables
 QLast Update : Thu Mar 23 01:07:33 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.323	2.651	28239490	35499524	12.141m	17.784 #
28) SA Decachlor...	8.748	7.766	25080733	28734464	14.014	14.489

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041723\
Data File : PL082153.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Apr 2023 22:22
Operator : AR\AJ
Sample : 02314-01
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
QUARTERLY-OUTFALL-002


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 04/18/2023
Supervised By : Ankita Jodhani 04/18/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 18 04:55:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032223.M
Quant Title : GC Extractables
QLast Update : Thu Mar 23 01:07:33 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

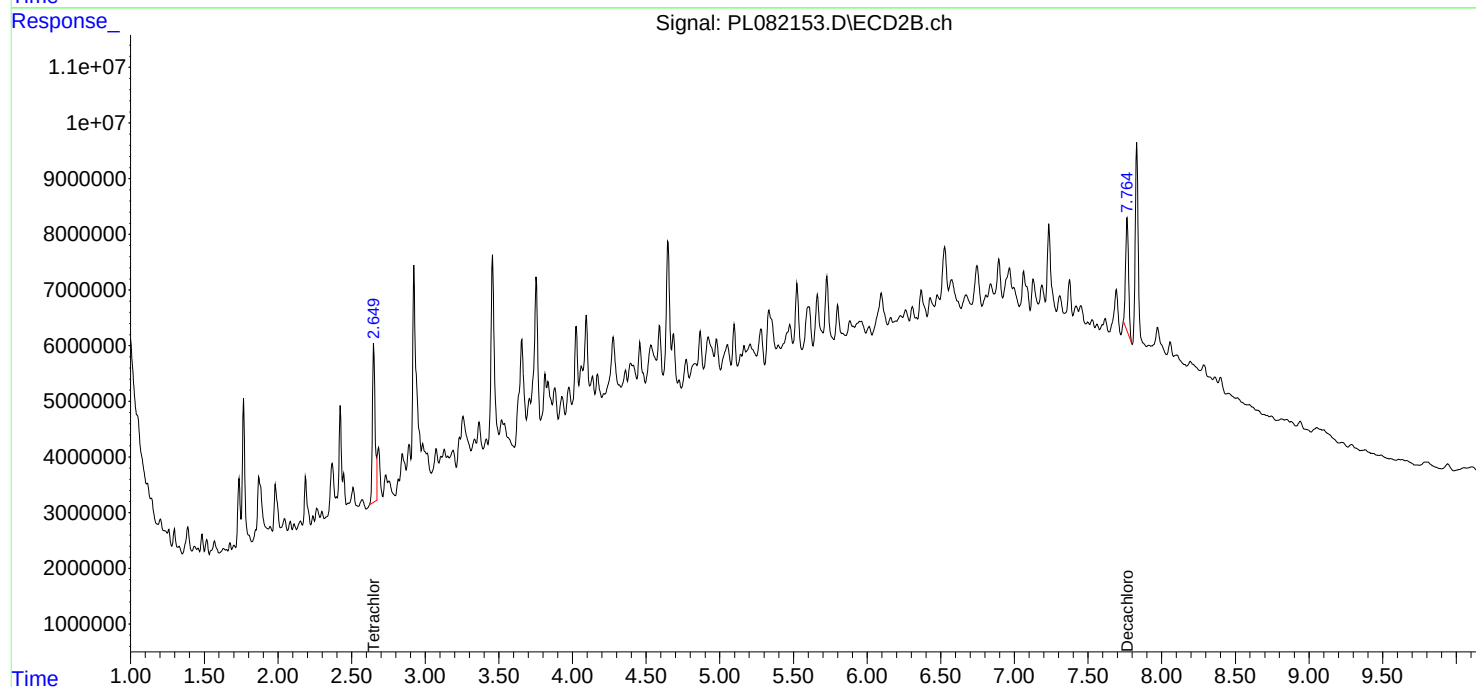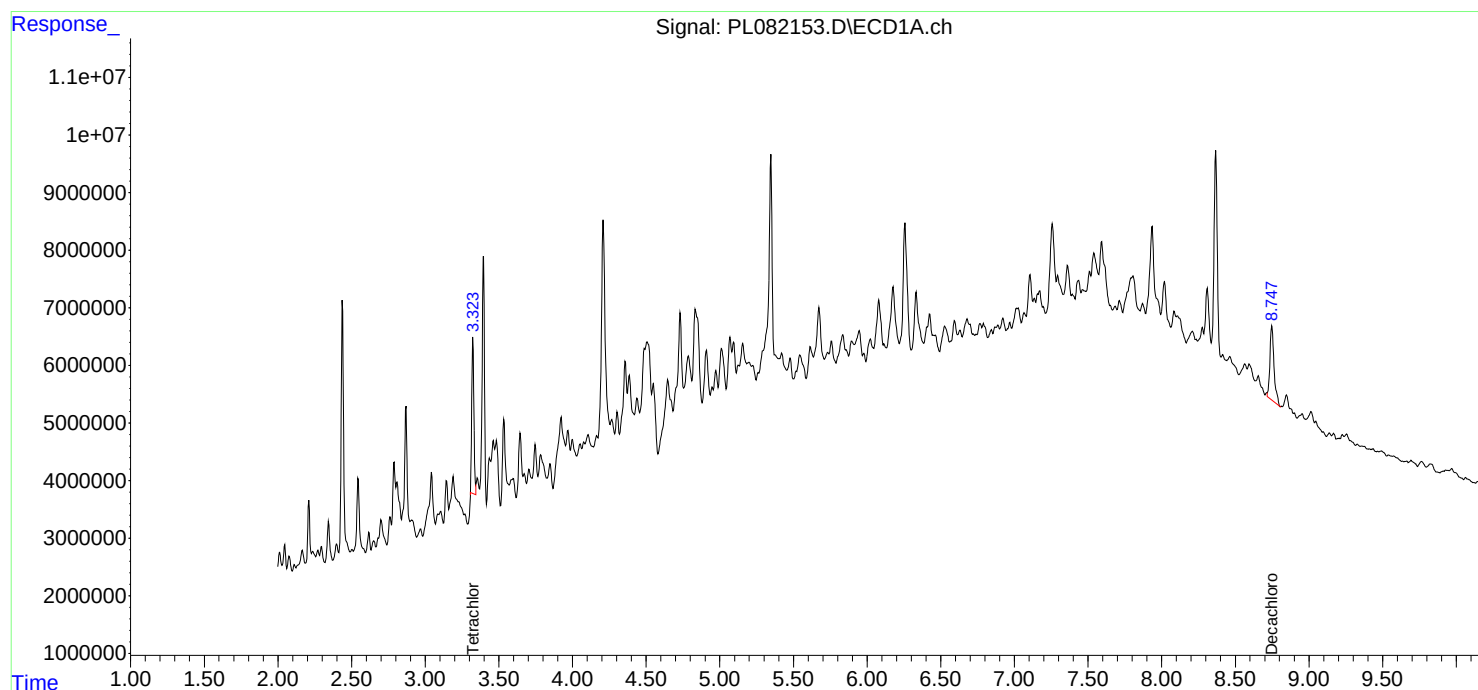

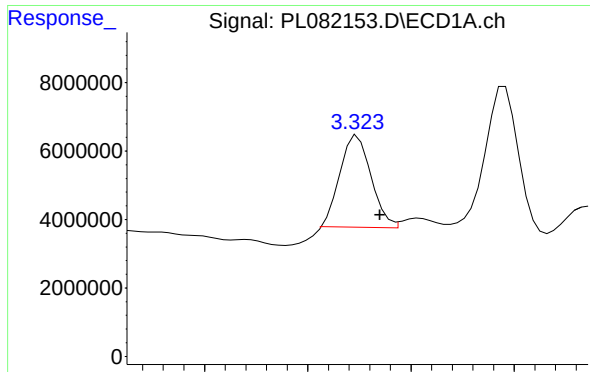


#1 Tetrachloro-m-xylene

R.T.: 3.323 min
Delta R.T.: -0.012 min
Response: 28239490
Conc: 12.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
QUARTERLY-OUTFALL-002


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/18/2023
Supervised By :Ankita Jodhani 04/18/2023

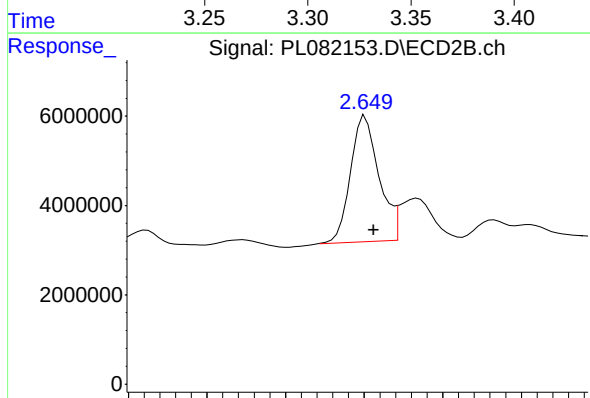


#1 Tetrachloro-m-xylene

R.T.: 2.651 min
Delta R.T.: -0.005 min
Response: 35499524
Conc: 17.78 ng/ml

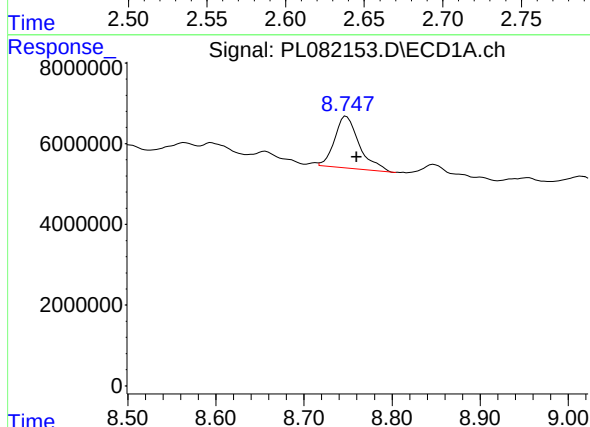

#28 Decachlorobiphenyl

R.T.: 8.748 min
Delta R.T.: -0.011 min
Response: 25080733
Conc: 14.01 ng/ml

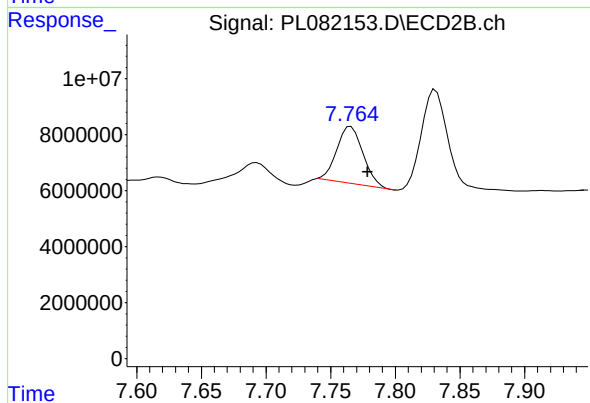

#28 Decachlorobiphenyl

R.T.: 7.766 min
Delta R.T.: -0.013 min
Response: 28734464
Conc: 14.49 ng/ml