

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041819\
 Data File : PL047559.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Apr 2019 12:31
 Operator : AJ\SJ
 Sample : K2442-16
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-21-D

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: 07 Apr 19 01:09:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.361	3.976	147.9E6	46291870	20.330	20.218
28) SA Decachlor...	8.035	9.029	169.2E6	49900902	20.118	21.523
Target Compounds						
6) B beta-BHC	0.000	4.853f	0	4065407	N.D.	3.067 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041819\
Data File : PL047559.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Apr 2019 12:31
Operator : AJ\SJ
Sample : K2442-16
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-21-D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 19 01:09:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

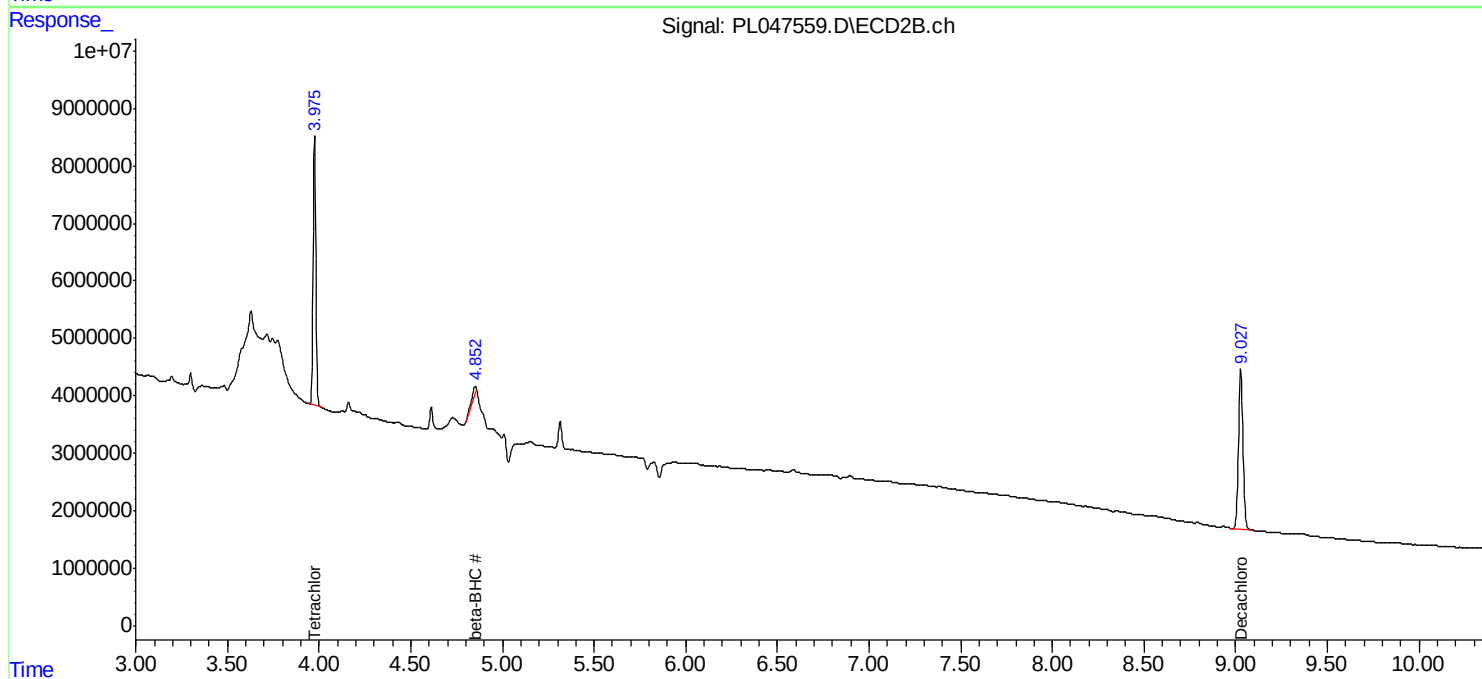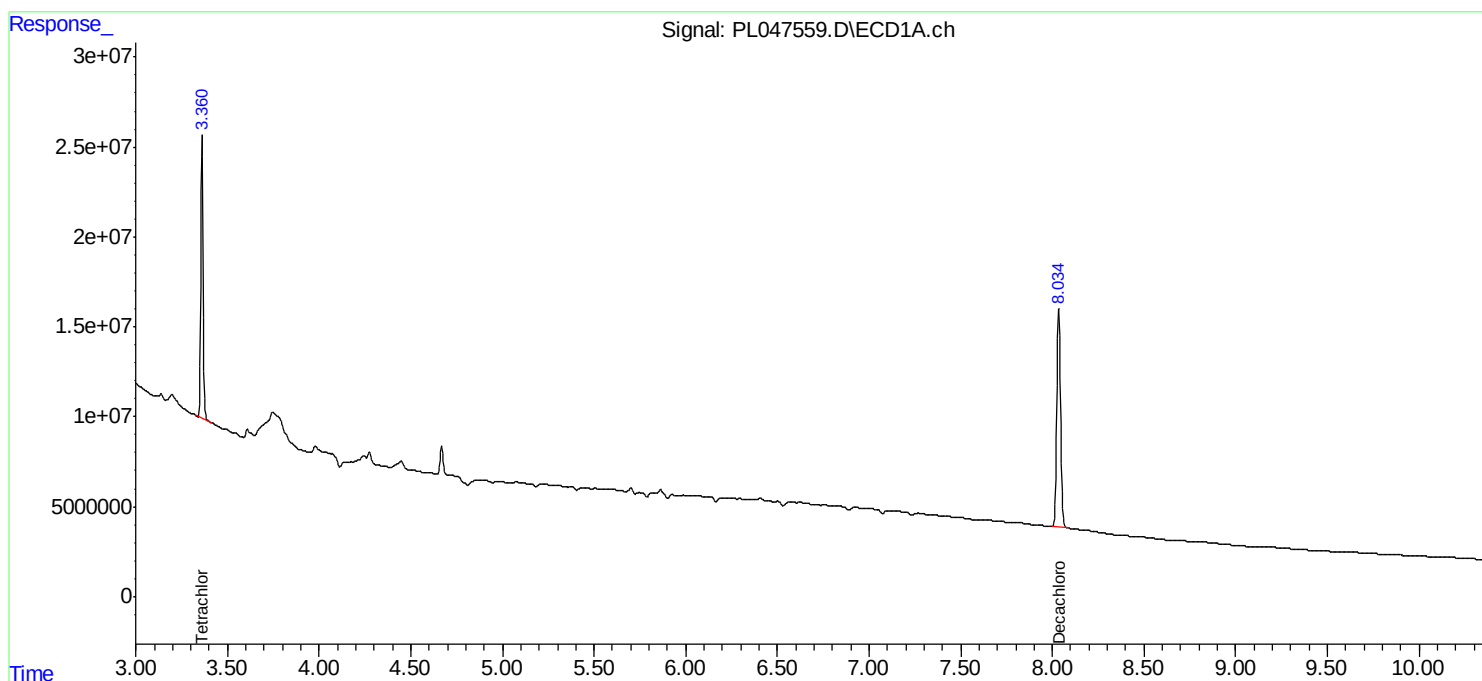


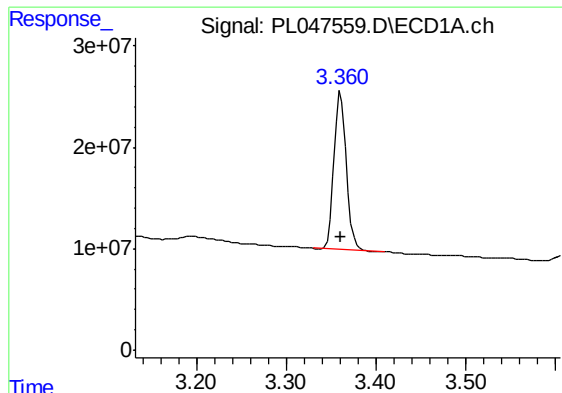

#1 Tetrachloro-m-xylene


R.T.: 3.361 min
Delta R.T.: 0.000 min
Response: 147894661
Conc: 20.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-21-D

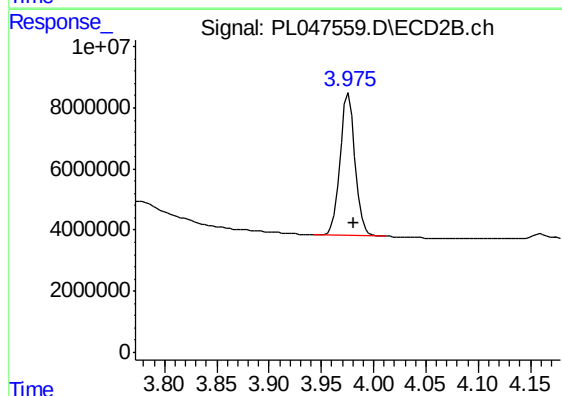


#1 Tetrachloro-m-xylene

R.T.: 3.976 min
Delta R.T.: -0.004 min
Response: 46291870
Conc: 20.22 ng/ml

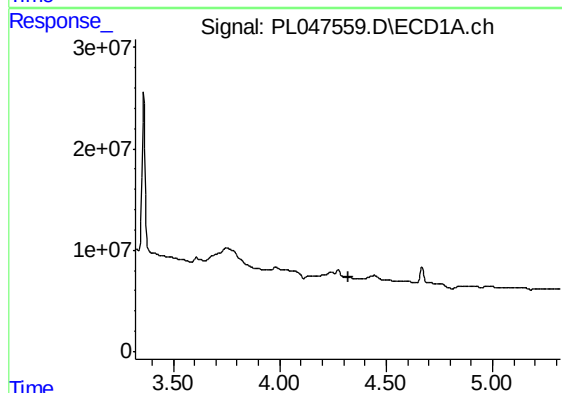


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.321 min
Response: 0
Conc: N.D.

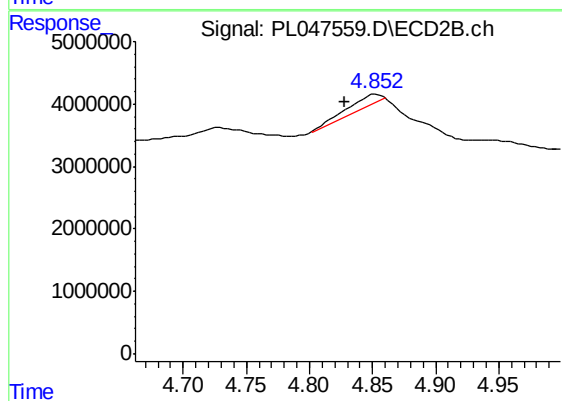

#6 beta-BHC


R.T.: 4.853 min
Delta R.T.: 0.025 min
Response: 4065407
Conc: 3.07 ng/ml

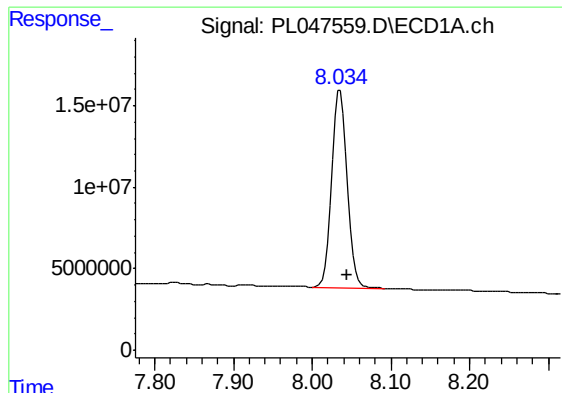

#28 Decachlorobiphenyl

R.T.: 8.035 min
Delta R.T.: -0.009 min
Response: 169214220
Conc: 20.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-21-D

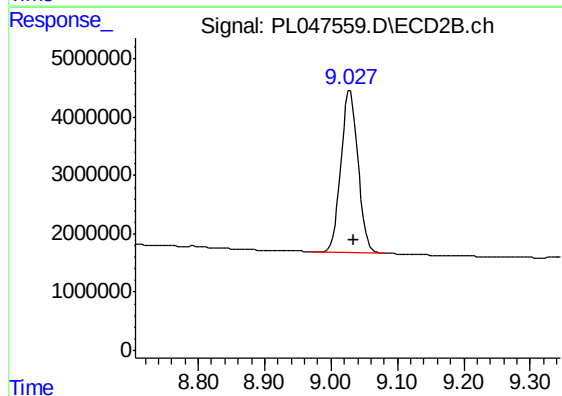

#28 Decachlorobiphenyl

R.T.: 9.029 min
Delta R.T.: -0.006 min
Response: 49900902
Conc: 21.52 ng/ml