

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041823\
 Data File : PL082177.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Apr 2023 15:43
 Operator : AR\AJ
 Sample : 02386-15
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SPA-4WC-23-04

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 18 22:25:35 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032223.M
 Quant Title : GC Extractables
 QLast Update : Thu Mar 23 01:07:33 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.330	2.648	24738616	483.4E6	10.636m	242.178 #
28)	SA Decachlor...	8.751	7.774	21038038	42409107	11.755	21.384 #
Target Compounds							
16)	A 4,4'-DDD	6.477	5.650	13130.4E6	8866.7E6	7280.558	5842.837



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041823\
Data File : PL082177.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Apr 2023 15:43
Operator : AR\AJ
Sample : 02386-15
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SPA-4WC-23-04

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 18 22:25:35 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032223.M
Quant Title : GC Extractables
QLast Update : Thu Mar 23 01:07:33 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

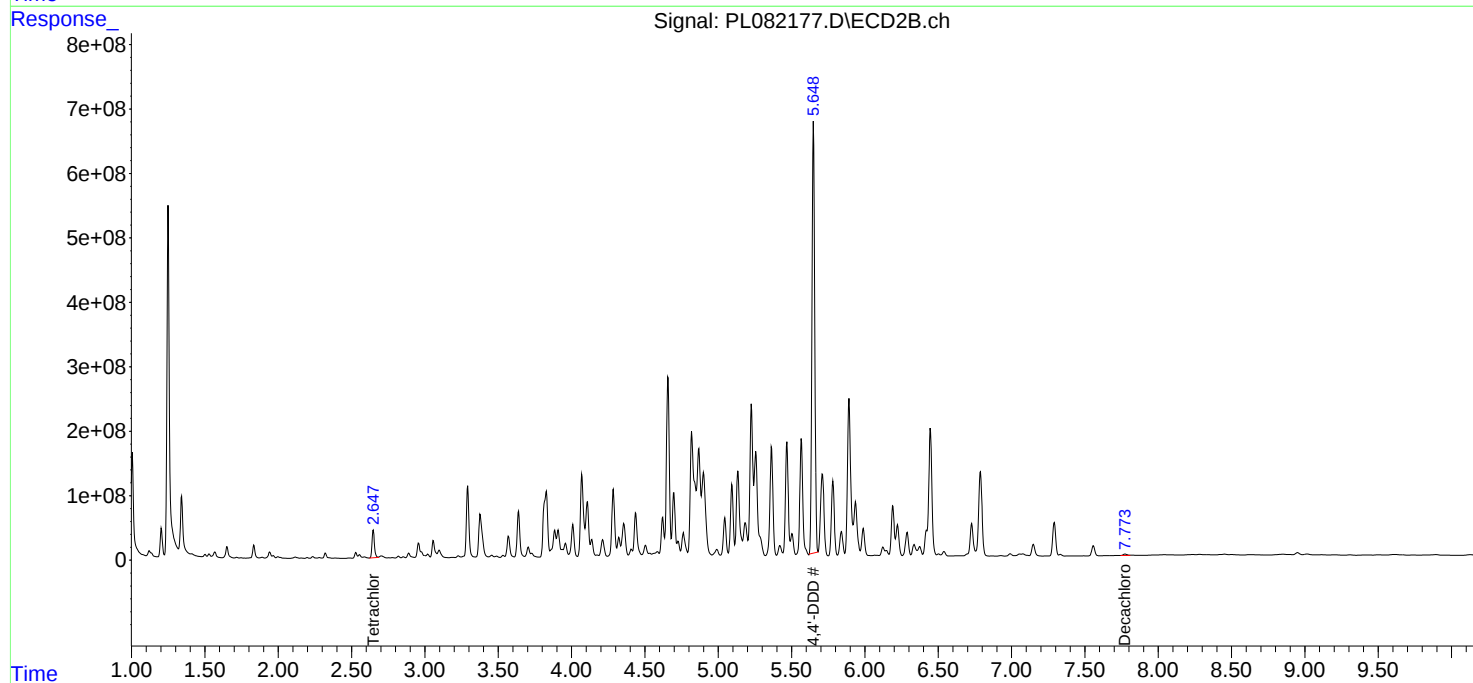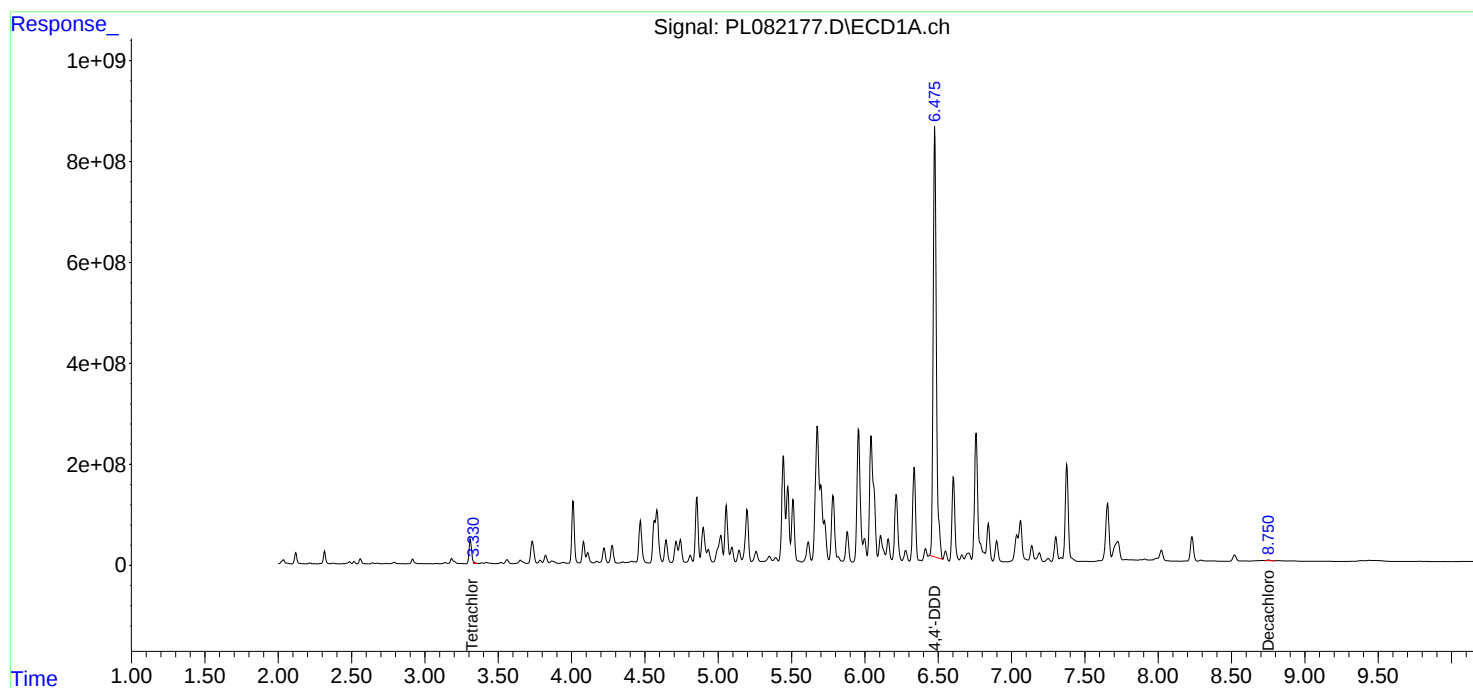


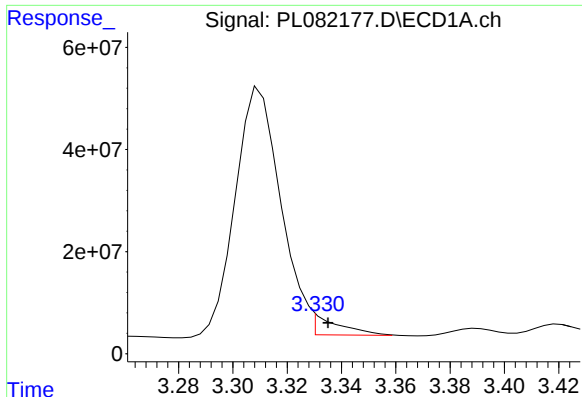

#1 Tetrachloro-m-xylene


R.T.: 3.330 min
Delta R.T.: -0.005 min
Response: 24738616
Conc: 10.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
SPA-4WC-23-04

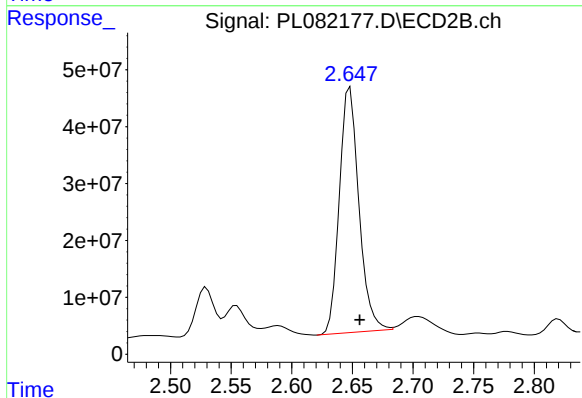


#1 Tetrachloro-m-xylene

R.T.: 2.648 min
Delta R.T.: -0.008 min
Response: 483423942
Conc: 242.18 ng/ml

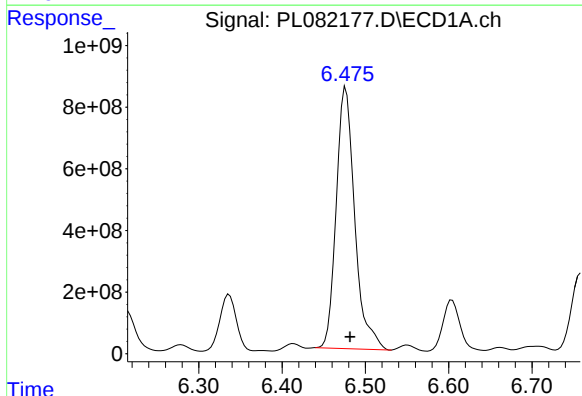


#16 4,4'-DDD

R.T.: 6.477 min
Delta R.T.: -0.005 min
Response: 13130386215
Conc: 7280.56 ng/ml

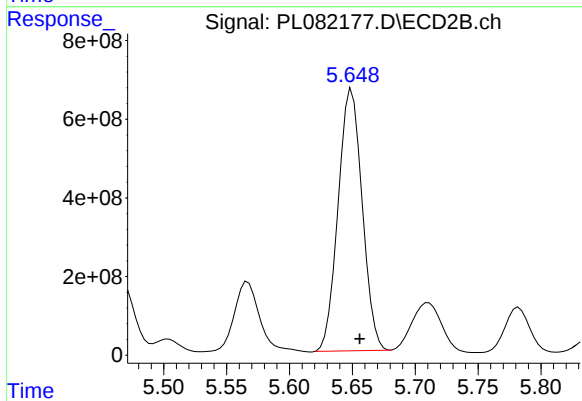

#16 4,4'-DDD


R.T.: 5.650 min
Delta R.T.: -0.006 min
Response: 8866705989
Conc: 5842.84 ng/ml

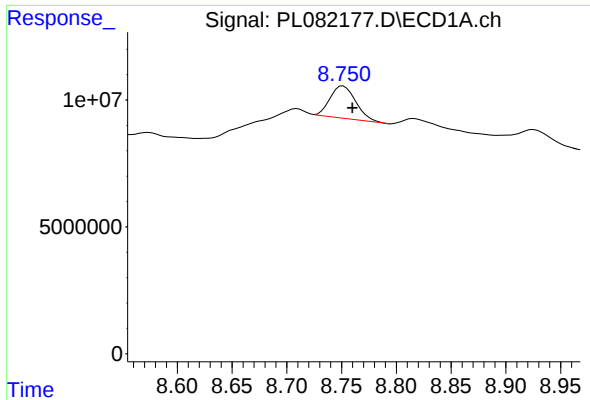

#28 Decachlorobiphenyl

R.T.: 8.751 min
Delta R.T.: -0.008 min
Response: 21038038
Conc: 11.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
SPA-4WC-23-04

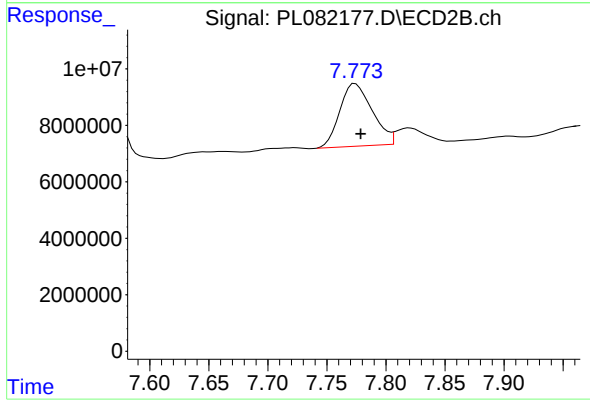

#28 Decachlorobiphenyl

R.T.: 7.774 min
Delta R.T.: -0.004 min
Response: 42409107
Conc: 21.38 ng/ml