

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL041824\  
 Data File : PL089084.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 18 Apr 2024 15:25  
 Operator : AR\AJ  
 Sample : P2151-01  
 Misc :  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 ECD\_L  
 ClientSampleId :  
 WATER-COMP

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 19 01:51:08 2024  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL041524.M  
 Quant Title : GC Extractables  
 QLast Update : Mon Apr 15 18:43:22 2024  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

|                             | Compound        | RT#1  | RT#2  | Resp#1   | Resp#2   | ng/ml  | ng/ml  |
|-----------------------------|-----------------|-------|-------|----------|----------|--------|--------|
| -----                       |                 |       |       |          |          |        |        |
| System Monitoring Compounds |                 |       |       |          |          |        |        |
| 1)                          | SA Tetrachlo... | 3.552 | 2.798 | 35108021 | 23210224 | 16.519 | 17.414 |
| 28)                         | SA Decachlor... | 9.066 | 7.951 | 12909424 | 12405911 | 10.135 | 9.264  |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL041824\  
Data File : PL089084.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 18 Apr 2024 15:25  
Operator : AR\AJ  
Sample : P2151-01  
Misc :  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
ECD\_L  
ClientSampleId :  
WATER-COMP

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Apr 19 01:51:08 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL041524.M  
Quant Title : GC Extractables  
QLast Update : Mon Apr 15 18:43:22 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

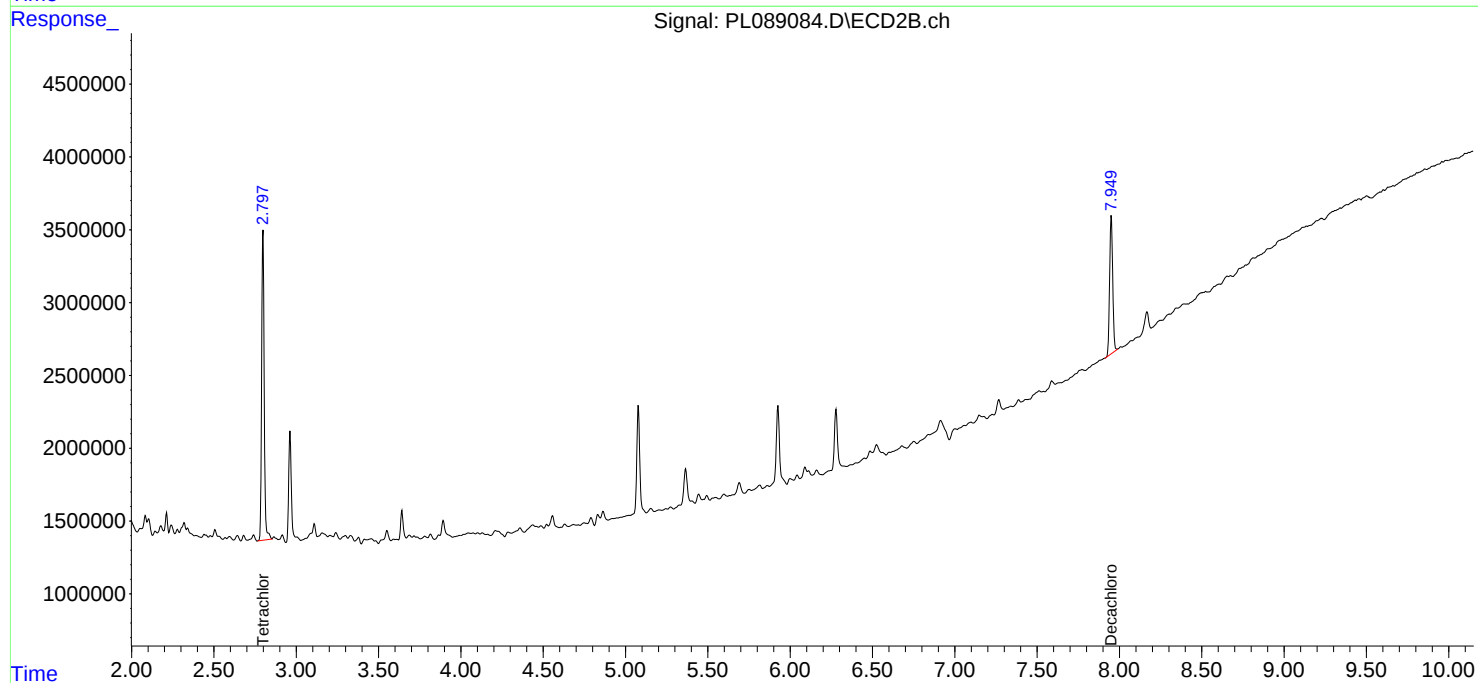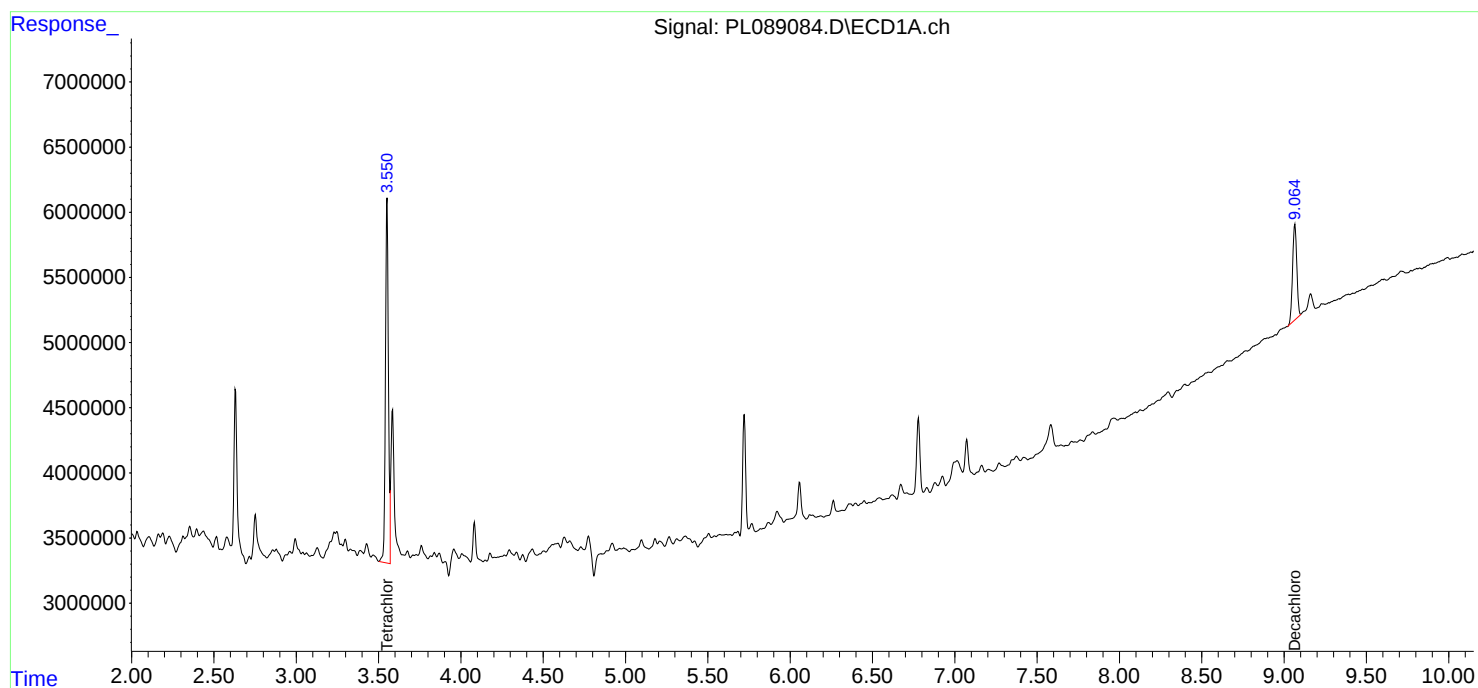


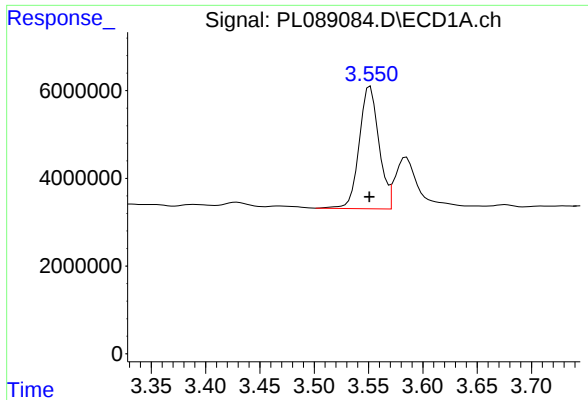

#1 Tetrachloro-m-xylene


R.T.: 3.552 min  
Delta R.T.: 0.000 min  
Response: 35108021  
Conc: 16.52 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :  
WATER-COMP

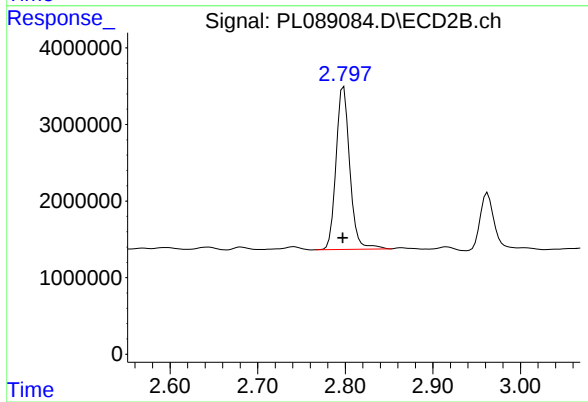


#1 Tetrachloro-m-xylene

R.T.: 2.798 min  
Delta R.T.: 0.001 min  
Response: 23210224  
Conc: 17.41 ng/ml

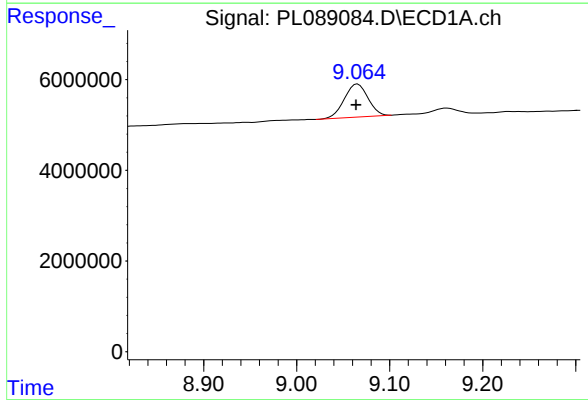

#28 Decachlorobiphenyl

R.T.: 9.066 min  
Delta R.T.: 0.002 min  
Response: 12909424  
Conc: 10.13 ng/ml

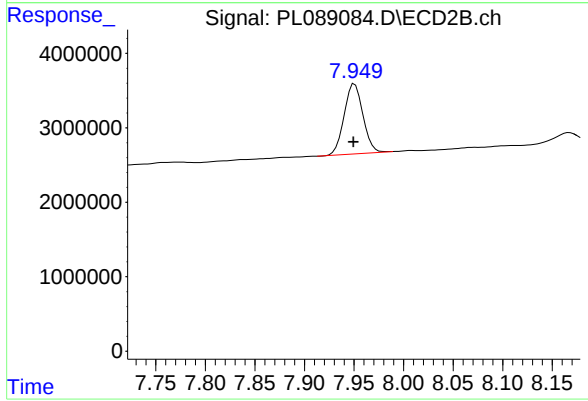

#28 Decachlorobiphenyl

R.T.: 7.951 min  
Delta R.T.: 0.001 min  
Response: 12405911  
Conc: 9.26 ng/ml