

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041919\
 Data File : PL047585.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Apr 2019 16:14
 Operator : AJ\SJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 19 16:50:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041919.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 19 16:45:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.330	3.940	442.0E6	117.7E6	50.000	50.000
28)	SA Decachlor...	8.004	8.975	474.9E6	131.3E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.173	4.927	196.7E6	56479763	500.000	500.000
24)	Chlordane-2	4.664	5.394	225.7E6	59732426	500.000	500.000
25)	Chlordane-3	5.221	6.037	685.6E6	200.6E6	500.000	500.000
26)	Chlordane-4	5.276	6.110	633.8E6	236.2E6	500.000	500.000
27)	Chlordane-5	6.099	6.912	195.2E6	47308765	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041919\
Data File : PL047585.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Apr 2019 16:14
Operator : AJ\SJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 19 16:50:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041919.M
Quant Title : GC Extractables
QLast Update : Fri Apr 19 16:45:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

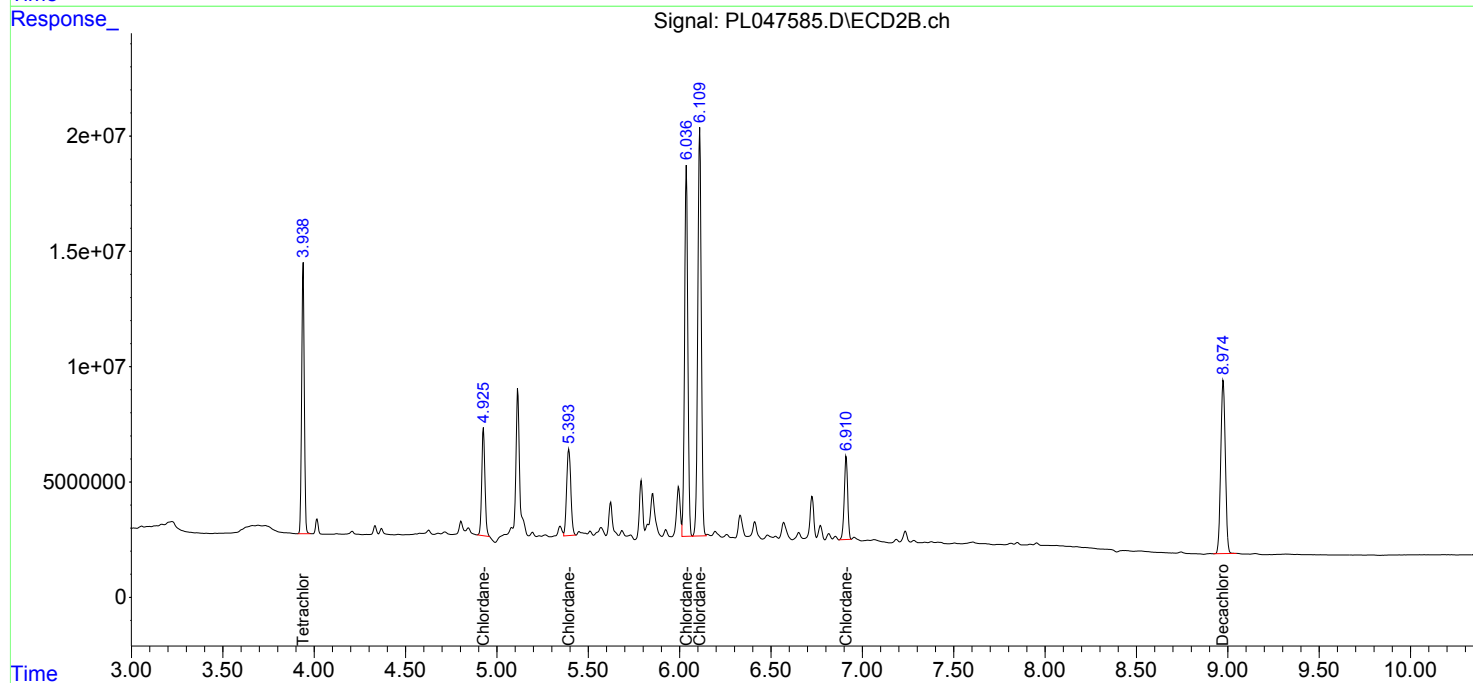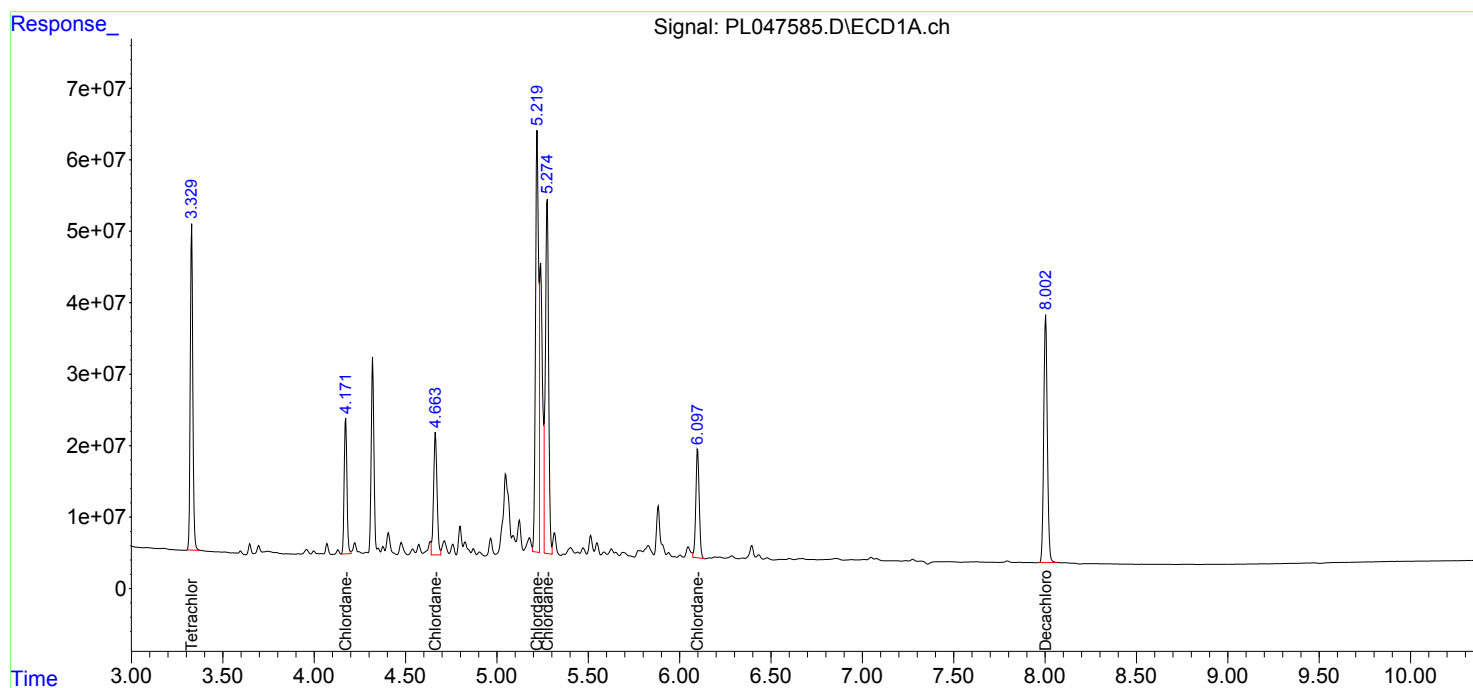


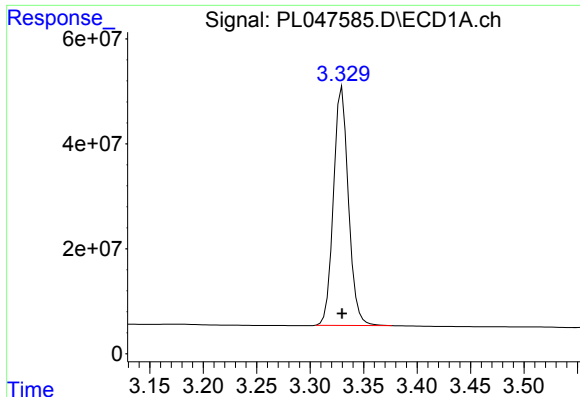

#1 Tetrachloro-m-xylene


R.T.: 3.330 min
Delta R.T.: 0.000 min
Response: 442038564
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

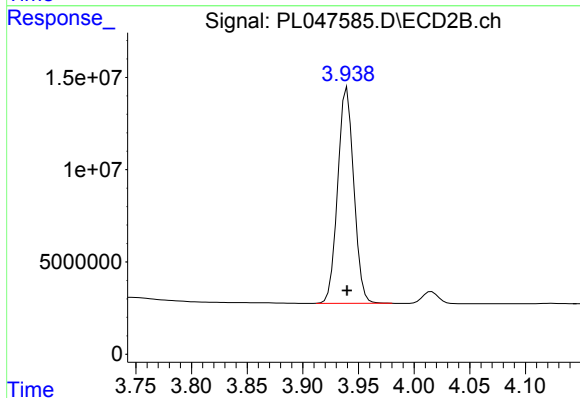


#1 Tetrachloro-m-xylene

R.T.: 3.940 min
Delta R.T.: 0.000 min
Response: 117660639
Conc: 50.00 ng/ml

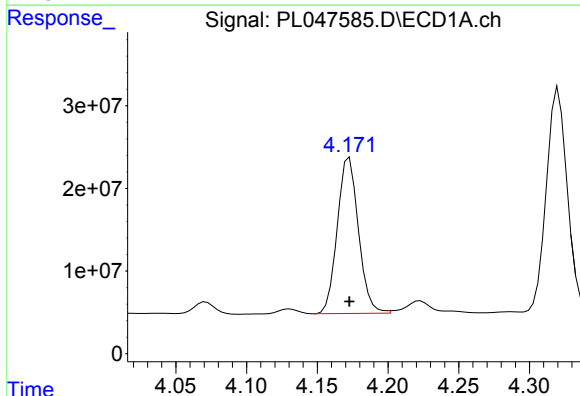


#23 Chlordane-1

R.T.: 4.173 min
Delta R.T.: 0.000 min
Response: 196728804
Conc: 500.00 ng/ml

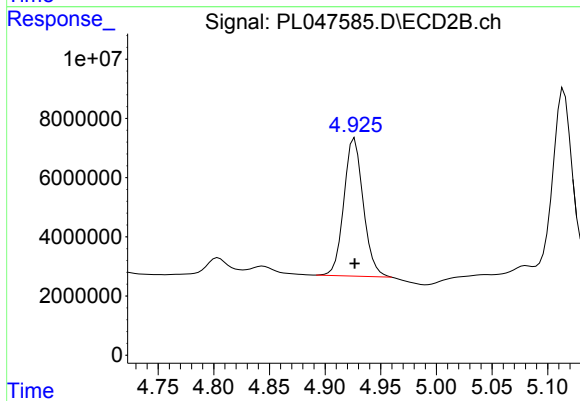

#23 Chlordane-1


R.T.: 4.927 min
Delta R.T.: 0.000 min
Response: 56479763
Conc: 500.00 ng/ml

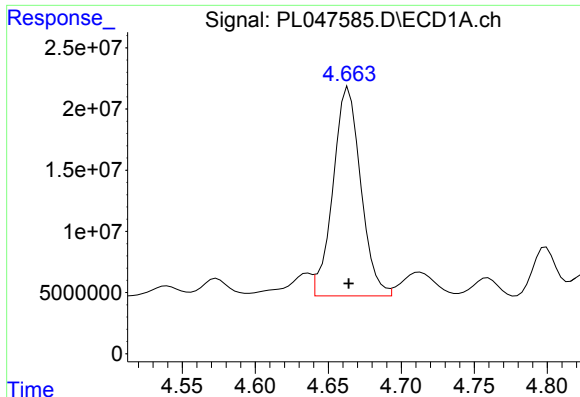

#24 Chlordane-2


R.T.: 4.664 min
Delta R.T.: 0.000 min
Response: 225665627
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

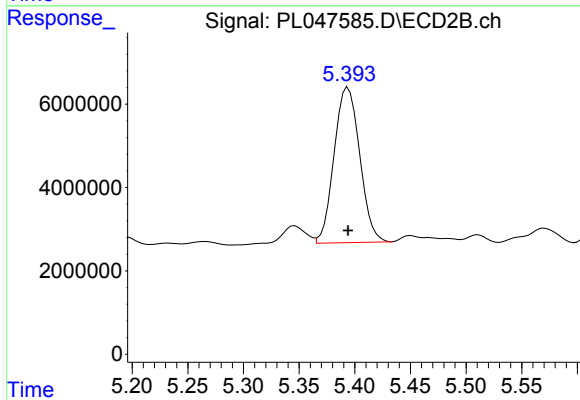


#24 Chlordane-2

R.T.: 5.394 min
Delta R.T.: 0.000 min
Response: 59732426
Conc: 500.00 ng/ml

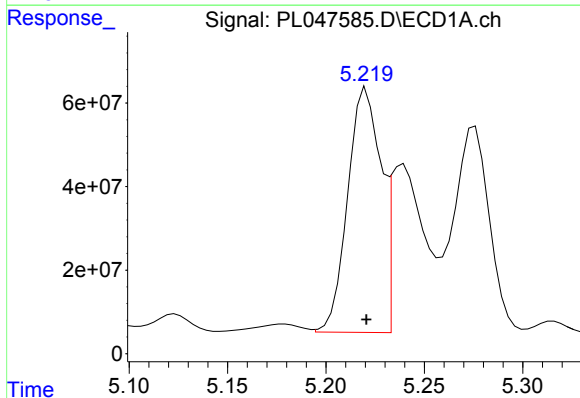


#25 Chlordane-3

R.T.: 5.221 min
Delta R.T.: 0.000 min
Response: 685553890
Conc: 500.00 ng/ml

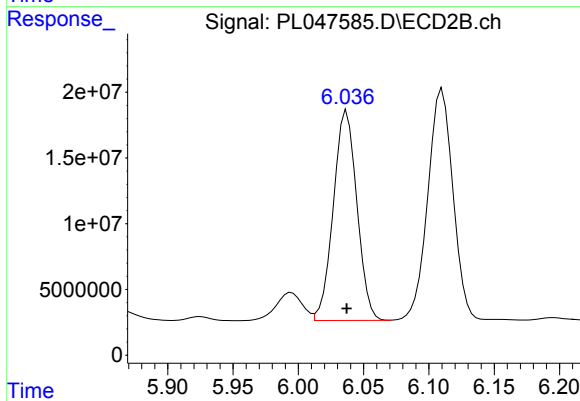

#25 Chlordane-3


R.T.: 6.037 min
Delta R.T.: 0.000 min
Response: 200599486
Conc: 500.00 ng/ml

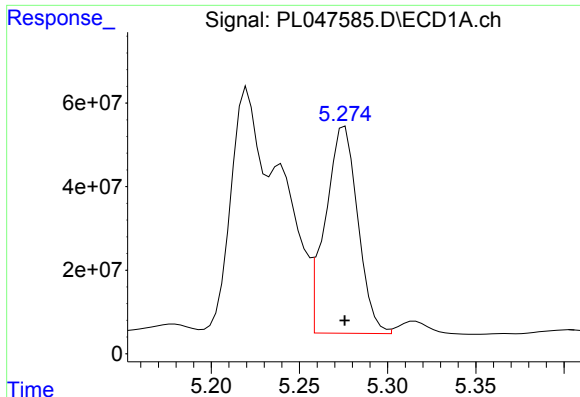

#26 Chlordane-4


R.T.: 5.276 min
Delta R.T.: 0.000 min
Response: 633764310
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

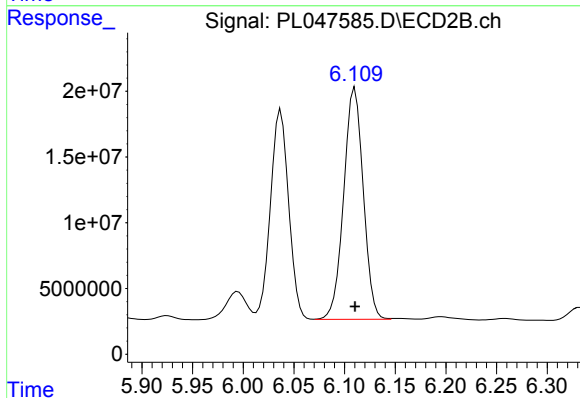


#26 Chlordane-4

R.T.: 6.110 min
Delta R.T.: 0.000 min
Response: 236206106
Conc: 500.00 ng/ml

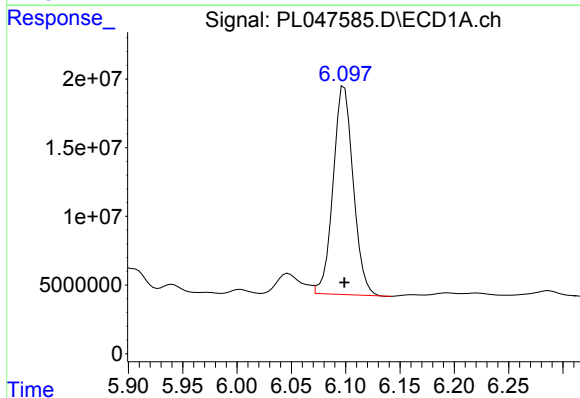


#27 Chlordane-5

R.T.: 6.099 min
Delta R.T.: 0.000 min
Response: 195154334
Conc: 500.00 ng/ml

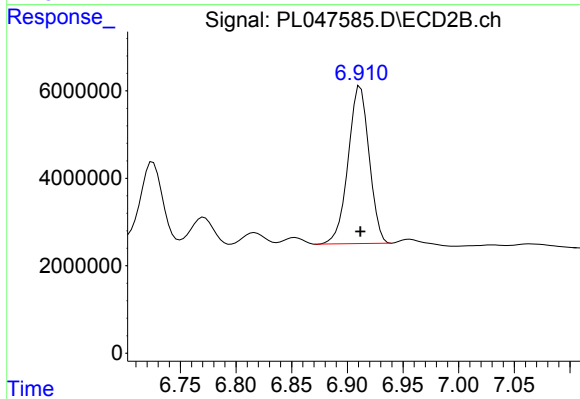

#27 Chlordane-5


R.T.: 6.912 min
Delta R.T.: 0.000 min
Response: 47308765
Conc: 500.00 ng/ml

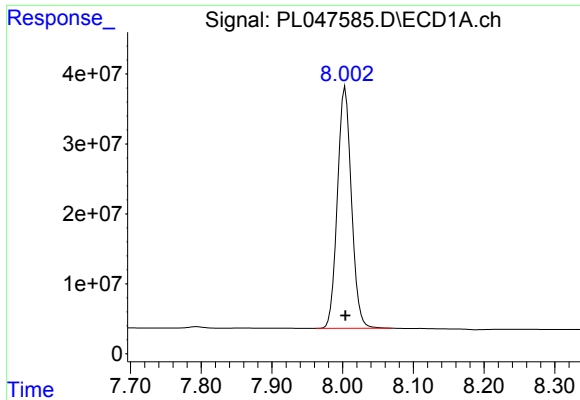

#28 Decachlorobiphenyl

R.T.: 8.004 min
Delta R.T.: 0.000 min
Response: 474946637
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

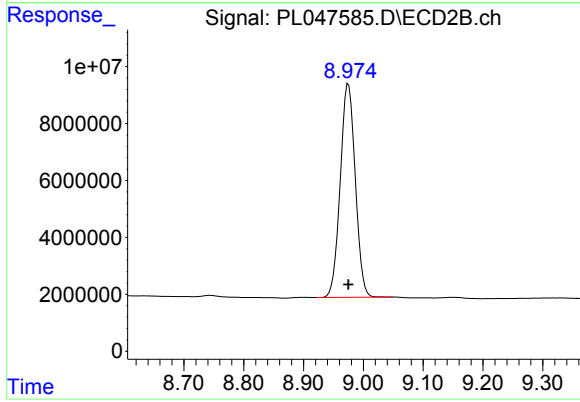

#28 Decachlorobiphenyl

R.T.: 8.975 min
Delta R.T.: 0.000 min
Response: 131289699
Conc: 50.00 ng/ml