

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041919\
 Data File : PL047591.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Apr 2019 20:41
 Operator : AJ\SJ
 Sample : PB119048BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PSTDCCC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 19 23:32:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041919.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 19 16:51:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.330	3.941	187.6E6	51532539	21.146	19.305
28) SA Decachlor...	8.005	8.975	177.7E6	54342804	17.588	17.902
Target Compounds						
4) MA Heptachlor	0.000	5.101	0	3091993	N.D.	0.839 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041919\
Data File : PL047591.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Apr 2019 20:41
Operator : AJ\SJ
Sample : PB119048BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 19 23:32:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041919.M
Quant Title : GC Extractables
QLast Update : Fri Apr 19 16:51:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

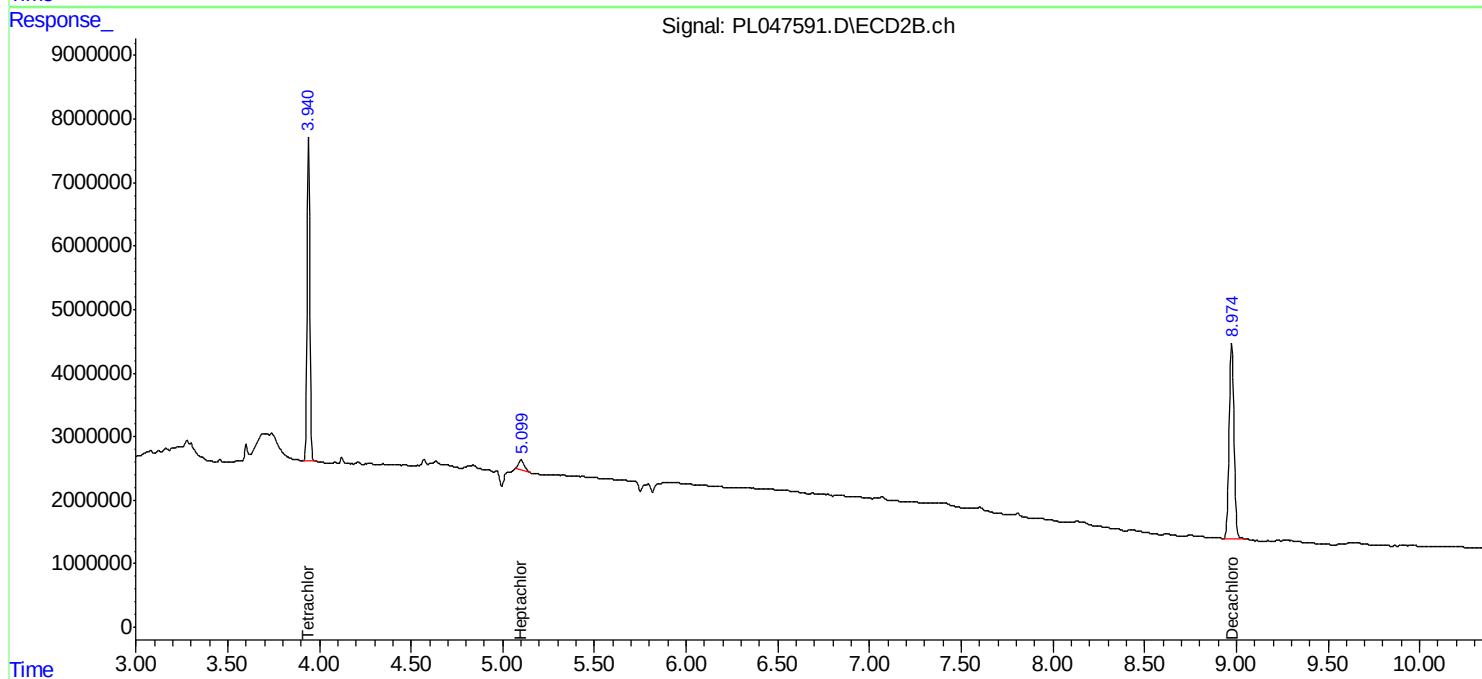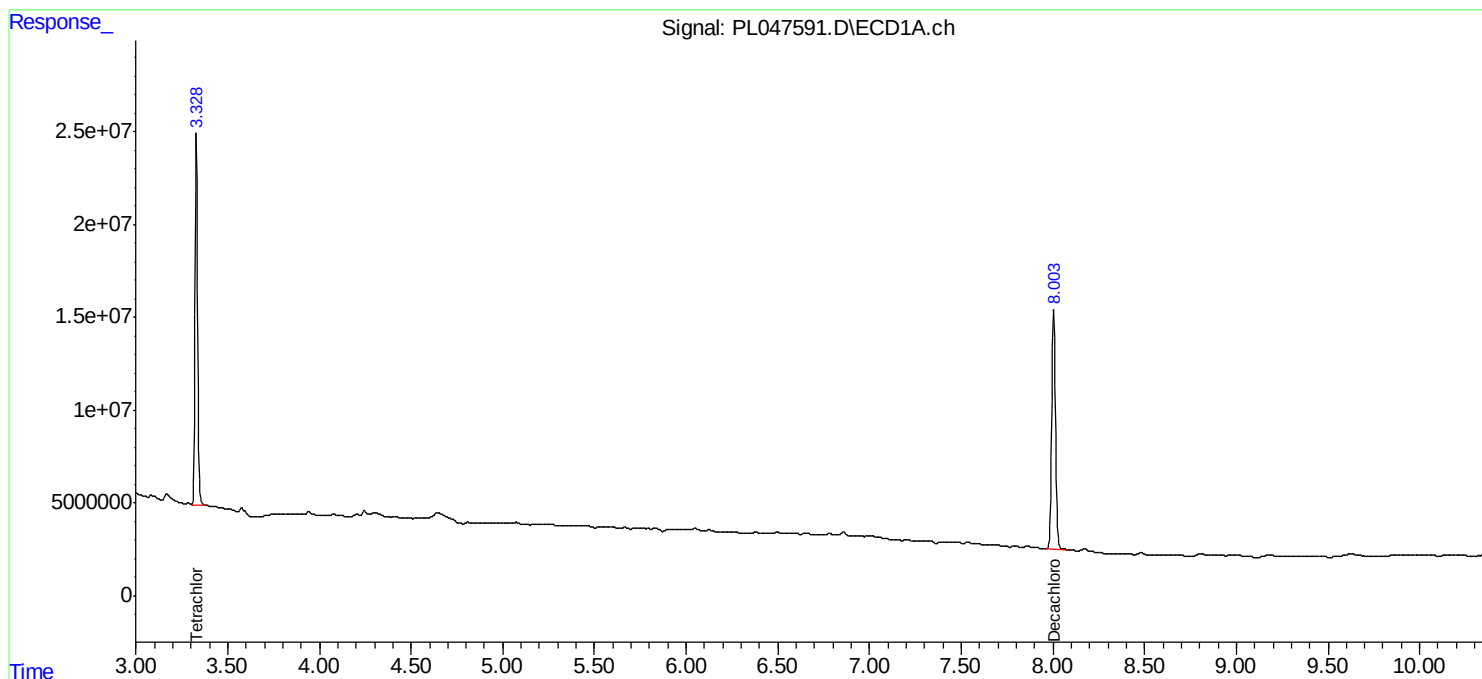


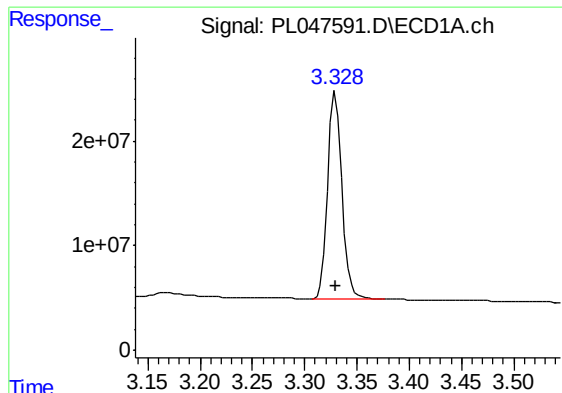

#1 Tetrachloro-m-xylene


R.T.: 3.330 min
Delta R.T.: 0.000 min
Response: 187622024
Conc: 21.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

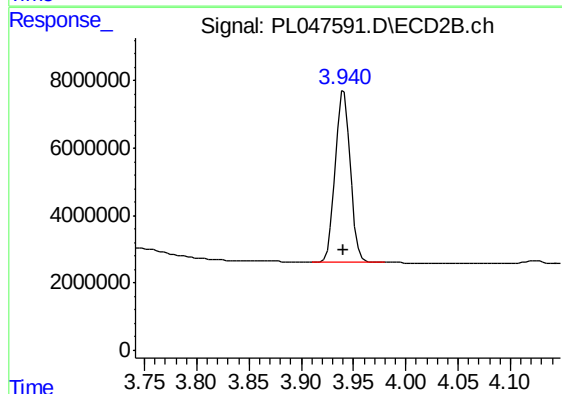


#1 Tetrachloro-m-xylene

R.T.: 3.941 min
Delta R.T.: 0.000 min
Response: 51532539
Conc: 19.30 ng/ml

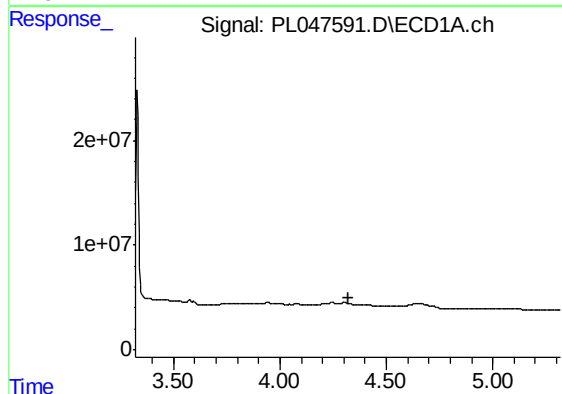


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.320 min
Response: 0
Conc: N.D.

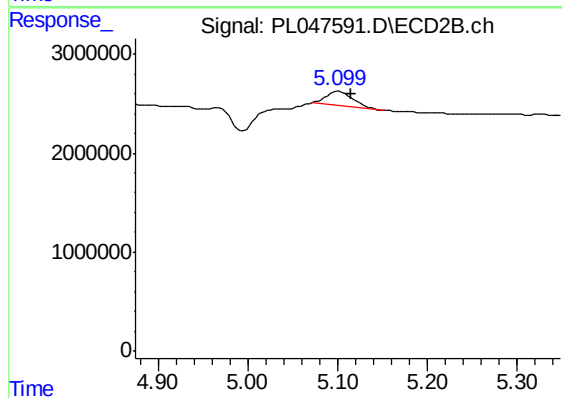

#4 Heptachlor


R.T.: 5.101 min
Delta R.T.: -0.014 min
Response: 3091993
Conc: 0.84 ng/ml

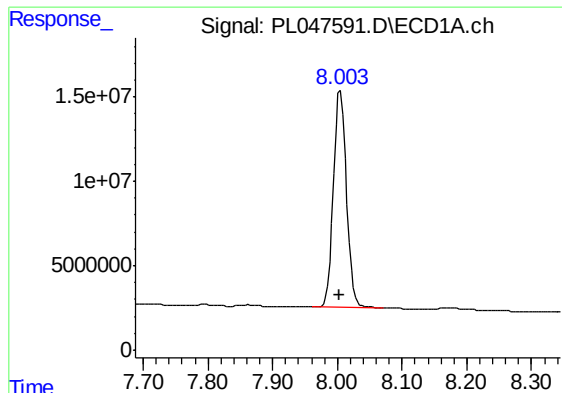

#28 Decachlorobiphenyl

R.T.: 8.005 min
Delta R.T.: 0.002 min
Response: 177668577
Conc: 17.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

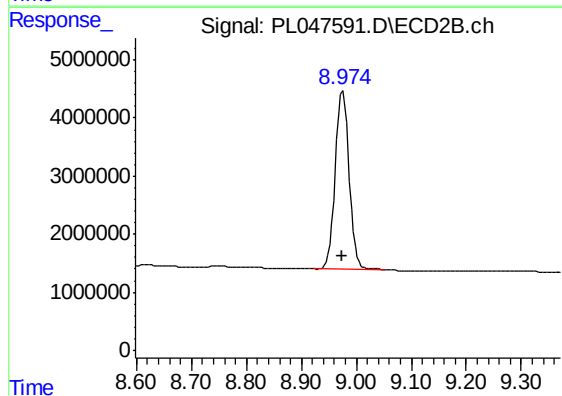

#28 Decachlorobiphenyl

R.T.: 8.975 min
Delta R.T.: 0.000 min
Response: 54342804
Conc: 17.90 ng/ml