

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041919\
 Data File : PL047608.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2019 00:58
 Operator : AJ\SJ
 Sample : K2198-06
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-TRACK-74-75

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 20 01:16:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041919.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 19 16:51:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.331	3.941	191.0E6	52293599	21.526	19.590
28)	SA Decachlor...	8.004	8.975	159.3E6	46444434	15.772	15.300
Target Compounds							
4)	MA Heptachlor	0.000	5.120	0	6293425	N.D.	1.708 #
12)	B 4,4'-DDE	5.432	0.000	16386882	0	1.409	N.D. #
17)	MA 4,4'-DDT	0.000	7.071f	0	2202666	N.D.	0.886 #
24)	Chlordane-2	4.654	0.000	36234740	0	80.284	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041919\
Data File : PL047608.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2019 00:58
Operator : AJ\SJ
Sample : K2198-06
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-TRACK-74-75

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 20 01:16:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041919.M
Quant Title : GC Extractables
QLast Update : Fri Apr 19 16:51:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

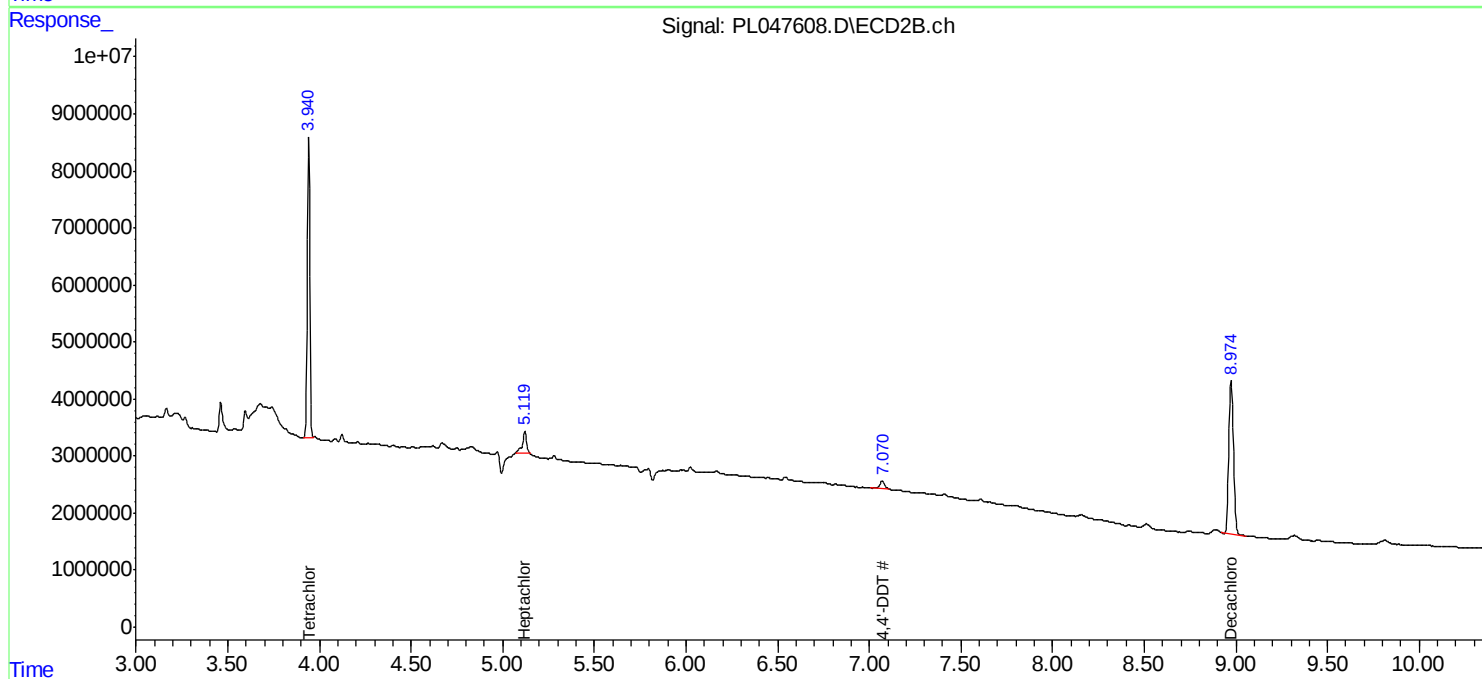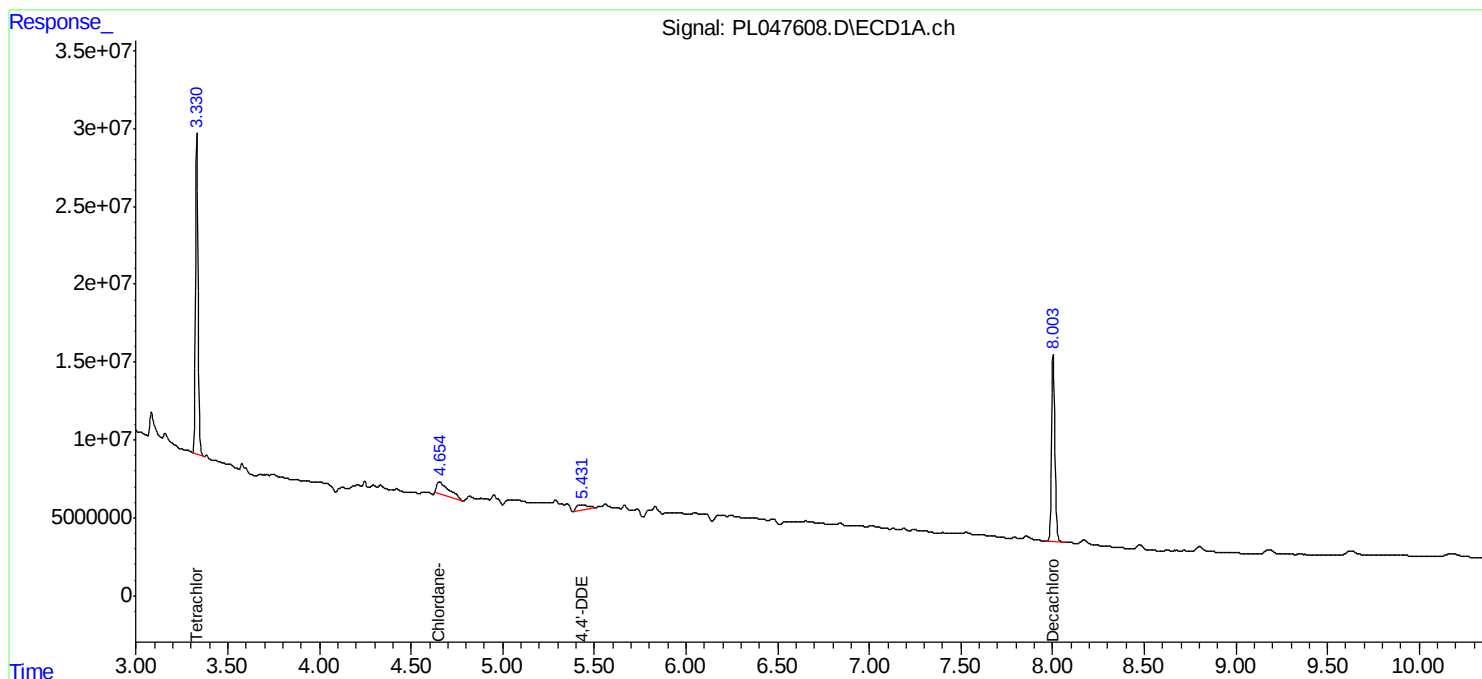


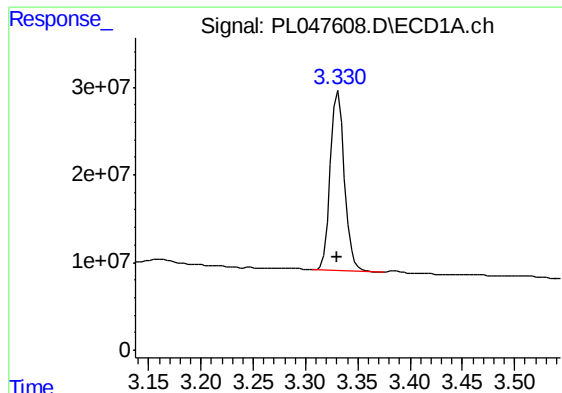

#1 Tetrachloro-m-xylene


R.T.: 3.331 min
Delta R.T.: 0.001 min
Response: 190992694
Conc: 21.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-TRACK-74-75

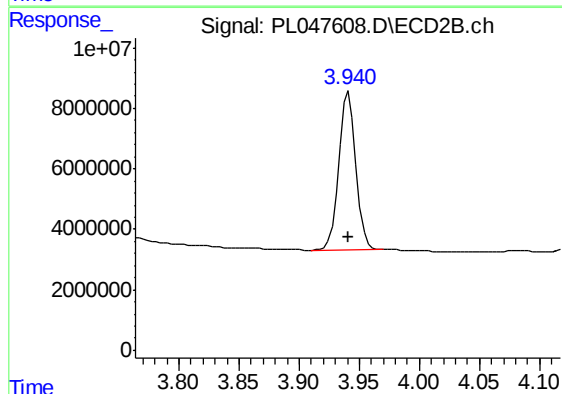


#1 Tetrachloro-m-xylene

R.T.: 3.941 min
Delta R.T.: 0.000 min
Response: 52293599
Conc: 19.59 ng/ml

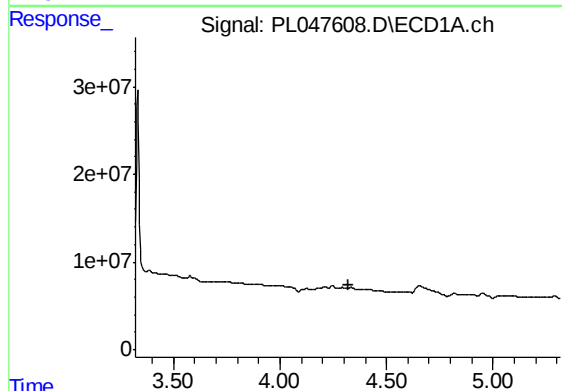


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.320 min
Response: 0
Conc: N.D.

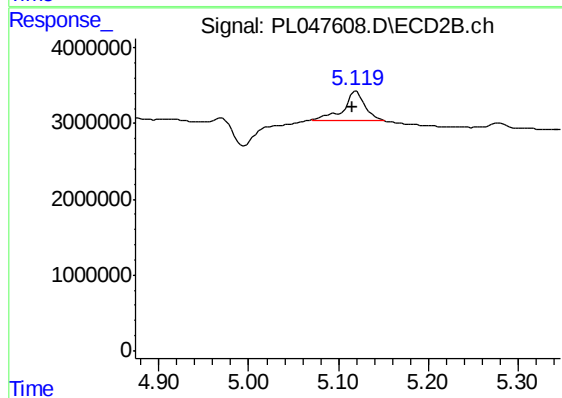

#4 Heptachlor


R.T.: 5.120 min
Delta R.T.: 0.005 min
Response: 6293425
Conc: 1.71 ng/ml

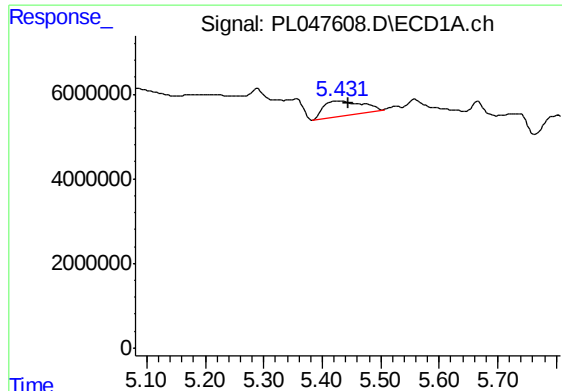

#12 4,4'-DDE


R.T.: 5.432 min
Delta R.T.: -0.012 min
Response: 16386882
Conc: 1.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-TRACK-74-75

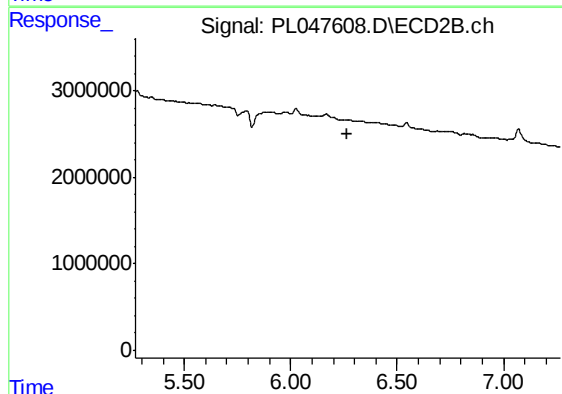


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.268 min
Response: 0
Conc: N.D.

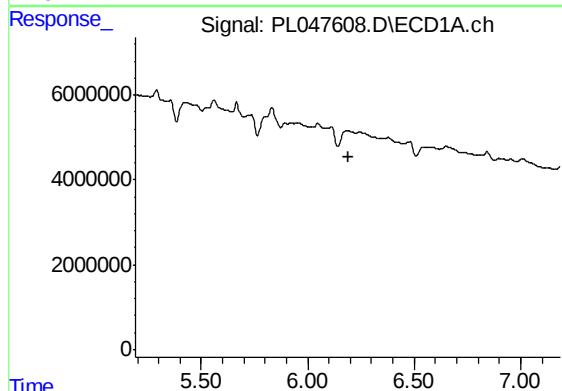


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.190 min
Response: 0
Conc: N.D.

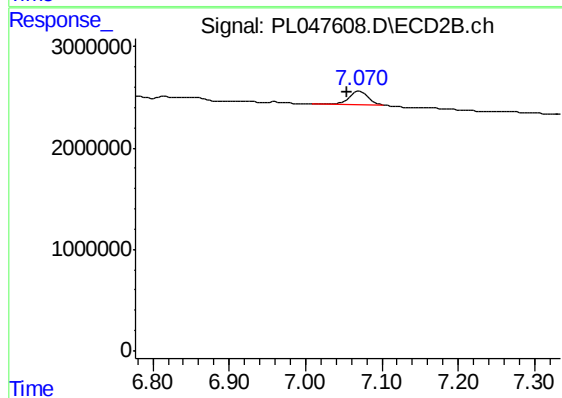

#17 4,4'-DDT


R.T.: 7.071 min
Delta R.T.: 0.016 min
Response: 2202666
Conc: 0.89 ng/ml

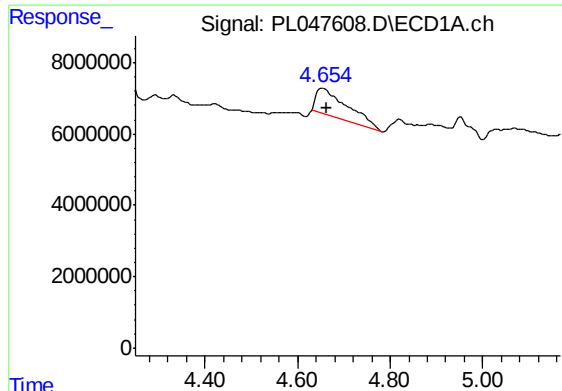

#24 Chlordane-2


R.T.: 4.654 min
Delta R.T.: -0.010 min
Response: 36234740
Conc: 80.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-TRACK-74-75

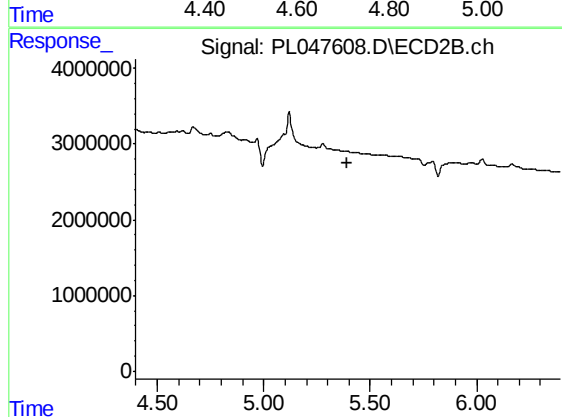


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.394 min
Response: 0
Conc: N.D.

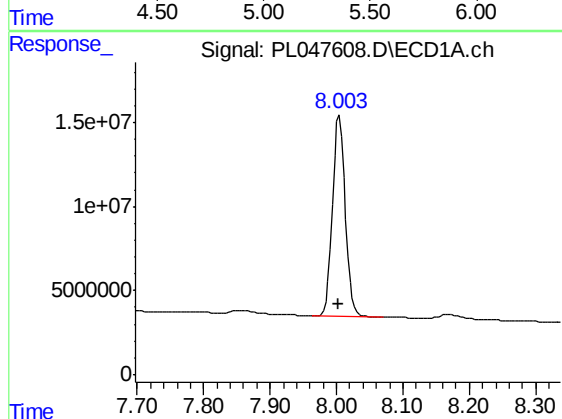

#28 Decachlorobiphenyl

R.T.: 8.004 min
Delta R.T.: 0.001 min
Response: 159315919
Conc: 15.77 ng/ml

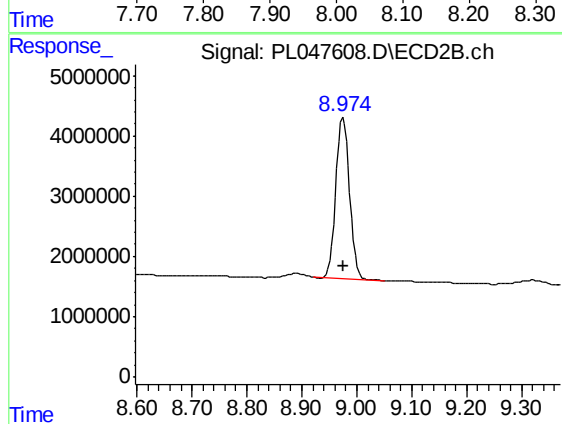

#28 Decachlorobiphenyl

R.T.: 8.975 min
Delta R.T.: 0.000 min
Response: 46444434
Conc: 15.30 ng/ml