

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041922\
 Data File : PL074171.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Apr 2022 09:12
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 19 16:50:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 14 09:29:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.639	5.490	8232532	44544530	25.479	24.983
28)	SA Decachlor...	10.415	11.338	12149878	40665440	23.364	23.023
Target Compounds							
6)	B beta-BHC	0.000	6.682	0	940116	N.D.	0.834 #
7)	B delta-BHC	0.000	6.958	0	2852445	N.D.	1.168 #
10)	B gamma-Chl...	0.000	8.201	0	607400	N.D.	0.272 #
11)	B alpha-Chl...	0.000	8.260f	0	117166	N.D.	0.054 #
13)	MA Dieldrin	7.802f	8.609	87662	64571	0.204	0.032 #
14)	MA Endrin	8.089f	8.858	288293	434252	0.710	0.256 #
15)	B Endosulfa...	8.352f	9.059	60814	570575	0.148	0.328 #
16)	A 4,4'-DDD	0.000	9.007f	0	1049710	N.D.	0.682 #
23)	Chlordane-1	0.000	6.858	0	1145465	N.D.	14.354 #
25)	Chlordane-3	0.000	8.201	0	607400	N.D.	1.795 #
26)	Chlordane-4	0.000	8.260f	0	117166	N.D.	0.295 #
27)	Chlordane-5	8.352f	0.000	60814	0	3.487	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041922\
Data File : PL074171.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Apr 2022 09:12
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 19 16:50:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
Quant Title : GC Extractables
QLast Update : Thu Apr 14 09:29:23 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

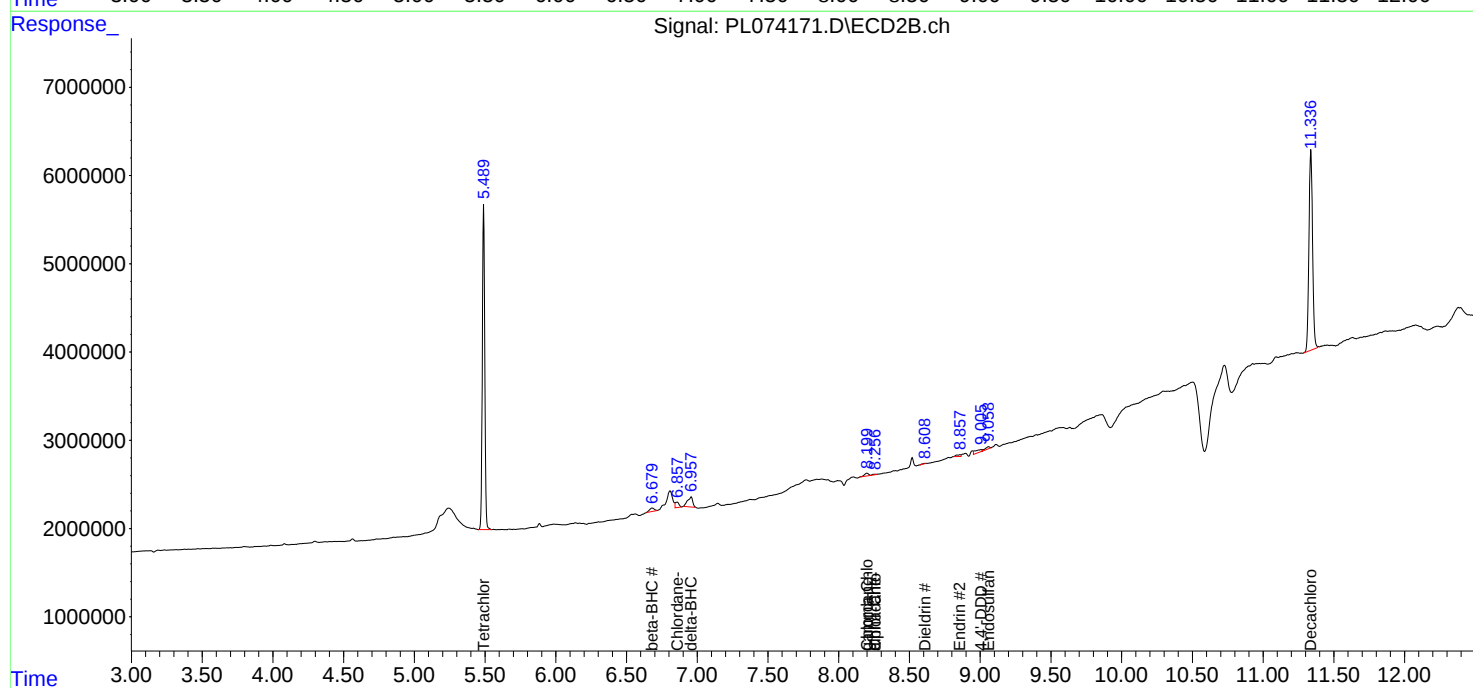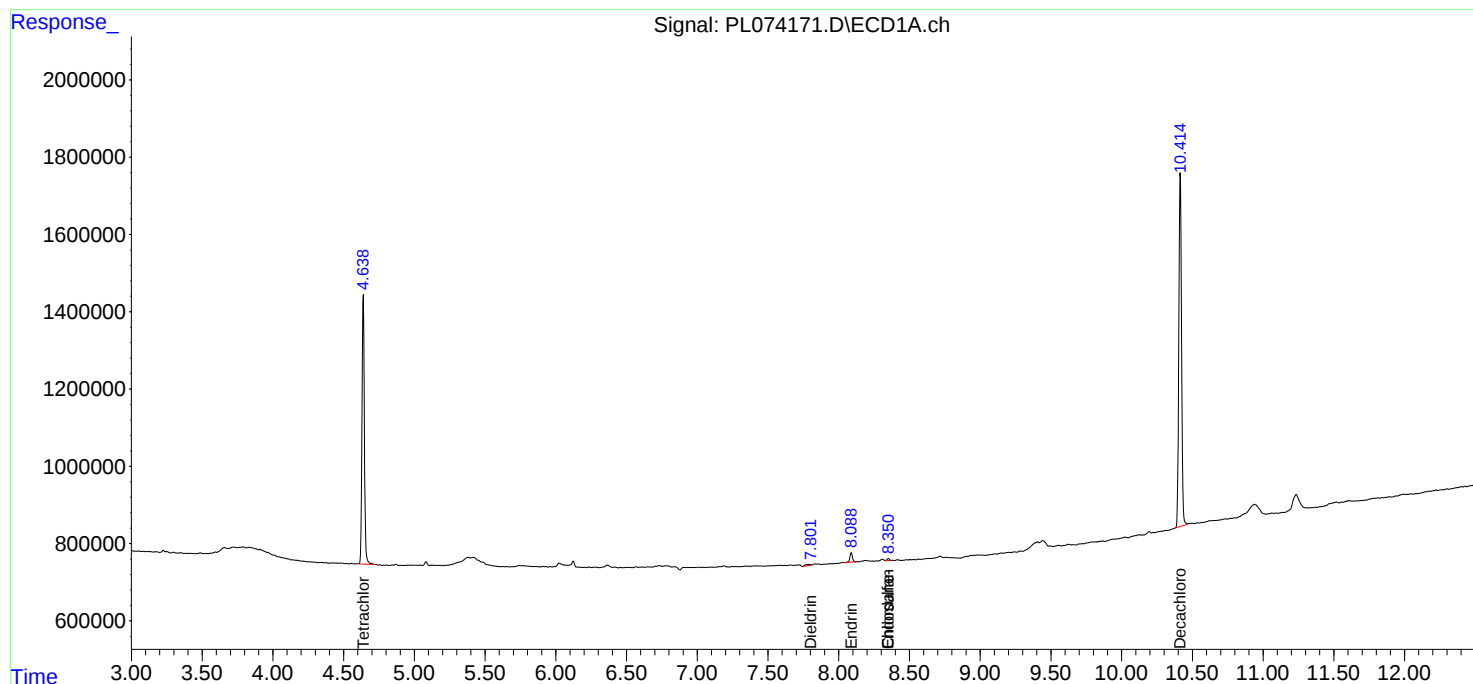


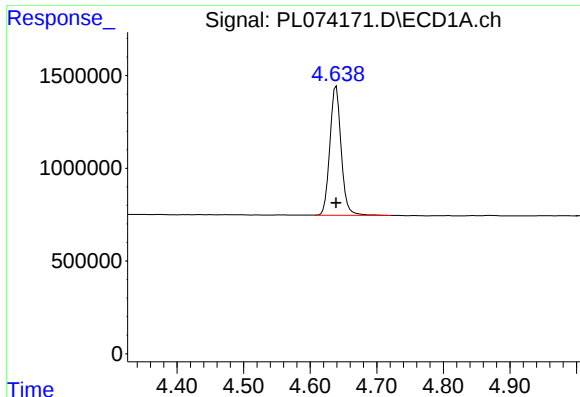

#1 Tetrachloro-m-xylene


R.T.: 4.639 min
Delta R.T.: 0.000 min
Response: 8232532
Conc: 25.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

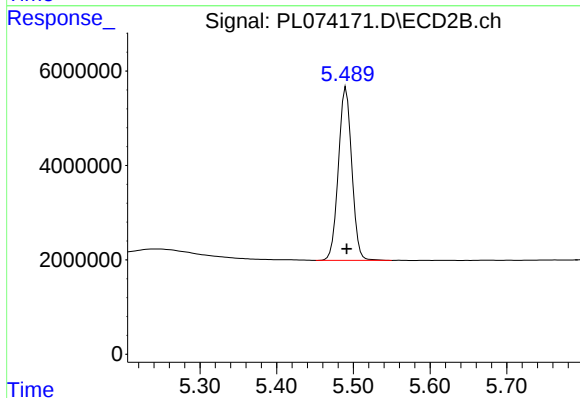


#1 Tetrachloro-m-xylene

R.T.: 5.490 min
Delta R.T.: -0.001 min
Response: 44544530
Conc: 24.98 ng/ml

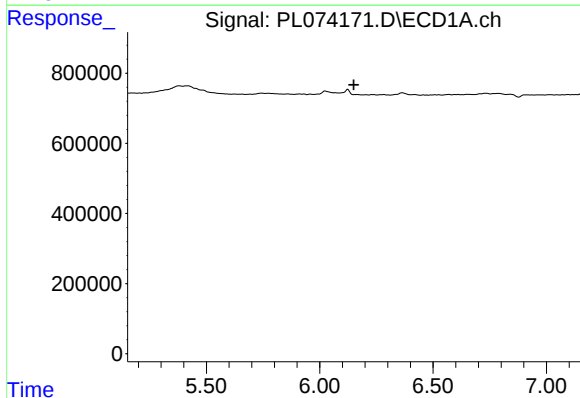


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.151 min
Response: 0
Conc: N.D.

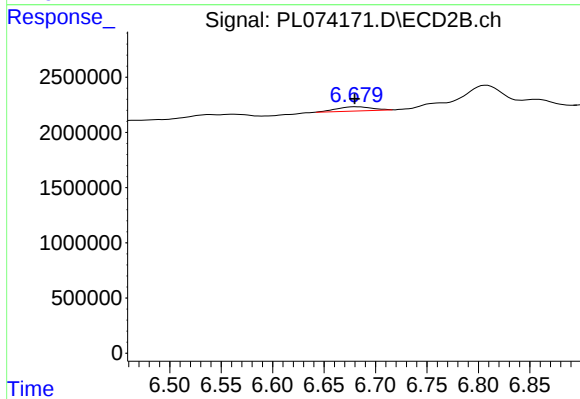

#6 beta-BHC


R.T.: 6.682 min
Delta R.T.: 0.002 min
Response: 940116
Conc: 0.83 ng/ml

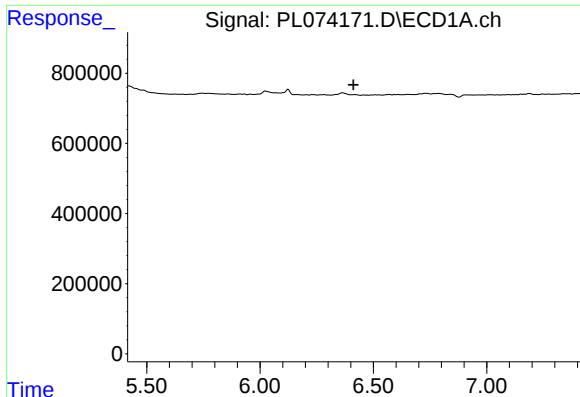

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.412 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

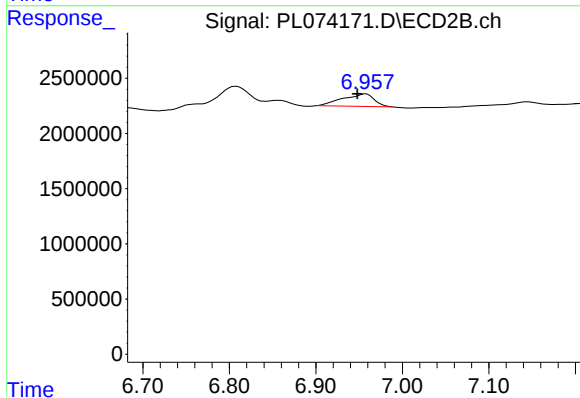


#7 delta-BHC

R.T.: 6.958 min
Delta R.T.: 0.010 min
Response: 2852445
Conc: 1.17 ng/ml

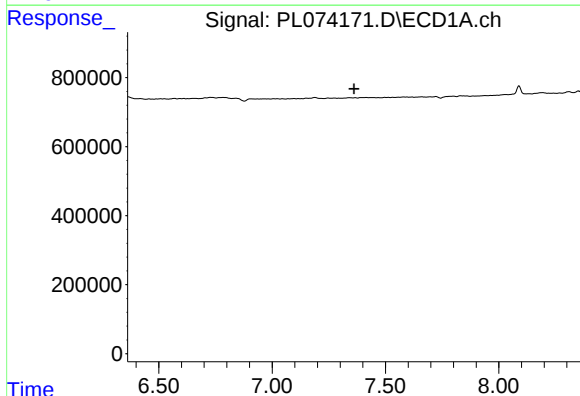


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.362 min
Response: 0
Conc: N.D.

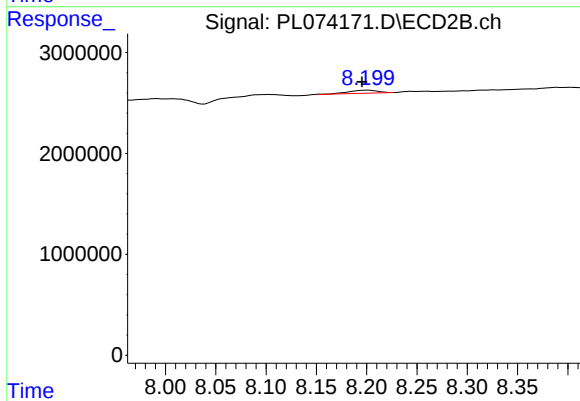

#10 gamma-Chlordane


R.T.: 8.201 min
Delta R.T.: 0.005 min
Response: 607400
Conc: 0.27 ng/ml

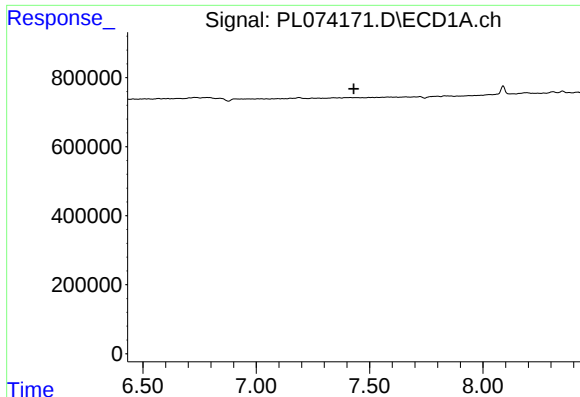

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.431 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

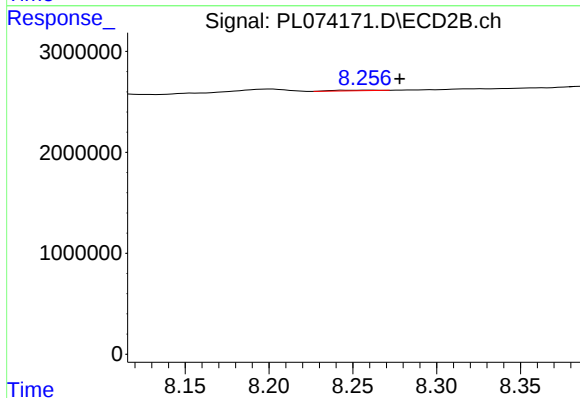


#11 alpha-Chlordane

R.T.: 8.260 min
Delta R.T.: -0.018 min
Response: 117166
Conc: 0.05 ng/ml

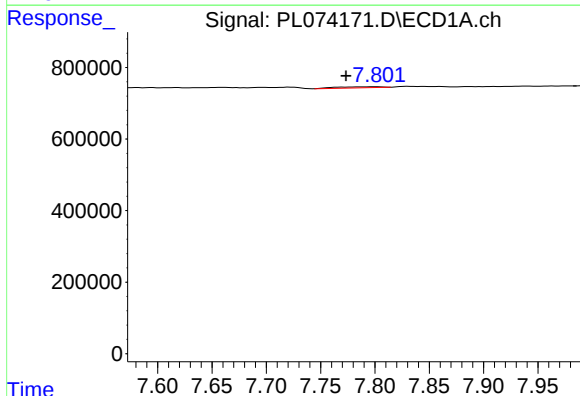


#13 Dieldrin

R.T.: 7.802 min
Delta R.T.: 0.029 min
Response: 87662
Conc: 0.20 ng/ml

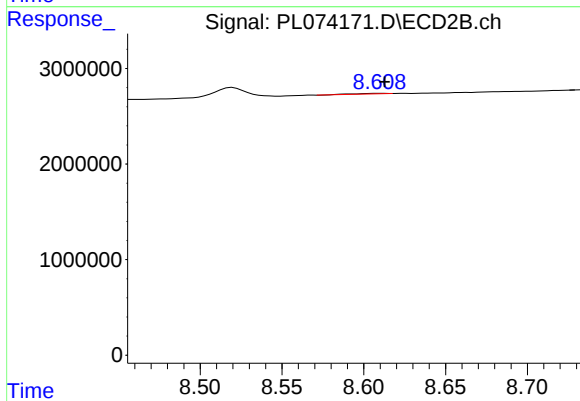

#13 Dieldrin


R.T.: 8.609 min
Delta R.T.: -0.003 min
Response: 64571
Conc: 0.03 ng/ml

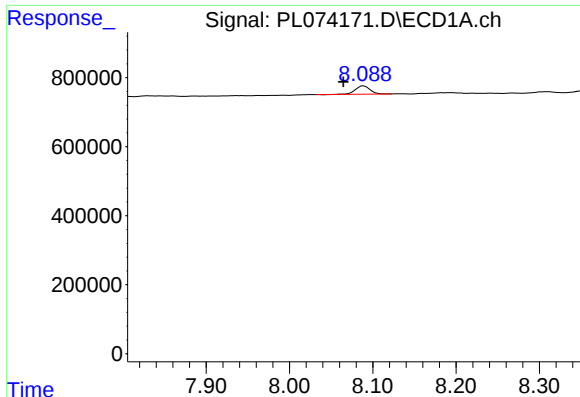

#14 Endrin


R.T.: 8.089 min
Delta R.T.: 0.024 min
Response: 288293
Conc: 0.71 ng/ml

Instrument :
ECD_L
ClientSampleId :

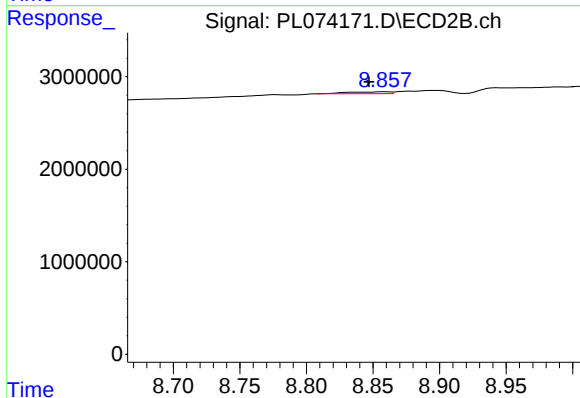


#14 Endrin

R.T.: 8.858 min
Delta R.T.: 0.011 min
Response: 434252
Conc: 0.26 ng/ml

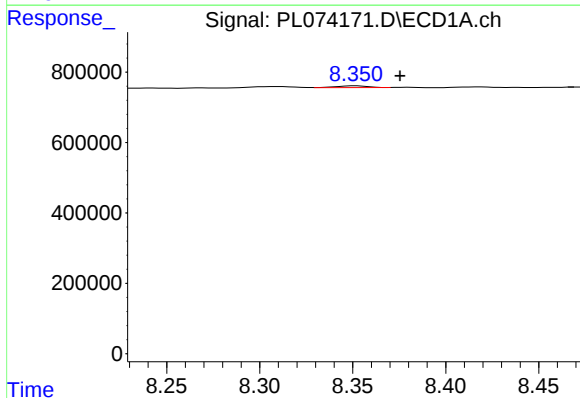


#15 Endosulfan II

R.T.: 8.352 min
Delta R.T.: -0.024 min
Response: 60814
Conc: 0.15 ng/ml

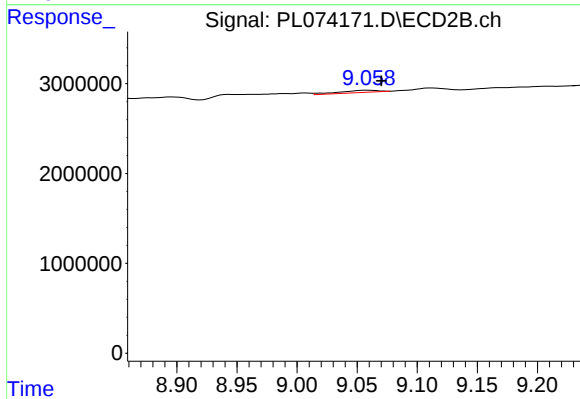

#15 Endosulfan II


R.T.: 9.059 min
Delta R.T.: -0.011 min
Response: 570575
Conc: 0.33 ng/ml

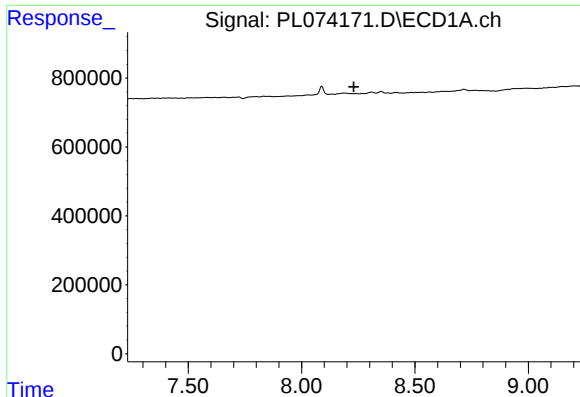

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.231 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

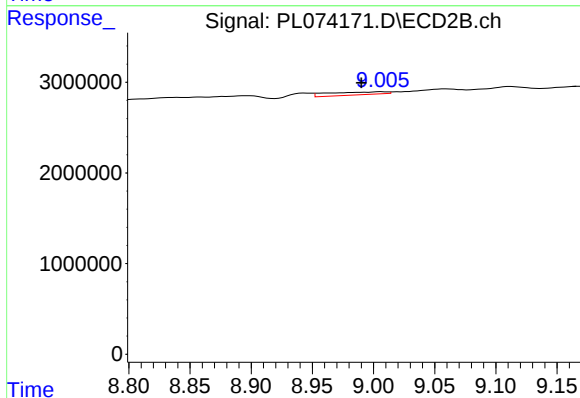


#16 4,4'-DDD

R.T.: 9.007 min
Delta R.T.: 0.017 min
Response: 1049710
Conc: 0.68 ng/ml

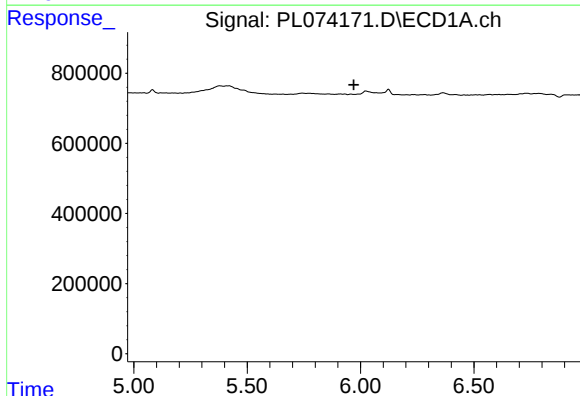


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.970 min
Response: 0
Conc: N.D.

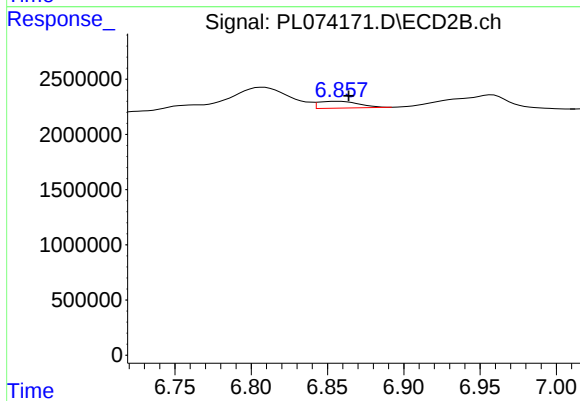

#23 Chlordane-1


R.T.: 6.858 min
Delta R.T.: -0.006 min
Response: 1145465
Conc: 14.35 ng/ml

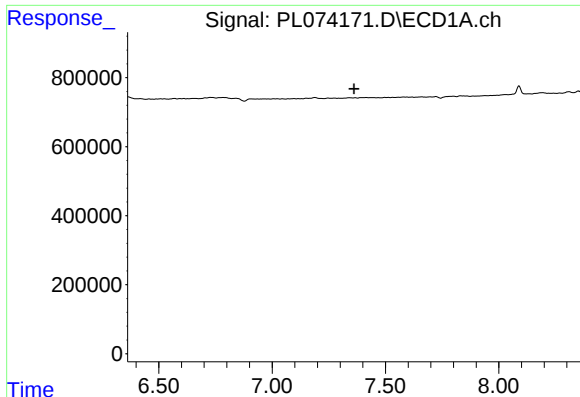

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

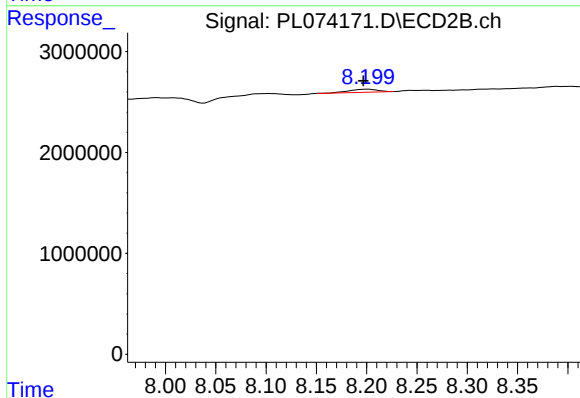


#25 Chlordane-3

R.T.: 8.201 min
Delta R.T.: 0.004 min
Response: 607400
Conc: 1.80 ng/ml

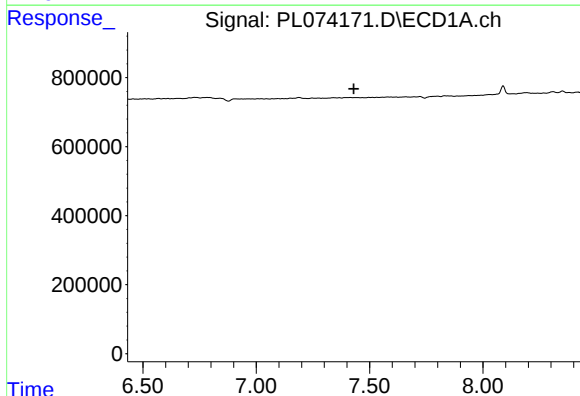


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.430 min
Response: 0
Conc: N.D.

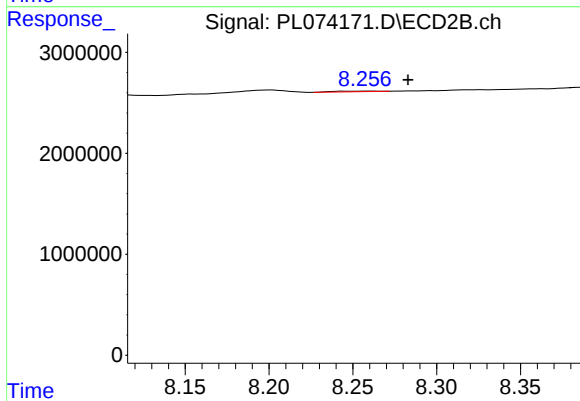

#26 Chlordane-4


R.T.: 8.260 min
Delta R.T.: -0.023 min
Response: 117166
Conc: 0.30 ng/ml

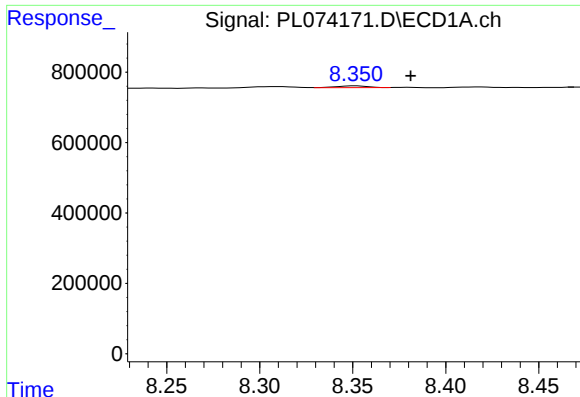

#27 Chlordane-5


R.T.: 8.352 min
Delta R.T.: -0.030 min
Response: 60814
Conc: 3.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

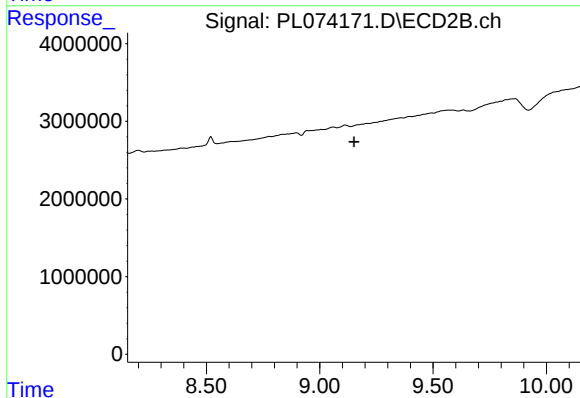


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.152 min
Response: 0
Conc: N.D.

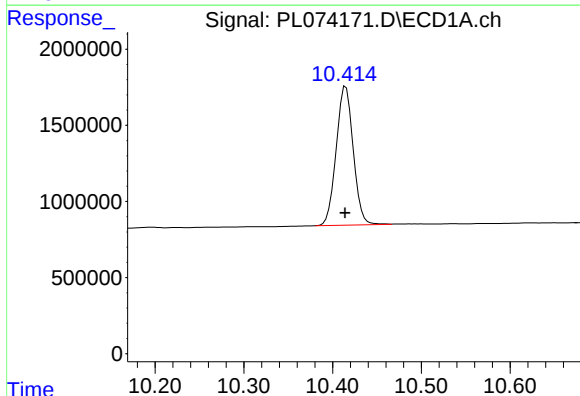

#28 Decachlorobiphenyl

R.T.: 10.415 min
Delta R.T.: 0.001 min
Response: 12149878
Conc: 23.36 ng/ml

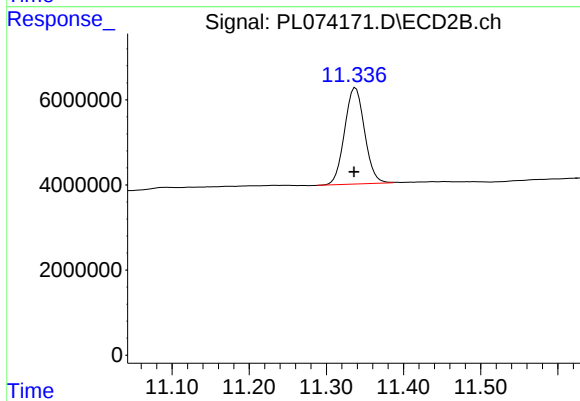

#28 Decachlorobiphenyl

R.T.: 11.338 min
Delta R.T.: 0.002 min
Response: 40665440
Conc: 23.02 ng/ml