

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041923\
 Data File : PS022749.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Apr 2023 09:35
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 19 22:17:36 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041223.M
 Quant Title : 8080.M
 QLast Update : Wed Apr 12 14:05:56 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.489	0.000	4315438	0	1.733	N.D. #
Target Compounds							
1) T	Dalapon	2.583	0.000	4172943	0	1.413	N.D. #
2) T	3,5-DICHL...	5.842	0.000	411539	0	<MDL	N.D. #
3) T	4-Nitroph...	6.326	0.000	17114662	0	9.223	N.D. #
6) T	MCP	6.826	7.178f	7263439	1358225	<MDL	<MDL #
8) T	DICHLORPROP	7.262	7.668	5715348	1847416	1.879	1.659
9) T	2,4-D	7.458	7.939	10800009	2092685	2.917	1.634 #
10) T	Pentachlo...	7.707	0.000	9931735	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.238	8.688f	31375690	1465410	1.712	<MDL #
12) T	2,4,5-T	8.498	9.154	4563583	4367081	<MDL	<MDL #
13) T	2,4-DB	8.999	9.629	34246546	5652711	8.014	7.544
14) T	DINOSEB	10.062	0.000	133805	0	<MDL	N.D. #
15) T	Picloram	9.910	10.916	83099493	19232278	2.790	2.365
16) T	DCPA	10.327	10.916	3683194	19232278	<MDL	2.770 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS041923\
Data File : PS022749.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Apr 2023 09:35
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 19 22:17:36 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS041223.M
Quant Title : 8080.M
QLast Update : Wed Apr 12 14:05:56 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

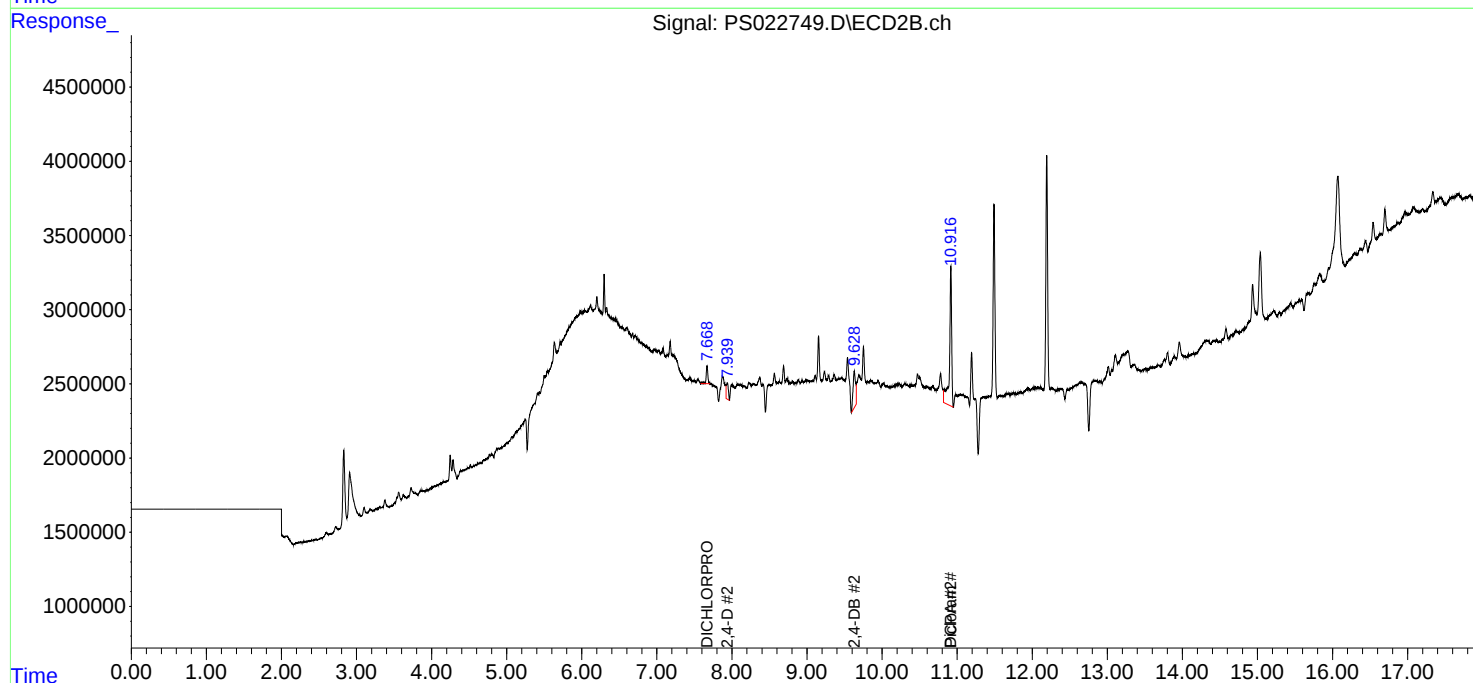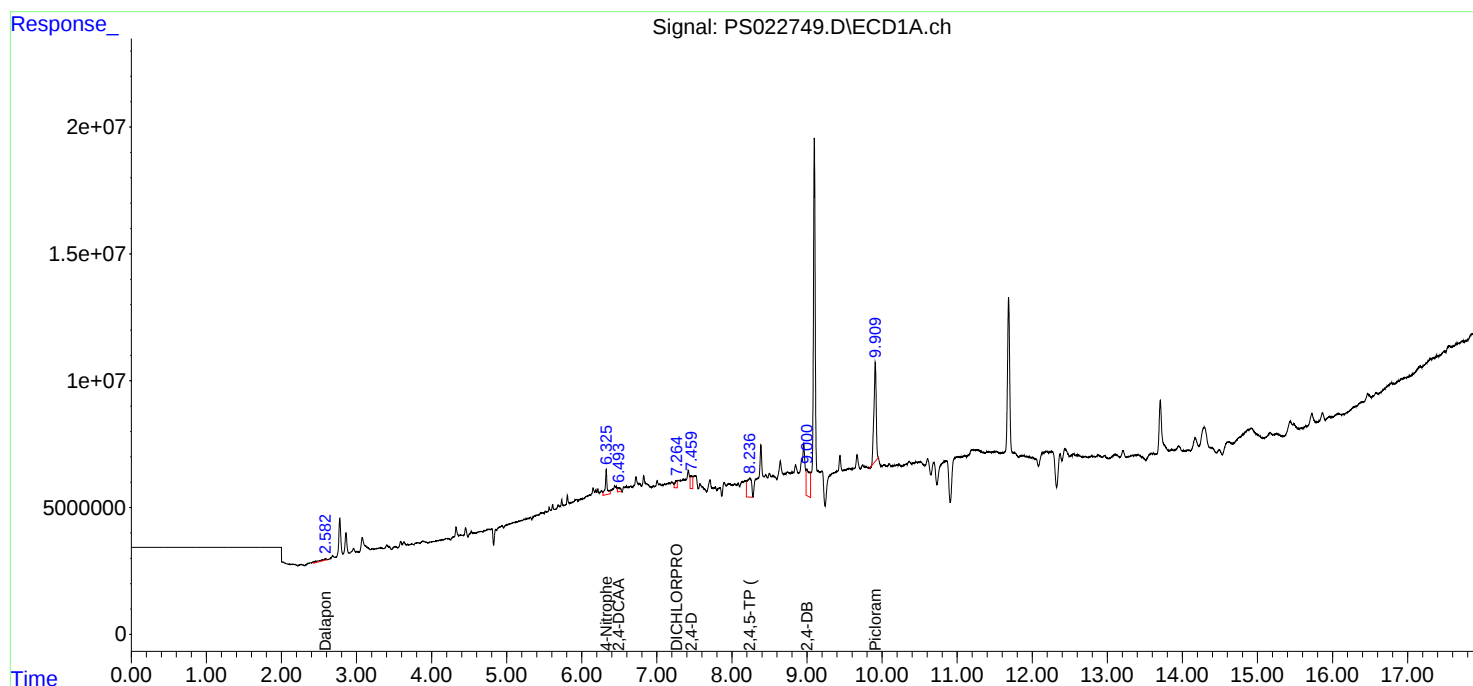


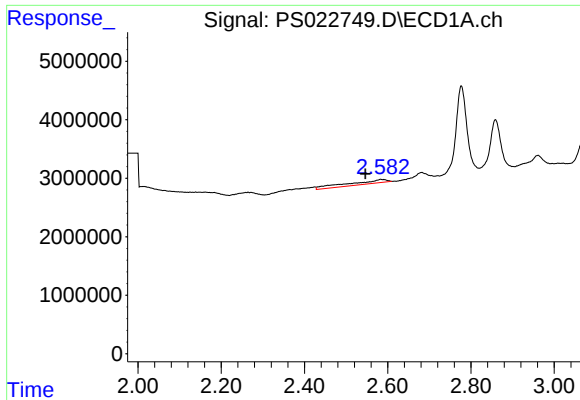

#1 Dalapon


R.T.: 2.583 min
Delta R.T.: 0.036 min
Response: 4172943
Conc: 1.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

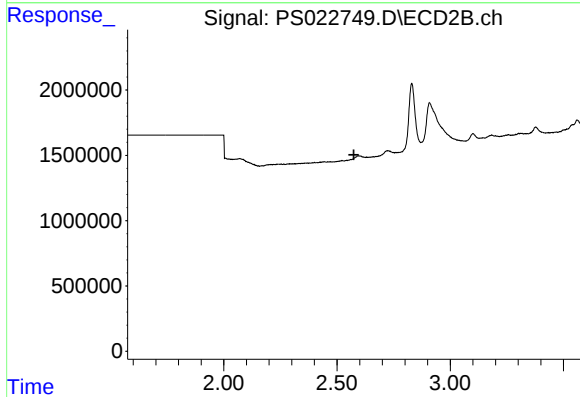


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.574 min
Response: 0
Conc: N.D.

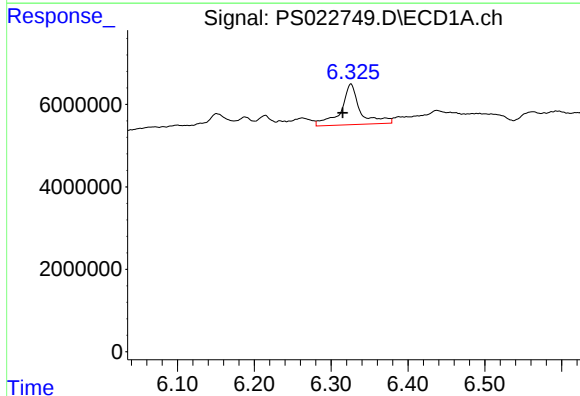


#3 4-Nitrophenol

R.T.: 6.326 min
Delta R.T.: 0.010 min
Response: 17114662
Conc: 9.22 ng/ml

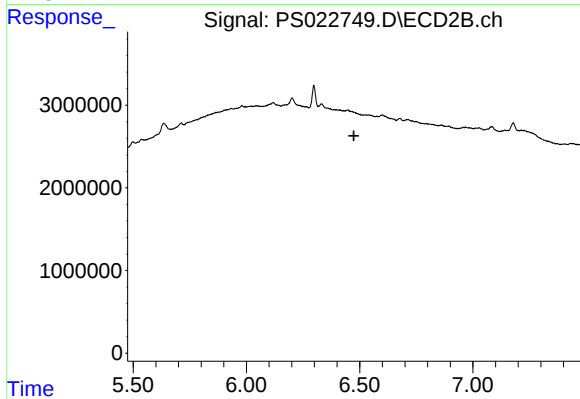

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.474 min
Response: 0
Conc: N.D.

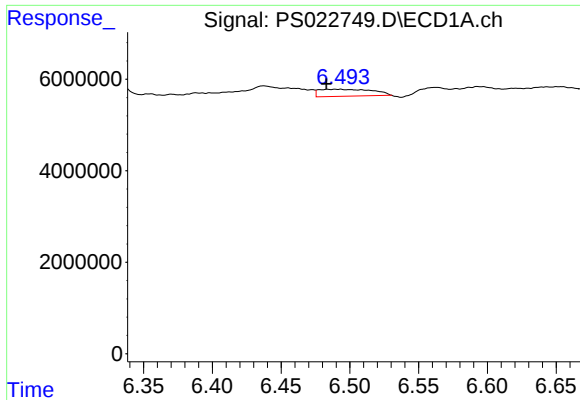

#4 2,4-DCAA


R.T.: 6.489 min
Delta R.T.: 0.006 min
Response: 4315438
Conc: 1.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

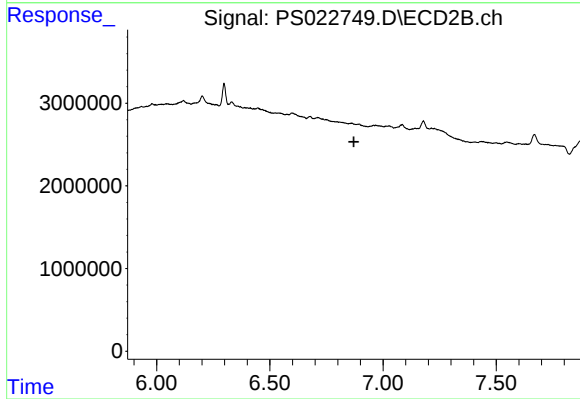


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.871 min
Response: 0
Conc: N.D.

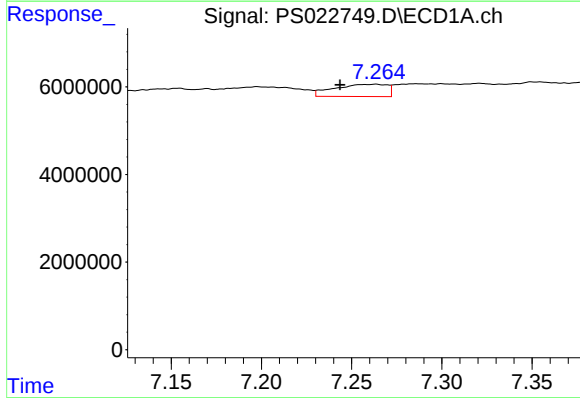


#8 DICHLORPROP

R.T.: 7.262 min
Delta R.T.: 0.019 min
Response: 5715348
Conc: 1.88 ng/ml

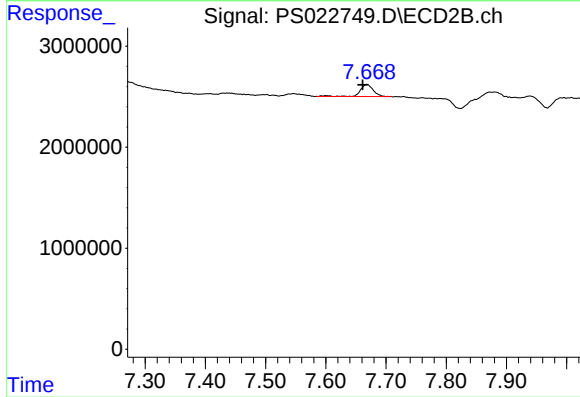

#8 DICHLORPROP


R.T.: 7.668 min
Delta R.T.: 0.007 min
Response: 1847416
Conc: 1.66 ng/ml

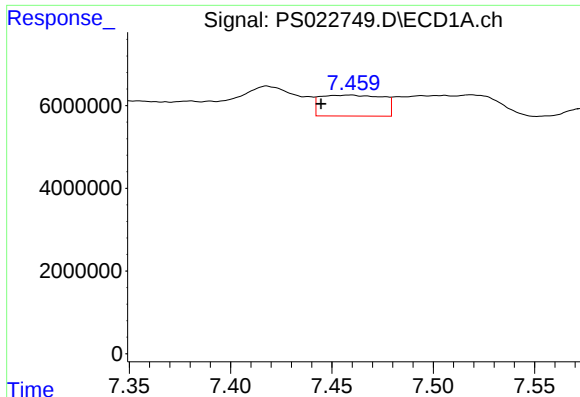

#9 2,4-D


R.T.: 7.458 min
Delta R.T.: 0.013 min
Response: 10800009
Conc: 2.92 ng/ml

Instrument :
ECD_L
ClientSampleId :

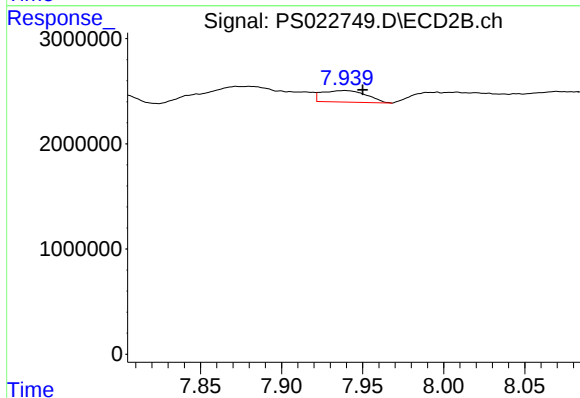


#9 2,4-D

R.T.: 7.939 min
Delta R.T.: -0.011 min
Response: 2092685
Conc: 1.63 ng/ml

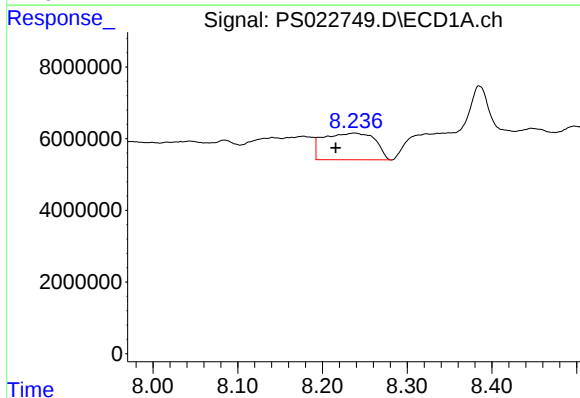


#11 2,4,5-TP (SILVEX)

R.T.: 8.238 min
Delta R.T.: 0.022 min
Response: 31375690
Conc: 1.71 ng/ml

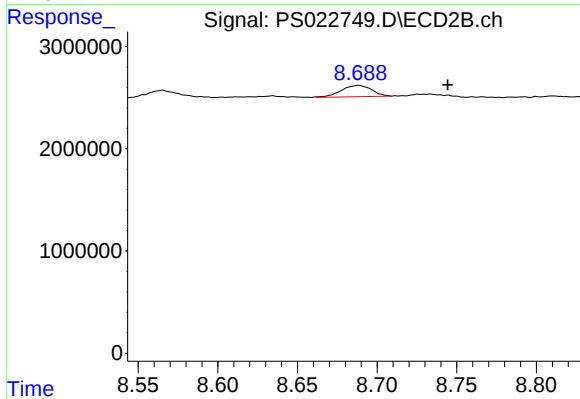

#11 2,4,5-TP (SILVEX)


R.T.: 8.688 min
Delta R.T.: -0.056 min
Response: 1465410
Conc: N.D.

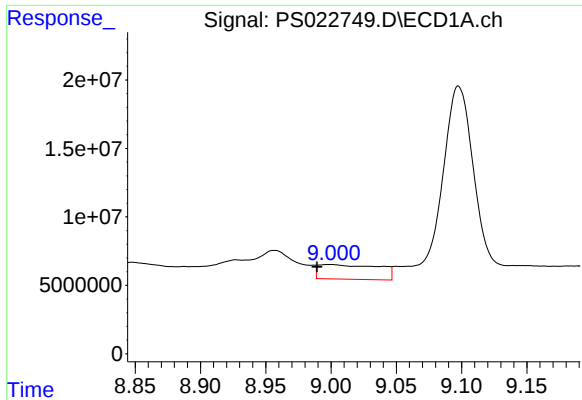

#13 2,4-DB


R.T.: 8.999 min
Delta R.T.: 0.010 min
Response: 34246546
Conc: 8.01 ng/ml

Instrument :
ECD_L
ClientSampleId :

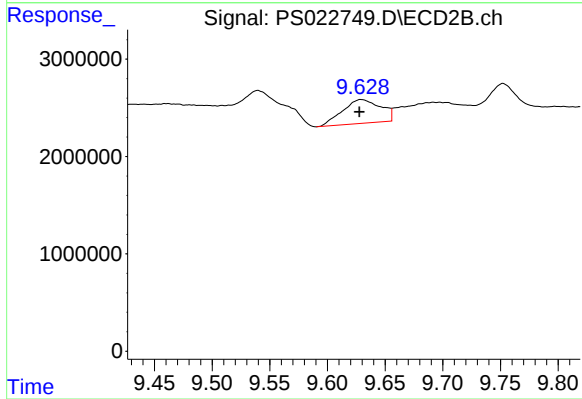


#13 2,4-DB

R.T.: 9.629 min
Delta R.T.: 0.002 min
Response: 5652711
Conc: 7.54 ng/ml

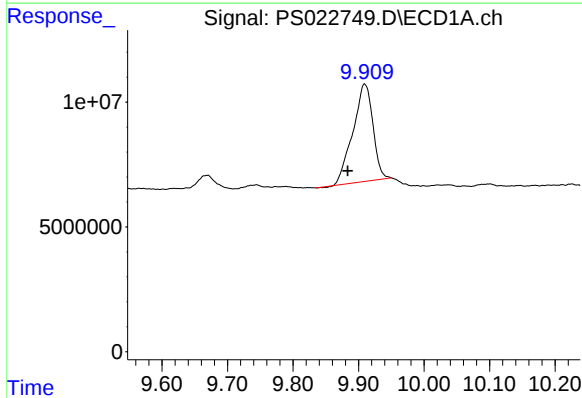


#15 Picloram

R.T.: 9.910 min
Delta R.T.: 0.026 min
Response: 83099493
Conc: 2.79 ng/ml

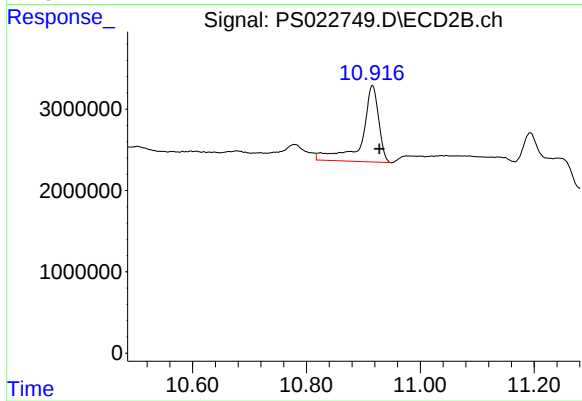

#15 Picloram


R.T.: 10.916 min
Delta R.T.: -0.012 min
Response: 19232278
Conc: 2.36 ng/ml

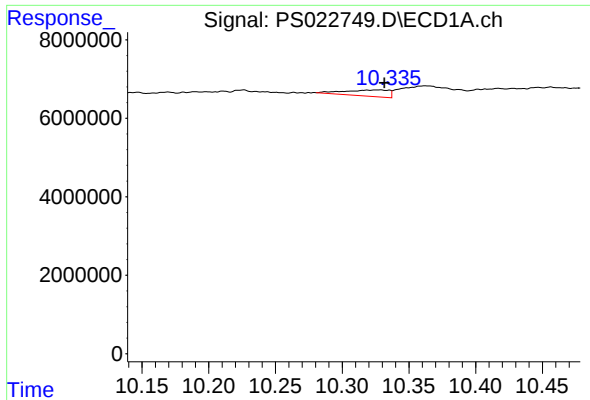

#16 DCPA

R.T.: 10.327 min
Delta R.T.: -0.004 min
Response: 3683194
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

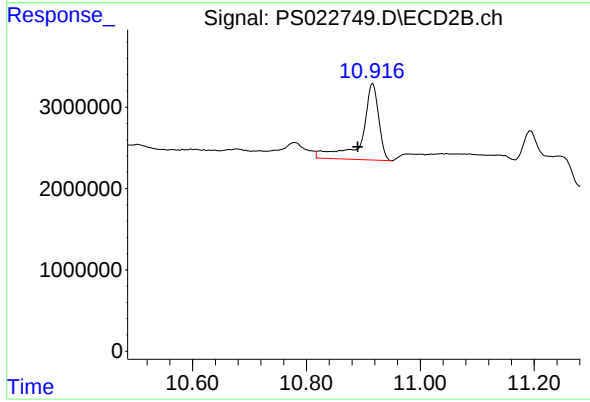

#16 DCPA

R.T.: 10.916 min
Delta R.T.: 0.026 min
Response: 19232278
Conc: 2.77 ng/ml