

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041923\
 Data File : PL082187.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Apr 2023 12:59
 Operator : AR\AJ
 Sample : 02386-03DL 1000X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SPA-1WC-23-04DL

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 04/20/2023
 Supervised By :Ankita Jodhani 04/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 19 22:04:37 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032223.M
 Quant Title : GC Extractables
 QLast Update : Thu Mar 23 01:07:33 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

16) A	4,4'-DDD	6.481	5.644	93704944	67786181	51.958	44.669m
-------	----------	-------	-------	----------	----------	--------	---------

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041923\
Data File : PL082187.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Apr 2023 12:59
Operator : AR\AJ
Sample : 02386-03DL 1000X
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SPA-1WC-23-04DL


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 04/20/2023
Supervised By : Ankita Jodhani 04/21/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 19 22:04:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032223.M
Quant Title : GC Extractables
QLast Update : Thu Mar 23 01:07:33 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

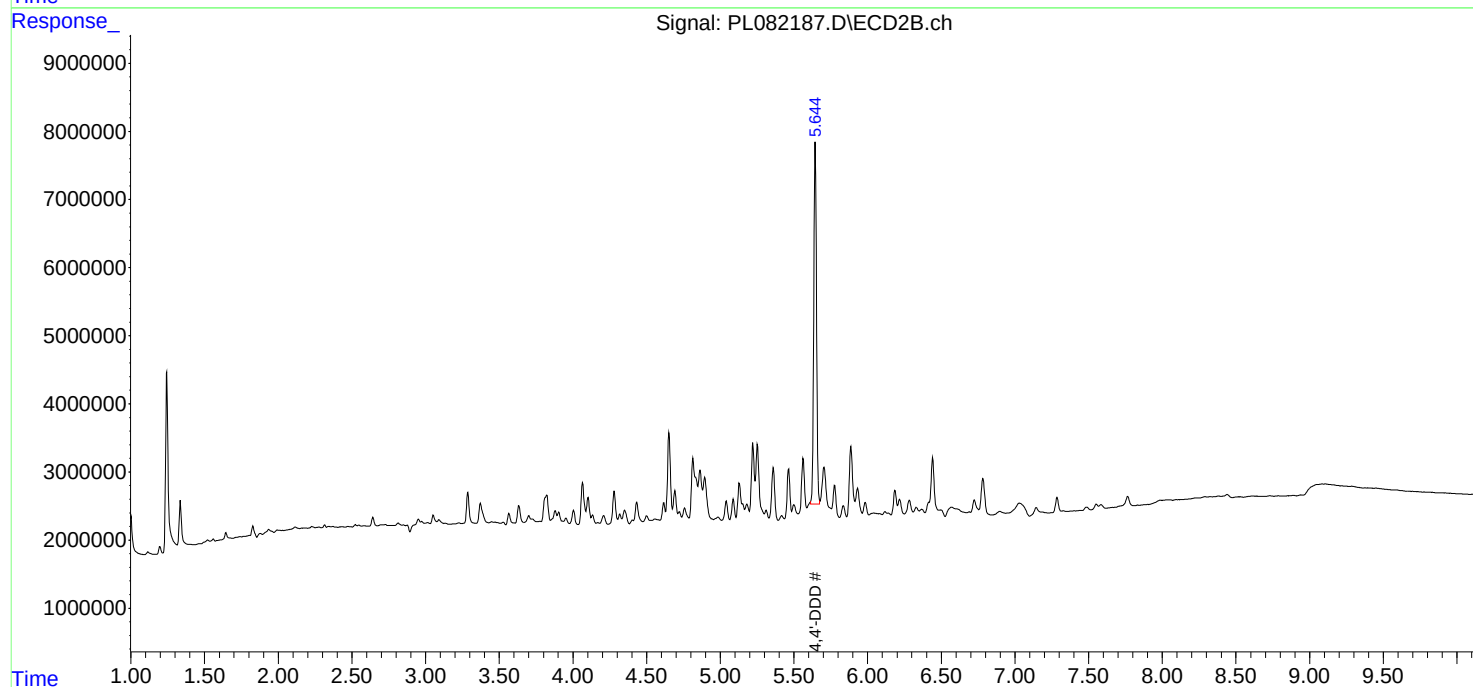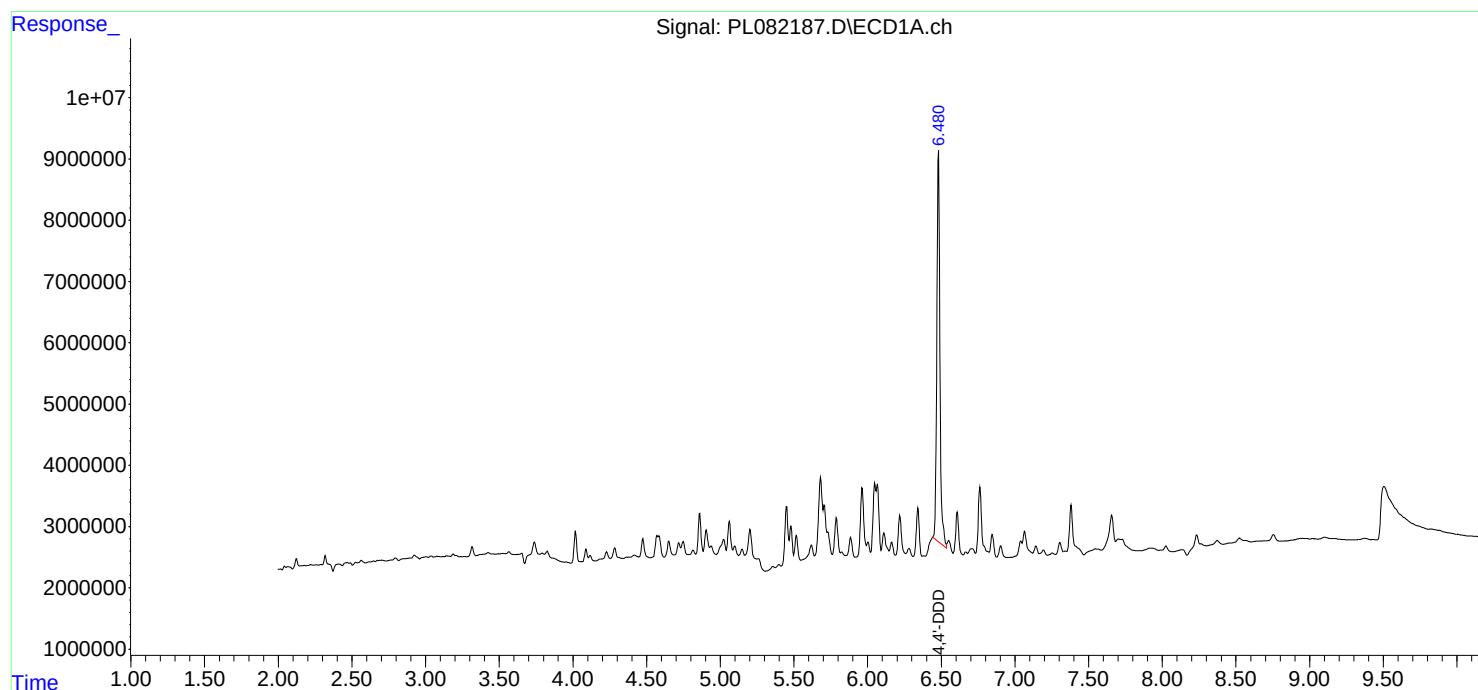

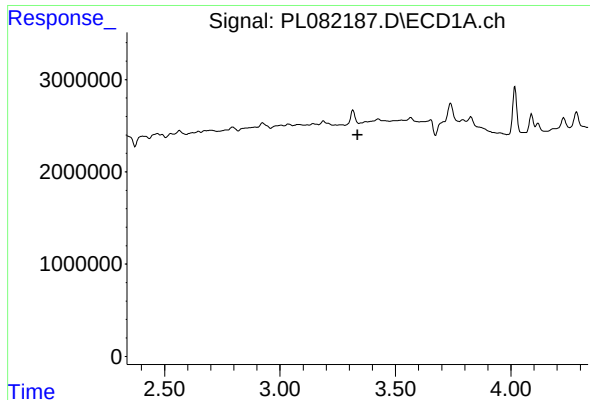


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 3.335 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SPA-1WC-23-04DL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/20/2023
Supervised By :Ankita Jodhani 04/21/2023

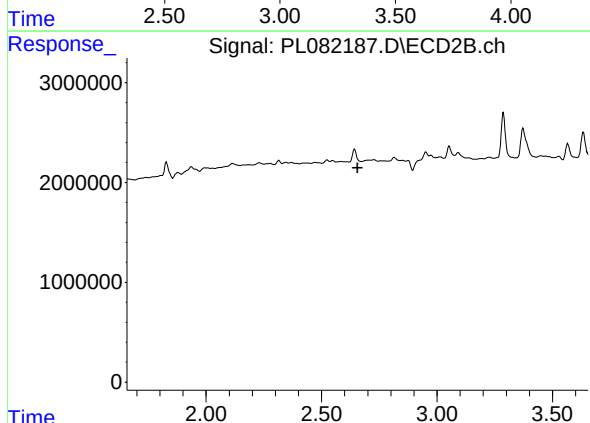


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 2.656 min
Response: 0
Conc: N.D.

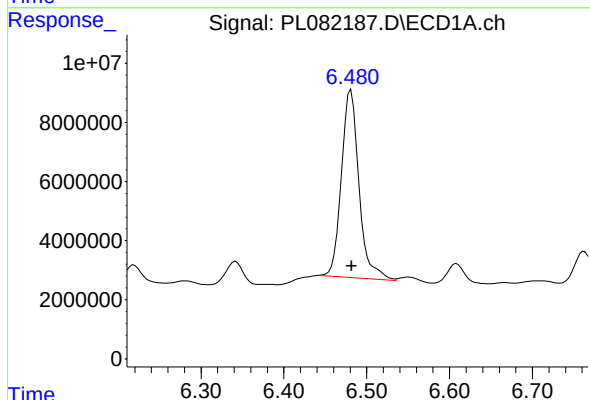


#16 4,4'-DDD

R.T.: 6.481 min
Delta R.T.: 0.000 min
Response: 93704944
Conc: 51.96 ng/ml

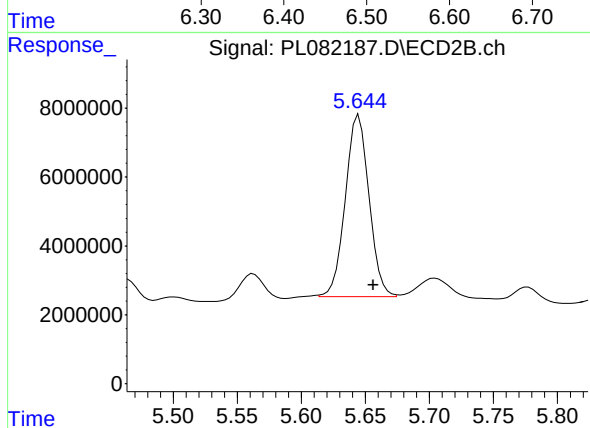

#16 4,4'-DDD

R.T.: 5.644 min
Delta R.T.: -0.012 min
Response: 67786181
Conc: 44.67 ng/ml m

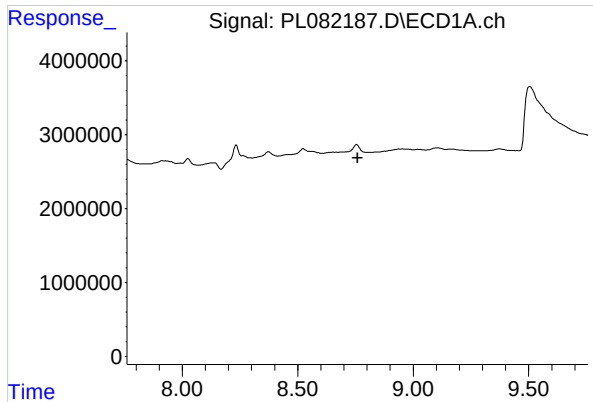


#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.760 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SPA-1WC-23-04DL

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/20/2023
Supervised By :Ankita Jodhani 04/21/2023

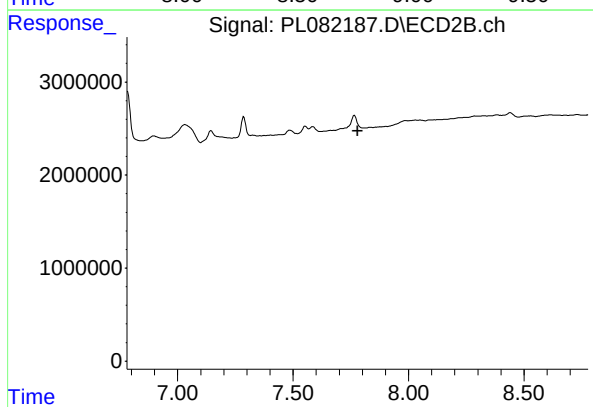

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 7.779 min
Response: 0
Conc: N.D.