

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042020\
 Data File : PL058190.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2020 17:52
 Operator : AJ\MA
 Sample : PB128351BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 05:02:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.456	3.955	239.2E6	48200891	23.723	22.211
28)	SA Decachlor...	8.205	8.978	186.3E6	44188261	18.075	19.782
Target Compounds							
2)	A alpha-BHC	3.886	0.000	4864952	0	0.280	N.D. #
4)	MA Heptachlor	0.000	5.135	0	1886400	N.D.	0.562 #
5)	MB Aldrin	4.730	0.000	531603	0	0.036	N.D. #
7)	B delta-BHC	0.000	4.985f	0	2905228	N.D.	3.140 #
15)	B Endosulfa...	0.000	6.868f	0	439327	N.D.	0.169 #
19)	B Endosulfa...	6.684f	0.000	567426	0	0.056	N.D. #
20)	A Methoxychlor	6.916	0.000	1853016	0	0.336	N.D. #
22)	Mirex	7.342	0.000	999428	0	0.122	N.D. #
23)	Chlordane-1	4.356f	0.000	3606235	0	9.751	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042020\
Data File : PL058190.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2020 17:52
Operator : AJ\MA
Sample : PB128351BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 05:02:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

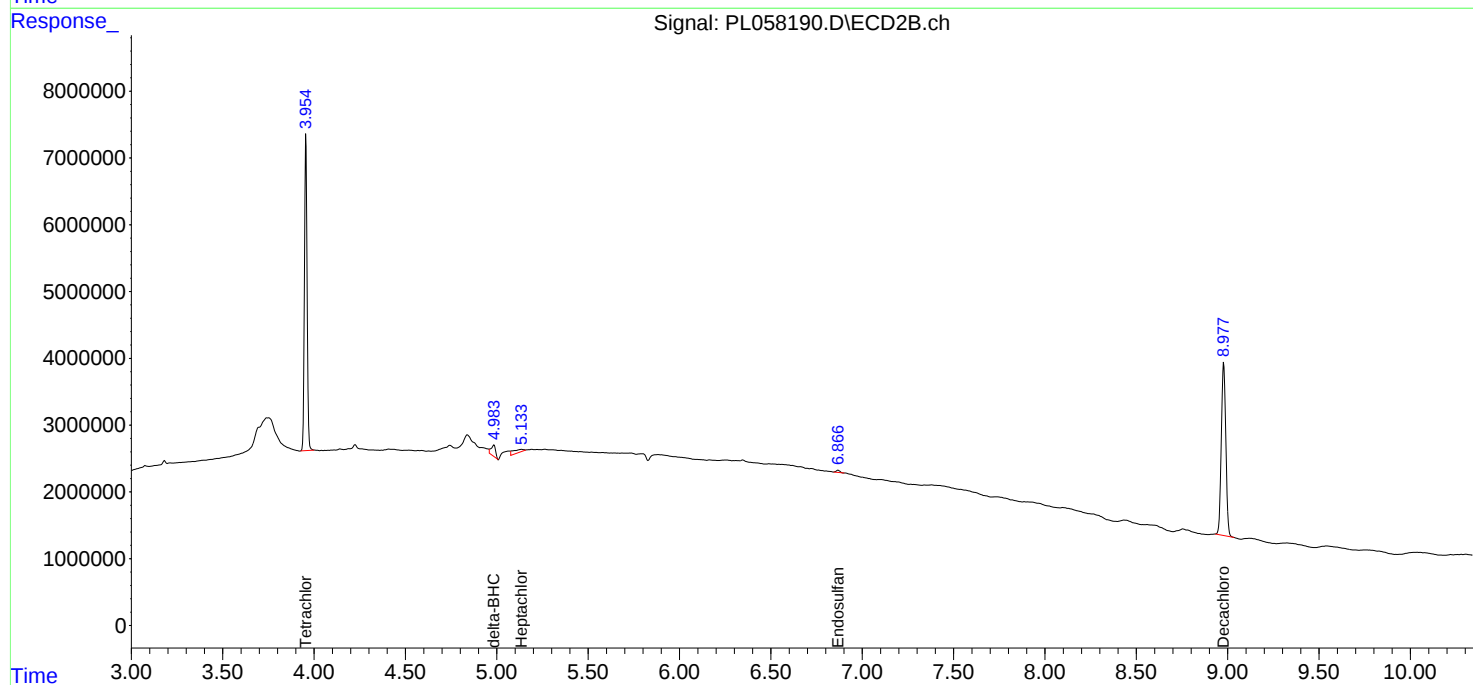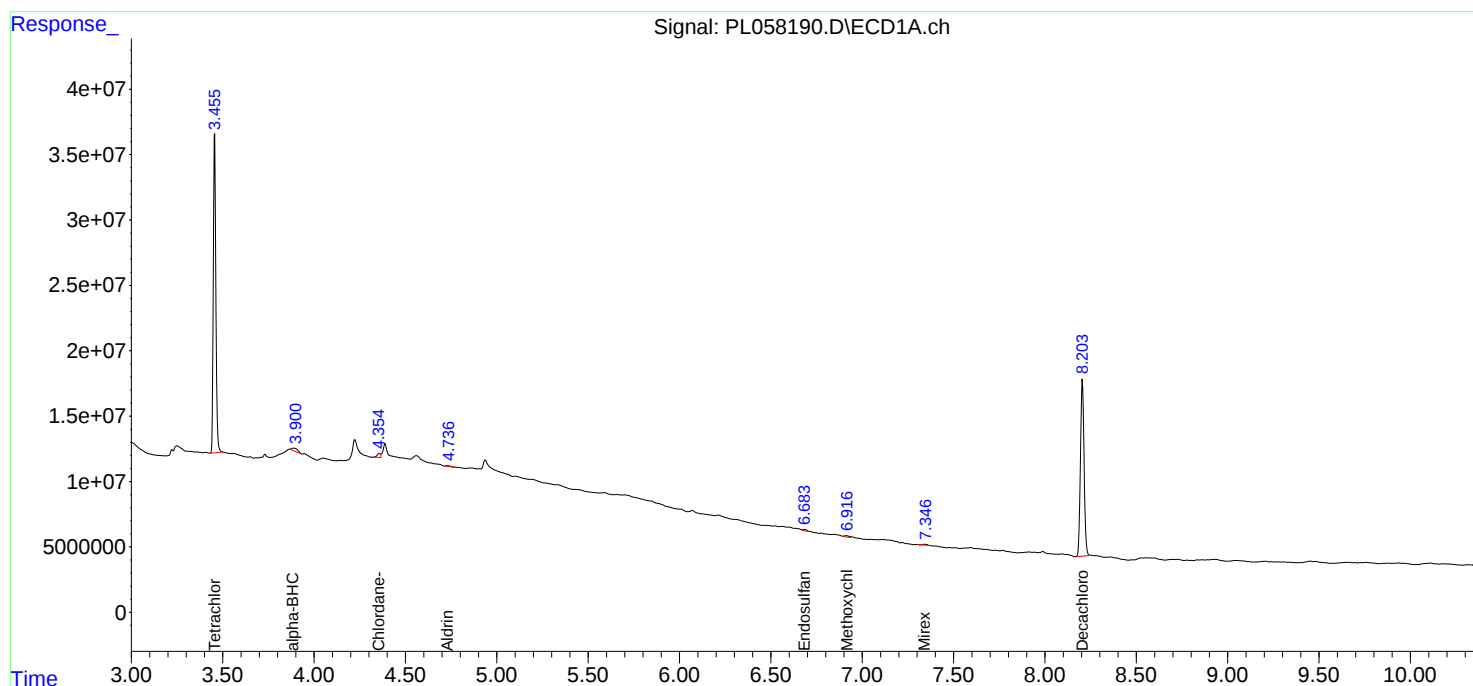


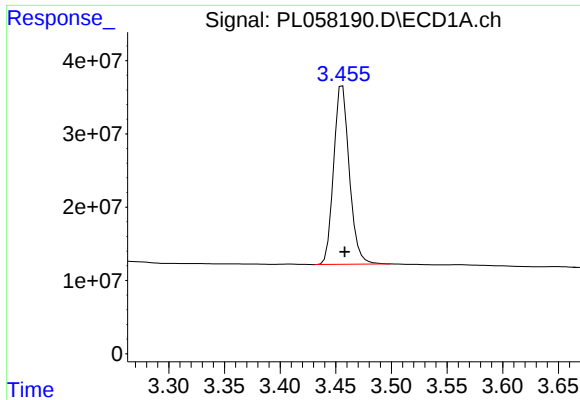

#1 Tetrachloro-m-xylene


R.T.: 3.456 min
Delta R.T.: -0.002 min
Response: 239156698
Conc: 23.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

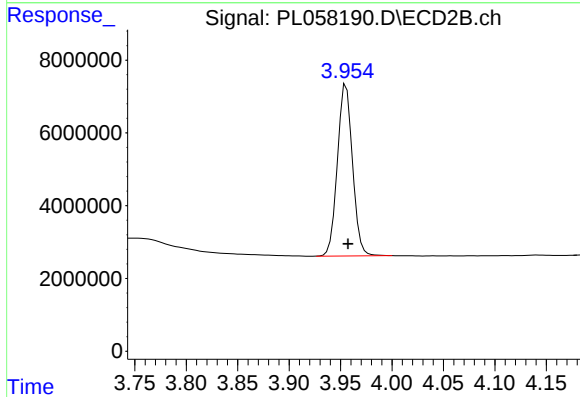


#1 Tetrachloro-m-xylene

R.T.: 3.955 min
Delta R.T.: -0.002 min
Response: 48200891
Conc: 22.21 ng/ml

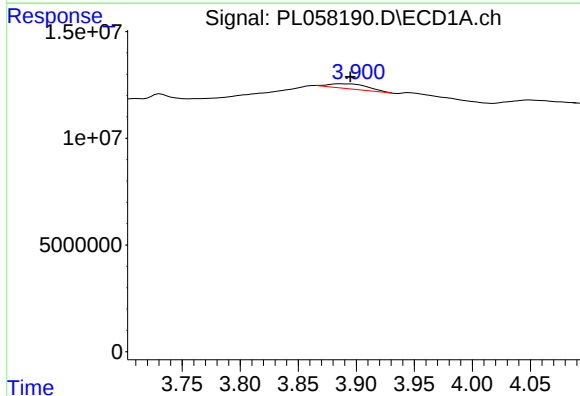


#2 alpha-BHC

R.T.: 3.886 min
Delta R.T.: -0.009 min
Response: 4864952
Conc: 0.28 ng/ml

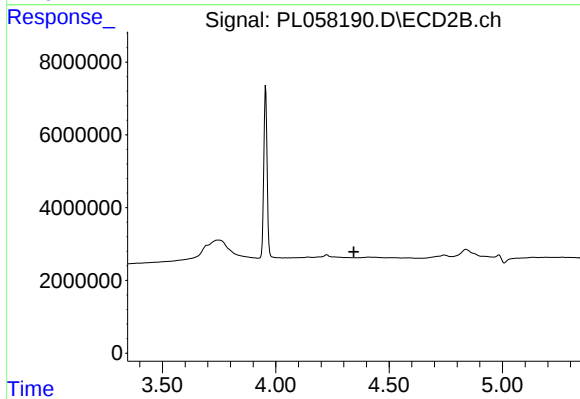

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.345 min
Response: 0
Conc: N.D.

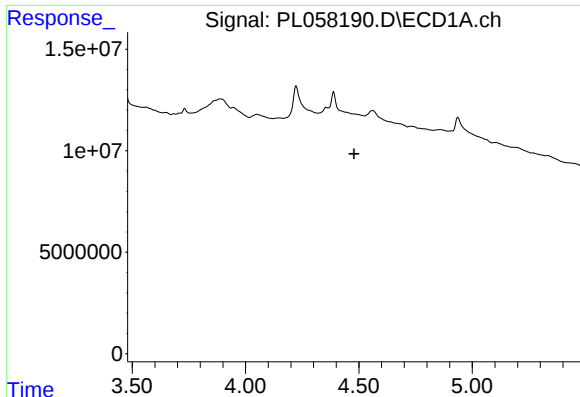

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

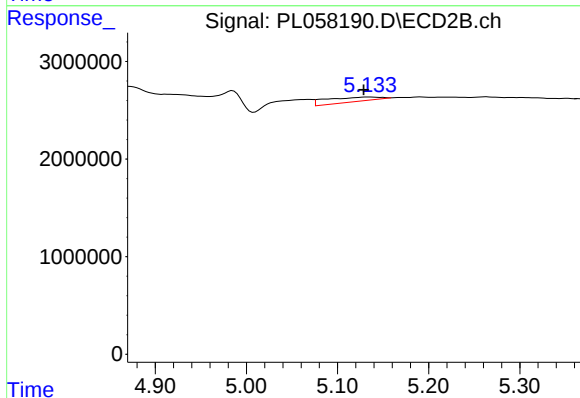


#4 Heptachlor

R.T.: 5.135 min
Delta R.T.: 0.006 min
Response: 1886400
Conc: 0.56 ng/ml

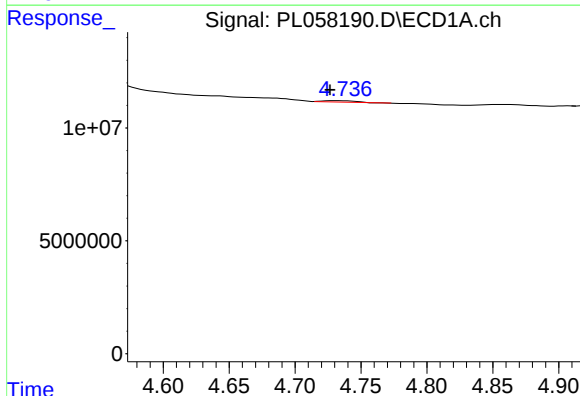


#5 Aldrin

R.T.: 4.730 min
Delta R.T.: 0.004 min
Response: 531603
Conc: 0.04 ng/ml

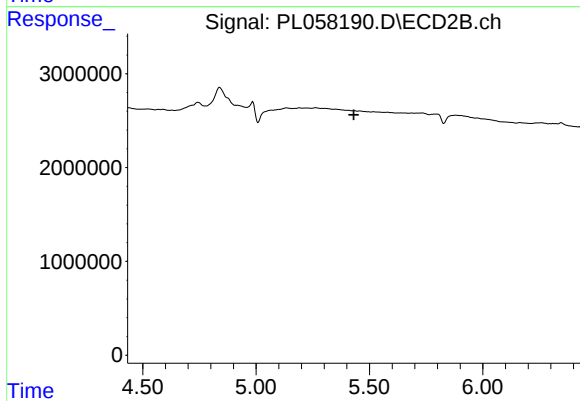

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.431 min
Response: 0
Conc: N.D.

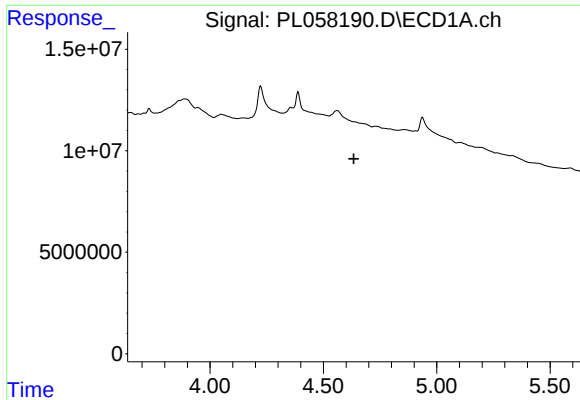

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.634 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

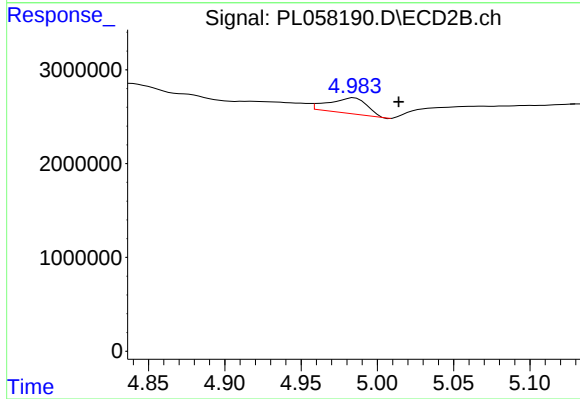


#7 delta-BHC

R.T.: 4.985 min
Delta R.T.: -0.029 min
Response: 2905228
Conc: 3.14 ng/ml

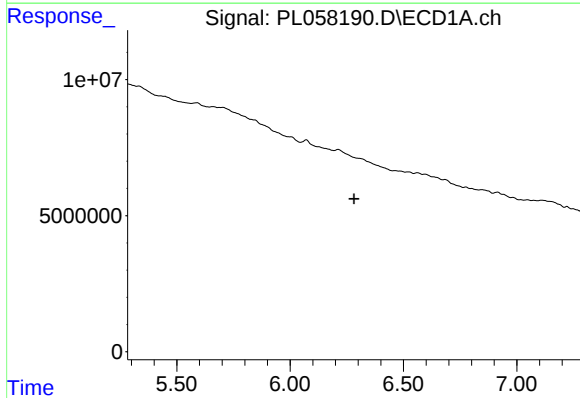


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.282 min
Response: 0
Conc: N.D.

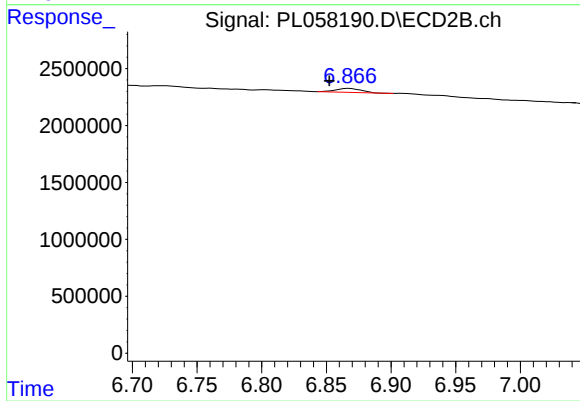

#15 Endosulfan II


R.T.: 6.868 min
Delta R.T.: 0.015 min
Response: 439327
Conc: 0.17 ng/ml

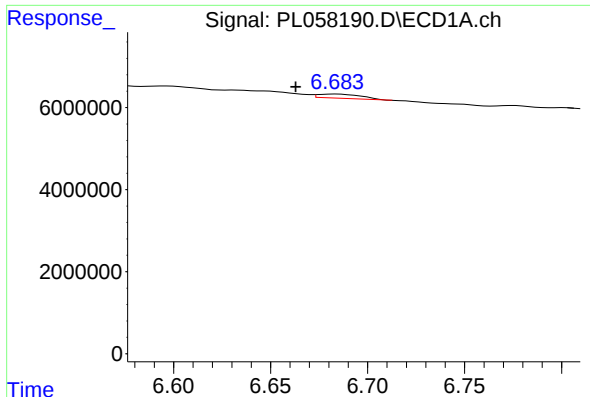

#19 Endosulfan Sulfate


R.T.: 6.684 min
Delta R.T.: 0.021 min
Response: 567426
Conc: 0.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

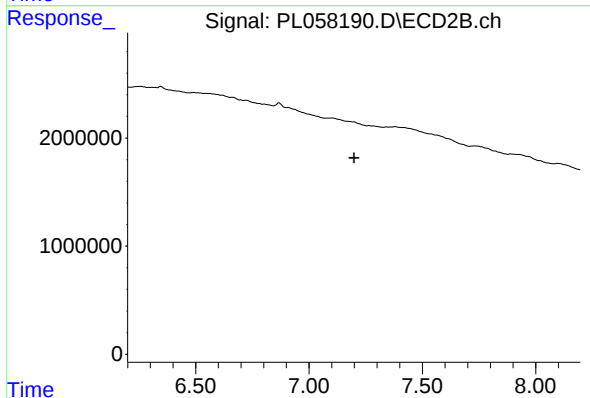


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.199 min
Response: 0
Conc: N.D.

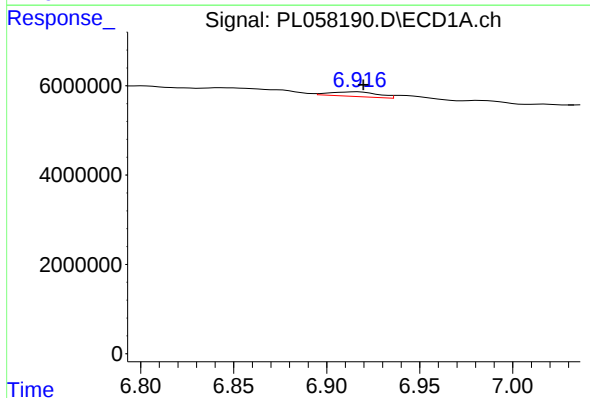


#20 Methoxychlor

R.T.: 6.916 min
Delta R.T.: -0.003 min
Response: 1853016
Conc: 0.34 ng/ml

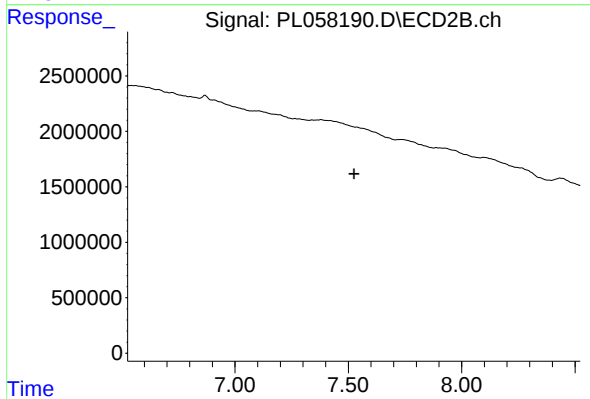

#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.525 min
Response: 0
Conc: N.D.

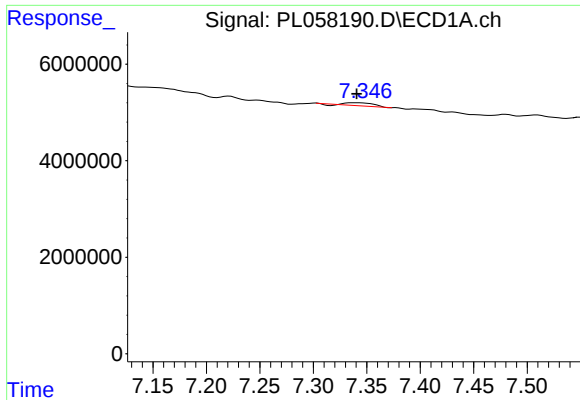

#22 Mirex


R.T.: 7.342 min

Delta R.T.: 0.001 min

Response: 999428

Conc: 0.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

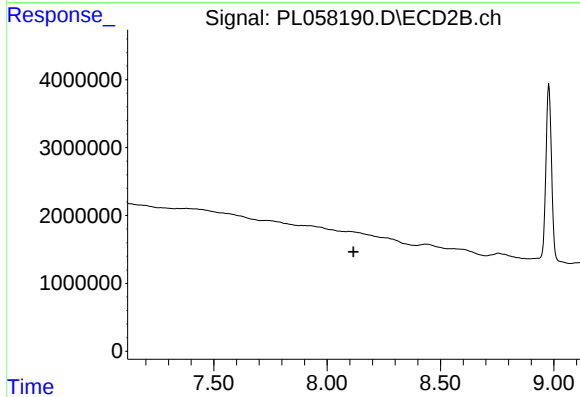


#22 Mirex

R.T.: 0.000 min

Exp R.T. : 8.117 min

Response: 0

Conc: N.D.

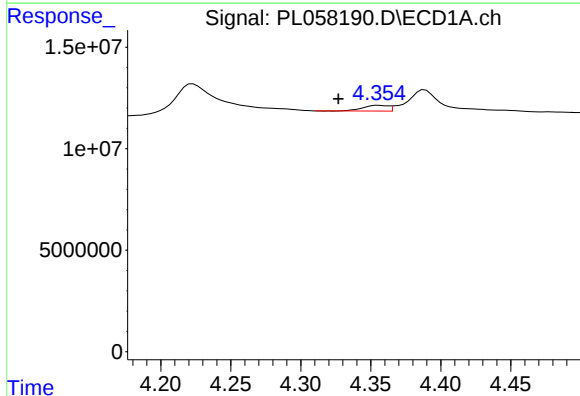


#23 Chlordane-1

R.T.: 4.356 min

Delta R.T.: 0.029 min

Response: 3606235

Conc: 9.75 ng/ml

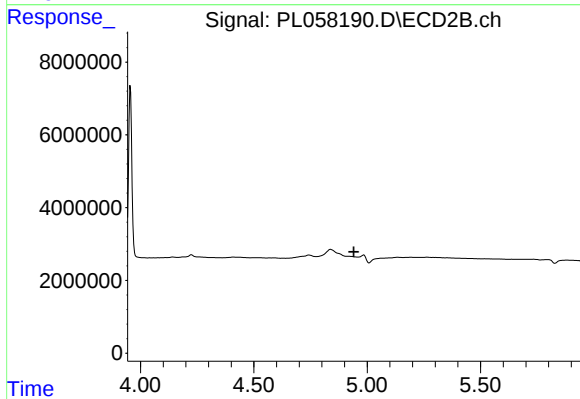


#23 Chlordane-1

R.T.: 0.000 min

Exp R.T. : 4.942 min

Response: 0


Conc: N.D.

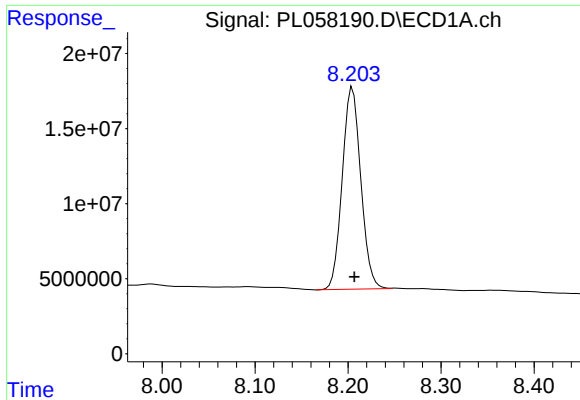

#28 Decachlorobiphenyl

R.T.: 8.205 min
Delta R.T.: -0.002 min
Response: 186327175
Conc: 18.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

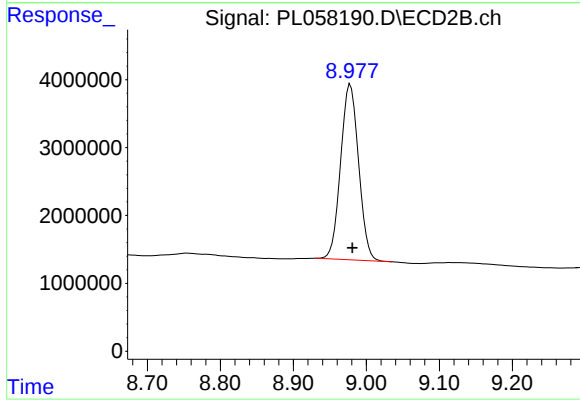

#28 Decachlorobiphenyl

R.T.: 8.978 min
Delta R.T.: -0.003 min
Response: 44188261
Conc: 19.78 ng/ml