

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042020\
 Data File : PL058192.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2020 18:21
 Operator : AJ\MA
 Sample : PB128351TB
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 05:02:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.456	3.956	237.5E6	49230906	23.563	22.686
28)	SA Decachlor...	8.206	8.979	192.8E6	44958737	18.706	20.127
Target Compounds							
2)	A alpha-BHC	3.891	0.000	5785261	0	0.333	N.D. #
4)	MA Heptachlor	0.000	5.134	0	1311352	N.D.	0.391 #
7)	B delta-BHC	0.000	4.984f	0	3147372	N.D.	3.233 #
15)	B Endosulfa...	0.000	6.870f	0	492498	N.D.	0.190 #
19)	B Endosulfa...	6.677	0.000	1118040	0	0.110	N.D. #
21)	B Endrin ke...	7.159	0.000	524146	0	0.047	N.D. #
22)	Mirex	7.342	0.000	501930	0	0.061	N.D. #
23)	Chlordane-1	4.353f	0.000	3004844	0	8.124	N.D. #
24)	Chlordane-2	4.847f	0.000	303348	0	0.751	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042020\
Data File : PL058192.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2020 18:21
Operator : AJ\MA
Sample : PB128351TB
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 05:02:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

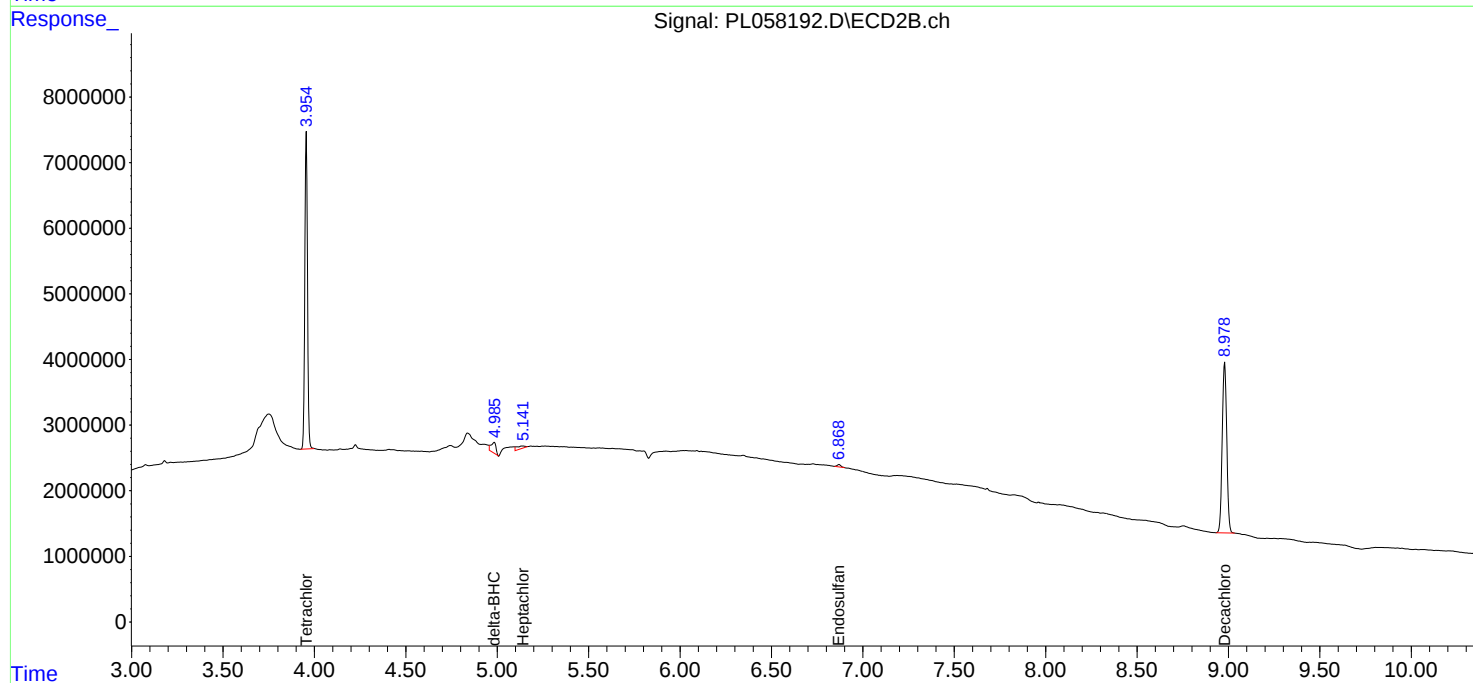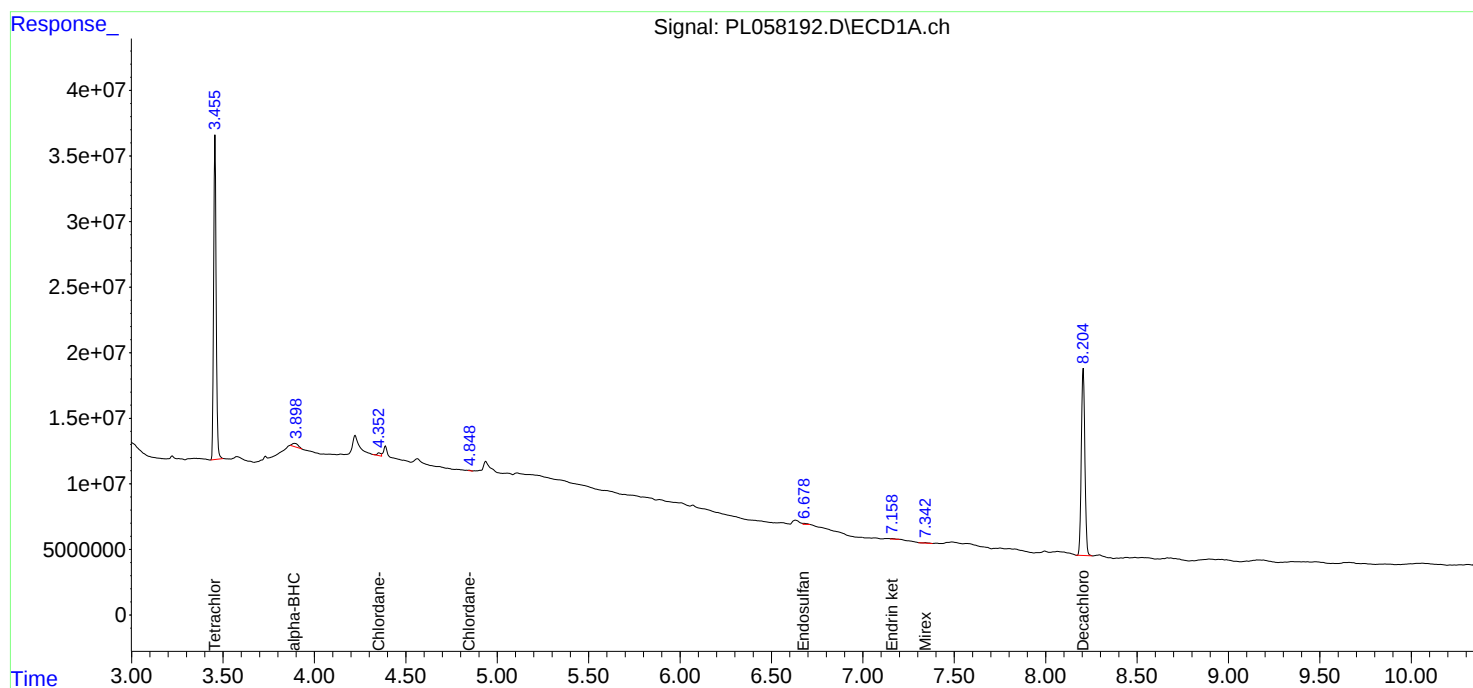


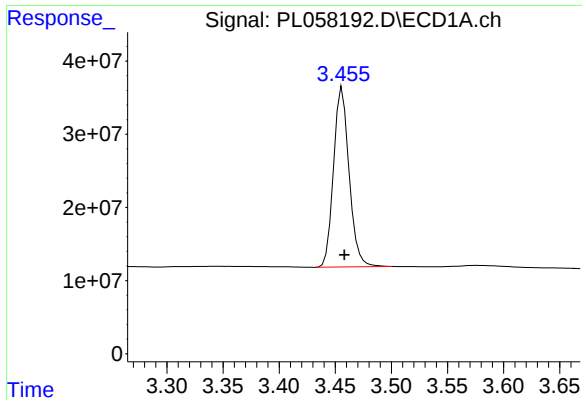

#1 Tetrachloro-m-xylene


R.T.: 3.456 min
Delta R.T.: -0.002 min
Response: 237534346
Conc: 23.56 ng/ml

Instrument :
ECD_L
ClientSampleId :

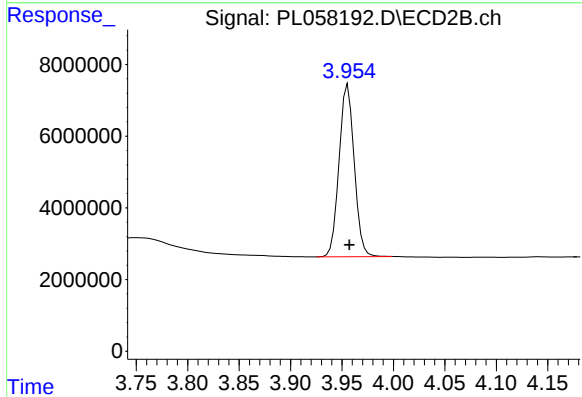


#1 Tetrachloro-m-xylene

R.T.: 3.956 min
Delta R.T.: -0.002 min
Response: 49230906
Conc: 22.69 ng/ml

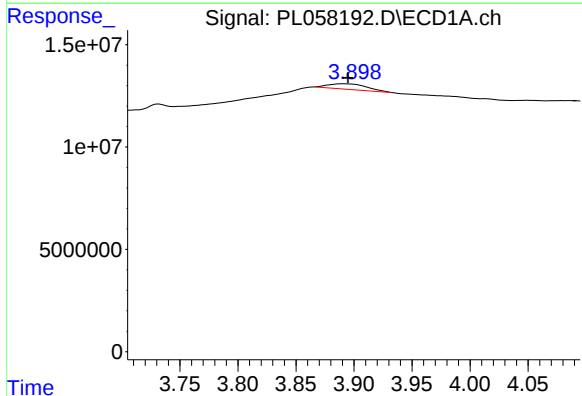


#2 alpha-BHC

R.T.: 3.891 min
Delta R.T.: -0.004 min
Response: 5785261
Conc: 0.33 ng/ml

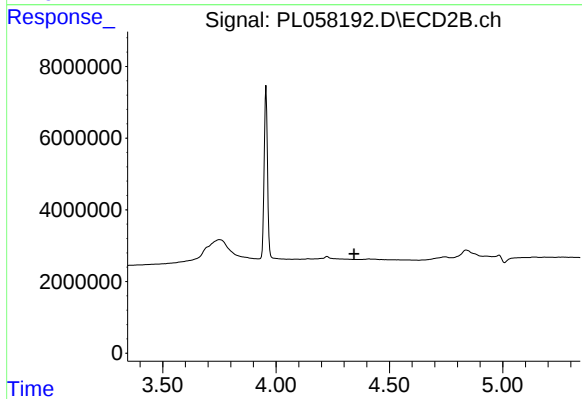

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.345 min
Response: 0
Conc: N.D.

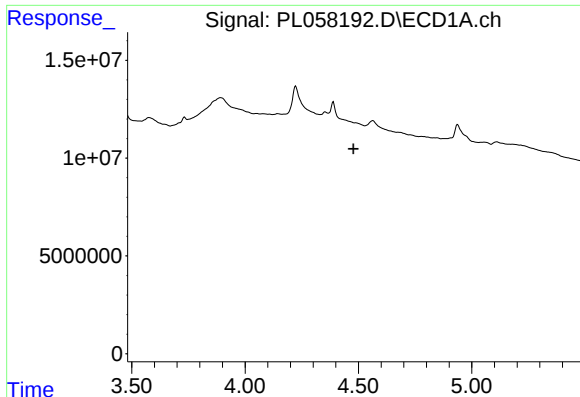

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

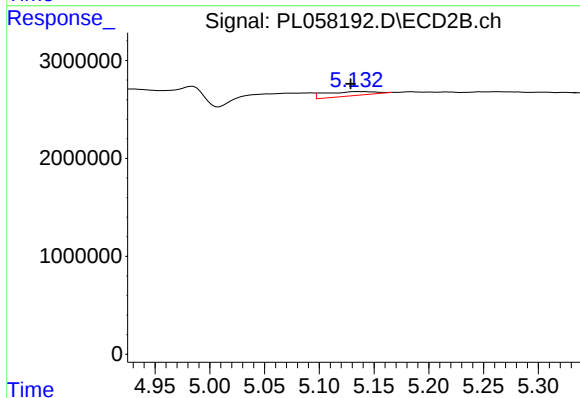


#4 Heptachlor

R.T.: 5.134 min
Delta R.T.: 0.005 min
Response: 1311352
Conc: 0.39 ng/ml

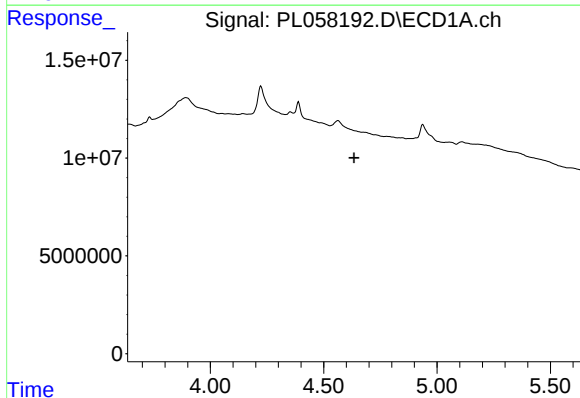


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.634 min
Response: 0
Conc: N.D.

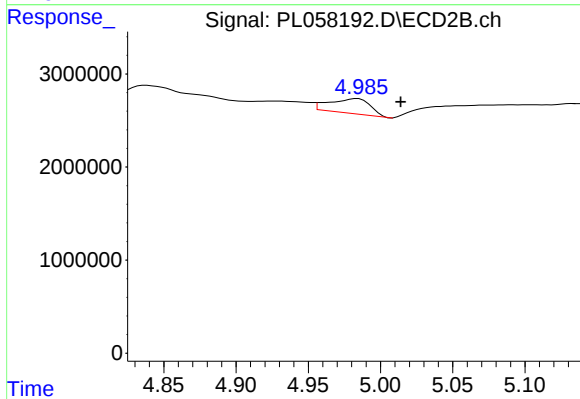

#7 delta-BHC


R.T.: 4.984 min
Delta R.T.: -0.030 min
Response: 3147372
Conc: 3.23 ng/ml

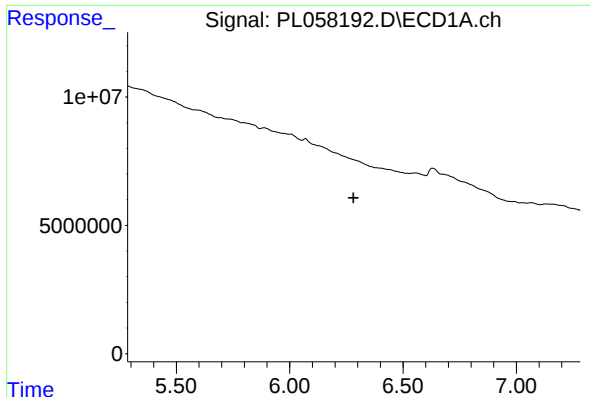

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.282 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

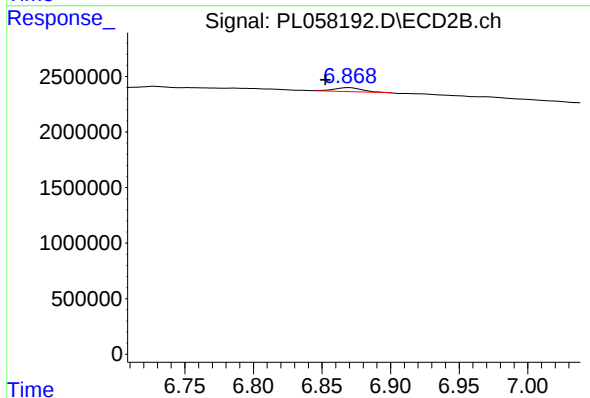


#15 Endosulfan II

R.T.: 6.870 min
Delta R.T.: 0.017 min
Response: 492498
Conc: 0.19 ng/ml

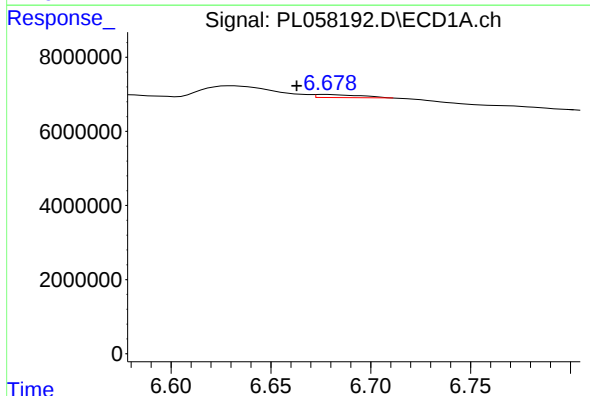


#19 Endosulfan Sulfate

R.T.: 6.677 min
Delta R.T.: 0.014 min
Response: 1118040
Conc: 0.11 ng/ml

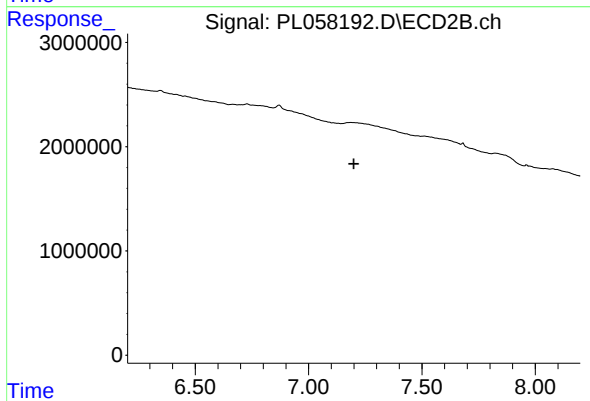

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.199 min
Response: 0
Conc: N.D.

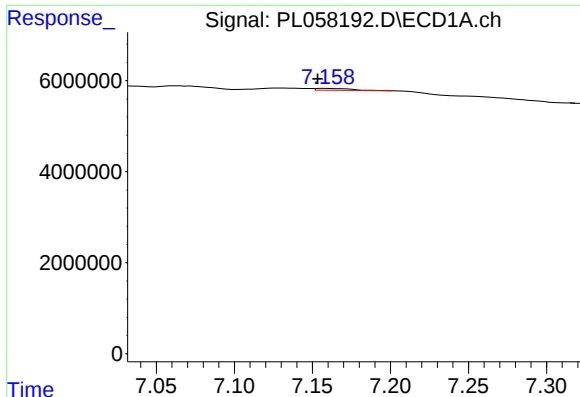

#21 Endrin ketone


R.T.: 7.159 min
Delta R.T.: 0.005 min
Response: 524146
Conc: 0.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

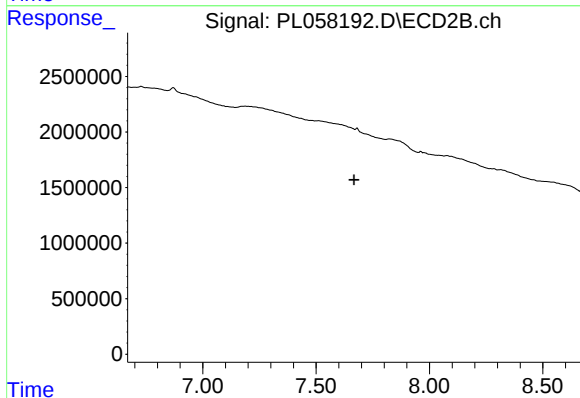


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.667 min
Response: 0
Conc: N.D.

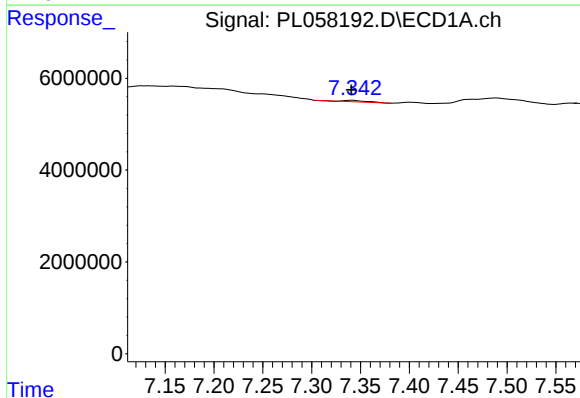


#22 Mirex

R.T.: 7.342 min
Delta R.T.: 0.002 min
Response: 501930
Conc: 0.06 ng/ml

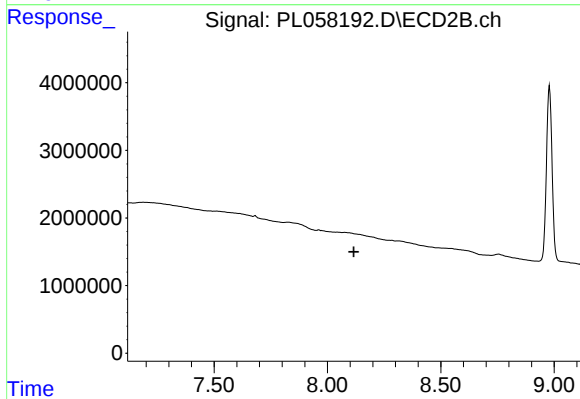

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 8.117 min
Response: 0
Conc: N.D.

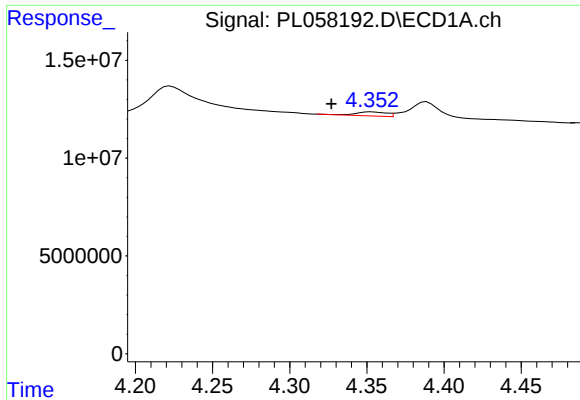

#23 Chlordane-1


R.T.: 4.353 min
Delta R.T.: 0.026 min
Response: 3004844
Conc: 8.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

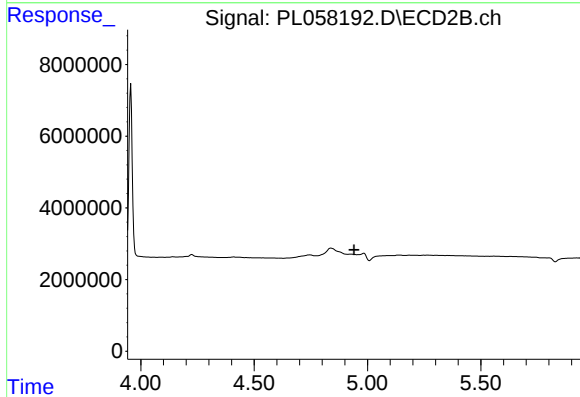


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

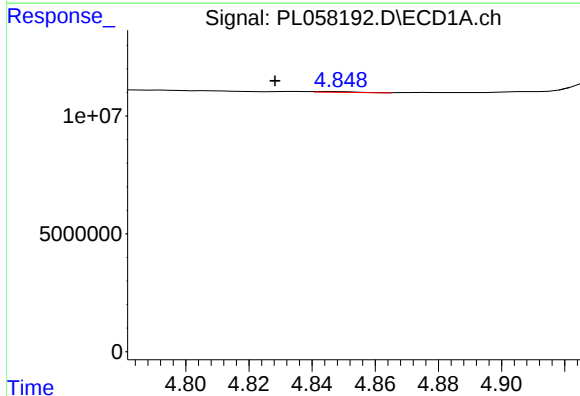


#24 Chlordane-2

R.T.: 4.847 min
Delta R.T.: 0.019 min
Response: 303348
Conc: 0.75 ng/ml

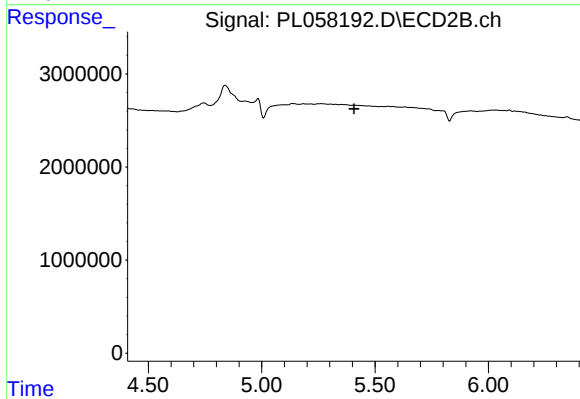

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.407 min
Response: 0
Conc: N.D.

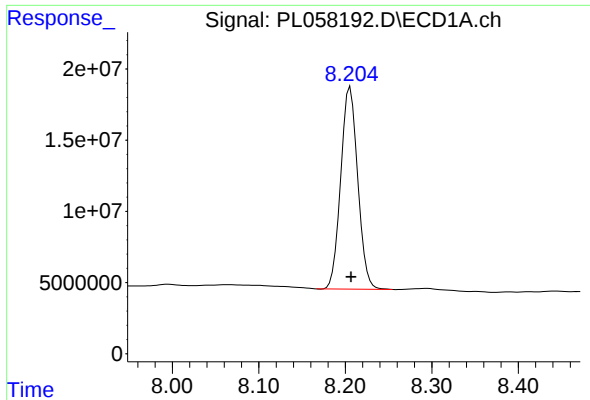

#28 Decachlorobiphenyl

R.T.: 8.206 min
Delta R.T.: -0.001 min
Response: 192830528
Conc: 18.71 ng/ml

Instrument :
ECD_L
ClientSampleId :

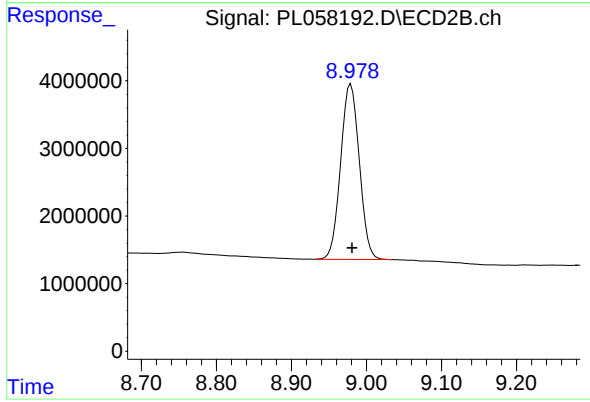

#28 Decachlorobiphenyl

R.T.: 8.979 min
Delta R.T.: -0.002 min
Response: 44958737
Conc: 20.13 ng/ml