

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042020\
 Data File : PL058196.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2020 19:17
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 05:03:59 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.456	3.955	246.0E6	51929999	24.403	23.929
28)	SA Decachlor...	8.205	8.979	206.5E6	45246743	20.033	20.256
Target Compounds							
2)	A alpha-BHC	3.894	0.000	4670079	0	0.269	N.D. #
4)	MA Heptachlor	4.483	5.141	906965	914341	0.057	0.272 #
15)	B Endosulfa...	0.000	6.869f	0	452264	N.D.	0.174 #
23)	Chlordane-1	4.356f	0.000	2818729	0	7.621	N.D. #
24)	Chlordane-2	4.814	0.000	417826	0	1.035	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042020\
Data File : PL058196.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2020 19:17
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 05:03:59 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

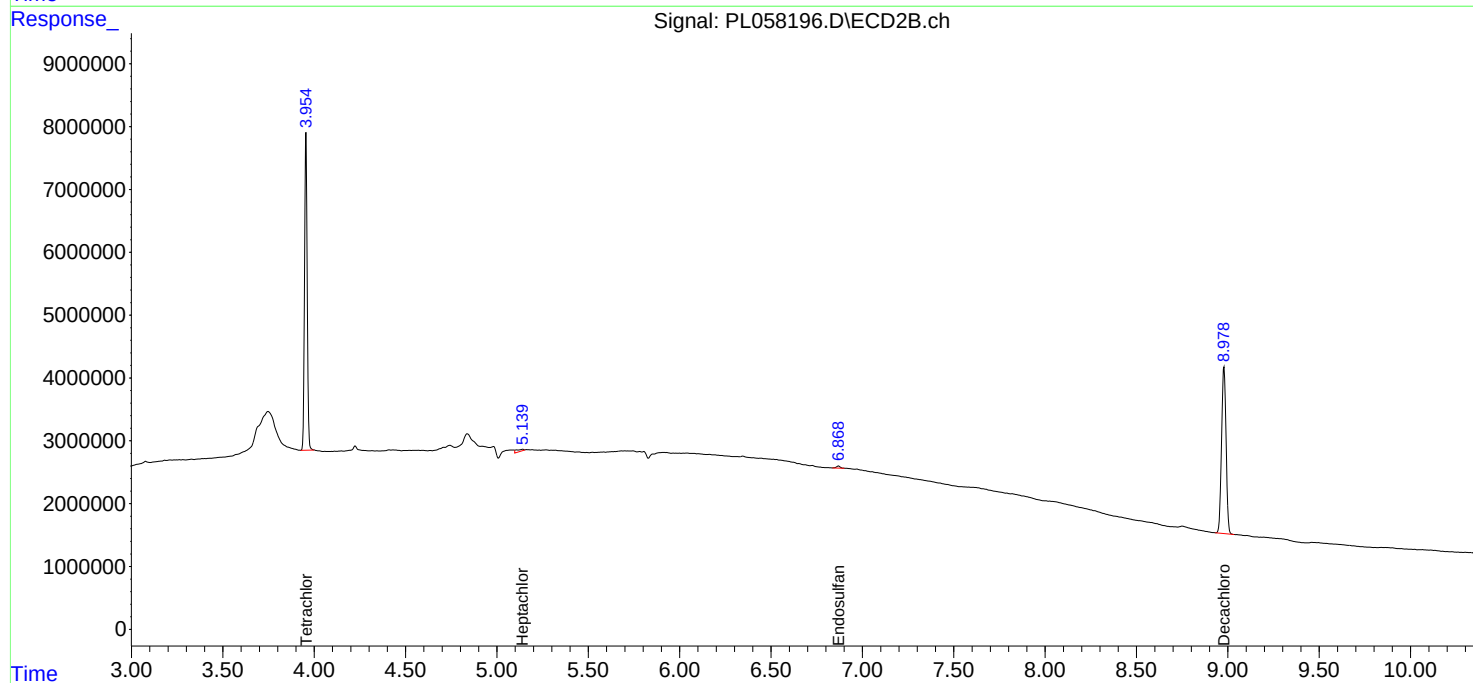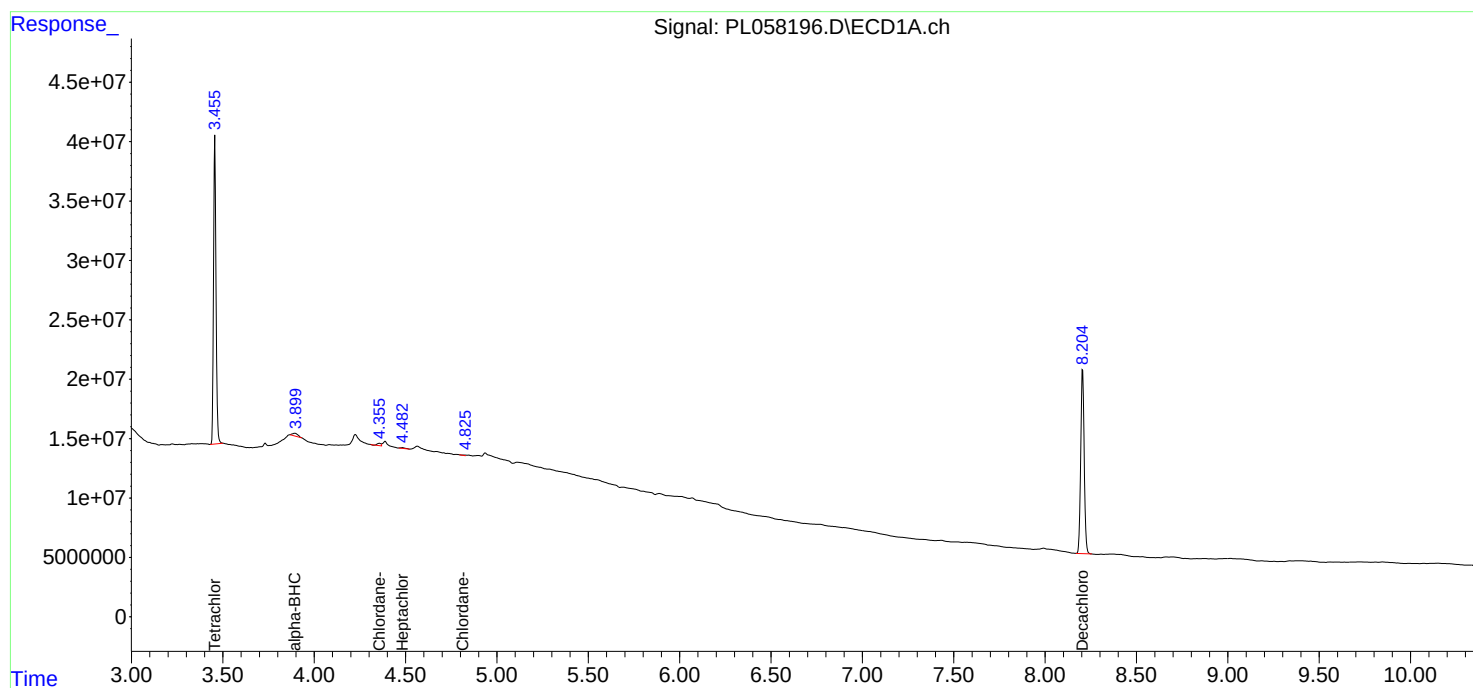


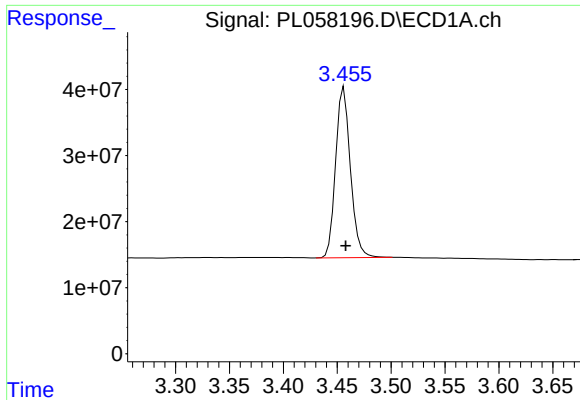

#1 Tetrachloro-m-xylene


R.T.: 3.456 min
Delta R.T.: -0.002 min
Response: 246003212
Conc: 24.40 ng/ml

Instrument :
ECD_L
ClientSampleId :

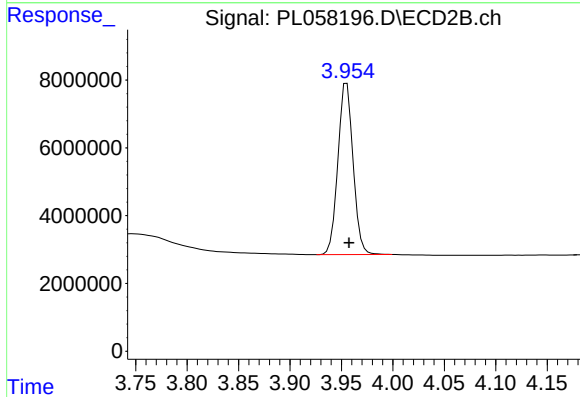


#1 Tetrachloro-m-xylene

R.T.: 3.955 min
Delta R.T.: -0.002 min
Response: 51929999
Conc: 23.93 ng/ml

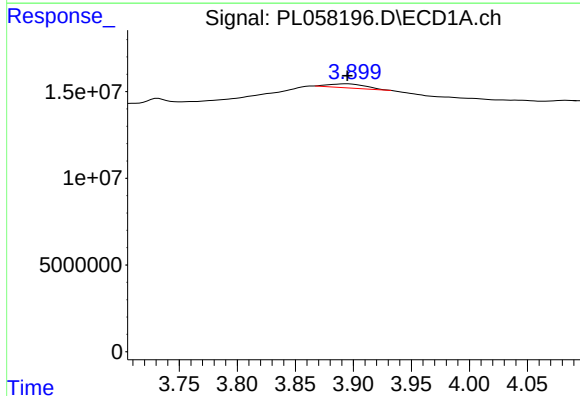


#2 alpha-BHC

R.T.: 3.894 min
Delta R.T.: -0.001 min
Response: 4670079
Conc: 0.27 ng/ml

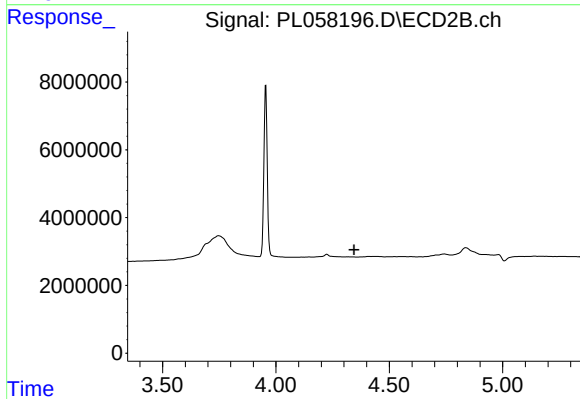

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.345 min
Response: 0
Conc: N.D.

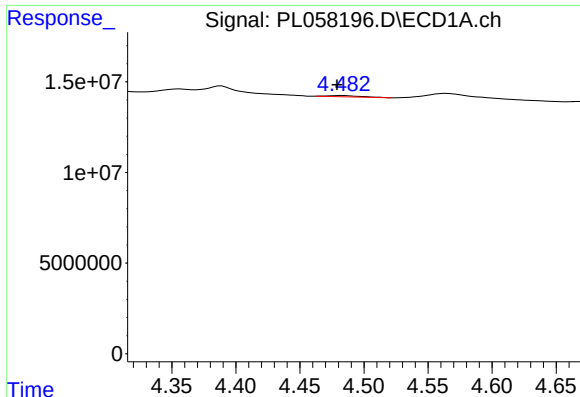

#4 Heptachlor


R.T.: 4.483 min
Delta R.T.: 0.004 min
Response: 906965
Conc: 0.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

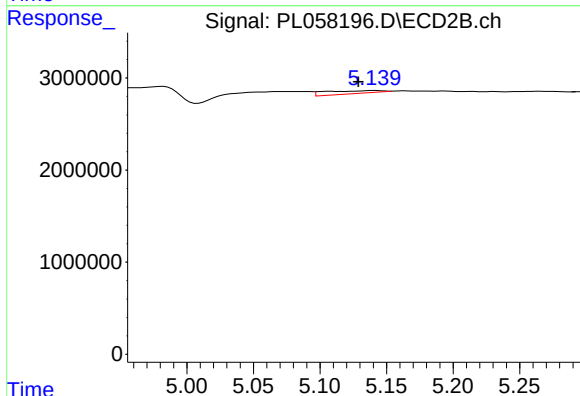


#4 Heptachlor

R.T.: 5.141 min
Delta R.T.: 0.012 min
Response: 914341
Conc: 0.27 ng/ml

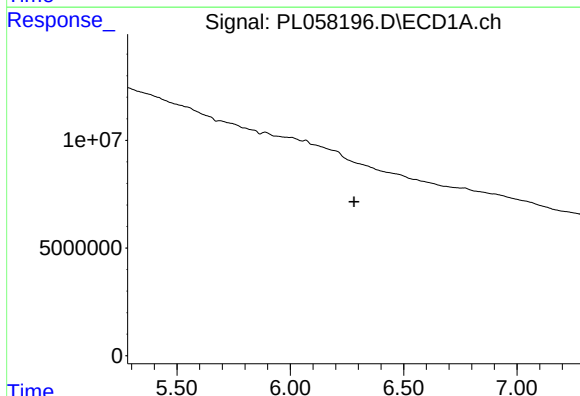


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.282 min
Response: 0
Conc: N.D.

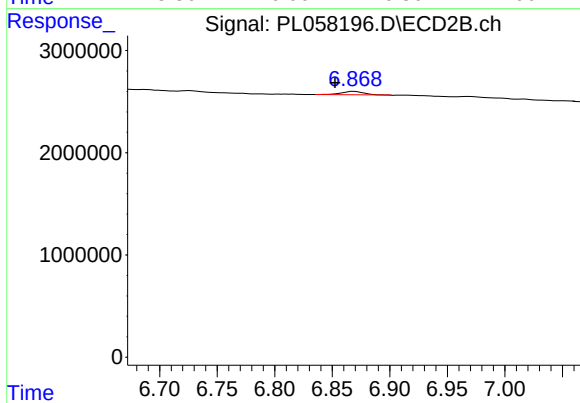

#15 Endosulfan II


R.T.: 6.869 min
Delta R.T.: 0.017 min
Response: 452264
Conc: 0.17 ng/ml

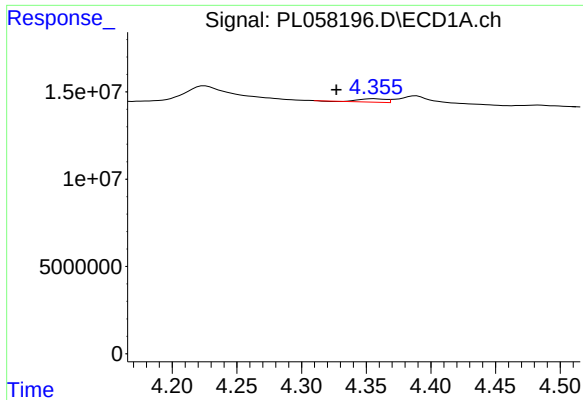

#23 Chlordane-1


R.T.: 4.356 min
Delta R.T.: 0.029 min
Response: 2818729
Conc: 7.62 ng/ml

Instrument :
ECD_L
ClientSampleId :

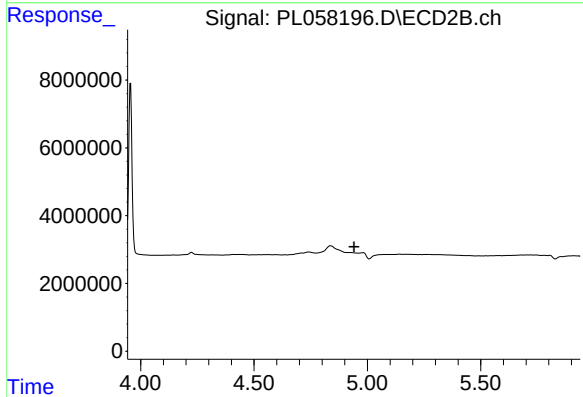


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

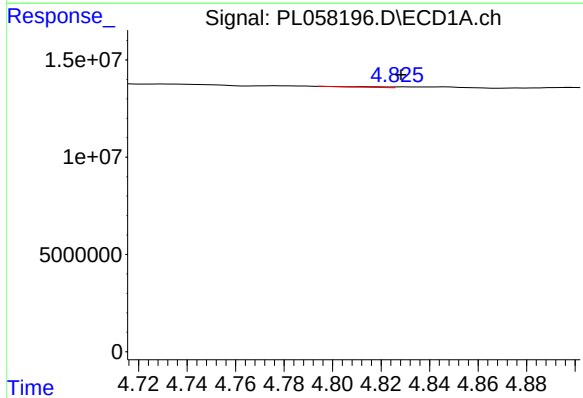


#24 Chlordane-2

R.T.: 4.814 min
Delta R.T.: -0.014 min
Response: 417826
Conc: 1.03 ng/ml

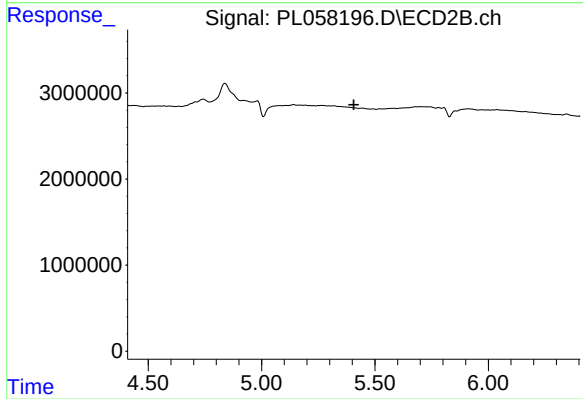

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.407 min
Response: 0
Conc: N.D.

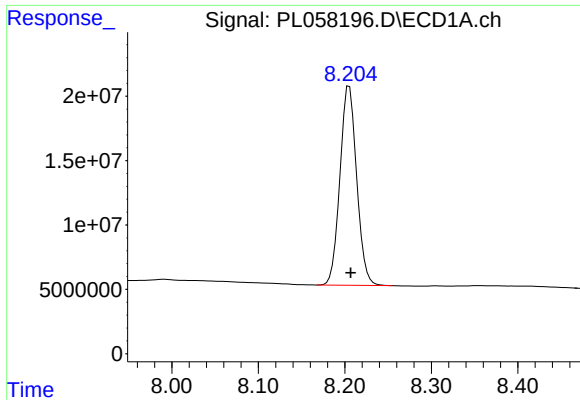

#28 Decachlorobiphenyl

R.T.: 8.205 min
Delta R.T.: -0.002 min
Response: 206506636
Conc: 20.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

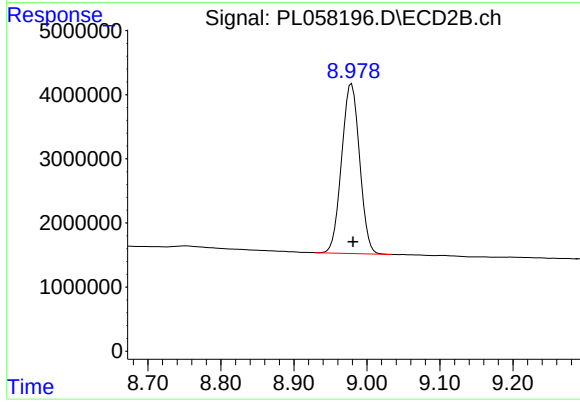

#28 Decachlorobiphenyl

R.T.: 8.979 min
Delta R.T.: -0.002 min
Response: 45246743
Conc: 20.26 ng/ml