

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042020\
 Data File : PL058216.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Apr 2020 00:16
 Operator : AJ\MA
 Sample : L2327-12
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 05:10:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.457	3.956	233.3E6	52923054	23.147	24.387
28)	SA Decachlor...	8.206	8.978	200.9E6	42618090	19.485	19.079
Target Compounds							
2)	A alpha-BHC	0.000	4.333	0	216335	N.D.	0.066 #
4)	MA Heptachlor	4.474	5.137	1029323	1366097	0.064	0.407 #
7)	B delta-BHC	0.000	4.984f	0	10175802	N.D.	5.931 #
8)	B Heptachlo...	0.000	5.802	0	4071621	N.D.	1.508 #
15)	B Endosulfa...	0.000	6.869f	0	687538	N.D.	0.265 #
19)	B Endosulfa...	6.681f	0.000	1534275	0	0.151	N.D. #
23)	Chlordane-1	4.355f	0.000	3286164	0	8.885	N.D. #
24)	Chlordane-2	4.840	0.000	3481045	0	8.623	N.D. #
27)	Chlordane-5	6.315f	0.000	26287884	0	69.494	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042020\
Data File : PL058216.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Apr 2020 00:16
Operator : AJ\MA
Sample : L2327-12
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 05:10:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

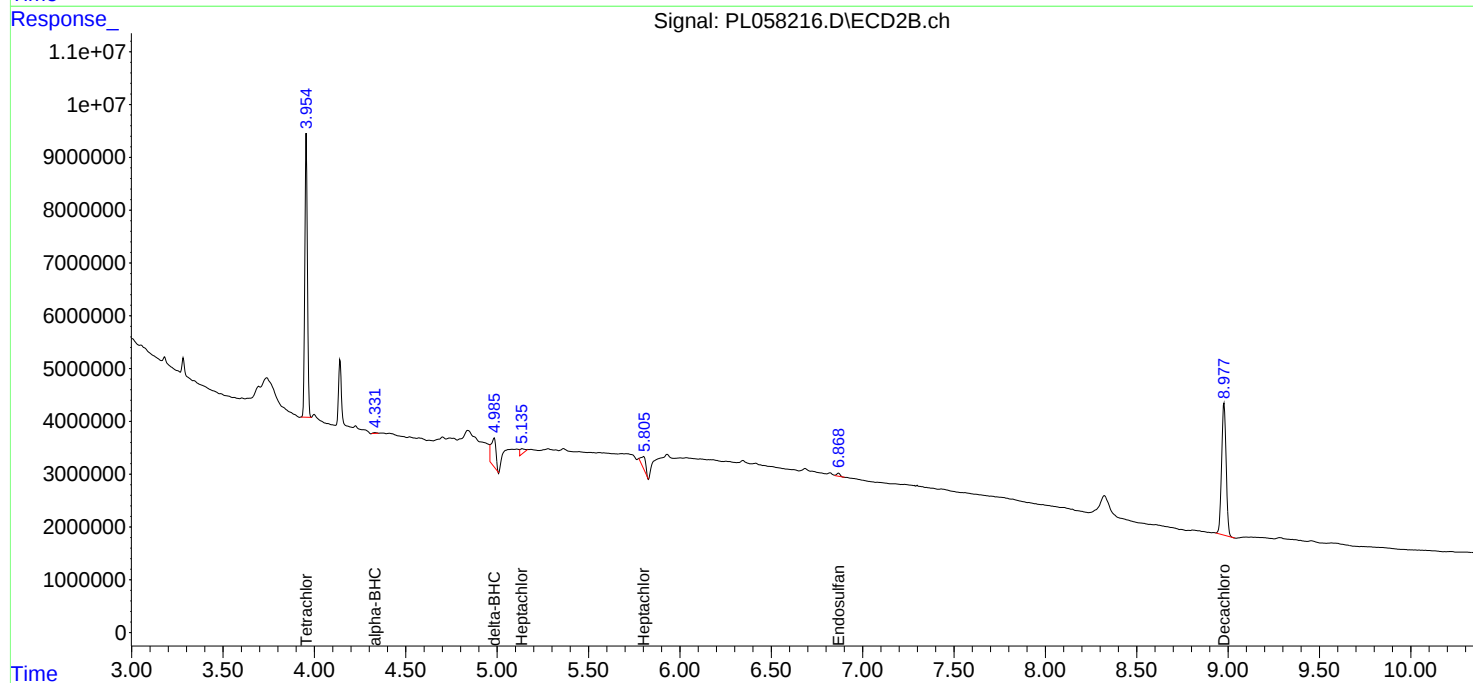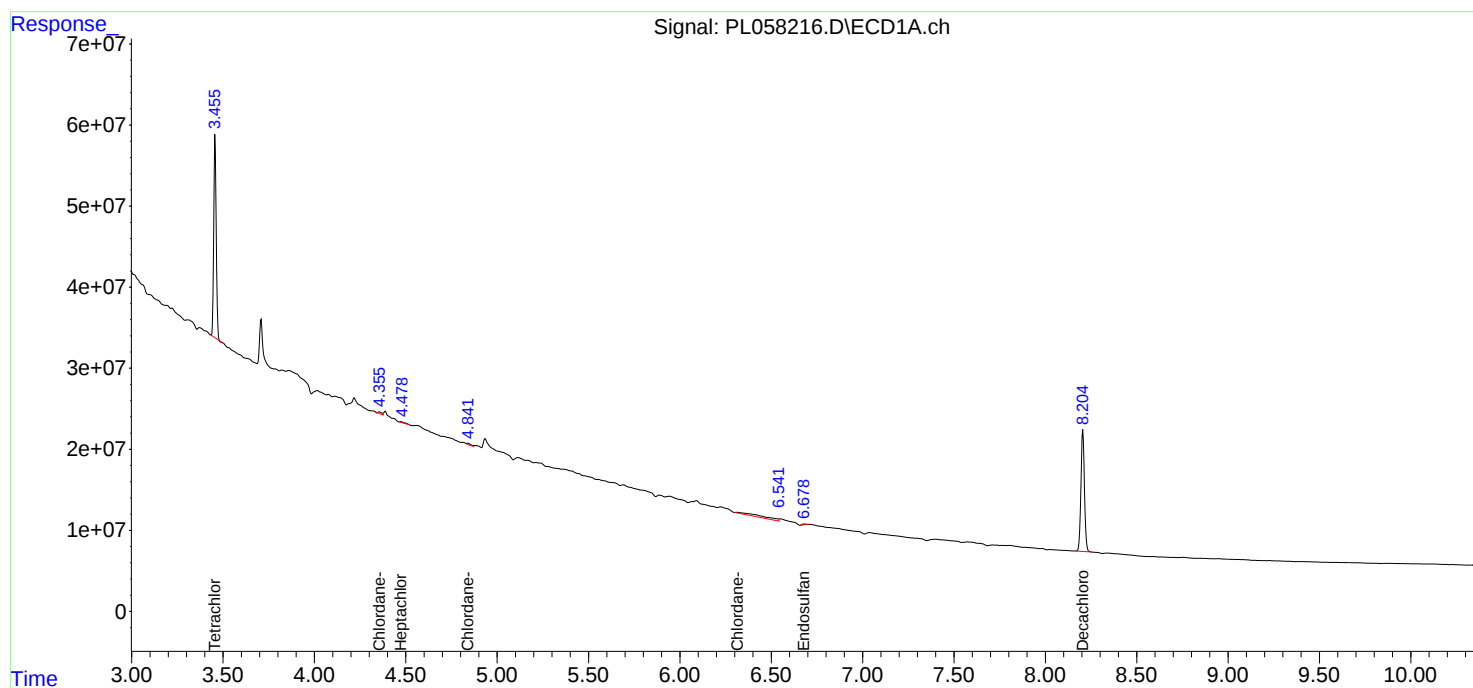


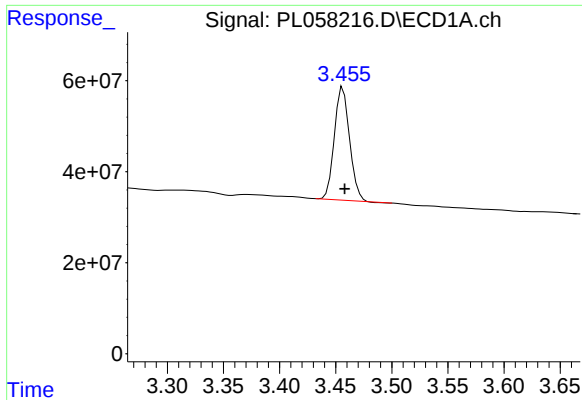

#1 Tetrachloro-m-xylene


R.T.: 3.457 min
Delta R.T.: -0.001 min
Response: 233346601
Conc: 23.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

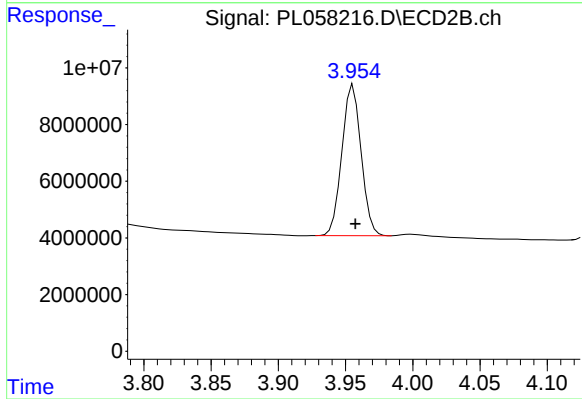


#1 Tetrachloro-m-xylene

R.T.: 3.956 min
Delta R.T.: -0.002 min
Response: 52923054
Conc: 24.39 ng/ml

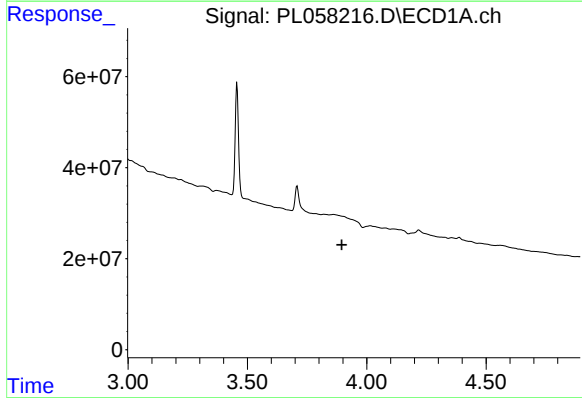


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.895 min
Response: 0
Conc: N.D.

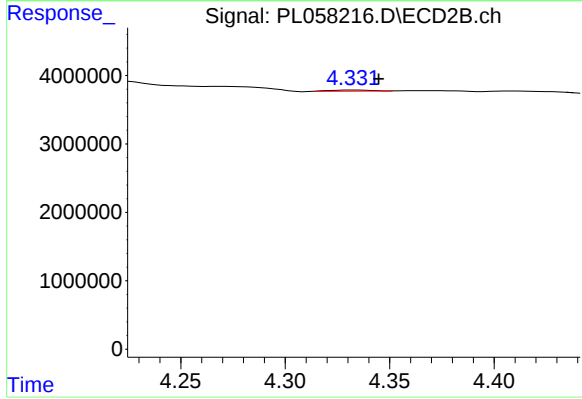

#2 alpha-BHC


R.T.: 4.333 min
Delta R.T.: -0.012 min
Response: 216335
Conc: 0.07 ng/ml

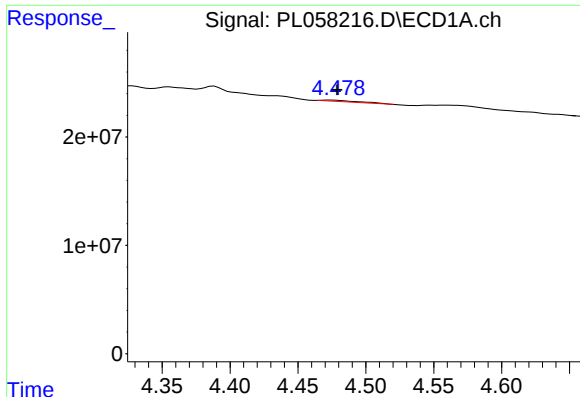

#4 Heptachlor


R.T.: 4.474 min
Delta R.T.: -0.005 min
Response: 1029323
Conc: 0.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

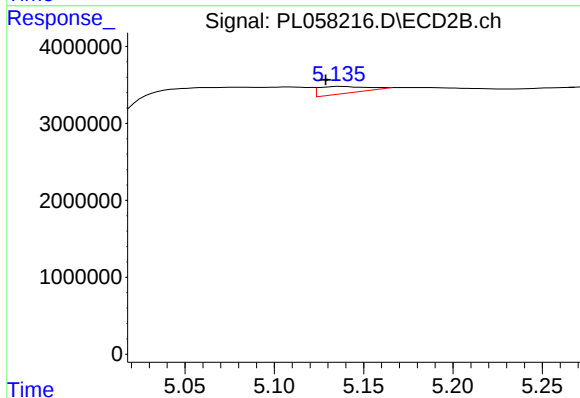


#4 Heptachlor

R.T.: 5.137 min
Delta R.T.: 0.008 min
Response: 1366097
Conc: 0.41 ng/ml

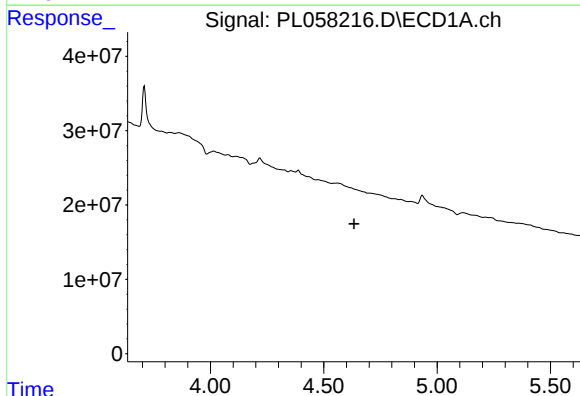


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.634 min
Response: 0
Conc: N.D.

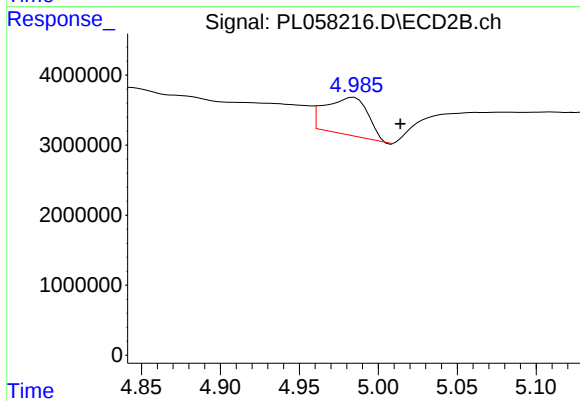

#7 delta-BHC


R.T.: 4.984 min
Delta R.T.: -0.030 min
Response: 10175802
Conc: 5.93 ng/ml

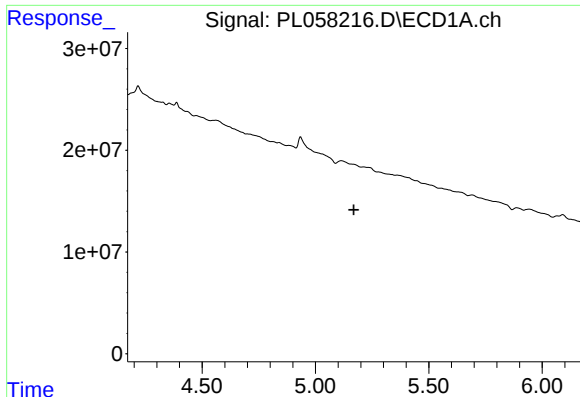

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.169 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

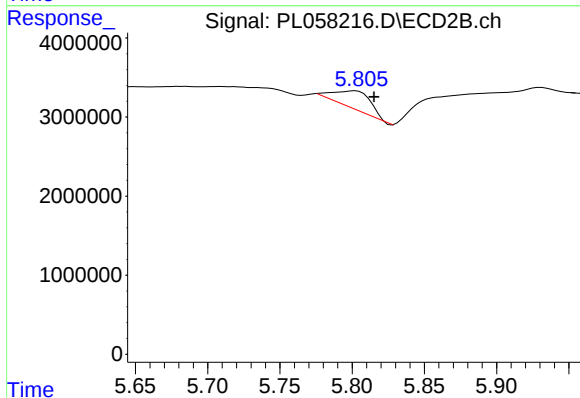


#8 Heptachlor epoxide

R.T.: 5.802 min
Delta R.T.: -0.013 min
Response: 4071621
Conc: 1.51 ng/ml

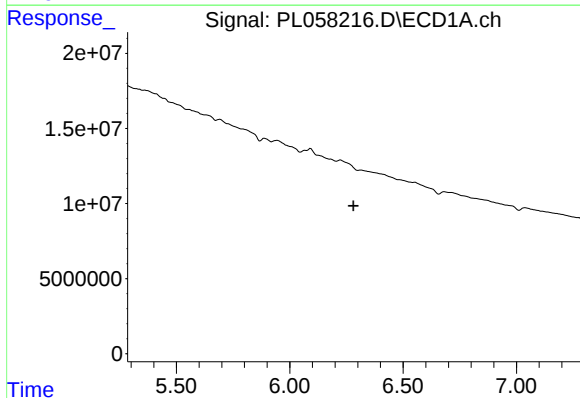


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.282 min
Response: 0
Conc: N.D.

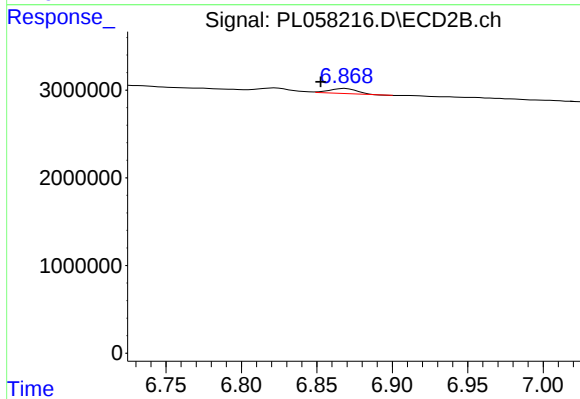

#15 Endosulfan II


R.T.: 6.869 min
Delta R.T.: 0.016 min
Response: 687538
Conc: 0.27 ng/ml

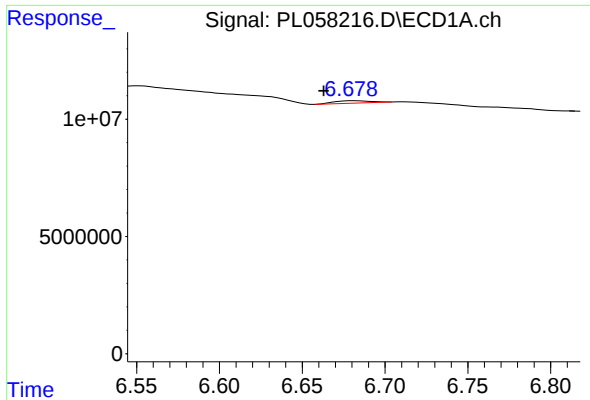

#19 Endosulfan Sulfate


R.T.: 6.681 min
Delta R.T.: 0.018 min
Response: 1534275
Conc: 0.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

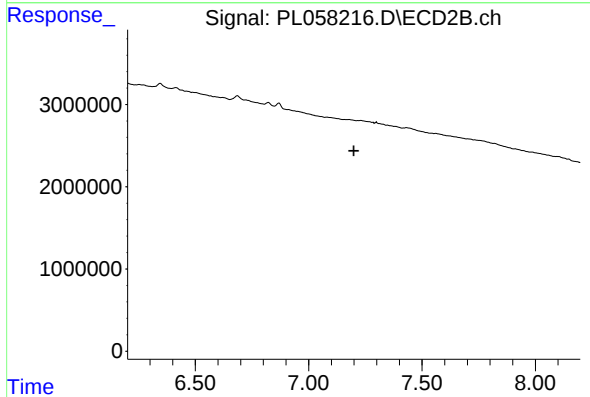


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.199 min
Response: 0
Conc: N.D.

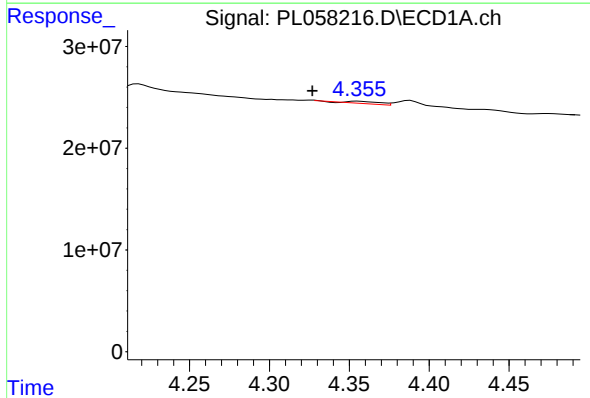


#23 Chlordane-1

R.T.: 4.355 min
Delta R.T.: 0.028 min
Response: 3286164
Conc: 8.89 ng/ml

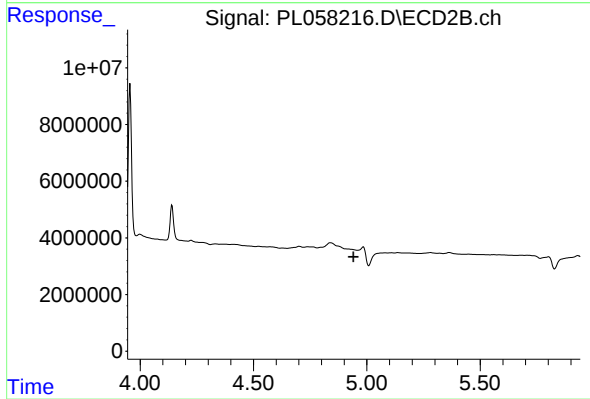

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

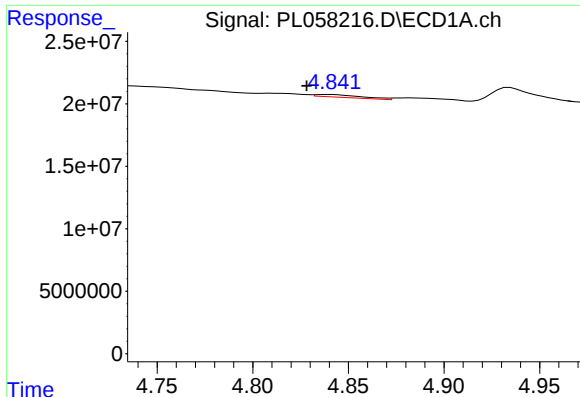

#24 Chlordane-2


R.T.: 4.840 min
Delta R.T.: 0.012 min
Response: 3481045
Conc: 8.62 ng/ml

Instrument :
ECD_L
ClientSampleId :

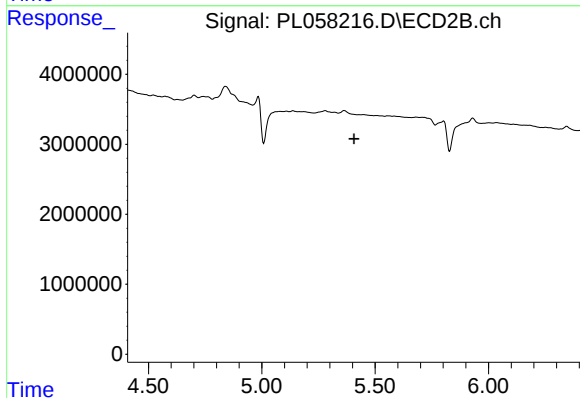


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.407 min
Response: 0
Conc: N.D.

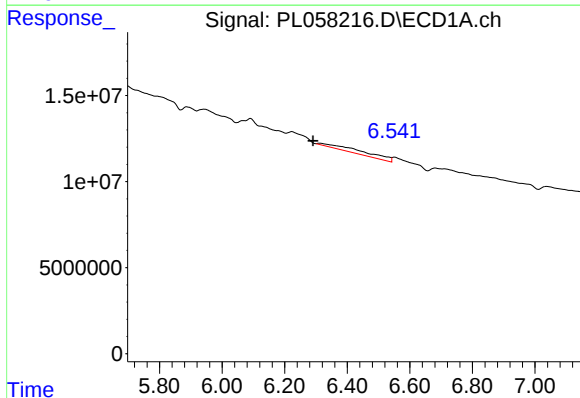


#27 Chlordane-5

R.T.: 6.315 min
Delta R.T.: 0.024 min
Response: 26287884
Conc: 69.49 ng/ml

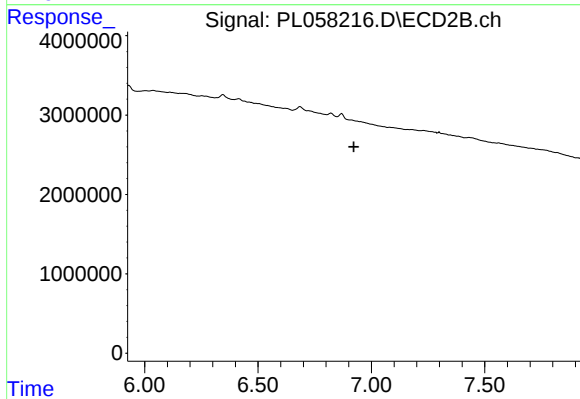

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 6.922 min
Response: 0
Conc: N.D.

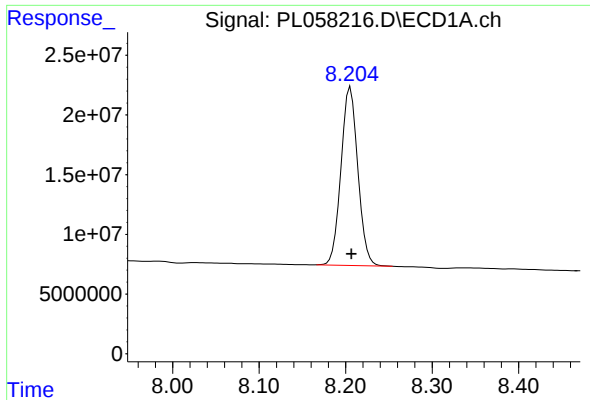

#28 Decachlorobiphenyl

R.T.: 8.206 min
Delta R.T.: -0.001 min
Response: 200864331
Conc: 19.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

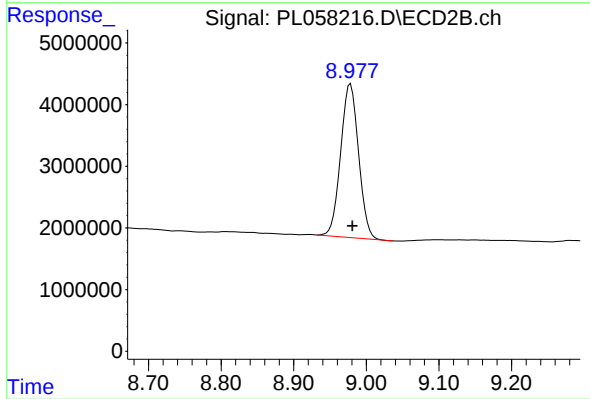

#28 Decachlorobiphenyl

R.T.: 8.978 min
Delta R.T.: -0.003 min
Response: 42618090
Conc: 19.08 ng/ml