

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042020\
 Data File : PL058219.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Apr 2020 00:58
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 05:10:46 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.457	3.956	239.9E6	50933349	23.794	23.470
28)	SA Decachlor...	8.205	8.979	220.6E6	45916815	21.402	20.556
Target Compounds							
2)	A alpha-BHC	3.892	0.000	5710325	0	0.329	N.D. #
4)	MA Heptachlor	4.473	5.138	992186	756056	0.062	0.225 #
6)	B beta-BHC	4.431	0.000	545800	0	0.086	N.D. #
8)	B Heptachlo...	5.172	5.811	1212266	3399196	0.090	1.259 #
9)	A Endosulfan I	5.514	0.000	269743	0	0.022	N.D. #
14)	MA Endrin	6.010	0.000	3865572	0	0.331	N.D. #
15)	B Endosulfa...	6.311f	6.868f	20647018	448950	1.866	0.173 #
23)	Chlordane-1	4.354f	0.000	2125381	0	5.747	N.D. #
24)	Chlordane-2	4.840	0.000	14621131	0	36.216	N.D. #
27)	Chlordane-5	6.311f	0.000	20647018	0	54.582	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042020\
Data File : PL058219.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Apr 2020 00:58
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 05:10:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

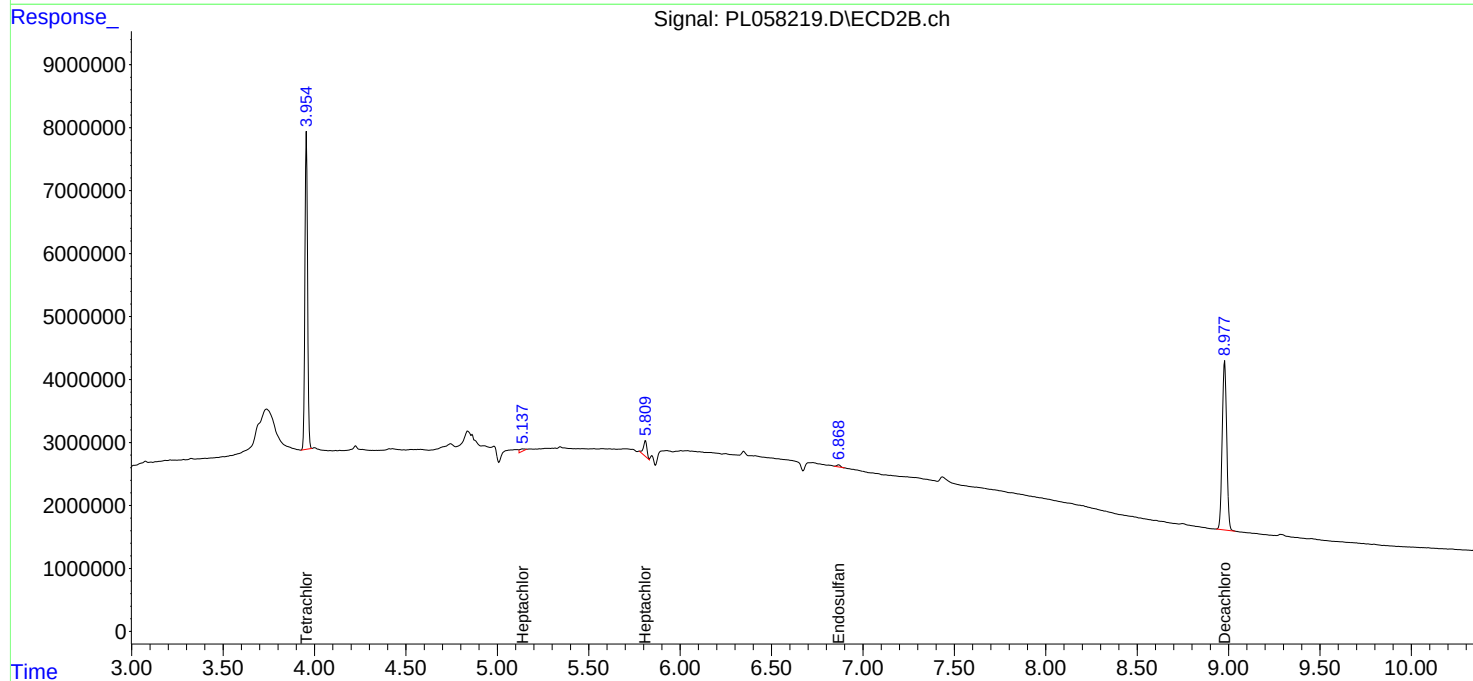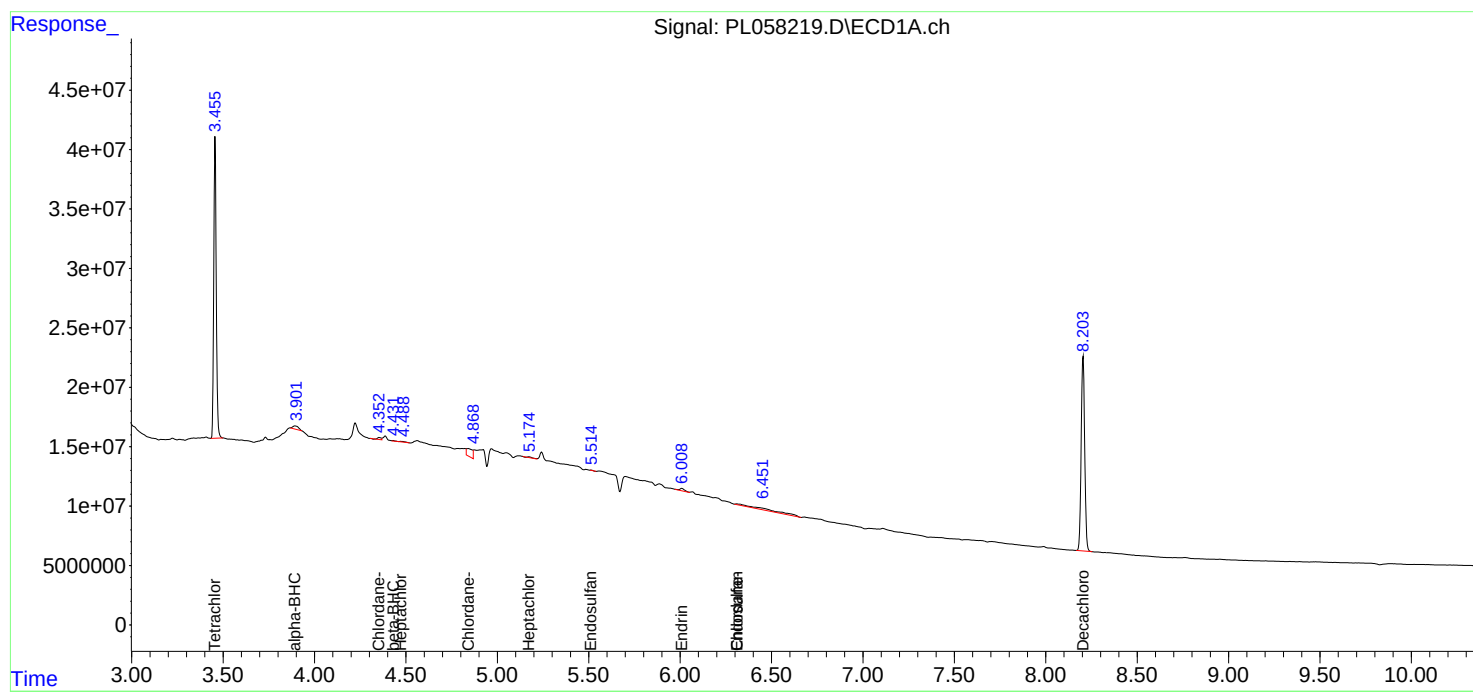


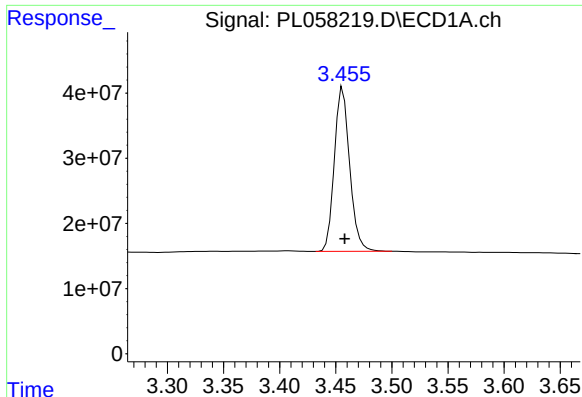

#1 Tetrachloro-m-xylene


R.T.: 3.457 min
Delta R.T.: -0.001 min
Response: 239864153
Conc: 23.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

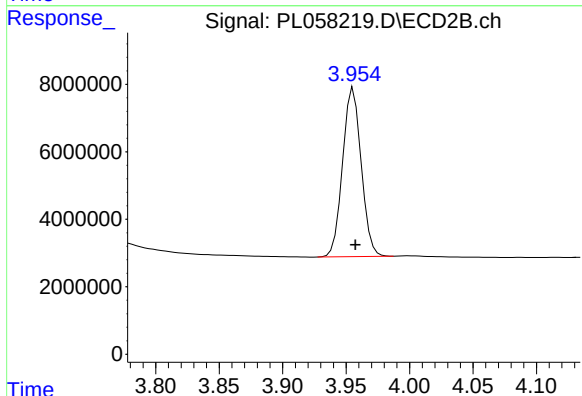


#1 Tetrachloro-m-xylene

R.T.: 3.956 min
Delta R.T.: -0.002 min
Response: 50933349
Conc: 23.47 ng/ml

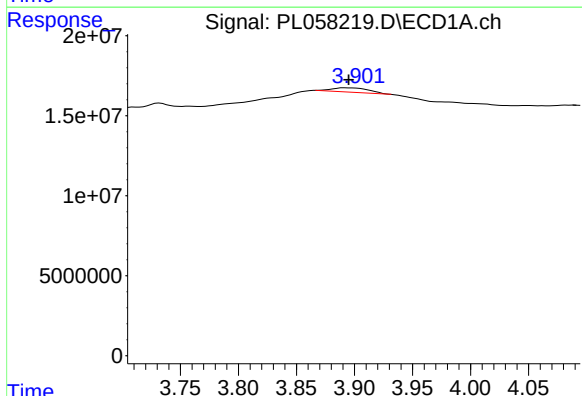


#2 alpha-BHC

R.T.: 3.892 min
Delta R.T.: -0.003 min
Response: 5710325
Conc: 0.33 ng/ml

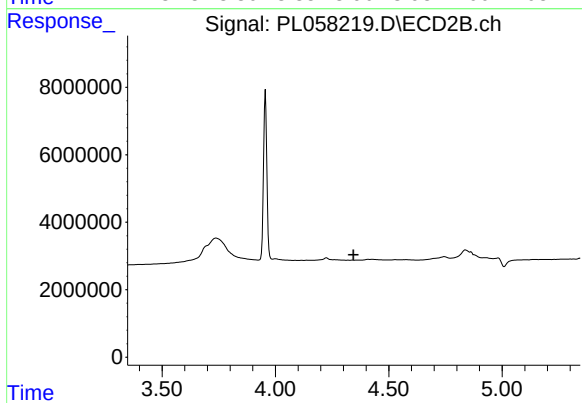

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.345 min
Response: 0
Conc: N.D.

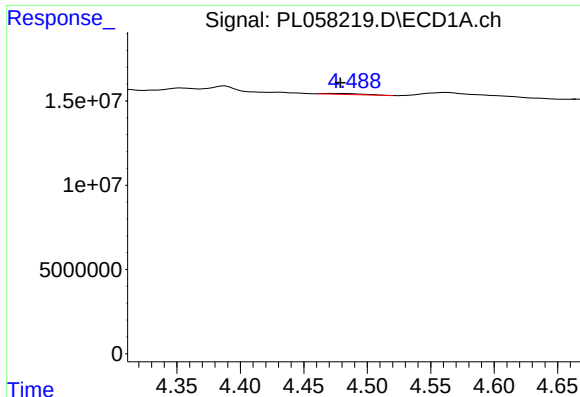

#4 Heptachlor


R.T.: 4.473 min
Delta R.T.: -0.006 min
Response: 992186
Conc: 0.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

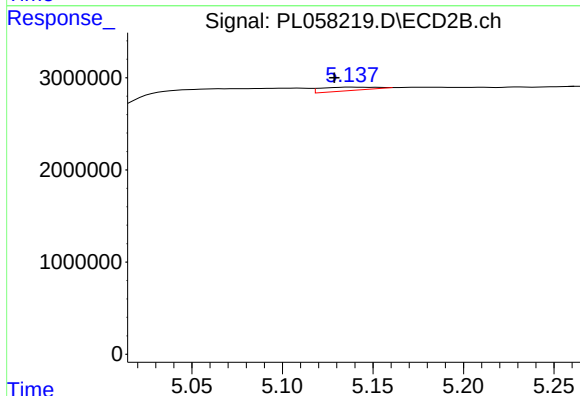


#4 Heptachlor

R.T.: 5.138 min
Delta R.T.: 0.010 min
Response: 756056
Conc: 0.23 ng/ml

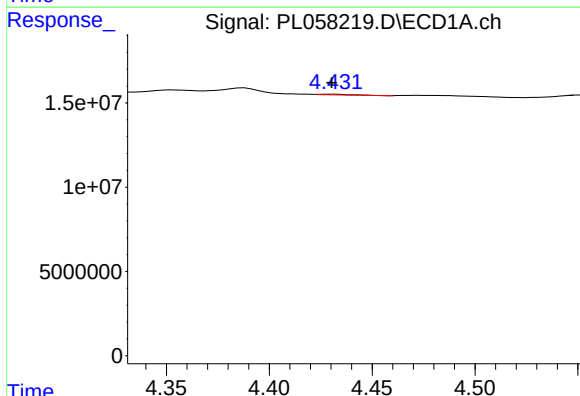


#6 beta-BHC

R.T.: 4.431 min
Delta R.T.: 0.000 min
Response: 545800
Conc: 0.09 ng/ml

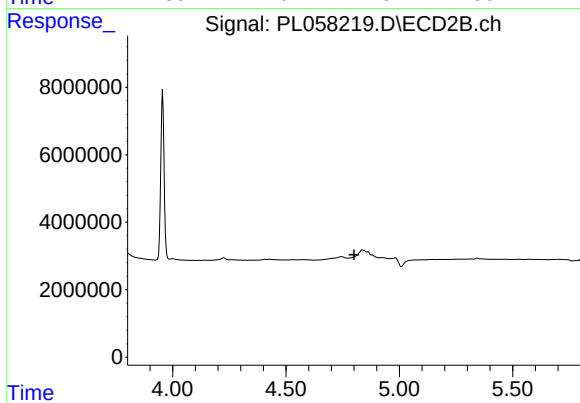

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.800 min
Response: 0
Conc: N.D.

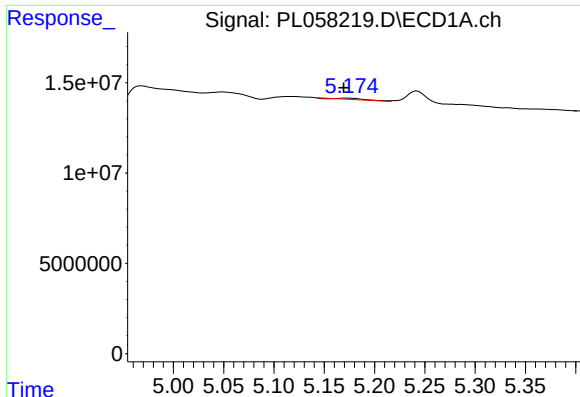

#8 Heptachlor epoxide


R.T.: 5.172 min
Delta R.T.: 0.003 min
Response: 1212266
Conc: 0.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

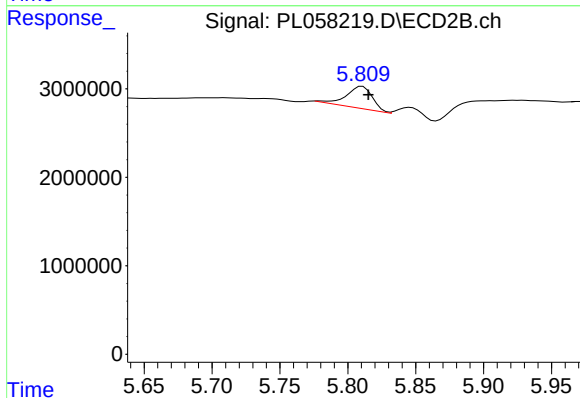


#8 Heptachlor epoxide

R.T.: 5.811 min
Delta R.T.: -0.004 min
Response: 3399196
Conc: 1.26 ng/ml

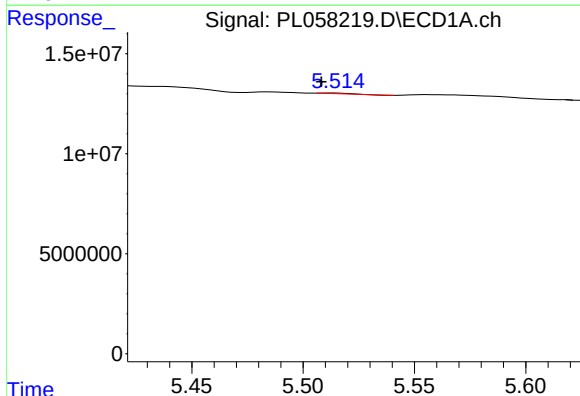


#9 Endosulfan I

R.T.: 5.514 min
Delta R.T.: 0.005 min
Response: 269743
Conc: 0.02 ng/ml

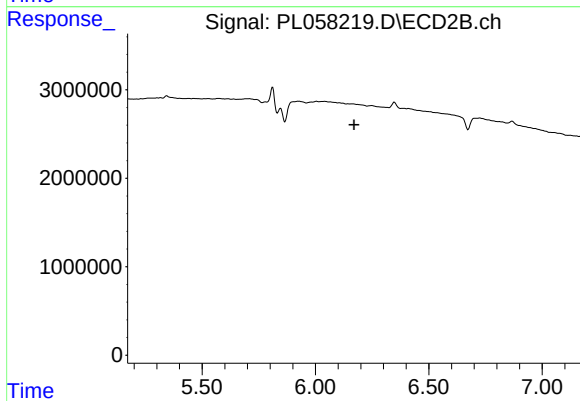

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.170 min
Response: 0
Conc: N.D.

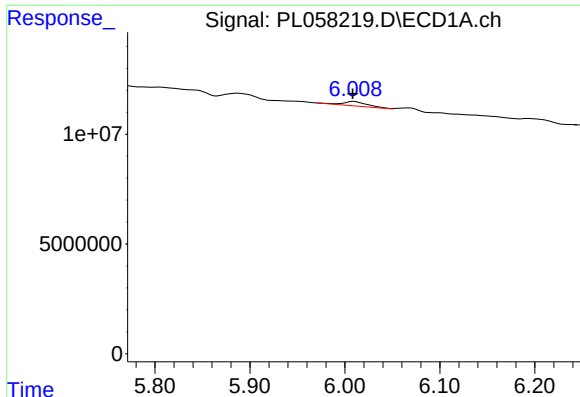

#14 Endrin


R.T.: 6.010 min
Delta R.T.: 0.001 min
Response: 3865572
Conc: 0.33 ng/ml

Instrument :
ECD_L
ClientSampleId :

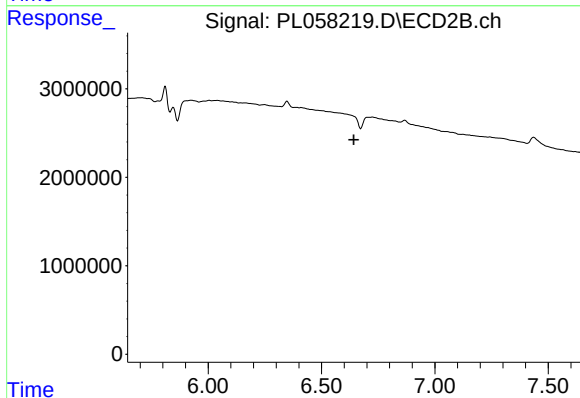


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.642 min
Response: 0
Conc: N.D.

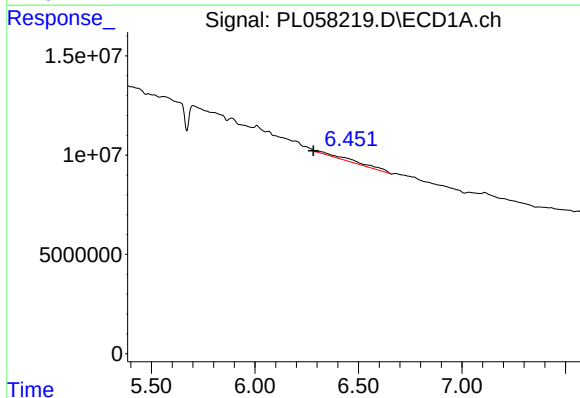


#15 Endosulfan II

R.T.: 6.311 min
Delta R.T.: 0.029 min
Response: 20647018
Conc: 1.87 ng/ml

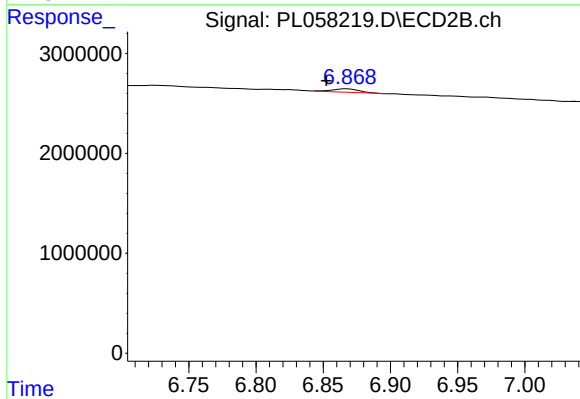

#15 Endosulfan II


R.T.: 6.868 min
Delta R.T.: 0.015 min
Response: 448950
Conc: 0.17 ng/ml

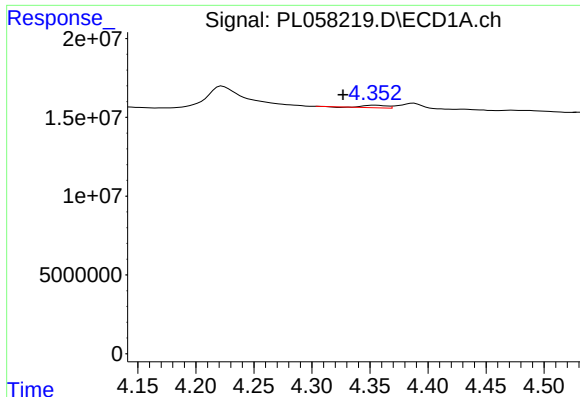

#23 Chlordane-1


R.T.: 4.354 min
Delta R.T.: 0.027 min
Response: 2125381
Conc: 5.75 ng/ml

Instrument :
ECD_L
ClientSampleId :

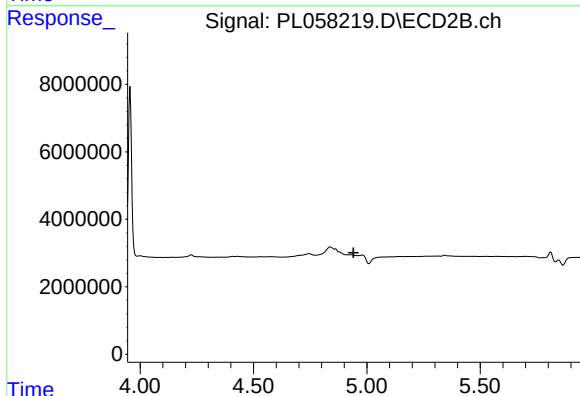


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

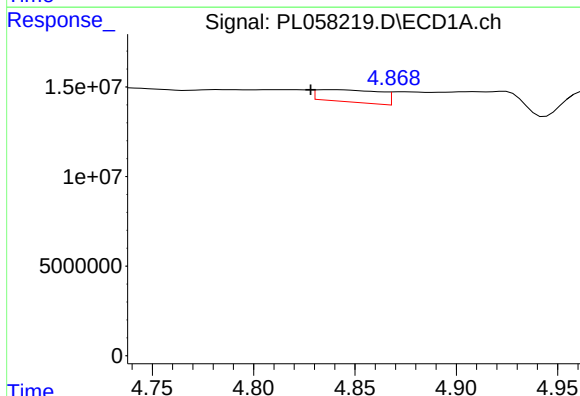


#24 Chlordane-2

R.T.: 4.840 min
Delta R.T.: 0.012 min
Response: 14621131
Conc: 36.22 ng/ml

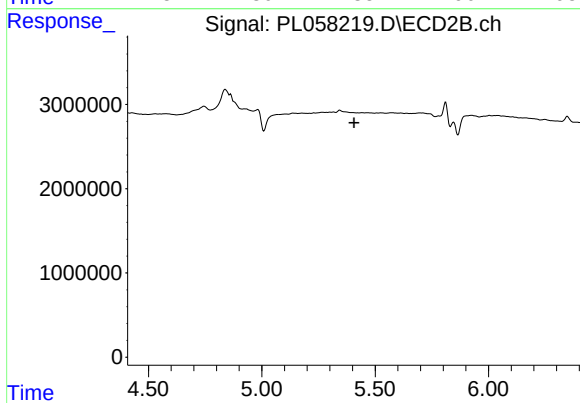

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.407 min
Response: 0
Conc: N.D.

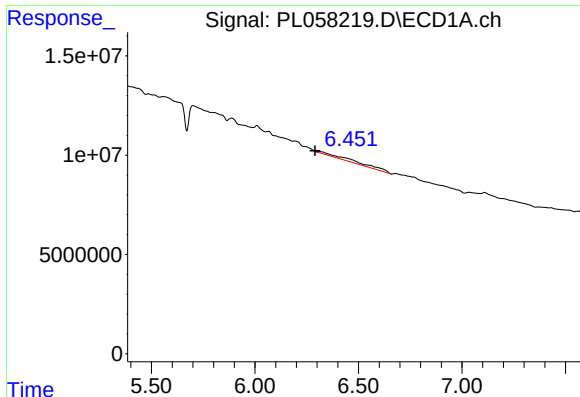

#27 Chlordane-5


R.T.: 6.311 min
Delta R.T.: 0.020 min
Response: 20647018
Conc: 54.58 ng/ml

Instrument :
ECD_L
ClientSampleId :

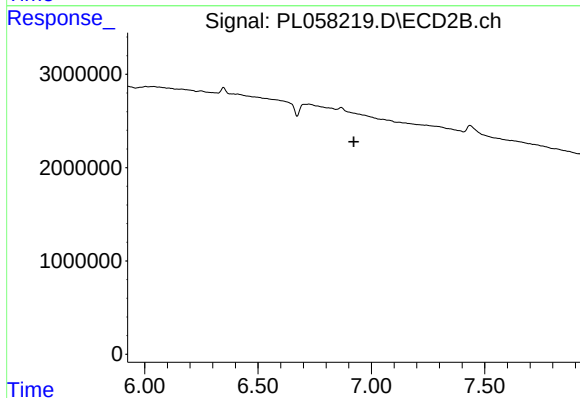


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.922 min
Response: 0
Conc: N.D.

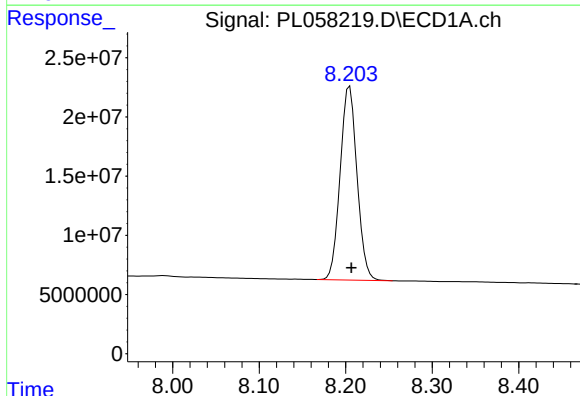

#28 Decachlorobiphenyl

R.T.: 8.205 min
Delta R.T.: -0.002 min
Response: 220617126
Conc: 21.40 ng/ml

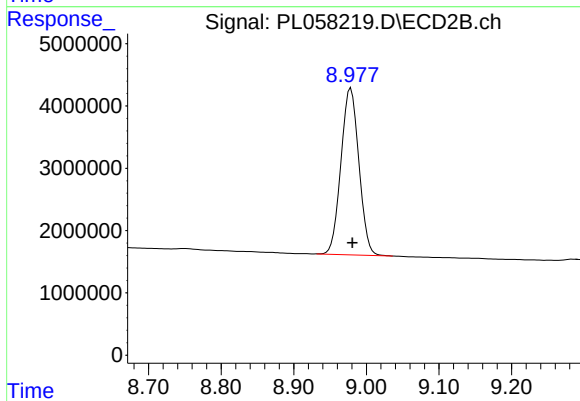

#28 Decachlorobiphenyl

R.T.: 8.979 min
Delta R.T.: -0.002 min
Response: 45916815
Conc: 20.56 ng/ml