

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042020\
 Data File : PL058229.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Apr 2020 03:35
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 05:13:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.457	3.956	255.3E6	54365821	25.321	25.052
28)	SA Decachlor...	8.206	8.980	230.2E6	48016783	22.334	21.496
Target Compounds							
2)	A alpha-BHC	3.898	0.000	5881848	0	0.339	N.D. #
4)	MA Heptachlor	4.476	5.137	262148	333745	0.016	0.099 #
5)	MB Aldrin	4.735	0.000	1125041	0	0.076	N.D. #
6)	B beta-BHC	4.433	0.000	925362	0	0.147	N.D. #
8)	B Heptachlo...	5.175	5.812	2279217	12883021	0.170	4.771 #
9)	A Endosulfan I	5.489f	0.000	853068	0	0.070	N.D. #
14)	MA Endrin	6.010	0.000	2349103	0	0.201	N.D. #
15)	B Endosulfa...	0.000	6.869f	0	436702	N.D.	0.168 #
23)	Chlordane-1	4.355f	0.000	3027596	0	8.186	N.D. #
24)	Chlordane-2	4.812f	0.000	42683106	0	105.726	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042020\
Data File : PL058229.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Apr 2020 03:35
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 05:13:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

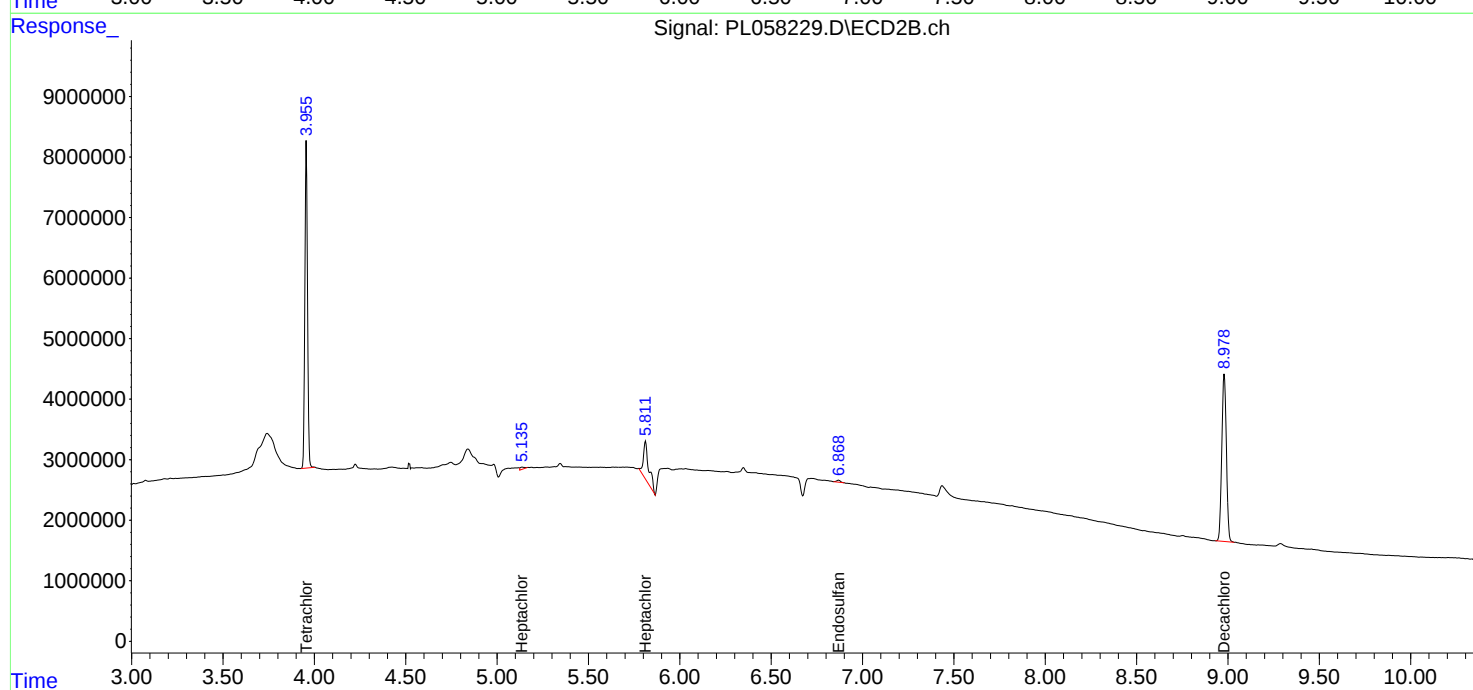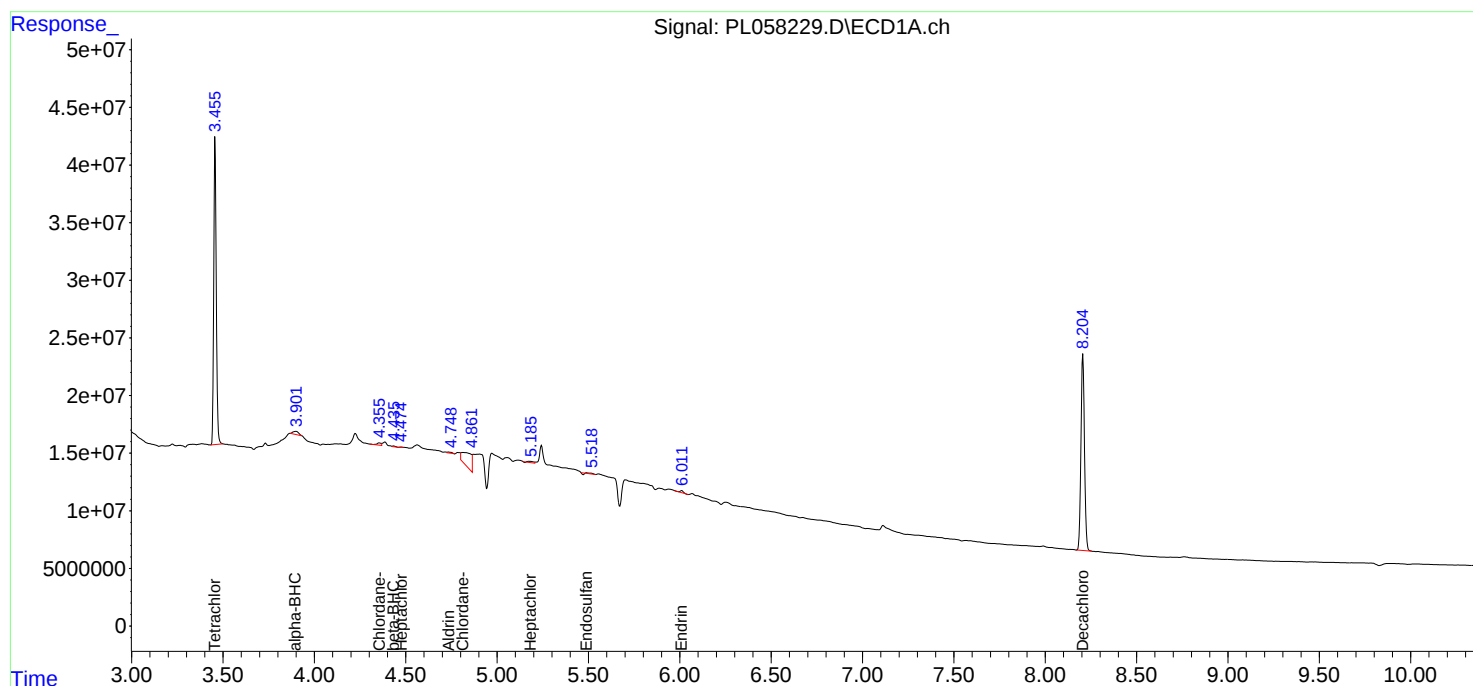


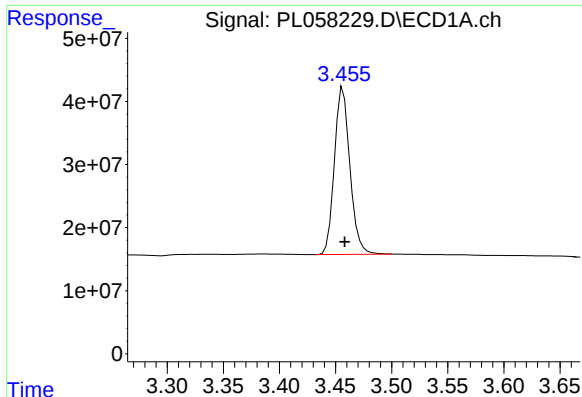

#1 Tetrachloro-m-xylene


R.T.: 3.457 min
Delta R.T.: -0.001 min
Response: 255263663
Conc: 25.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

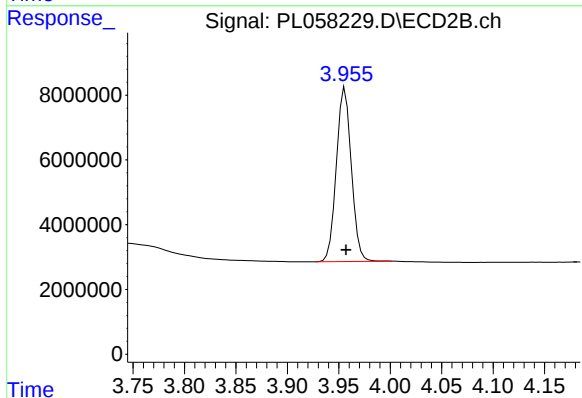


#1 Tetrachloro-m-xylene

R.T.: 3.956 min
Delta R.T.: -0.001 min
Response: 54365821
Conc: 25.05 ng/ml

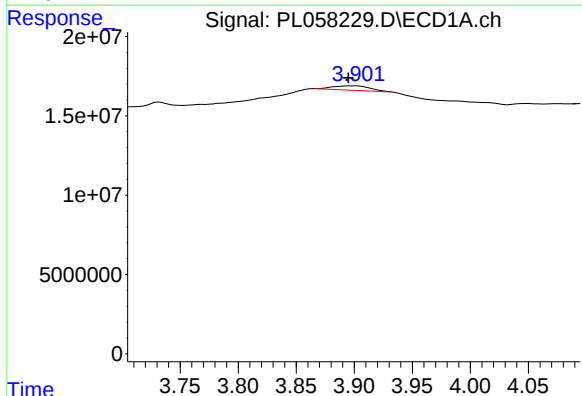


#2 alpha-BHC

R.T.: 3.898 min
Delta R.T.: 0.003 min
Response: 5881848
Conc: 0.34 ng/ml

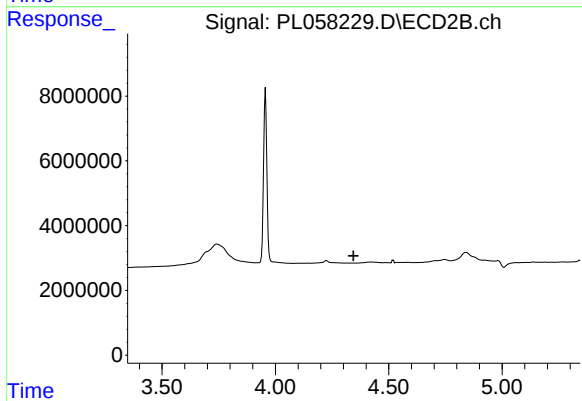

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.345 min
Response: 0
Conc: N.D.

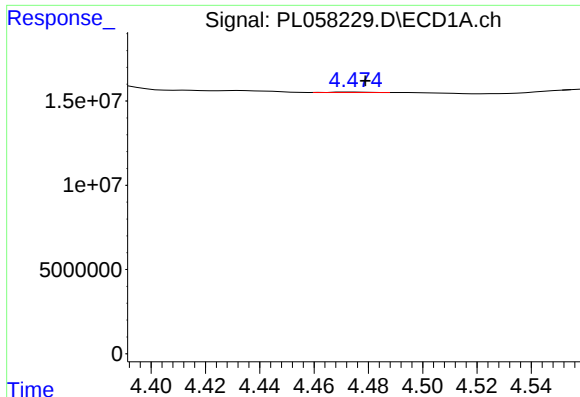

#4 Heptachlor


R.T.: 4.476 min
Delta R.T.: -0.003 min
Response: 262148
Conc: 0.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

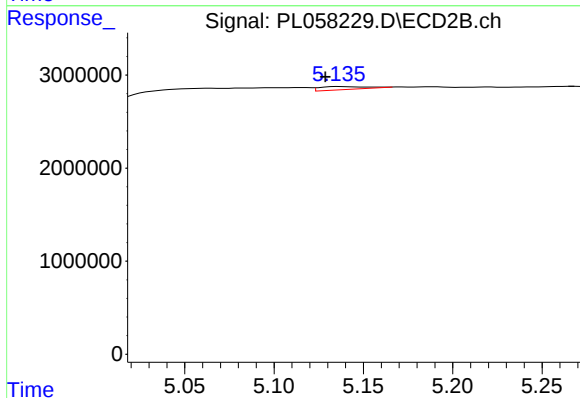


#4 Heptachlor

R.T.: 5.137 min
Delta R.T.: 0.008 min
Response: 333745
Conc: 0.10 ng/ml

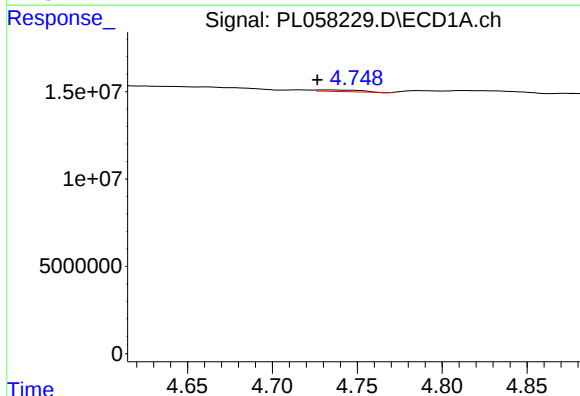


#5 Aldrin

R.T.: 4.735 min
Delta R.T.: 0.008 min
Response: 1125041
Conc: 0.08 ng/ml

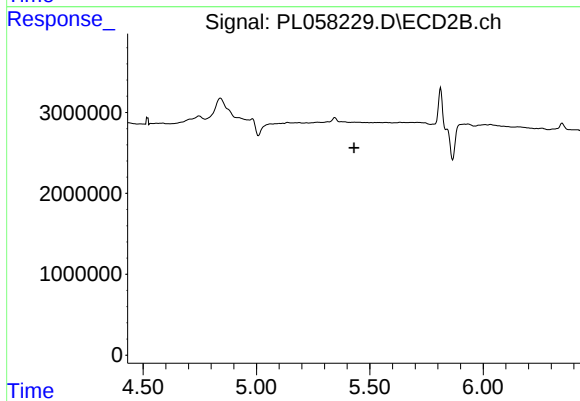

#5 Aldrin


R.T.: 0.000 min
Exp R.T. : 5.431 min
Response: 0
Conc: N.D.

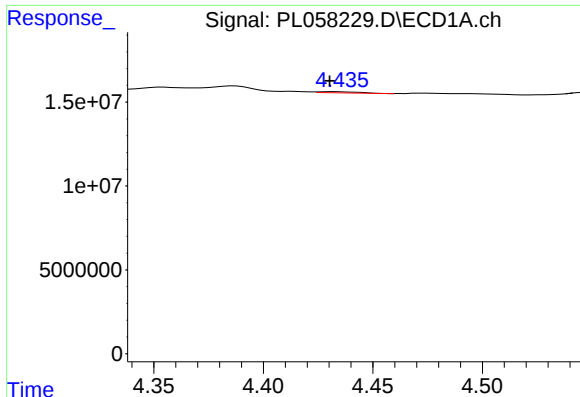

#6 beta-BHC


R.T.: 4.433 min
Delta R.T.: 0.003 min
Response: 925362
Conc: 0.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

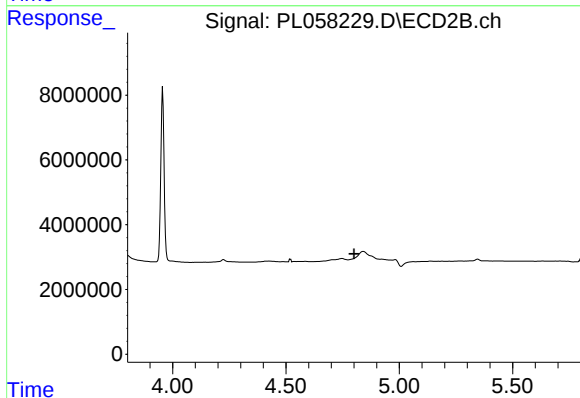


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.800 min
Response: 0
Conc: N.D.

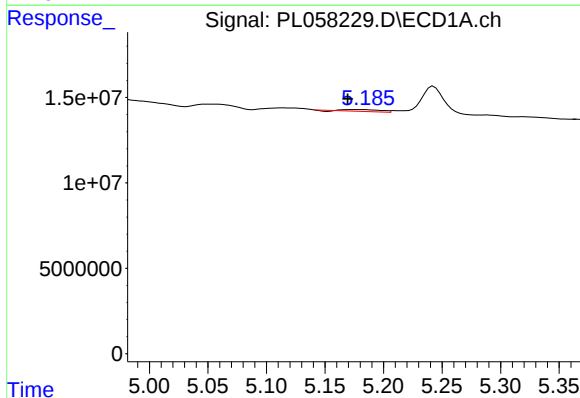


#8 Heptachlor epoxide

R.T.: 5.175 min
Delta R.T.: 0.005 min
Response: 2279217
Conc: 0.17 ng/ml

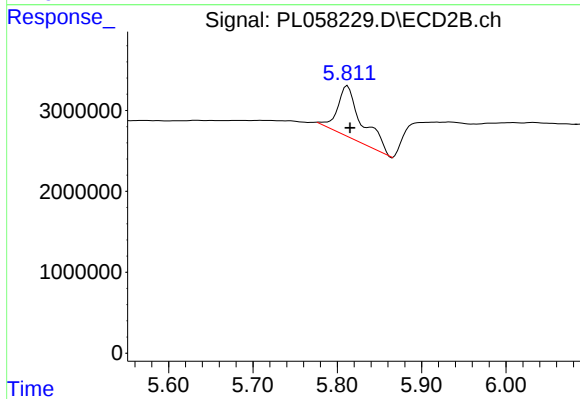

#8 Heptachlor epoxide


R.T.: 5.812 min
Delta R.T.: -0.003 min
Response: 12883021
Conc: 4.77 ng/ml

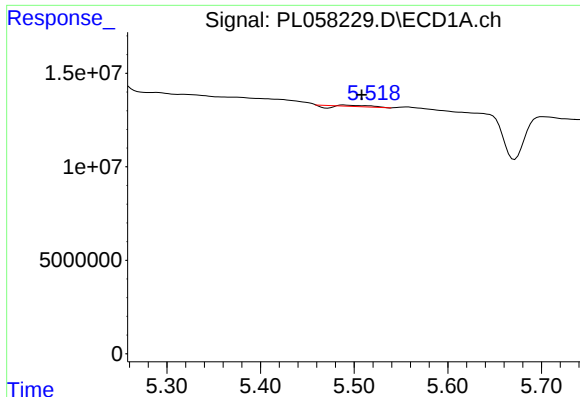

#9 Endosulfan I


R.T.: 5.489 min
Delta R.T.: -0.019 min
Response: 853068
Conc: 0.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

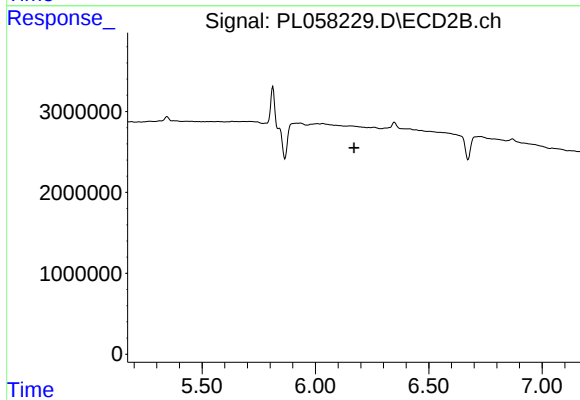


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.170 min
Response: 0
Conc: N.D.

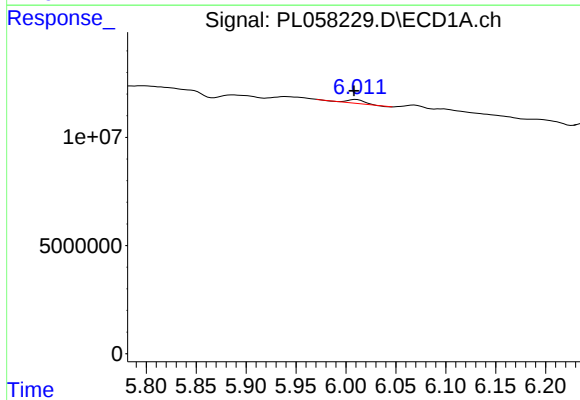


#14 Endrin

R.T.: 6.010 min
Delta R.T.: 0.002 min
Response: 2349103
Conc: 0.20 ng/ml

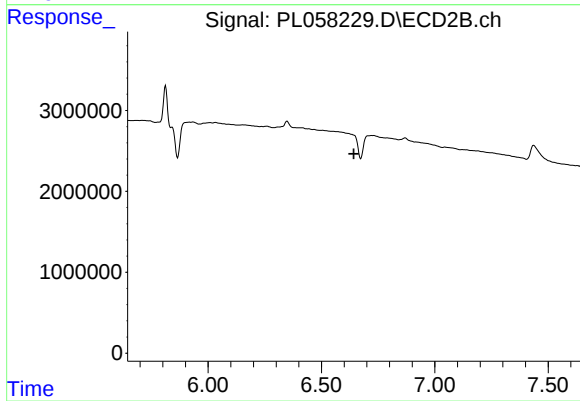

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.642 min
Response: 0
Conc: N.D.

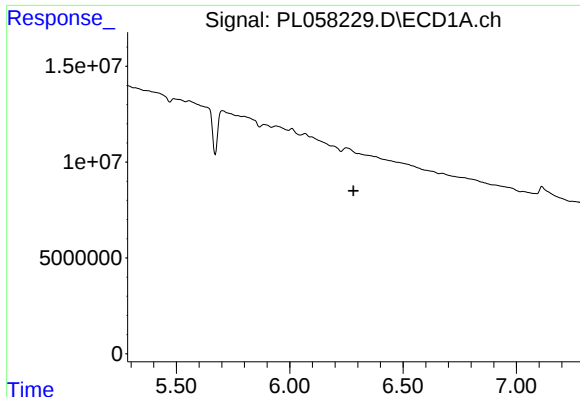

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.282 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

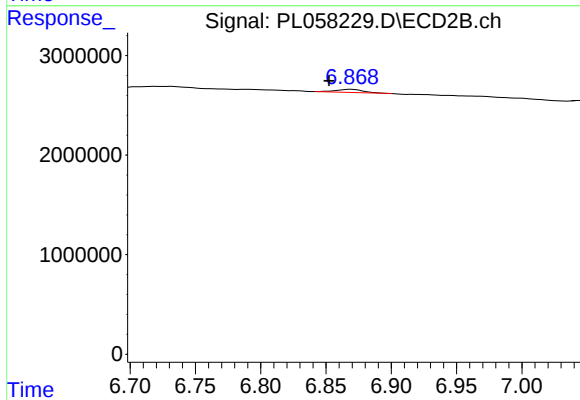


#15 Endosulfan II

R.T.: 6.869 min
Delta R.T.: 0.017 min
Response: 436702
Conc: 0.17 ng/ml

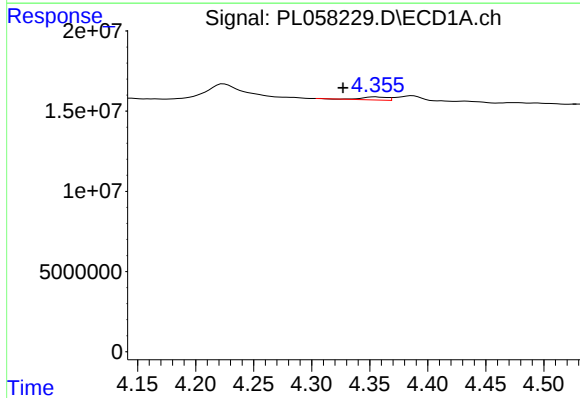


#23 Chlordane-1

R.T.: 4.355 min
Delta R.T.: 0.028 min
Response: 3027596
Conc: 8.19 ng/ml

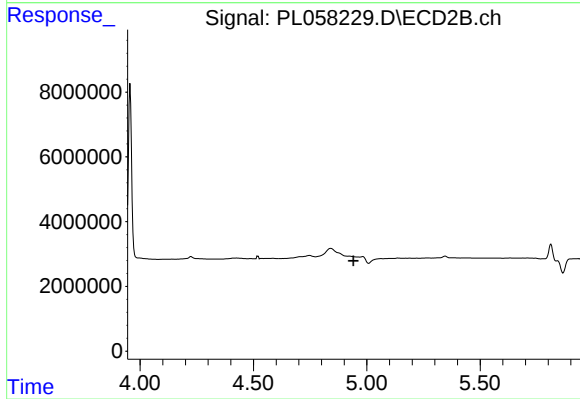

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.942 min
Response: 0
Conc: N.D.

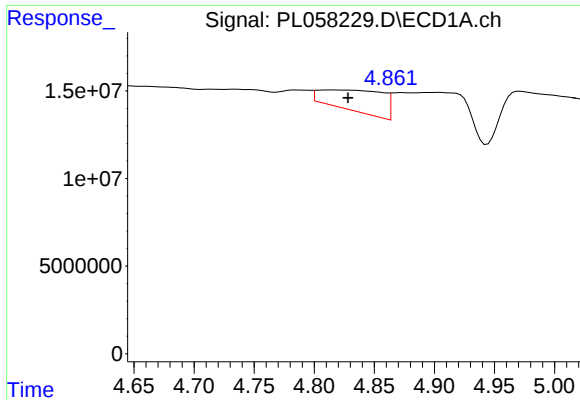

#24 Chlordane-2


R.T.: 4.812 min
Delta R.T.: -0.016 min
Response: 42683106
Conc: 105.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

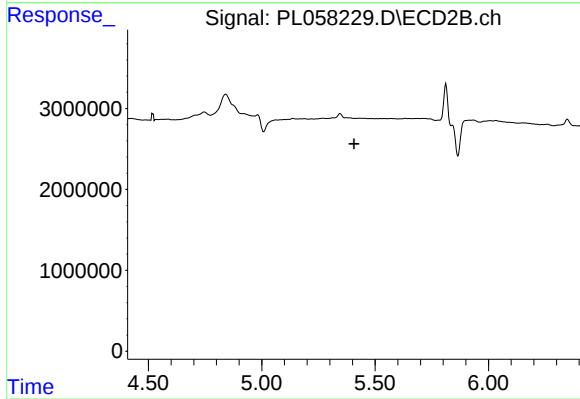


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 5.407 min
Response: 0
Conc: N.D.

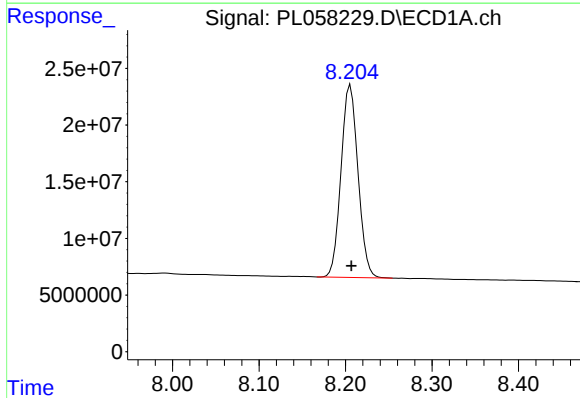

#28 Decachlorobiphenyl

R.T.: 8.206 min
Delta R.T.: -0.001 min
Response: 230227466
Conc: 22.33 ng/ml

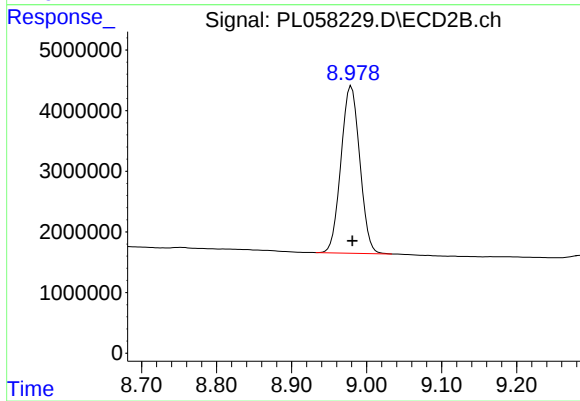

#28 Decachlorobiphenyl

R.T.: 8.980 min
Delta R.T.: -0.001 min
Response: 48016783
Conc: 21.50 ng/ml