

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL042020\  
 Data File : PL058221.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 21 Apr 2020 01:41  
 Operator : AJ\MA  
 Sample : L2327-21  
 Misc :  
 ALS Vial : 45 Sample Multiplier: 1

Instrument :  
 ECD\_L  
 ClientSampleId :  
 TP-3-S

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 21 05:11:19 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL040320.M  
 Quant Title : GC Extractables  
 QLast Update : Sat Apr 04 06:41:11 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

|                             | Compound        | RT#1  | RT#2  | Resp#1  | Resp#2   | ng/ml  | ng/ml  |
|-----------------------------|-----------------|-------|-------|---------|----------|--------|--------|
| -----                       |                 |       |       |         |          |        |        |
| System Monitoring Compounds |                 |       |       |         |          |        |        |
| 1)                          | SA Tetrachlo... | 3.457 | 3.956 | 226.5E6 | 50106946 | 22.467 | 23.089 |
| 28)                         | SA Decachlor... | 8.205 | 8.979 | 223.1E6 | 46117548 | 21.639 | 20.646 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL042020\  
Data File : PL058221.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 21 Apr 2020 01:41  
Operator : AJ\MA  
Sample : L2327-21  
Misc :  
ALS Vial : 45 Sample Multiplier: 1

Instrument :  
ECD\_L  
ClientSampleId :  
TP-3-S

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Apr 21 05:11:19 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL040320.M  
Quant Title : GC Extractables  
QLast Update : Sat Apr 04 06:41:11 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

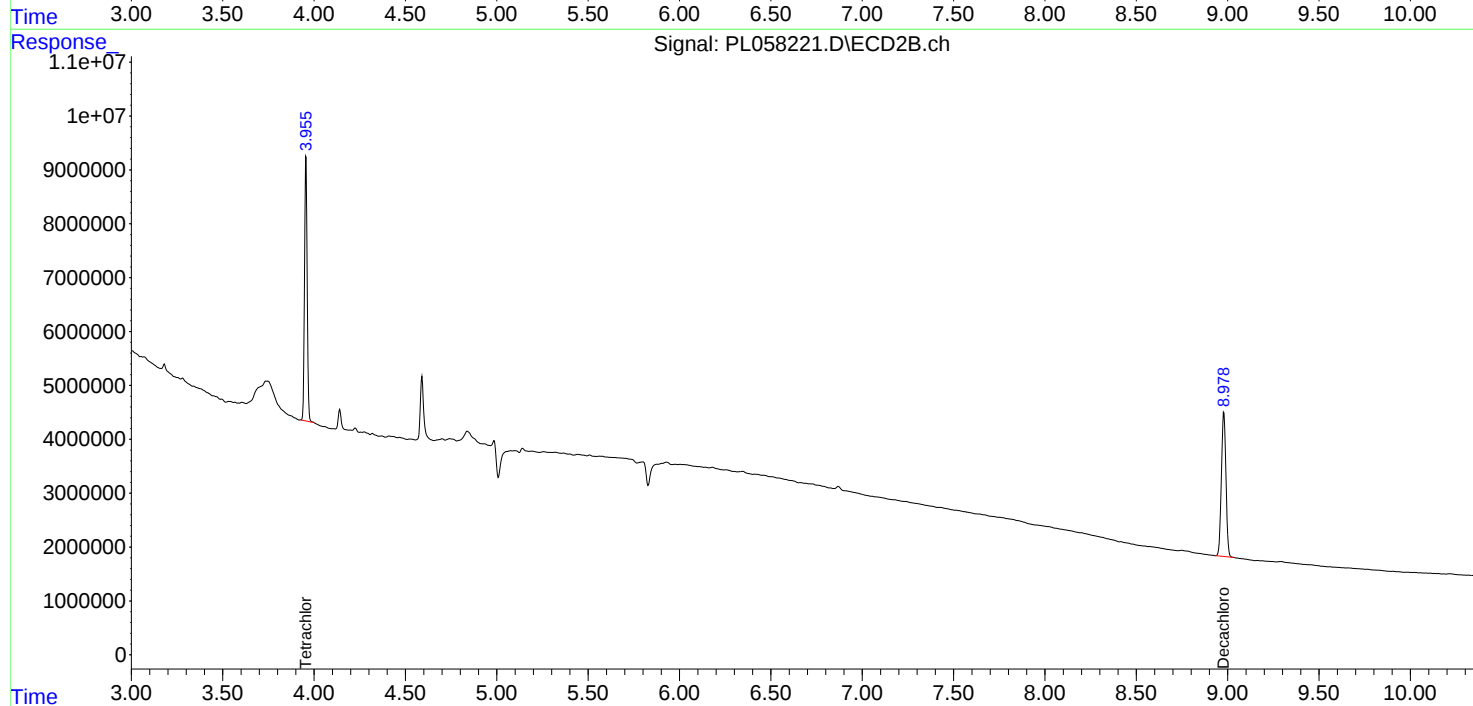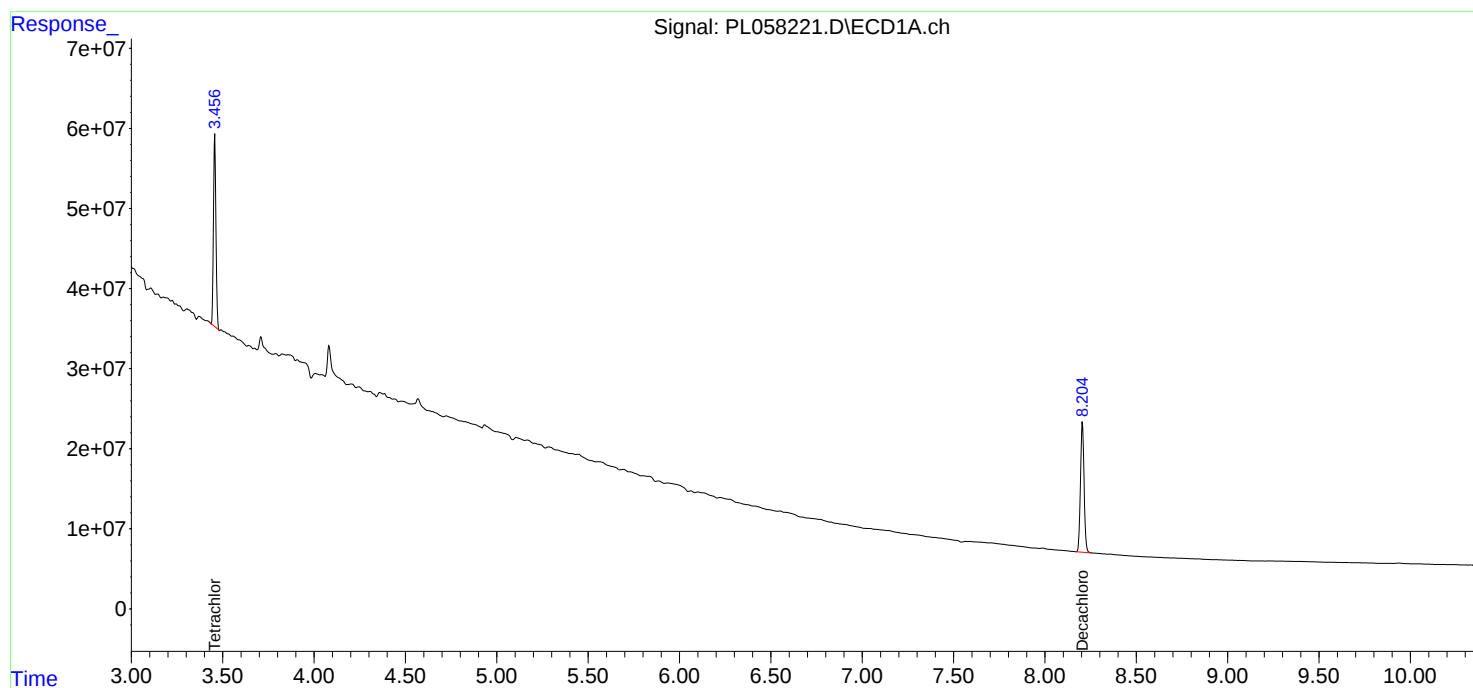


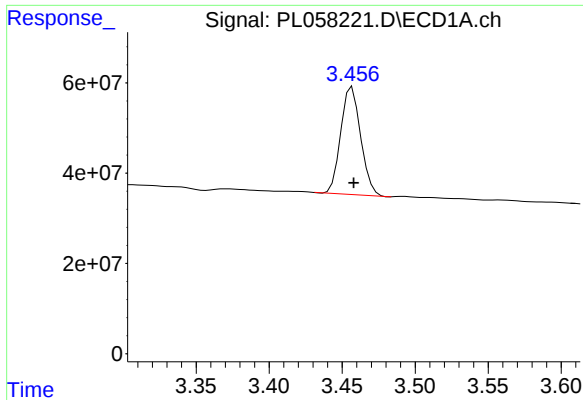

#1 Tetrachloro-m-xylene


R.T.: 3.457 min  
Delta R.T.: -0.001 min  
Response: 226492426  
Conc: 22.47 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :  
TP-3-S

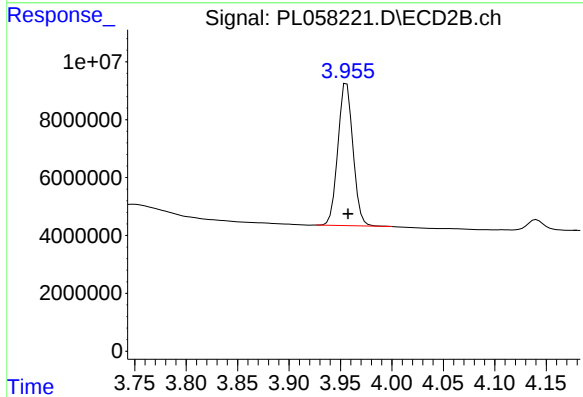


#1 Tetrachloro-m-xylene

R.T.: 3.956 min  
Delta R.T.: -0.001 min  
Response: 50106946  
Conc: 23.09 ng/ml

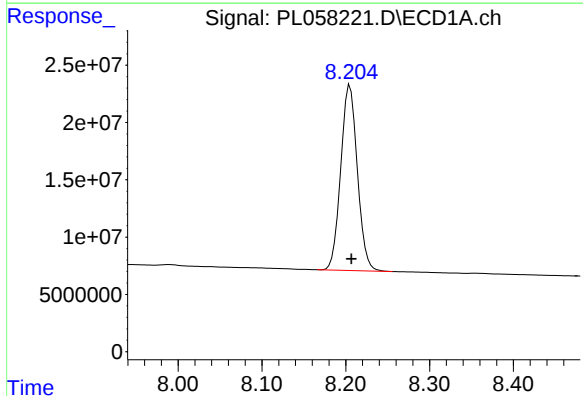

#28 Decachlorobiphenyl

R.T.: 8.205 min  
Delta R.T.: -0.002 min  
Response: 223066533  
Conc: 21.64 ng/ml

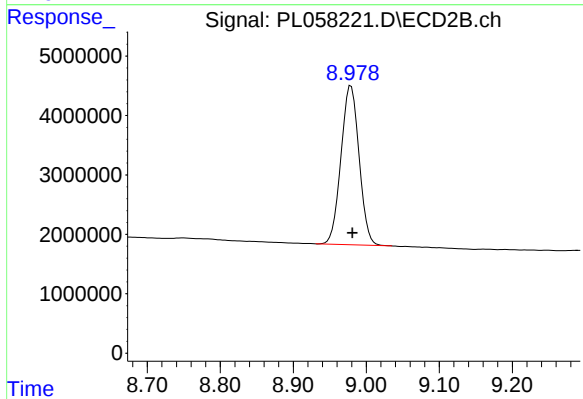

#28 Decachlorobiphenyl

R.T.: 8.979 min  
Delta R.T.: -0.002 min  
Response: 46117548  
Conc: 20.65 ng/ml