

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042020\
 Data File : PL058227.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Apr 2020 03:06
 Operator : AJ\MA
 Sample : L2340-03
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RECLAIM-SYSTEM-SEDIMENT-PIT

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 05:12:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.456	3.956	173.2E6	42928292	17.180	19.781
28)	SA Decachlor...	8.205	8.979	152.5E6	32598304	14.793	14.593

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042020\
Data File : PL058227.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Apr 2020 03:06
Operator : AJ\MA
Sample : L2340-03
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RECLAIM-SYSTEM-SEDIMENT-PIT

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 05:12:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

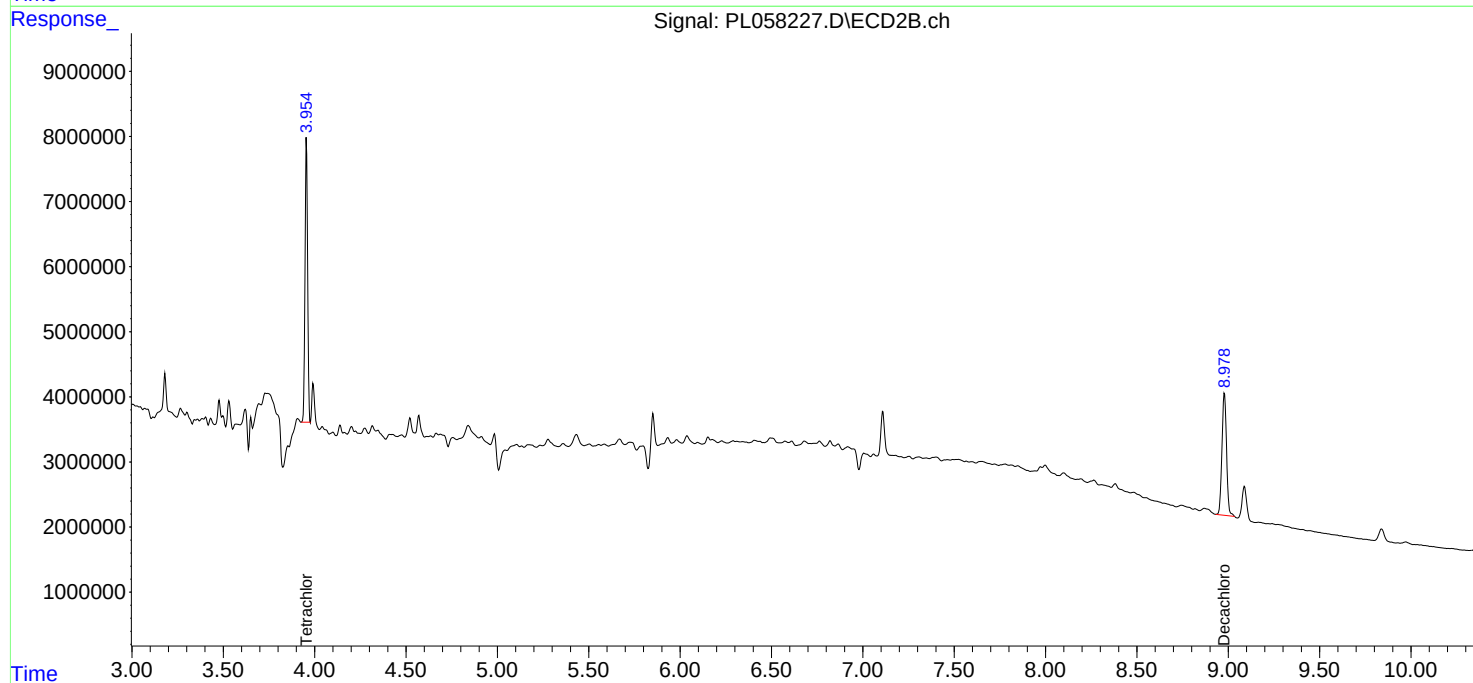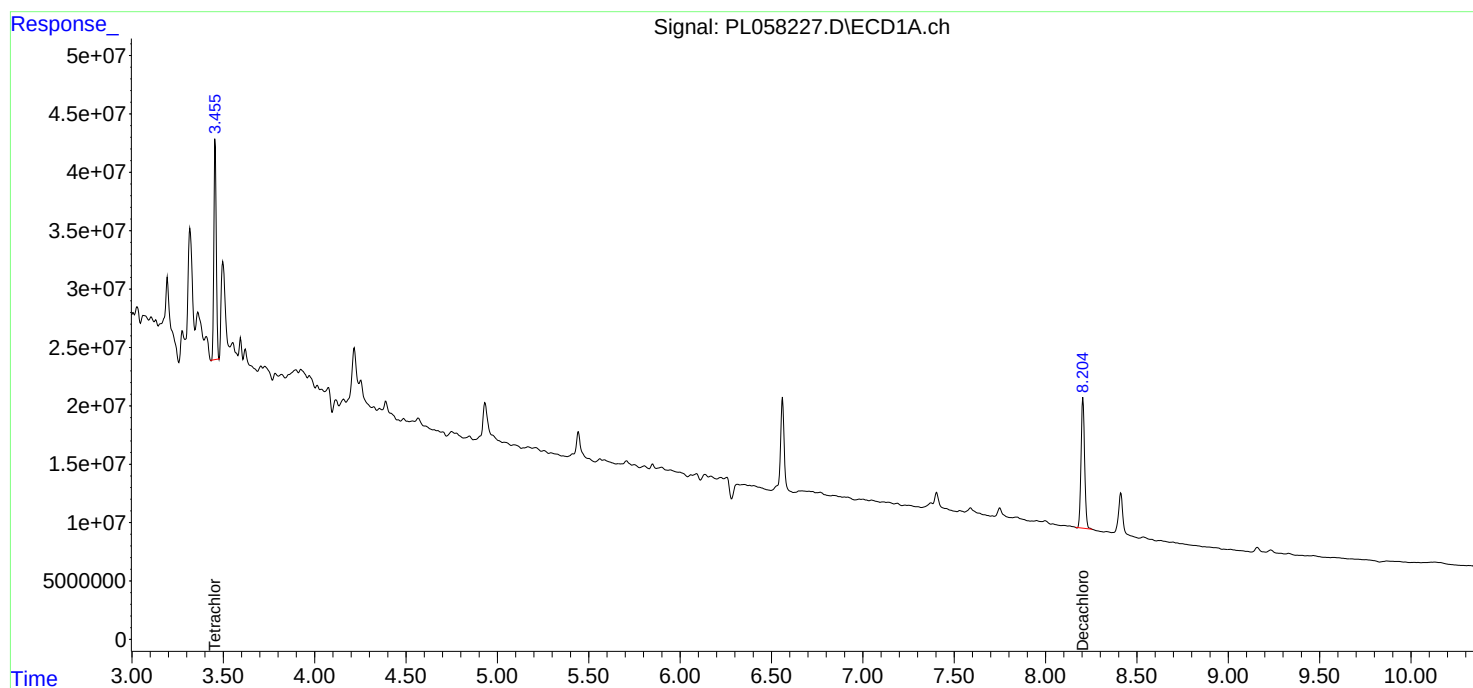


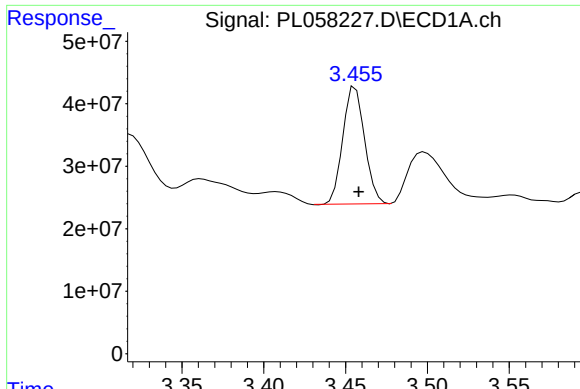

#1 Tetrachloro-m-xylene


R.T.: 3.456 min
Delta R.T.: -0.002 min
Response: 173190506
Conc: 17.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
RECLAIM-SYSTEM-SEDIMENT-PIT

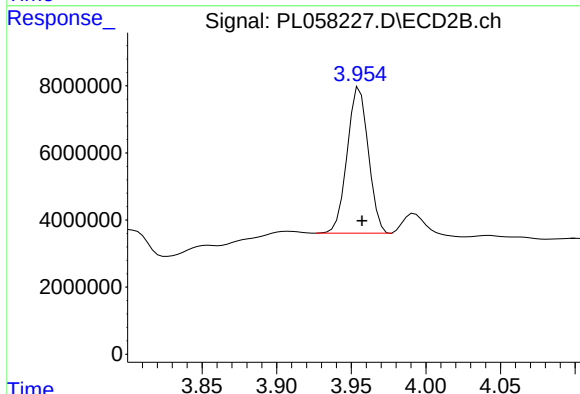


#1 Tetrachloro-m-xylene

R.T.: 3.956 min
Delta R.T.: -0.002 min
Response: 42928292
Conc: 19.78 ng/ml

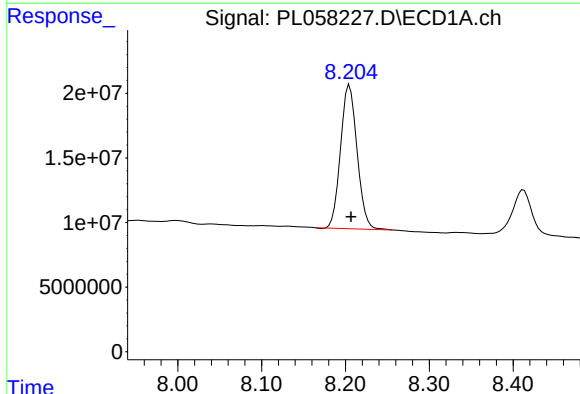

#28 Decachlorobiphenyl

R.T.: 8.205 min
Delta R.T.: -0.002 min
Response: 152493629
Conc: 14.79 ng/ml

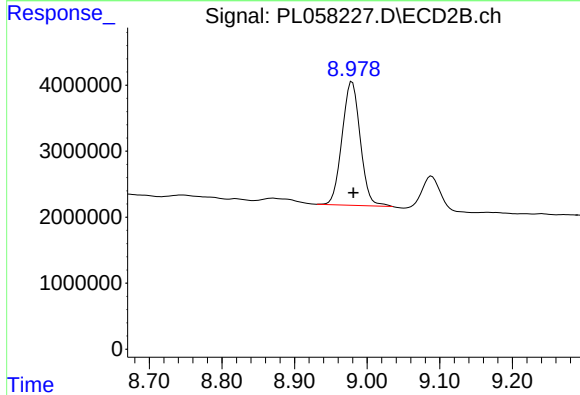

#28 Decachlorobiphenyl

R.T.: 8.979 min
Delta R.T.: -0.002 min
Response: 32598304
Conc: 14.59 ng/ml