

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042021\
 Data File : PL066334.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2021 09:14
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 08:13:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 15:37:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	4.153	48664738	78659541	19.120	19.555
28)	SA Decachlor...	8.166	9.351	49560942	64872093	20.778	19.863
Target Compounds							
4)	MA Heptachlor	0.000	5.350f	0	3307036	N.D.	0.594 #
5)	MB Aldrin	0.000	5.667	0	50367	N.D.	0.010 #
6)	B beta-BHC	4.419	5.033	1580499	11624534	0.897	0.256 #
15)	B Endosulfa...	0.000	7.127	0	2055501	N.D.	0.590 #
17)	MA 4,4'-DDT	0.000	7.340	0	1105618	N.D.	0.326 #
21)	B Endrin ke...	0.000	7.972	0	1265632	N.D.	0.344 #
23)	Chlordane-1	4.326f	0.000	2845821	0	24.893	N.D. #
24)	Chlordane-2	0.000	5.667f	0	50367	N.D.	0.286 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042021\
Data File : PL066334.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2021 09:14
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 08:13:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 15:37:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

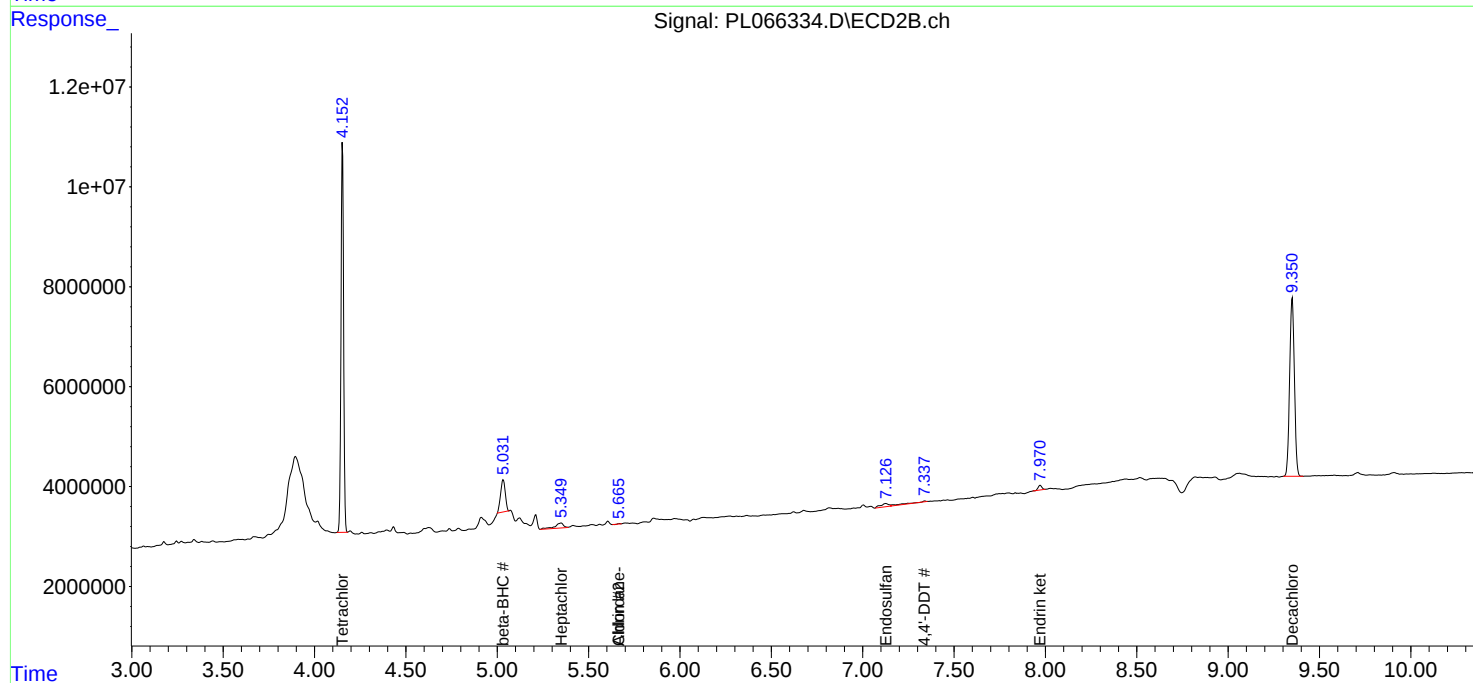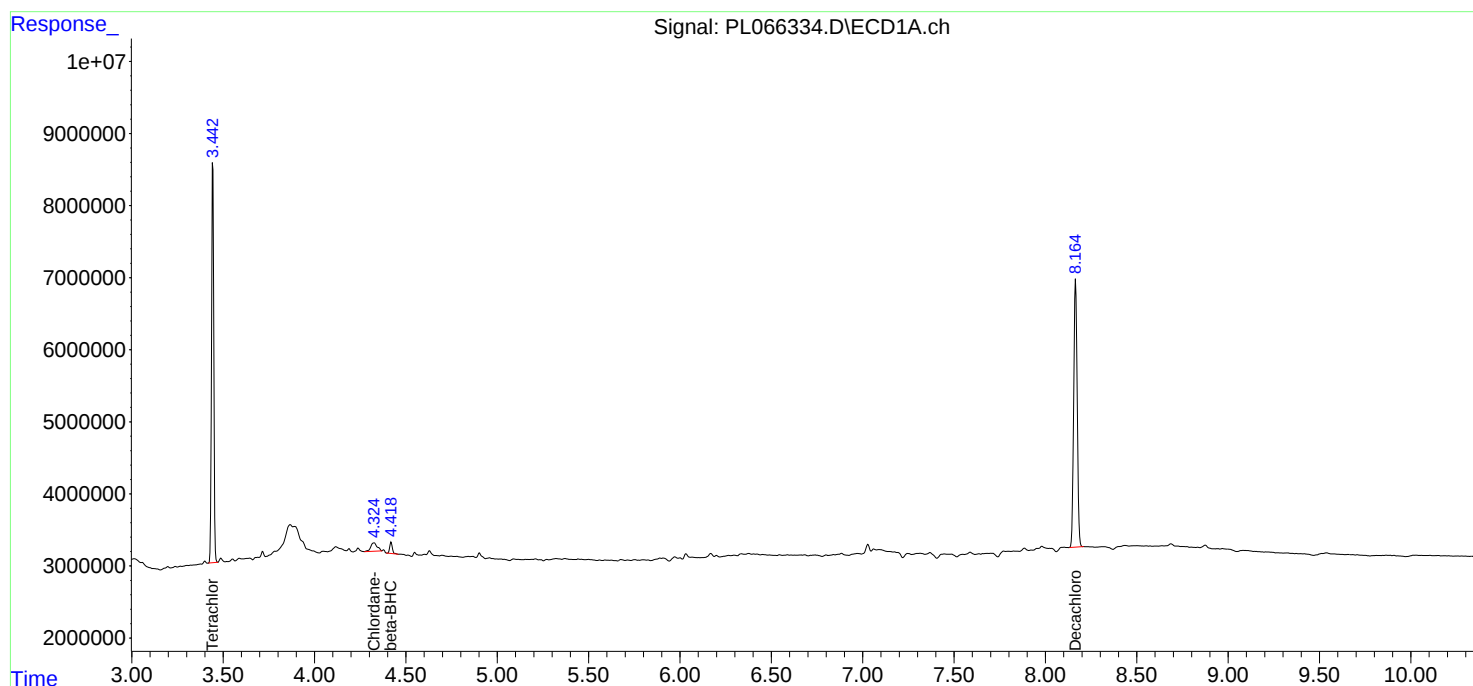


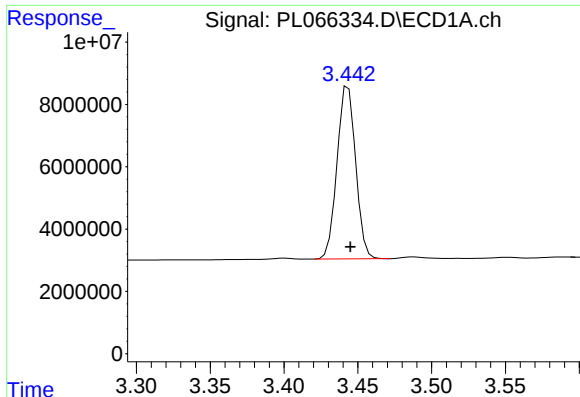

#1 Tetrachloro-m-xylene


R.T.: 3.444 min
Delta R.T.: -0.001 min
Response: 48664738
Conc: 19.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

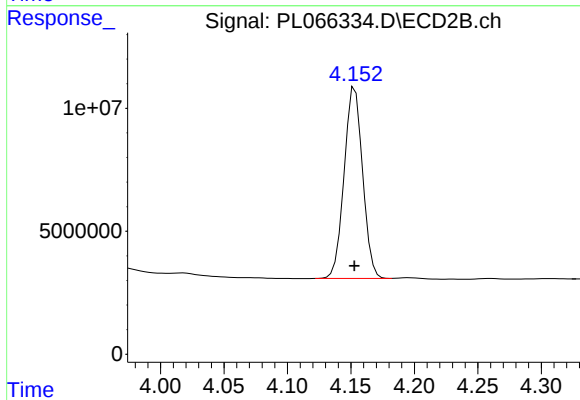


#1 Tetrachloro-m-xylene

R.T.: 4.153 min
Delta R.T.: 0.000 min
Response: 78659541
Conc: 19.55 ng/ml

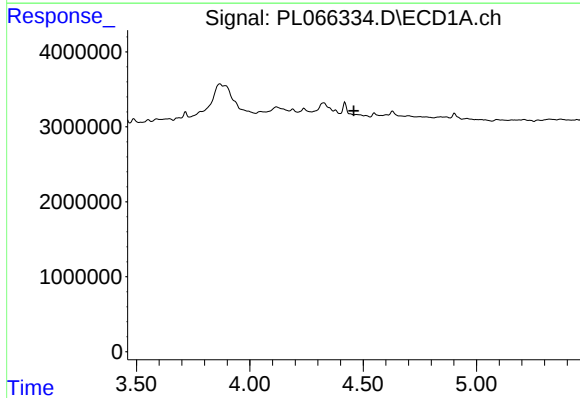


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.459 min
Response: 0
Conc: N.D.

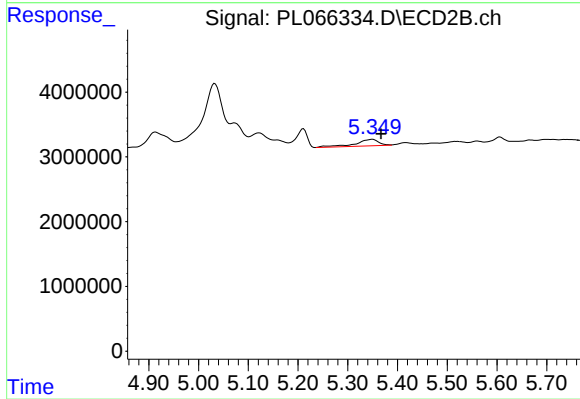

#4 Heptachlor


R.T.: 5.350 min
Delta R.T.: -0.017 min
Response: 3307036
Conc: 0.59 ng/ml

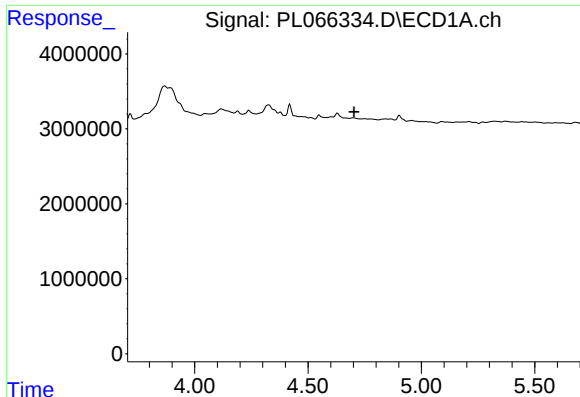

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 4.704 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

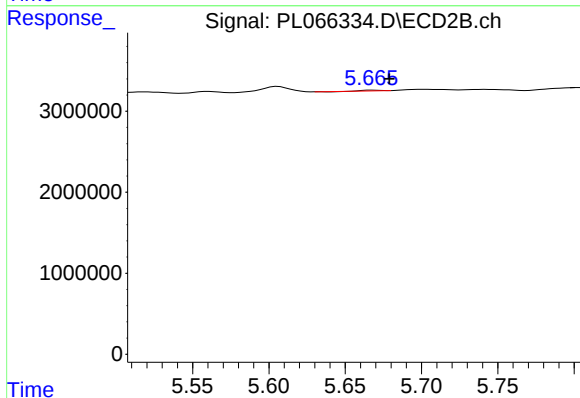


#5 Aldrin

R.T.: 5.667 min
Delta R.T.: -0.012 min
Response: 50367
Conc: 0.01 ng/ml

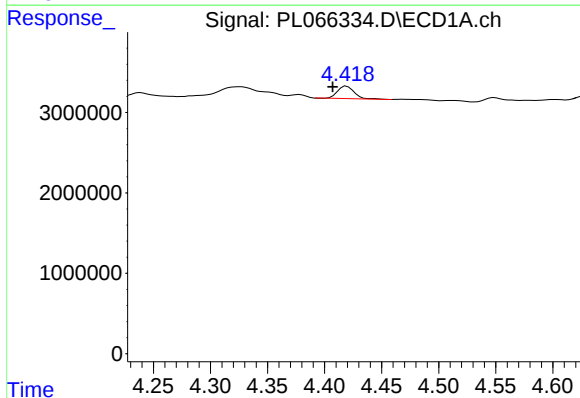


#6 beta-BHC

R.T.: 4.419 min
Delta R.T.: 0.012 min
Response: 1580499
Conc: 0.90 ng/ml

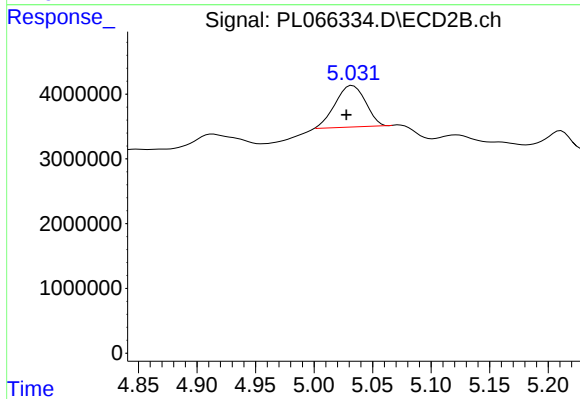

#6 beta-BHC


R.T.: 5.033 min
Delta R.T.: 0.005 min
Response: 11624534
Conc: 0.26 ng/ml

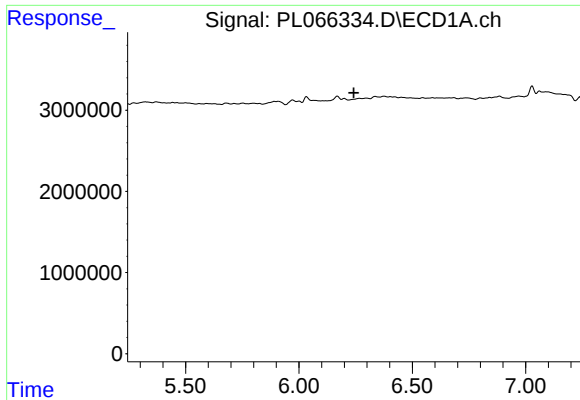

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.242 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

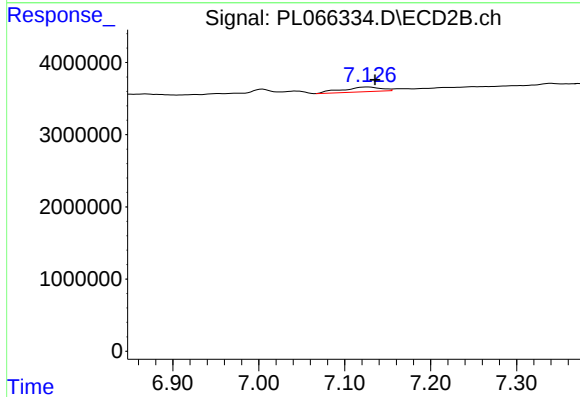


#15 Endosulfan II

R.T.: 7.127 min
Delta R.T.: -0.008 min
Response: 2055501
Conc: 0.59 ng/ml

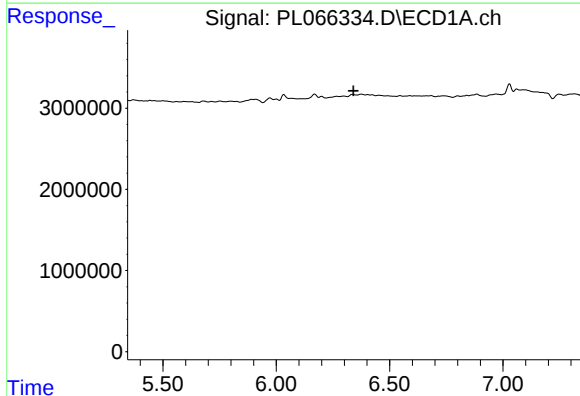


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.341 min
Response: 0
Conc: N.D.

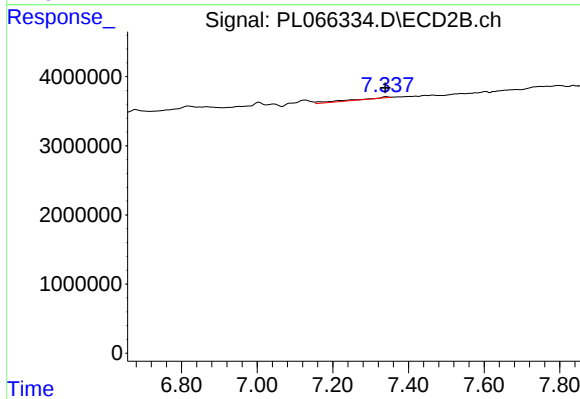

#17 4,4'-DDT


R.T.: 7.340 min
Delta R.T.: 0.000 min
Response: 1105618
Conc: 0.33 ng/ml

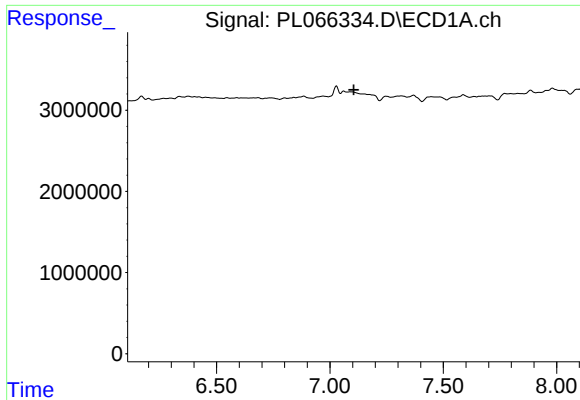

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.105 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

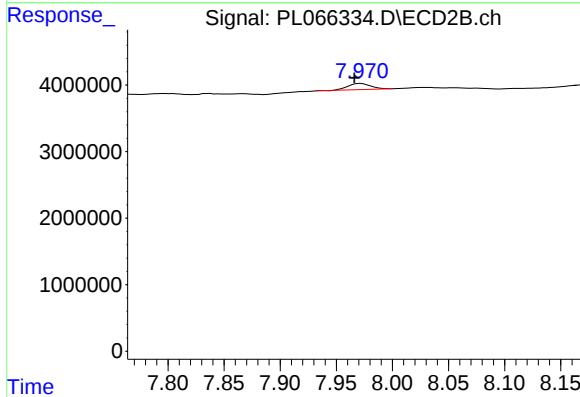


#21 Endrin ketone

R.T.: 7.972 min
Delta R.T.: 0.005 min
Response: 1265632
Conc: 0.34 ng/ml

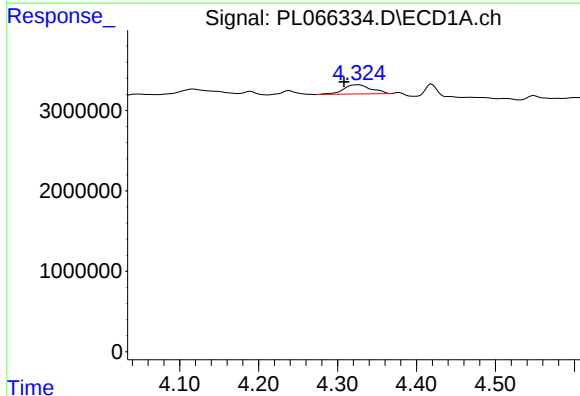


#23 Chlordane-1

R.T.: 4.326 min
Delta R.T.: 0.018 min
Response: 2845821
Conc: 24.89 ng/ml

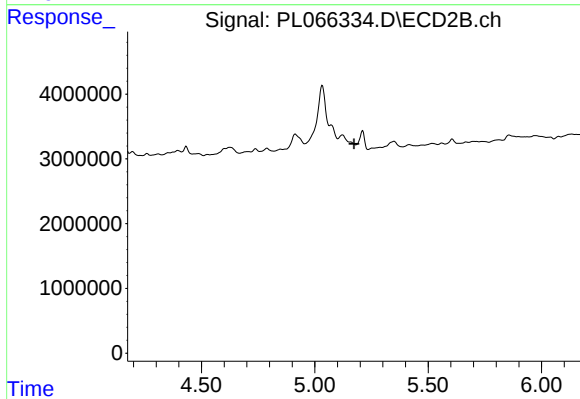

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.173 min
Response: 0
Conc: N.D.

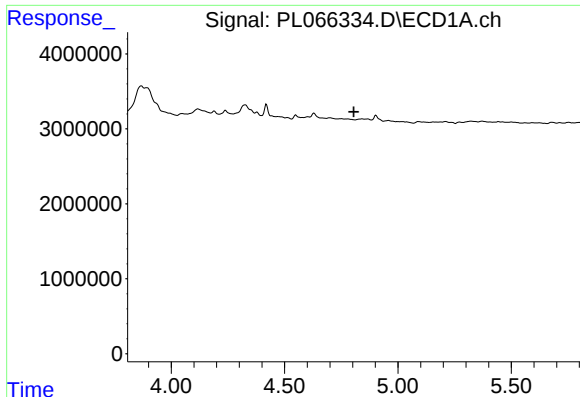

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.805 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

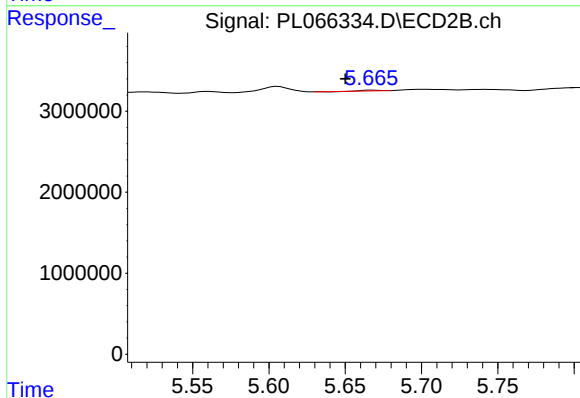


#24 Chlordane-2

R.T.: 5.667 min
Delta R.T.: 0.017 min
Response: 50367
Conc: 0.29 ng/ml

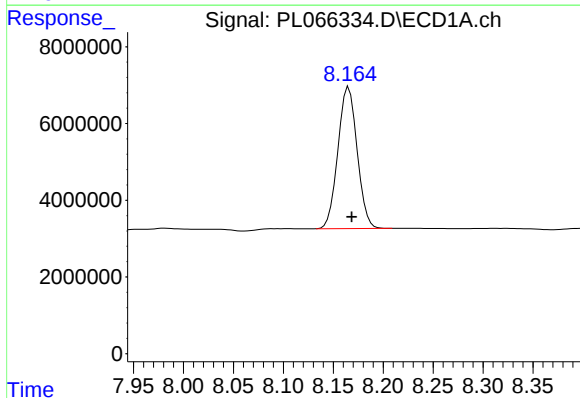

#28 Decachlorobiphenyl

R.T.: 8.166 min
Delta R.T.: -0.003 min
Response: 49560942
Conc: 20.78 ng/ml

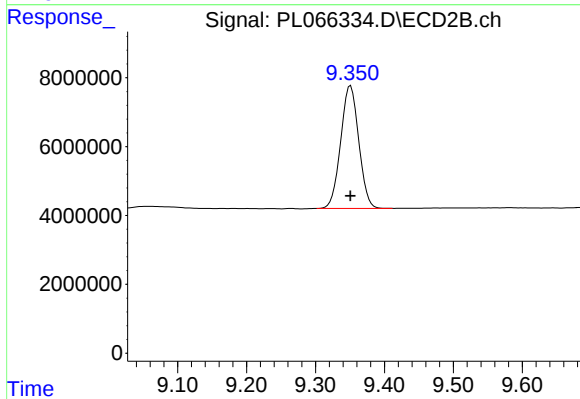

#28 Decachlorobiphenyl

R.T.: 9.351 min
Delta R.T.: 0.000 min
Response: 64872093
Conc: 19.86 ng/ml