

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042021\
 Data File : PL066347.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2021 13:04
 Operator : AR\AJ
 Sample : PB135862BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 08:15:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 15:37:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	4.153	46706256	76715825	18.350	19.071
28)	SA Decachlor...	8.165	9.351	48276858	63764655	20.240	19.524
Target Compounds							
3)	MA gamma-BHC...	4.156	0.000	4659862	0	1.196	N.D. #
4)	MA Heptachlor	0.000	5.351f	0	2334886	N.D.	0.419 #
5)	MB Aldrin	0.000	5.667	0	68190	N.D.	0.014 #
15)	B Endosulfa...	0.000	7.122	0	4674778	N.D.	1.341 #
17)	MA 4,4'-DDT	0.000	7.355f	0	1848181	N.D.	0.545 #
18)	B Endrin al...	0.000	7.256	0	3574232	N.D.	1.278 #
21)	B Endrin ke...	0.000	7.973	0	1652939	N.D.	0.449 #
23)	Chlordane-1	4.336f	0.000	4429880	0	38.750	N.D. #
24)	Chlordane-2	0.000	5.667f	0	68190	N.D.	0.388 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042021\
Data File : PL066347.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2021 13:04
Operator : AR\AJ
Sample : PB135862BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 08:15:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 15:37:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

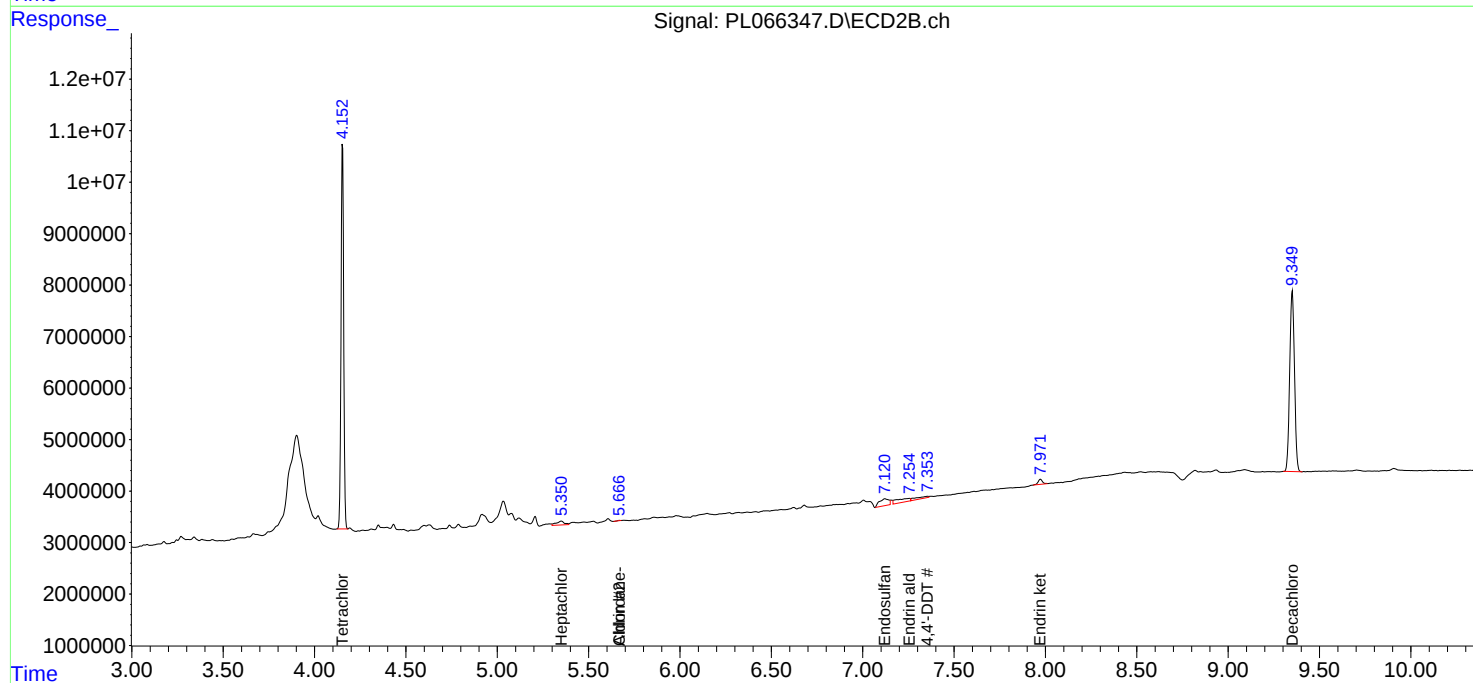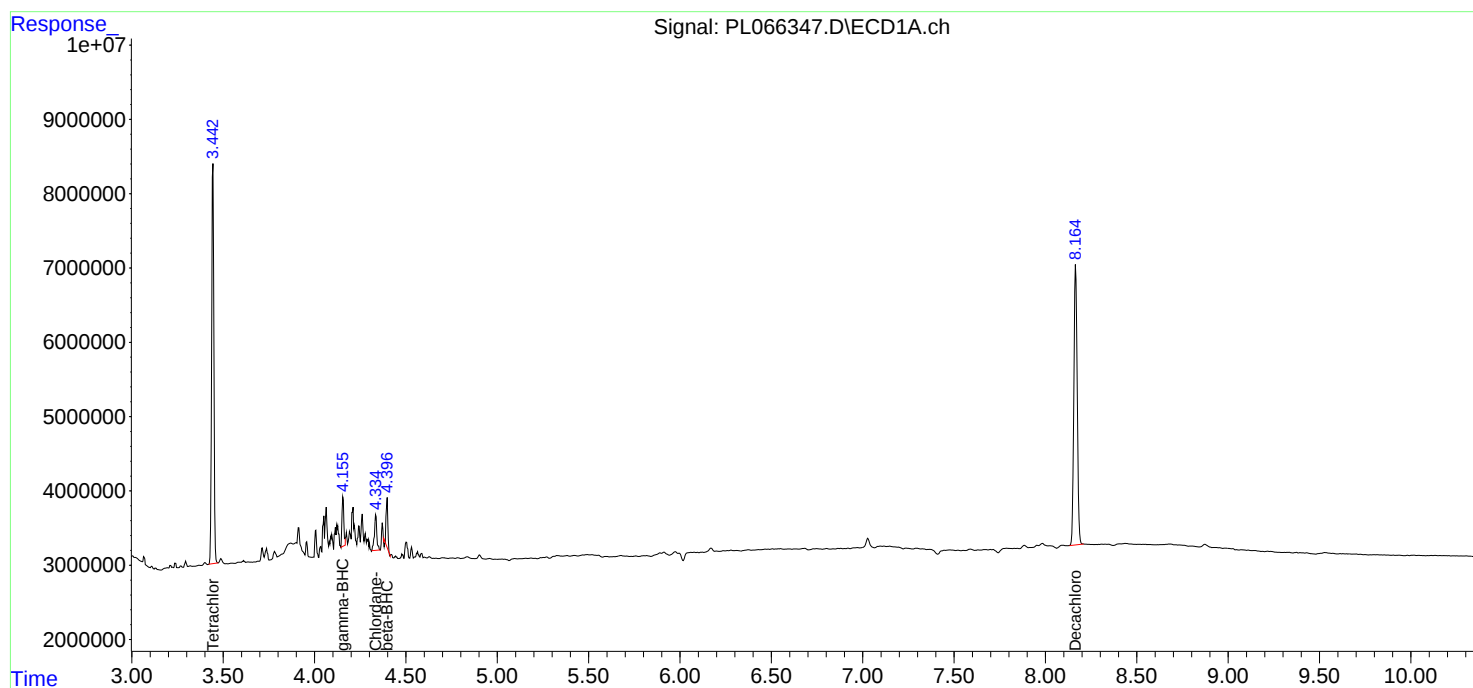


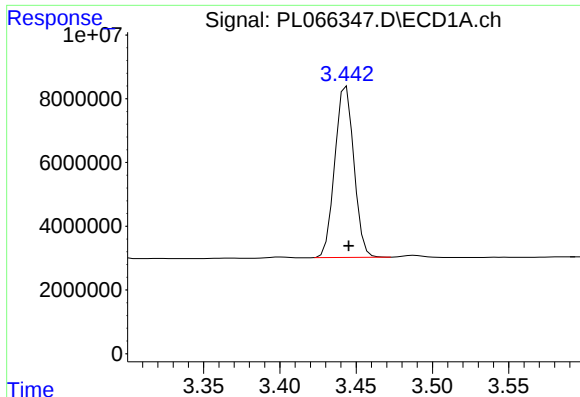

#1 Tetrachloro-m-xylene


R.T.: 3.444 min
Delta R.T.: -0.001 min
Response: 46706256
Conc: 18.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

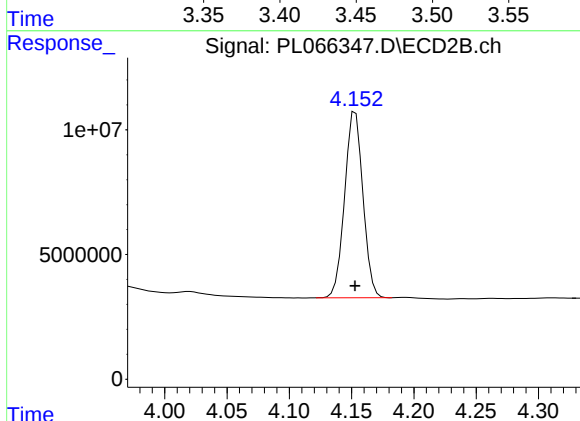


#1 Tetrachloro-m-xylene

R.T.: 4.153 min
Delta R.T.: 0.000 min
Response: 76715825
Conc: 19.07 ng/ml

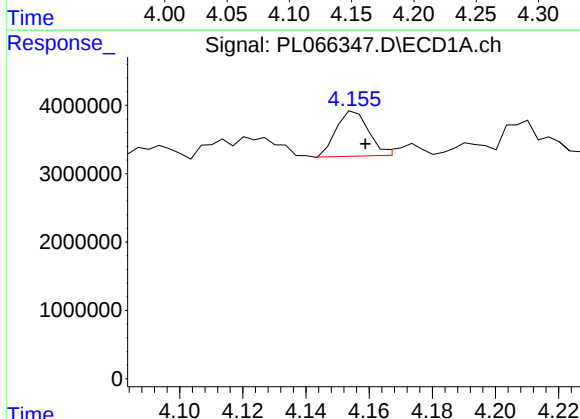


#3 gamma-BHC (Lindane)

R.T.: 4.156 min
Delta R.T.: -0.003 min
Response: 4659862
Conc: 1.20 ng/ml

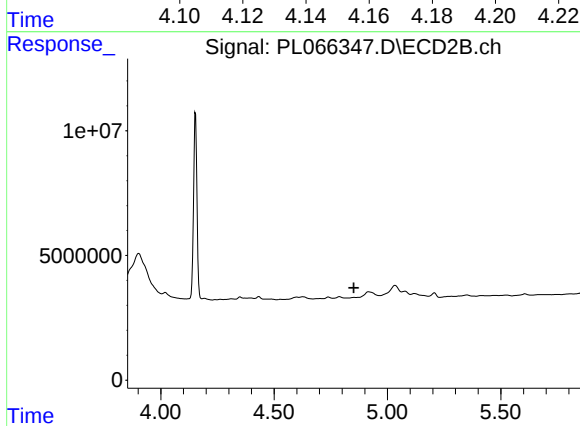

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.851 min
Response: 0
Conc: N.D.

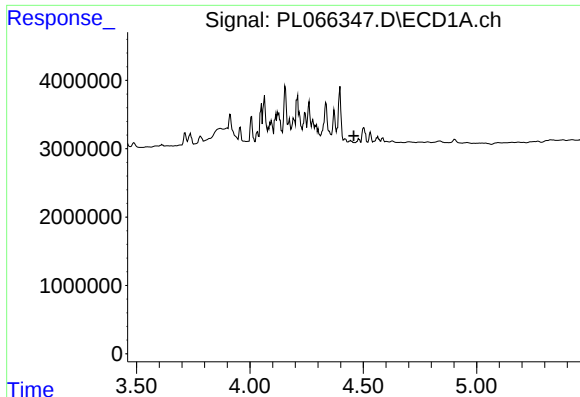

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.459 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

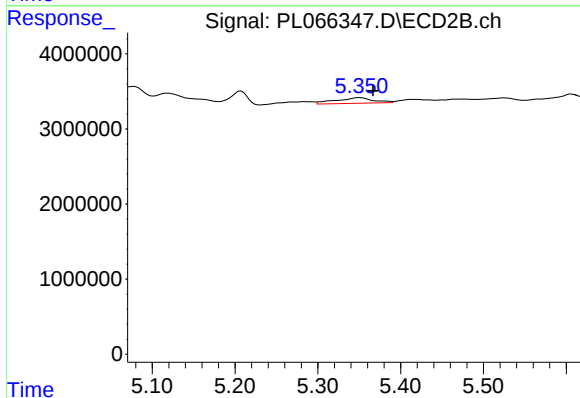


#4 Heptachlor

R.T.: 5.351 min
Delta R.T.: -0.016 min
Response: 2334886
Conc: 0.42 ng/ml

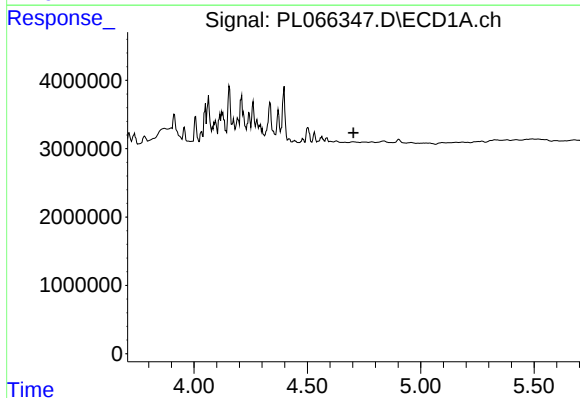


#5 Aldrin

R.T.: 0.000 min
Exp R.T.: 4.704 min
Response: 0
Conc: N.D.

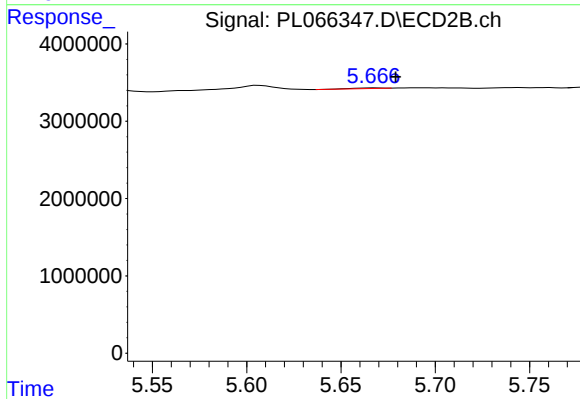

#5 Aldrin


R.T.: 5.667 min
Delta R.T.: -0.012 min
Response: 68190
Conc: 0.01 ng/ml

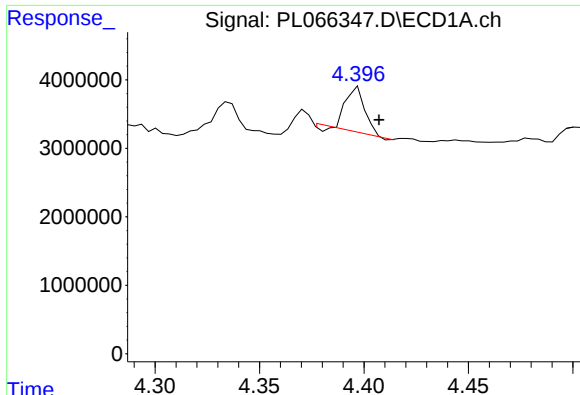

#6 beta-BHC


R.T.: 4.397 min
Delta R.T.: -0.010 min
Response: 4085304
Conc: 2.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

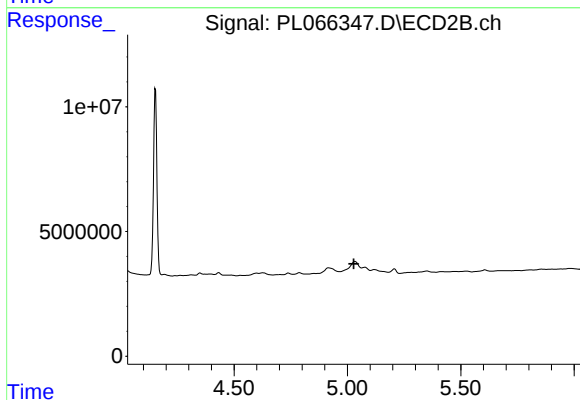


#6 beta-BHC

R.T.: 5.033 min
Delta R.T.: 0.006 min
Response: 5364909
Conc: N.D.

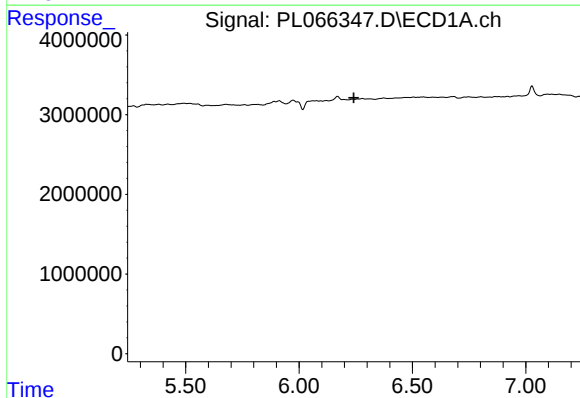


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.242 min
Response: 0
Conc: N.D.

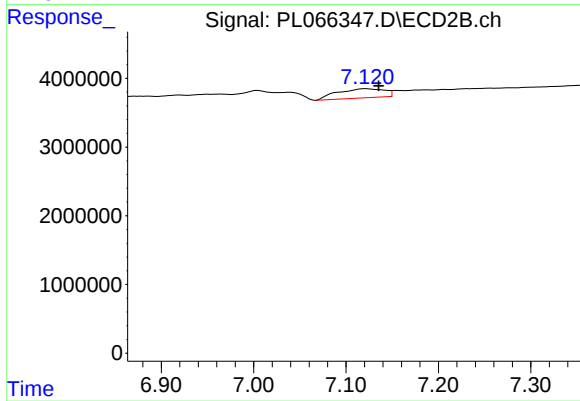

#15 Endosulfan II


R.T.: 7.122 min
Delta R.T.: -0.014 min
Response: 4674778
Conc: 1.34 ng/ml

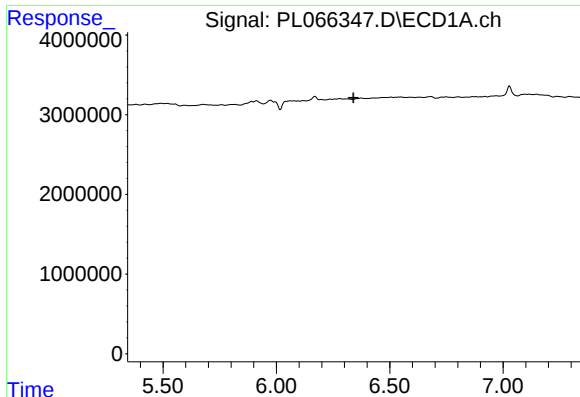

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.341 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

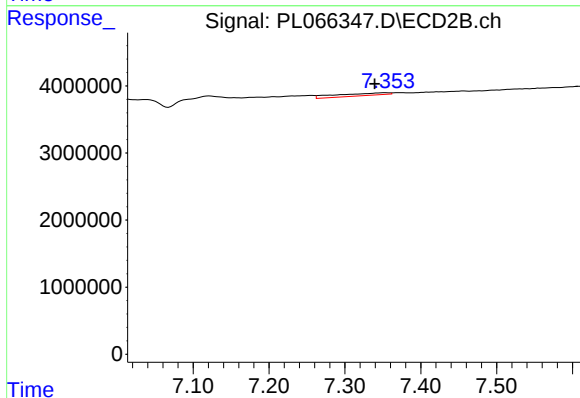


#17 4,4'-DDT

R.T.: 7.355 min
Delta R.T.: 0.016 min
Response: 1848181
Conc: 0.54 ng/ml

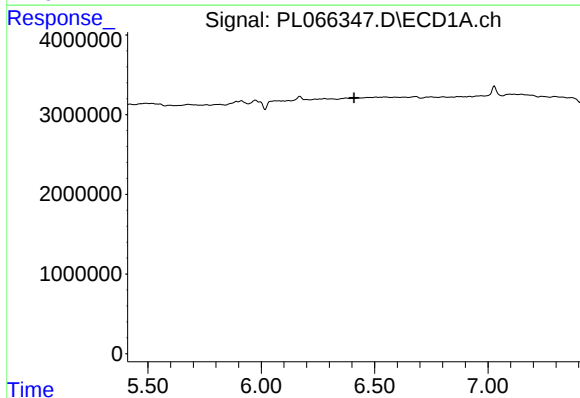


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.409 min
Response: 0
Conc: N.D.

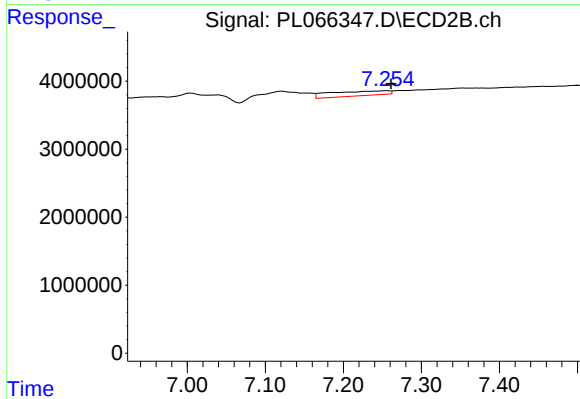

#18 Endrin aldehyde


R.T.: 7.256 min
Delta R.T.: -0.005 min
Response: 3574232
Conc: 1.28 ng/ml

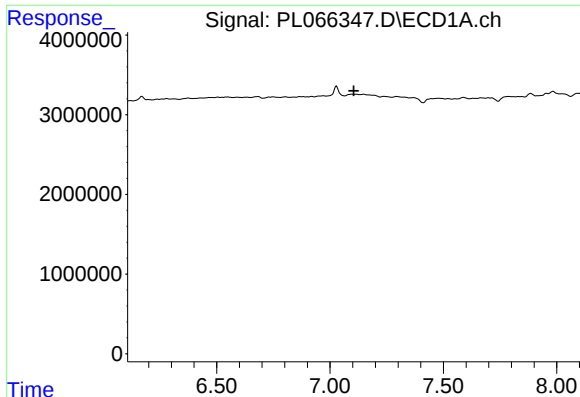

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.105 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

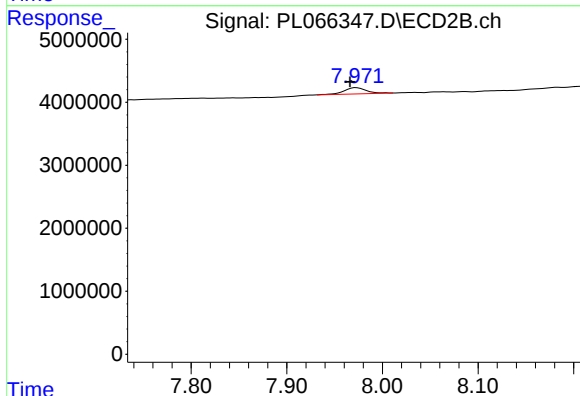


#21 Endrin ketone

R.T.: 7.973 min
Delta R.T.: 0.007 min
Response: 1652939
Conc: 0.45 ng/ml

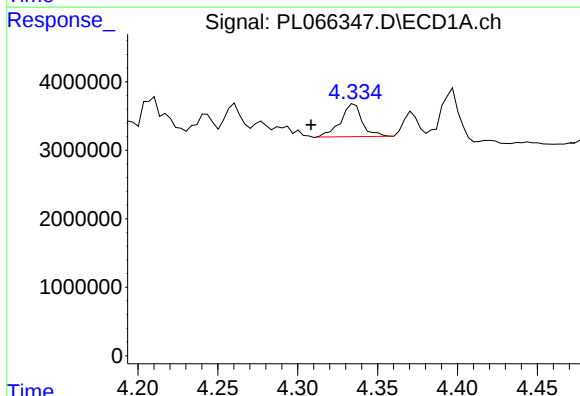


#23 Chlordane-1

R.T.: 4.336 min
Delta R.T.: 0.027 min
Response: 4429880
Conc: 38.75 ng/ml

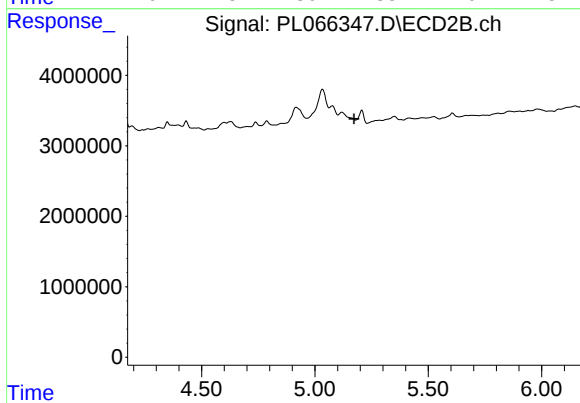

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.173 min
Response: 0
Conc: N.D.

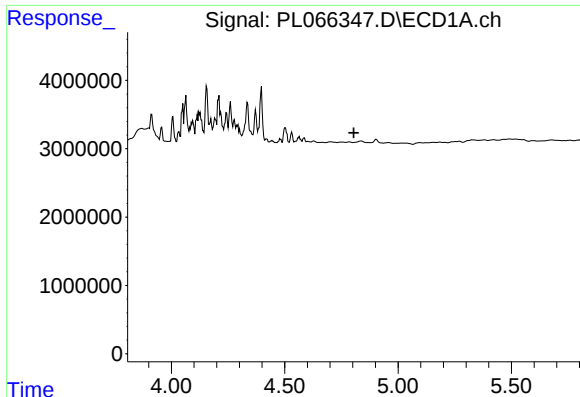

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.805 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

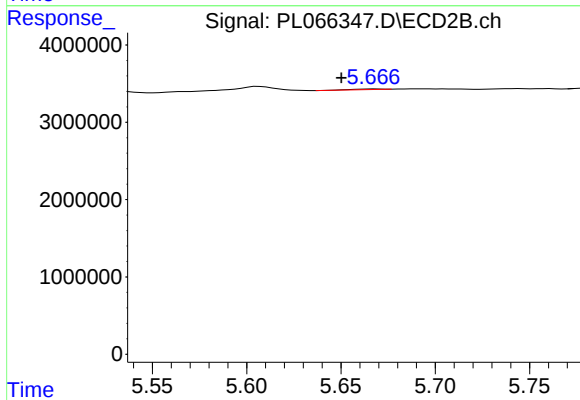


#24 Chlordane-2

R.T.: 5.667 min
Delta R.T.: 0.017 min
Response: 68190
Conc: 0.39 ng/ml

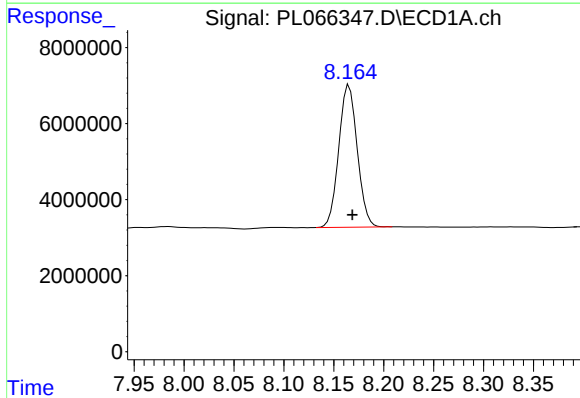

#28 Decachlorobiphenyl

R.T.: 8.165 min
Delta R.T.: -0.003 min
Response: 48276858
Conc: 20.24 ng/ml

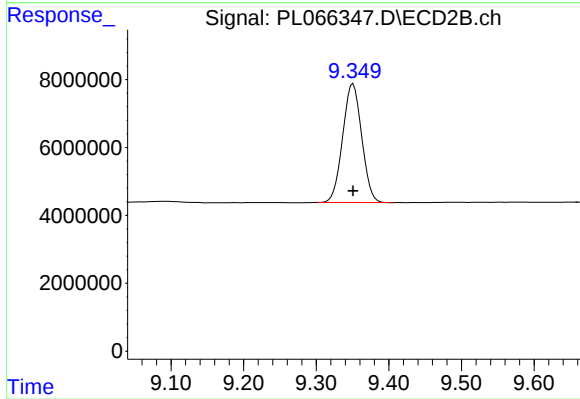

#28 Decachlorobiphenyl

R.T.: 9.351 min
Delta R.T.: 0.000 min
Response: 63764655
Conc: 19.52 ng/ml