

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042021\
 Data File : PL066363.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2021 17:47
 Operator : AR\AJ
 Sample : M2070-06
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 08:17:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 15:37:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	4.154	51048335	85324645	20.056	21.211
28)	SA Decachlor...	8.167	9.352	44526983	59098793	18.667	18.096
Target Compounds							
2)	A alpha-BHC	3.864f	0.000	1889886	0	0.459	N.D. #
4)	MA Heptachlor	0.000	5.353	0	1403091	N.D.	0.252 #
10)	B gamma-Chl...	0.000	6.315	0	421941	N.D.	0.092 #
15)	B Endosulfa...	0.000	7.122	0	1345524	N.D.	0.386 #
17)	MA 4,4'-DDT	0.000	7.342	0	1013834	N.D.	0.299 #
18)	B Endrin al...	0.000	7.257	0	724448	N.D.	0.259 #
21)	B Endrin ke...	0.000	7.973	0	1200783	N.D.	0.326 #
23)	Chlordane-1	4.334f	0.000	3777802	0	33.046	N.D. #
25)	Chlordane-3	0.000	6.315	0	421941	N.D.	0.642 #
27)	Chlordane-5	0.000	7.217	0	1220877	N.D.	9.109 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042021\
Data File : PL066363.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2021 17:47
Operator : AR\AJ
Sample : M2070-06
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 08:17:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 15:37:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

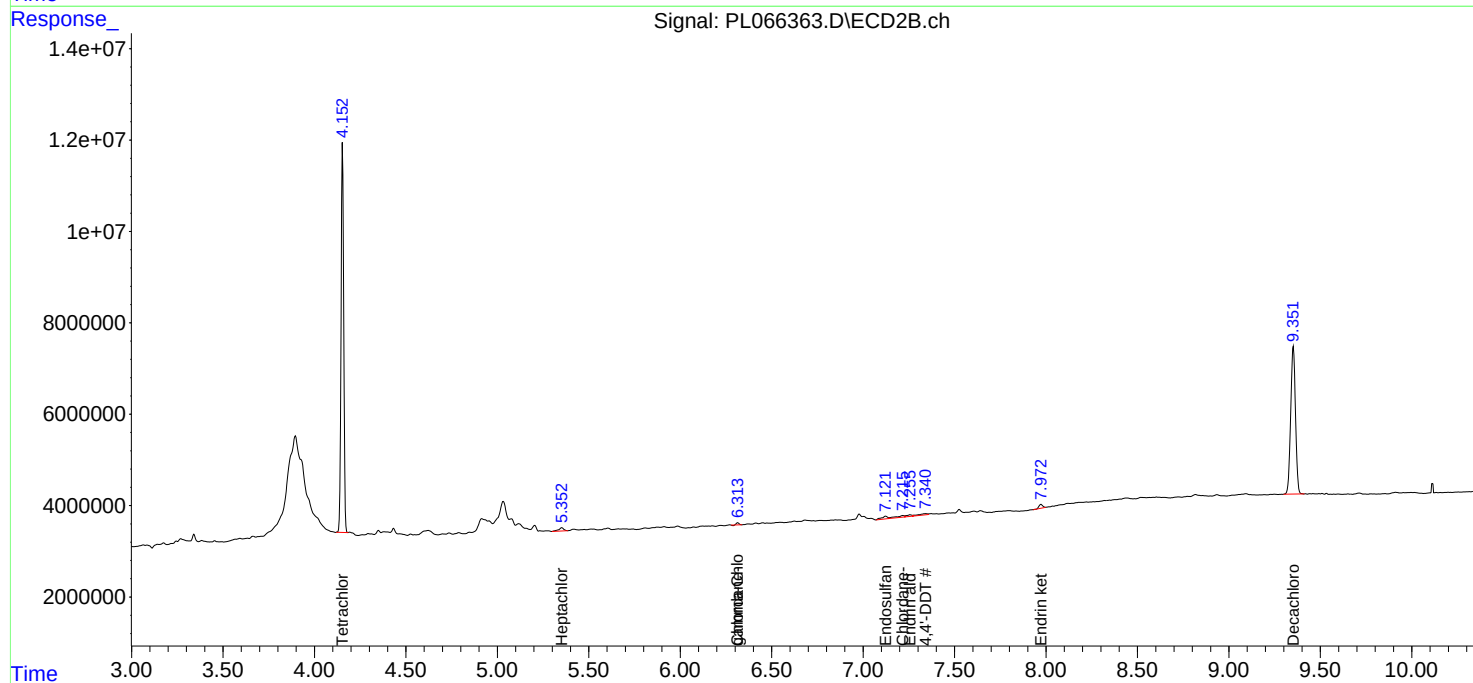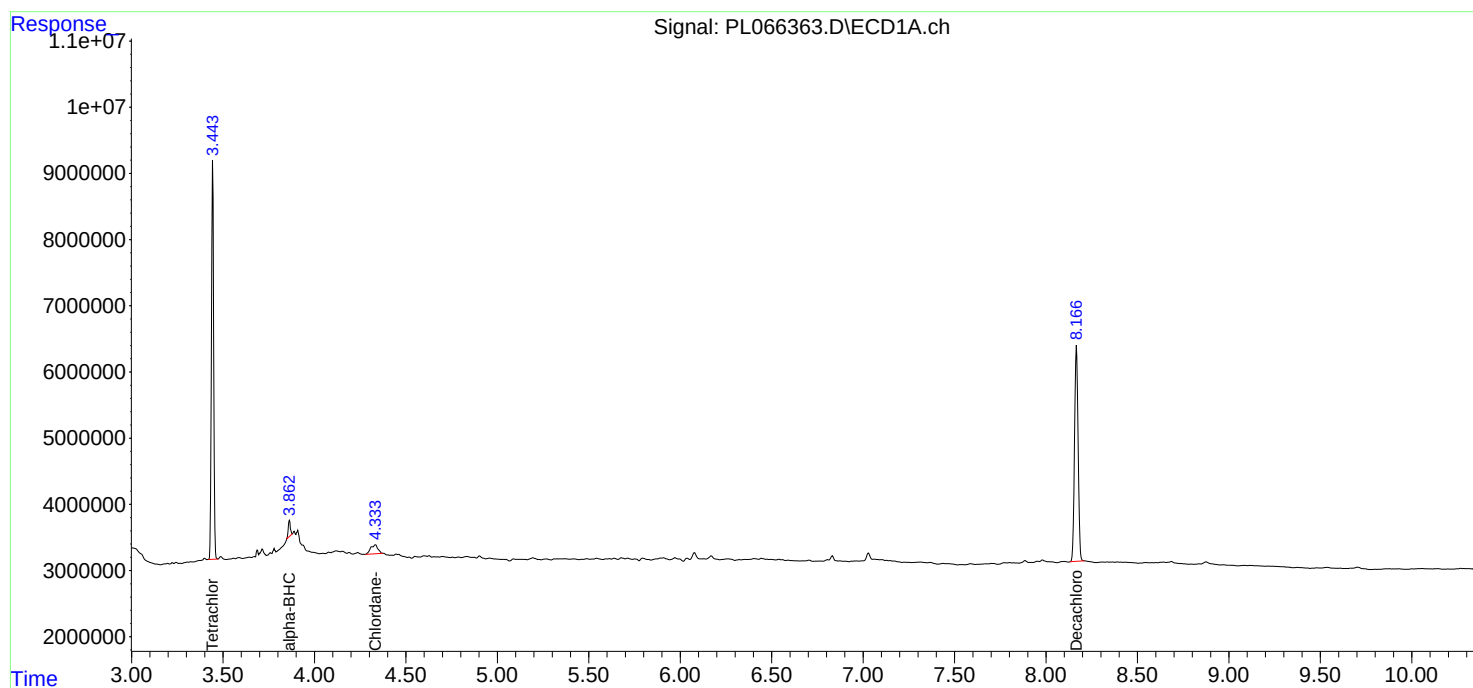


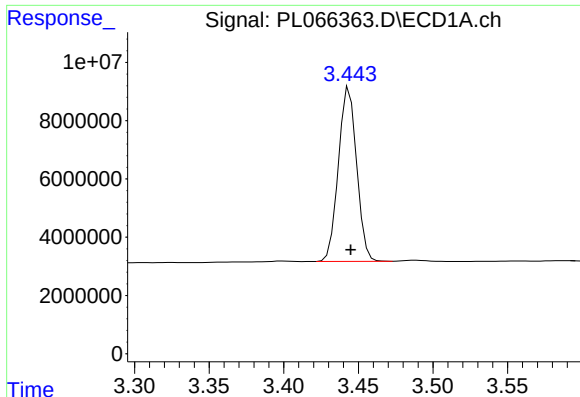

#1 Tetrachloro-m-xylene


R.T.: 3.444 min
Delta R.T.: 0.000 min
Response: 51048335
Conc: 20.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

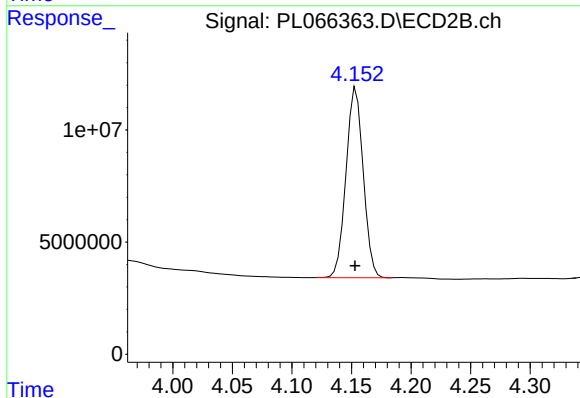


#1 Tetrachloro-m-xylene

R.T.: 4.154 min
Delta R.T.: 0.001 min
Response: 85324645
Conc: 21.21 ng/ml

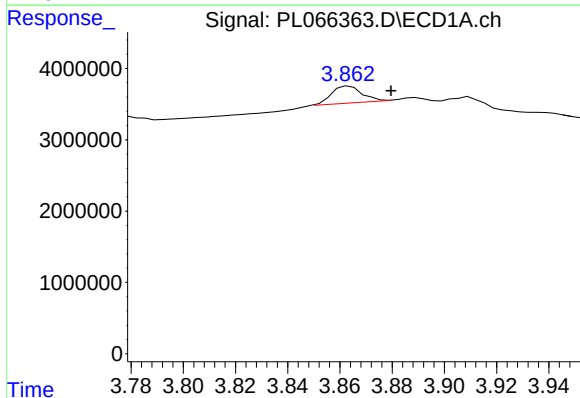


#2 alpha-BHC

R.T.: 3.864 min
Delta R.T.: -0.016 min
Response: 1889886
Conc: 0.46 ng/ml

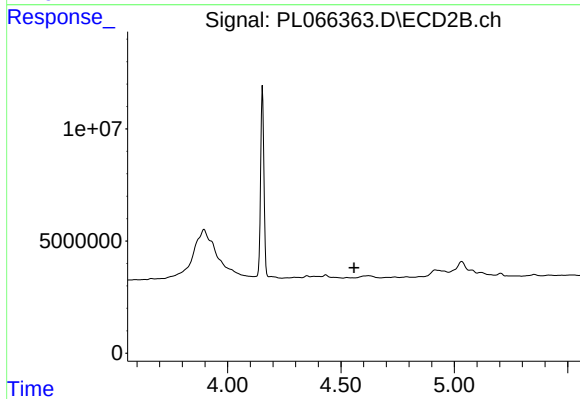

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.558 min
Response: 0
Conc: N.D.

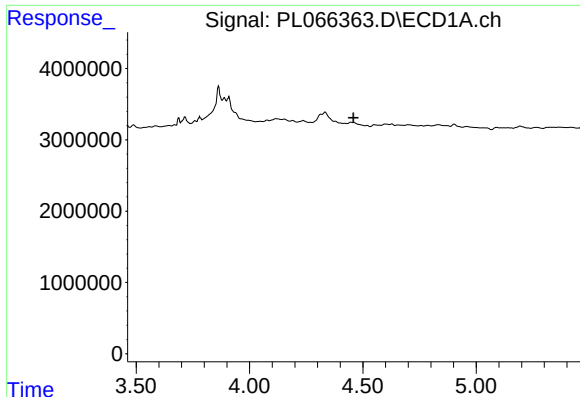

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.459 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

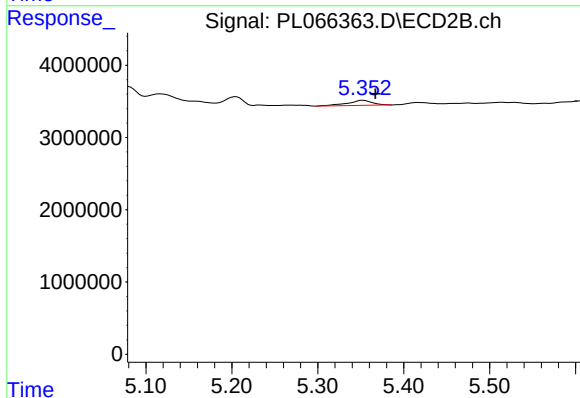


#4 Heptachlor

R.T.: 5.353 min
Delta R.T.: -0.014 min
Response: 1403091
Conc: 0.25 ng/ml

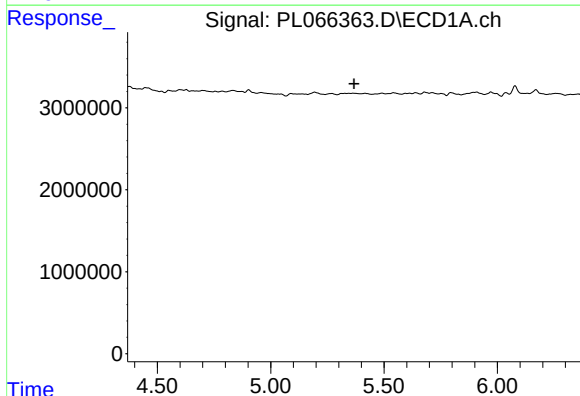


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.368 min
Response: 0
Conc: N.D.

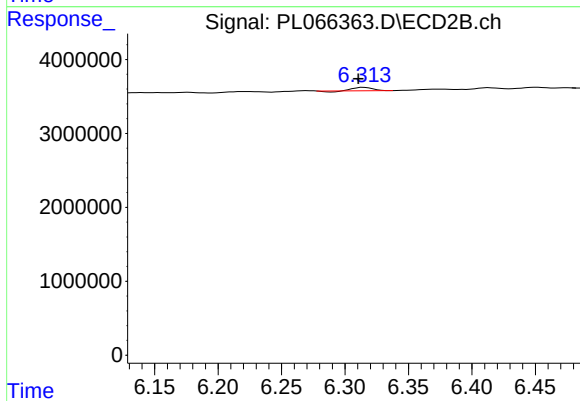

#10 gamma-Chlordane


R.T.: 6.315 min
Delta R.T.: 0.004 min
Response: 421941
Conc: 0.09 ng/ml

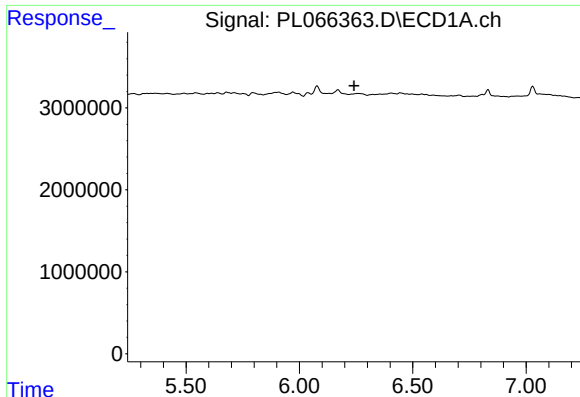

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.242 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

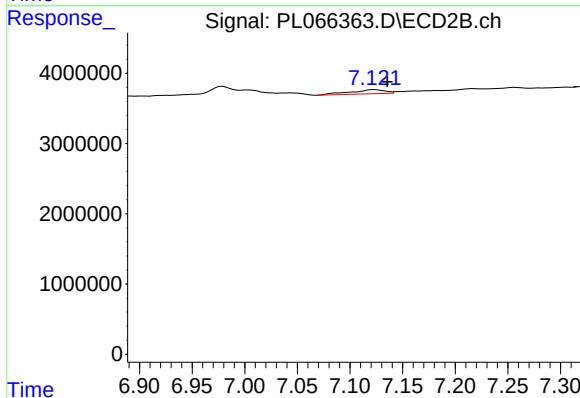


#15 Endosulfan II

R.T.: 7.122 min
Delta R.T.: -0.013 min
Response: 1345524
Conc: 0.39 ng/ml

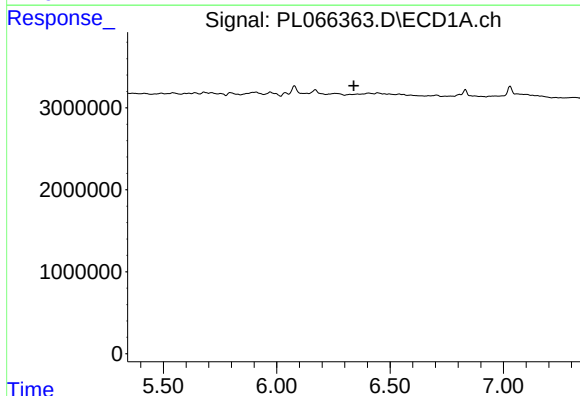


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.341 min
Response: 0
Conc: N.D.

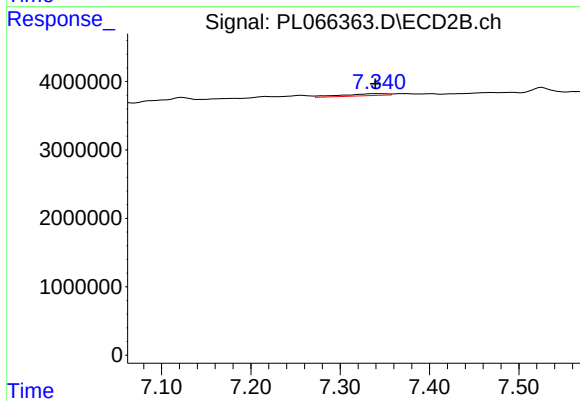

#17 4,4'-DDT


R.T.: 7.342 min
Delta R.T.: 0.003 min
Response: 1013834
Conc: 0.30 ng/ml

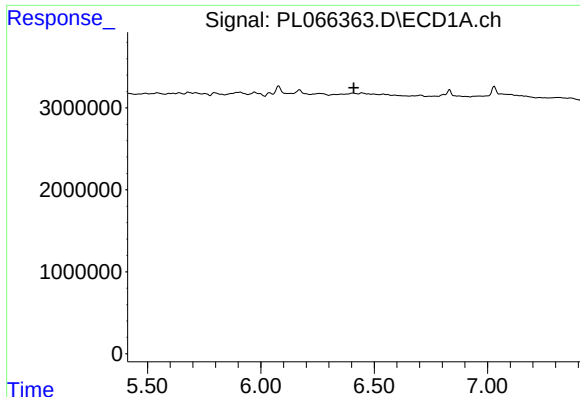

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.409 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

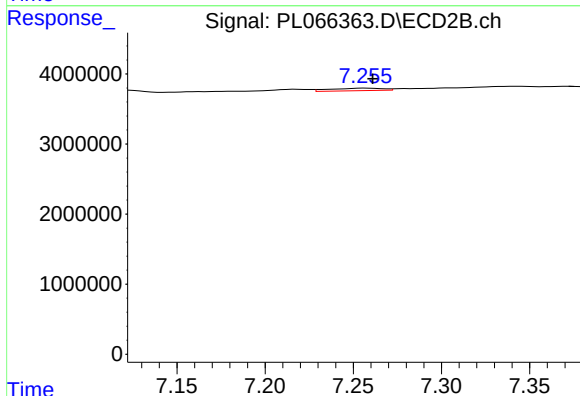


#18 Endrin aldehyde

R.T.: 7.257 min
Delta R.T.: -0.004 min
Response: 724448
Conc: 0.26 ng/ml

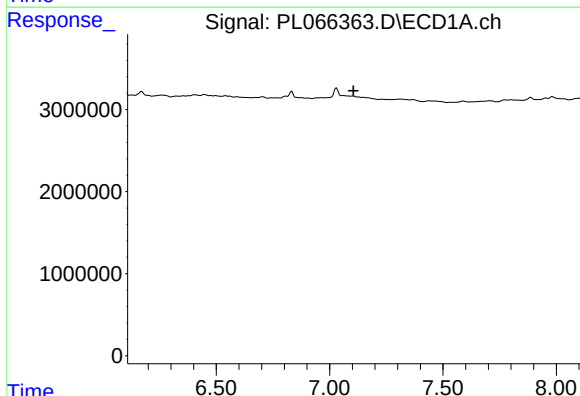


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 7.105 min
Response: 0
Conc: N.D.

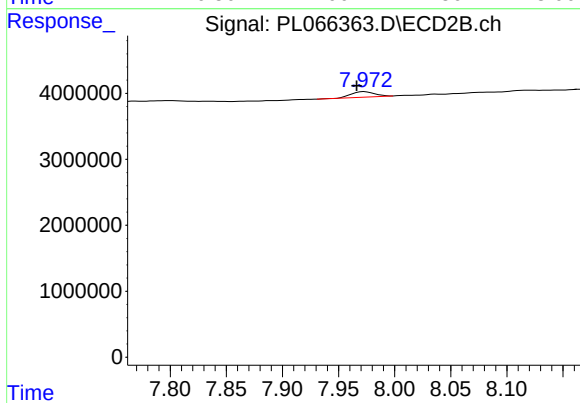

#21 Endrin ketone


R.T.: 7.973 min
Delta R.T.: 0.007 min
Response: 1200783
Conc: 0.33 ng/ml

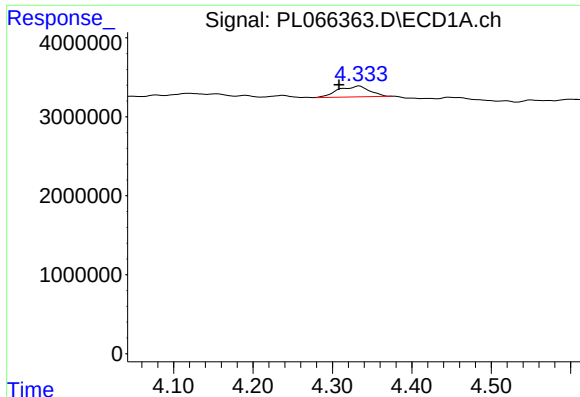

#23 Chlordane-1


R.T.: 4.334 min
Delta R.T.: 0.026 min
Response: 3777802
Conc: 33.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

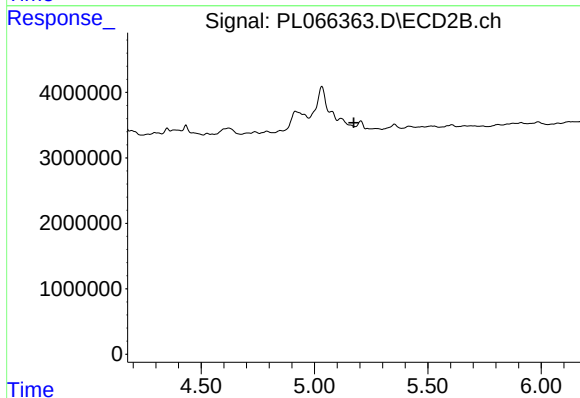


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.173 min
Response: 0
Conc: N.D.

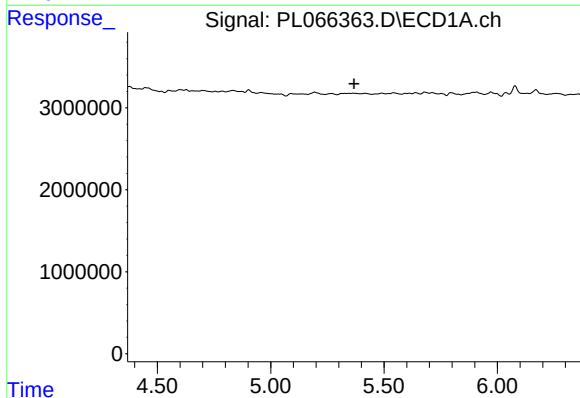


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.368 min
Response: 0
Conc: N.D.

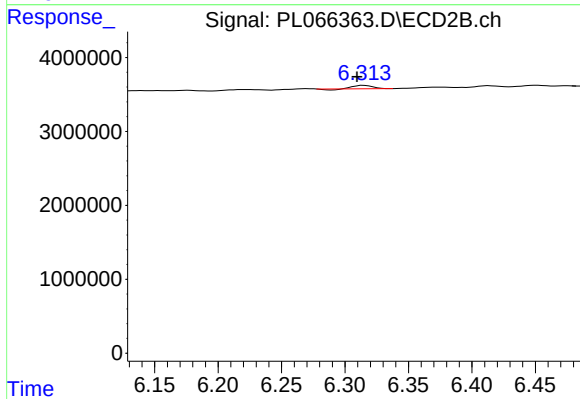

#25 Chlordane-3


R.T.: 6.315 min
Delta R.T.: 0.005 min
Response: 421941
Conc: 0.64 ng/ml

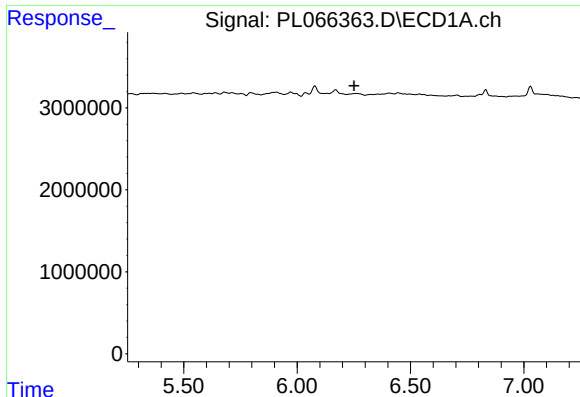

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.251 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

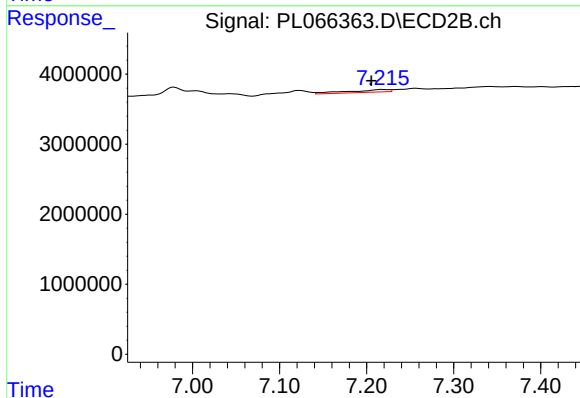


#27 Chlordane-5

R.T.: 7.217 min
Delta R.T.: 0.012 min
Response: 1220877
Conc: 9.11 ng/ml

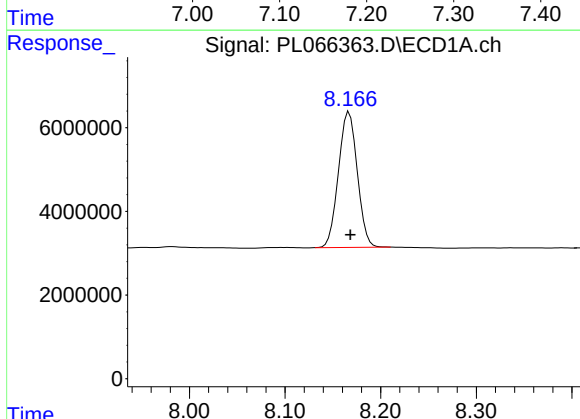

#28 Decachlorobiphenyl

R.T.: 8.167 min
Delta R.T.: -0.001 min
Response: 44526983
Conc: 18.67 ng/ml

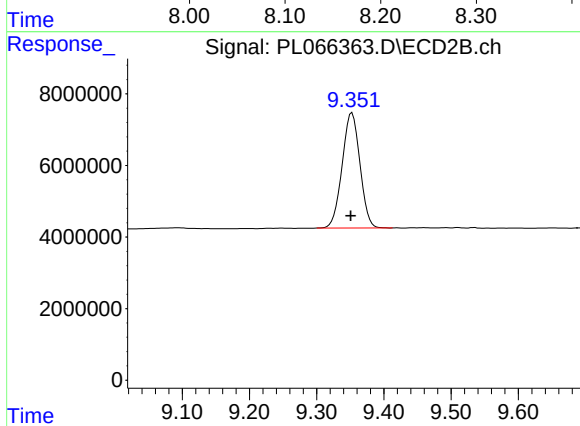

#28 Decachlorobiphenyl

R.T.: 9.352 min
Delta R.T.: 0.002 min
Response: 59098793
Conc: 18.10 ng/ml