

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042021\
 Data File : PL066338.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2021 10:42
 Operator : AR\AJ
 Sample : M2075-19
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-6-S

Manual Integrations
 APPROVED

Ankita
 4/21/2021 3:19:32 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 08:13:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 15:37:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.443	4.153	52007294	82105931	20.433m	20.411
28) SA Decachlor...	8.168	9.352	39338529	54428805	16.492	16.666
Target Compounds						
12) B 4,4'-DDE	5.588	6.538	4494982	7024456	1.205m	1.697 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042021\
Data File : PL066338.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2021 10:42
Operator : AR\AJ
Sample : M2075-19
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-6-S


Manual Integrations
APPROVED

Ankita
4/21/2021 3:19:32 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 08:13:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 15:37:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

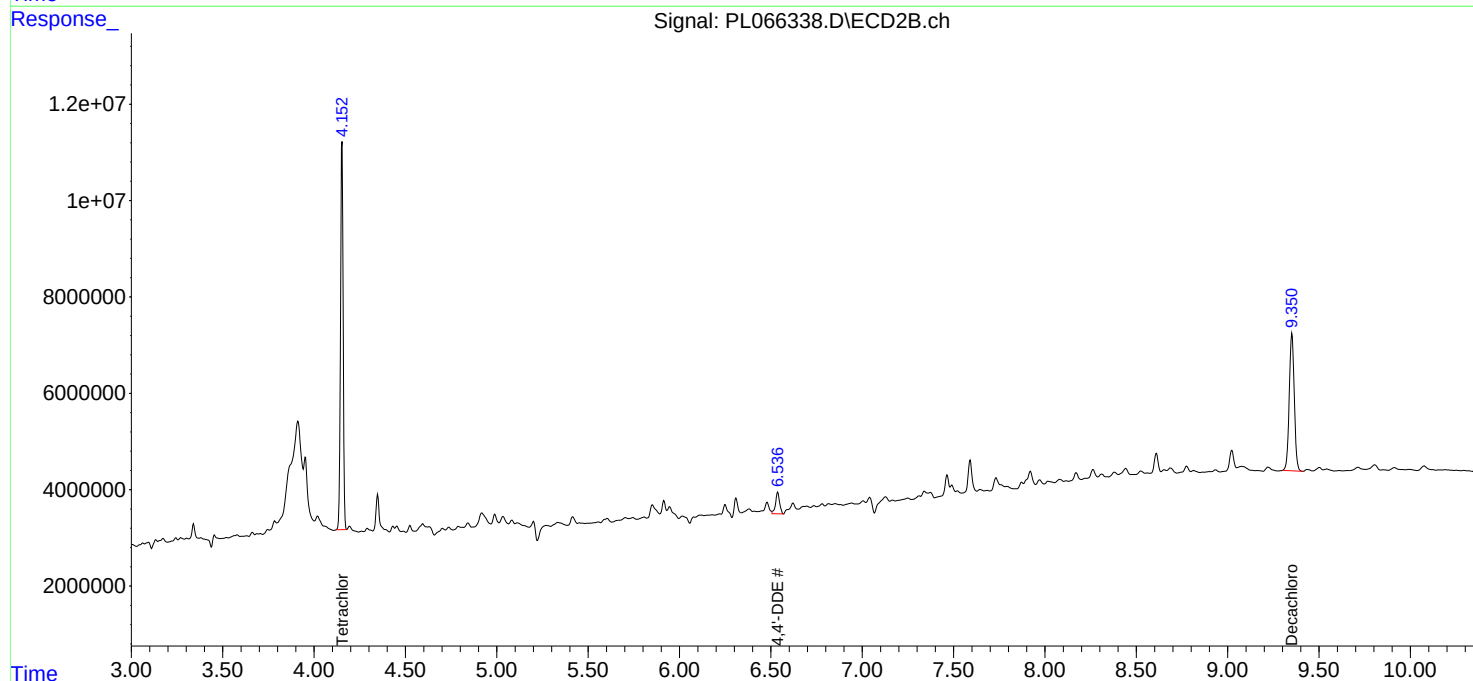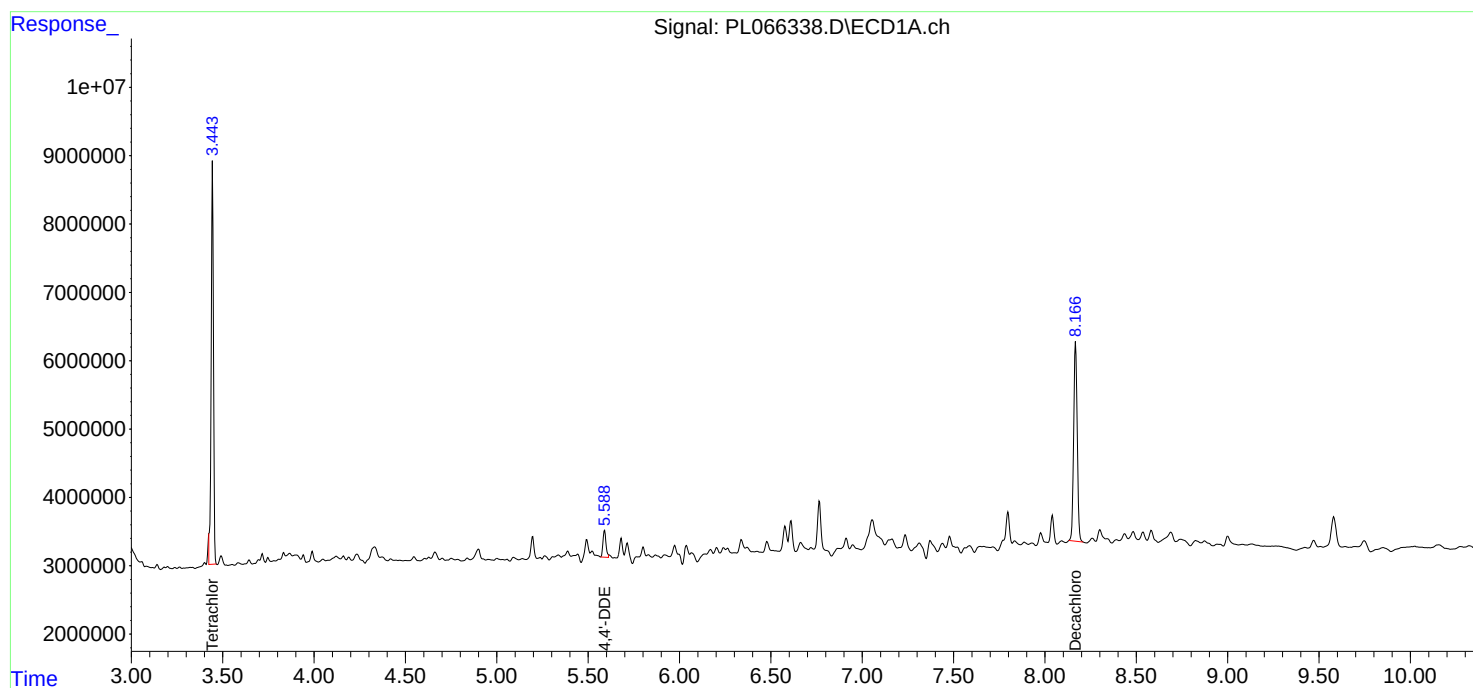

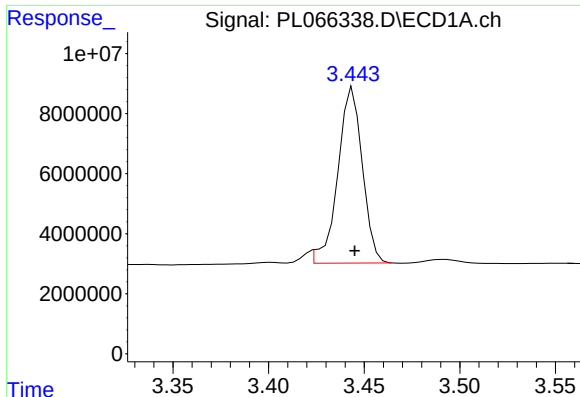


#1 Tetrachloro-m-xylene

R.T.: 3.443 min
Delta R.T.: -0.002 min
Response: 52007294
Conc: 20.43 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TP-6-S


Manual Integrations
APPROVED

Ankita
4/21/2021 3:19:32 PM

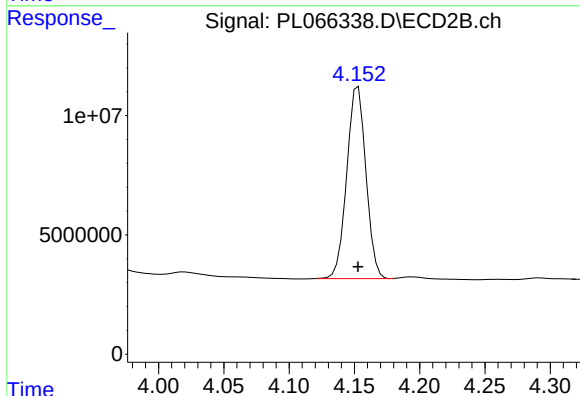


#1 Tetrachloro-m-xylene

R.T.: 4.153 min
Delta R.T.: 0.000 min
Response: 82105931
Conc: 20.41 ng/ml

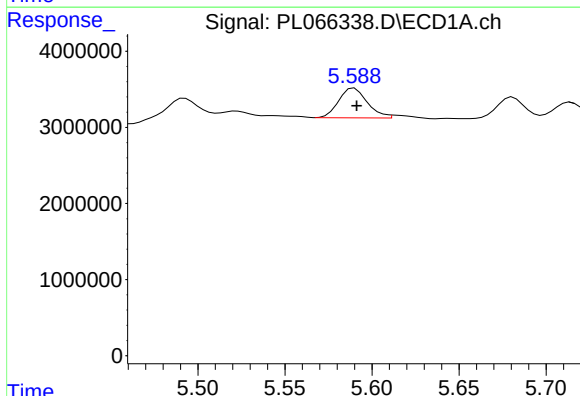


#12 4,4'-DDE

R.T.: 5.588 min
Delta R.T.: -0.003 min
Response: 4494982
Conc: 1.21 ng/ml m

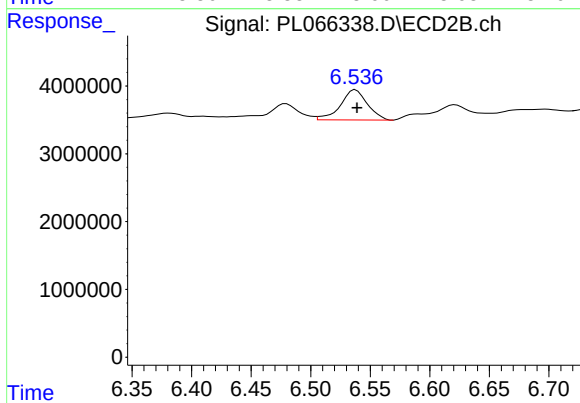

#12 4,4'-DDE

R.T.: 6.538 min
Delta R.T.: -0.001 min
Response: 7024456
Conc: 1.70 ng/ml

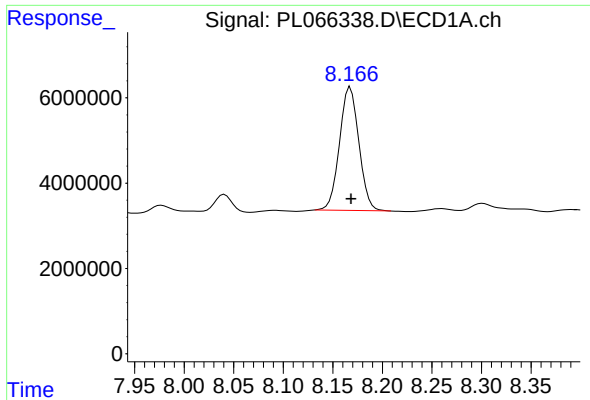


#28 Decachlorobiphenyl

R.T.: 8.168 min
Delta R.T.: 0.000 min
Response: 39338529
Conc: 16.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6-S

Manual Integrations
APPROVED

Ankita
4/21/2021 3:19:32 PM

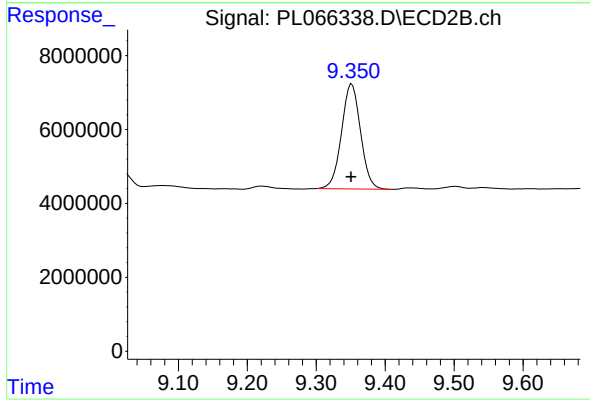

#28 Decachlorobiphenyl

R.T.: 9.352 min
Delta R.T.: 0.000 min
Response: 54428805
Conc: 16.67 ng/ml