

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042021\
 Data File : PL066344.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2021 12:21
 Operator : AR\AJ
 Sample : M2077-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-20-14.5-15.0

Manual Integrations
 APPROVED

Ankita
 4/21/2021 3:19:47 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 08:14:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 15:37:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	4.151	34512759	43521969	13.560m	10.819m
28)	SA Decachlor...	8.166	9.352	40766877	55563175	17.091	17.013

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042021\
Data File : PL066344.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2021 12:21
Operator : AR\AJ
Sample : M2077-04
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
SB-20-14.5-15.0


Manual Integrations
APPROVED

Ankita
4/21/2021 3:19:47 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 08:14:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041421.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 15:37:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

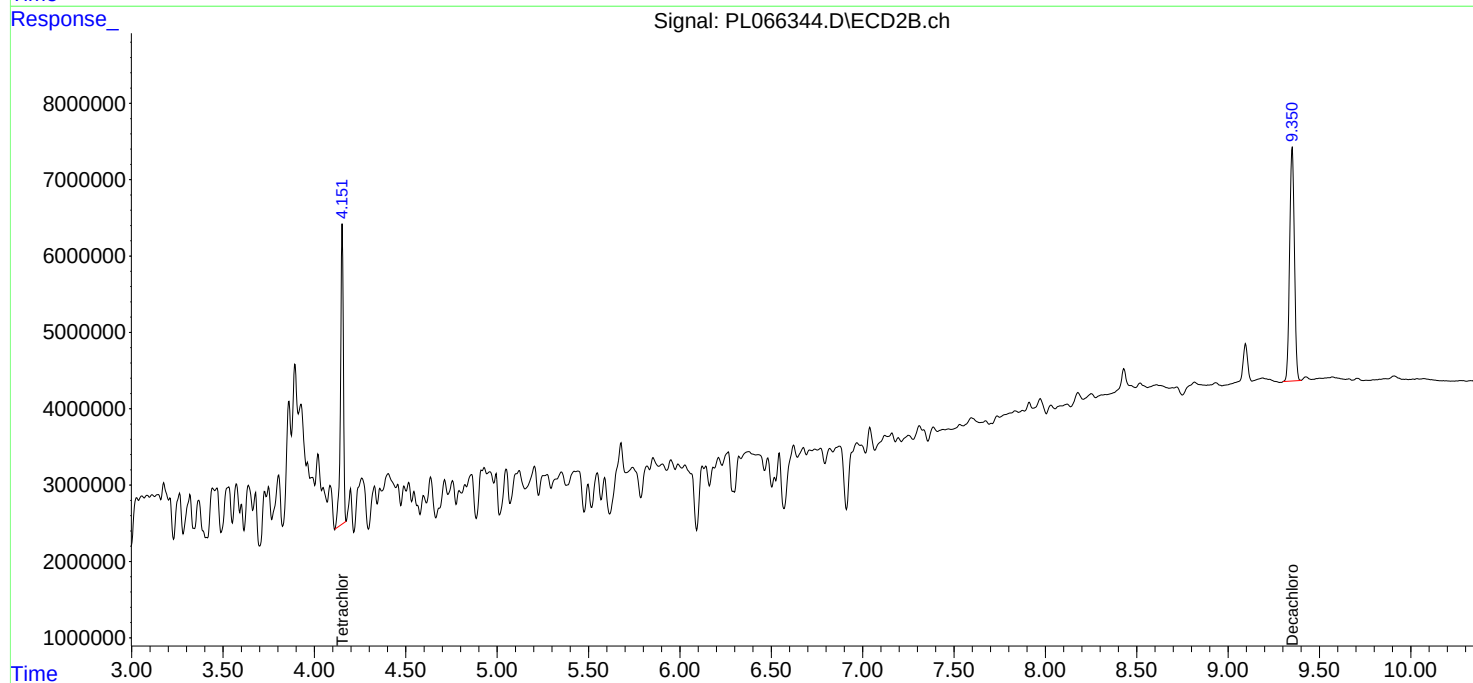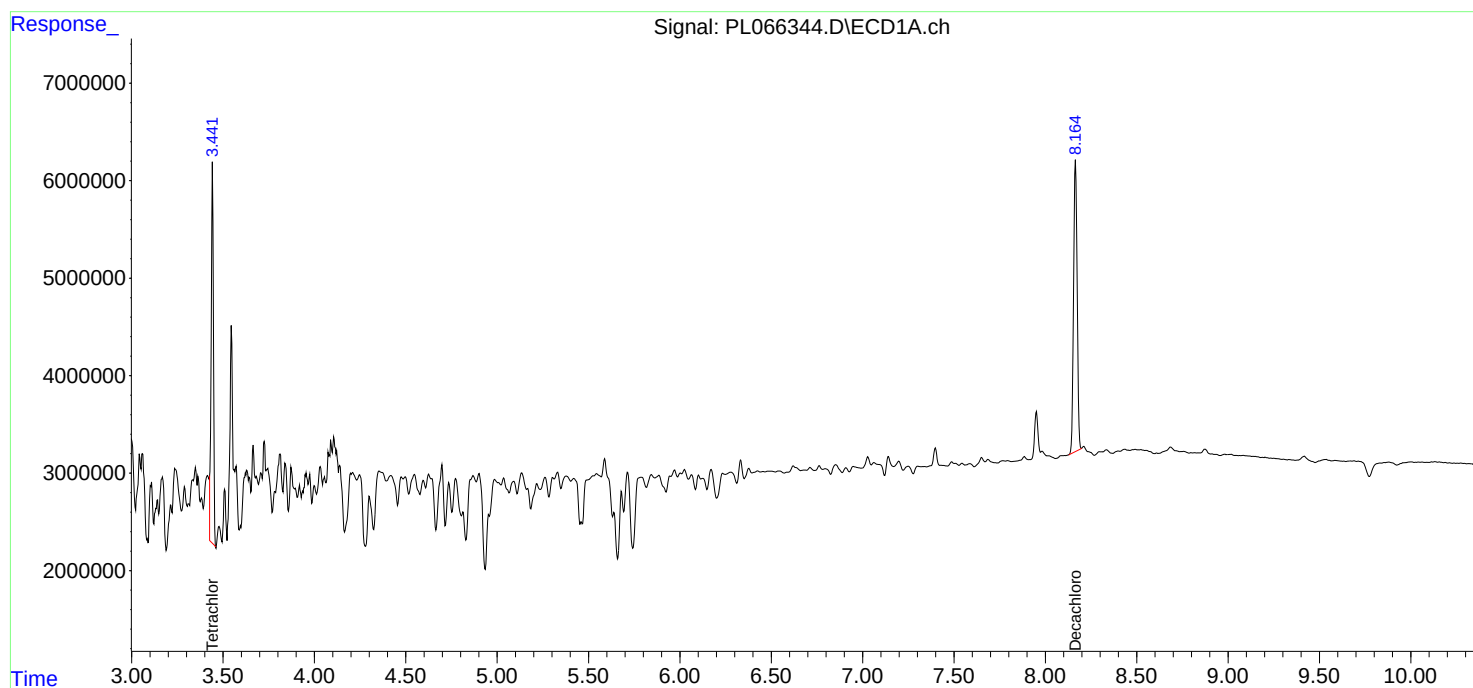

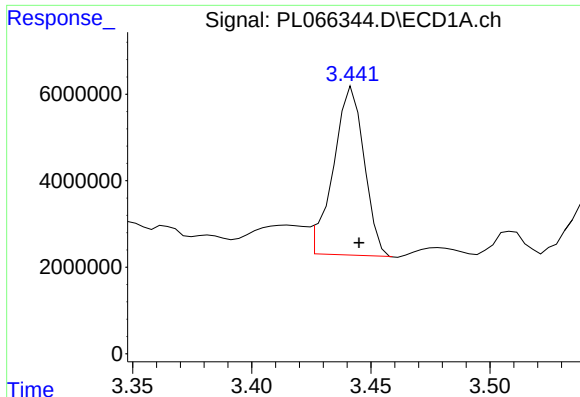


#1 Tetrachloro-m-xylene

R.T.: 3.441 min
Delta R.T.: -0.004 min
Response: 34512759
Conc: 13.56 ng/ml m

Instrument :
ECD_L
ClientSampleId :
SB-20-14.5-15.0


Manual Integrations
APPROVED

Ankita
4/21/2021 3:19:47 PM

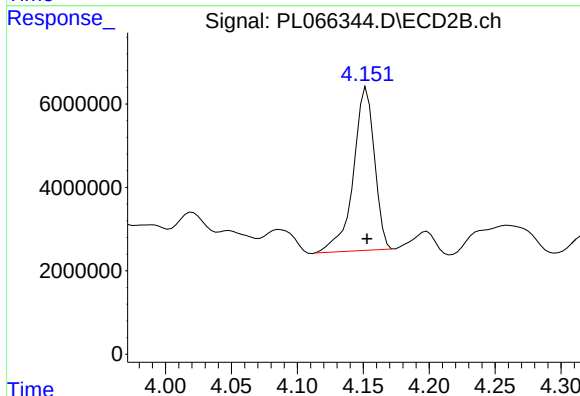


#1 Tetrachloro-m-xylene

R.T.: 4.151 min
Delta R.T.: -0.002 min
Response: 43521969
Conc: 10.82 ng/ml m

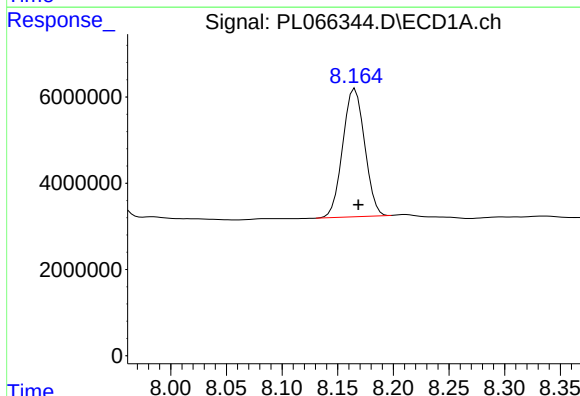

#28 Decachlorobiphenyl

R.T.: 8.166 min
Delta R.T.: -0.003 min
Response: 40766877
Conc: 17.09 ng/ml

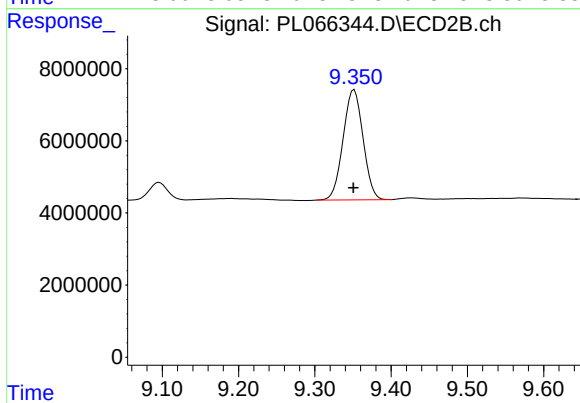

#28 Decachlorobiphenyl

R.T.: 9.352 min
Delta R.T.: 0.000 min
Response: 55563175
Conc: 17.01 ng/ml