

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042022\
 Data File : PL074231.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2022 23:24
 Operator : AR\AJ
 Sample : N2468-04
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WC-15-1-6

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 04/22/2022
 Supervised By : mohammad ahmed 04/22/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 03:00:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 14 09:29:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.635	5.489	7713024	40812817	23.871	22.890
2) SA Decachlor...	10.404	11.329	8689953	32497276	16.710m	18.398

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042022\
Data File : PL074231.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2022 23:24
Operator : AR\AJ
Sample : N2468-04
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
WC-15-1-6


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 04/22/2022
Supervised By : mohammad ahmed 04/22/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 03:00:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
Quant Title : GC Extractables
QLast Update : Thu Apr 14 09:29:23 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

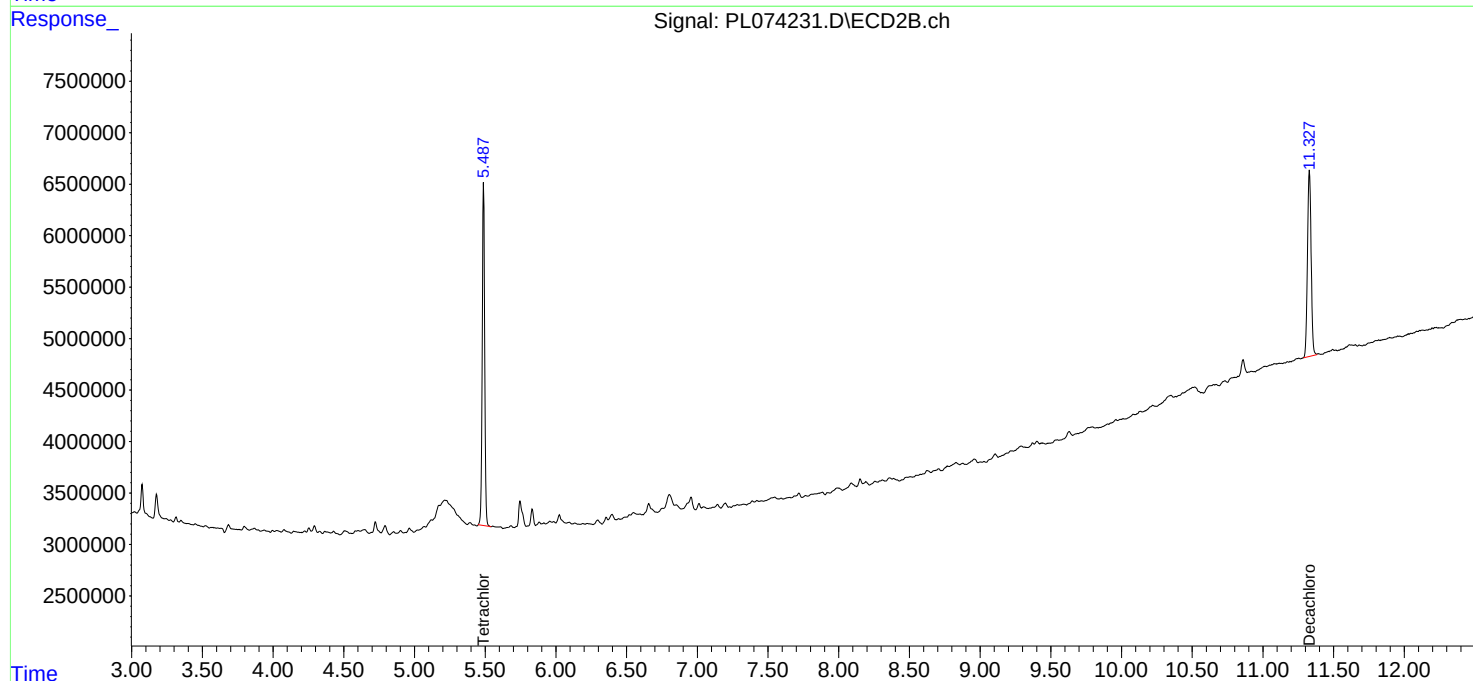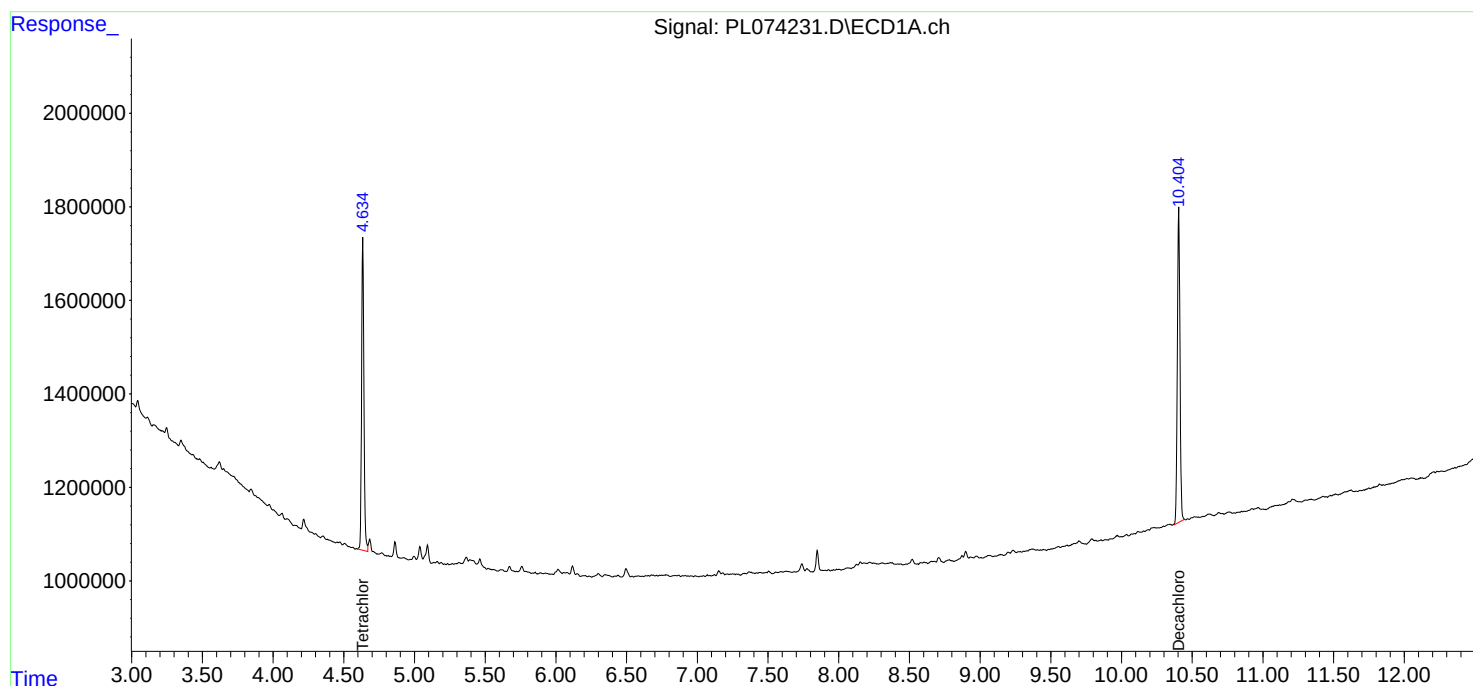

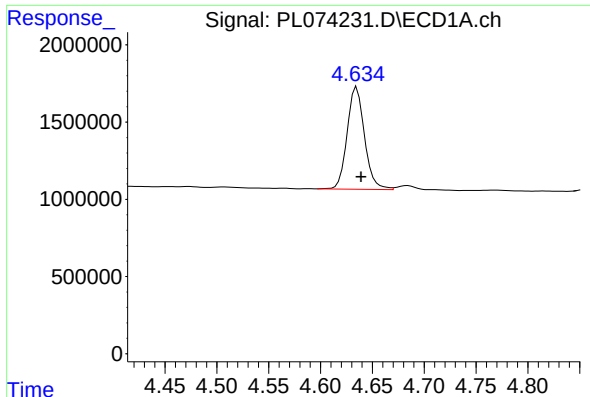


#1 Tetrachloro-m-xylene

R.T.: 4.635 min
Delta R.T.: -0.004 min
Response: 7713024
Conc: 23.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-15-1-6


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/22/2022
Supervised By :mohammad ahmed 04/22/2022

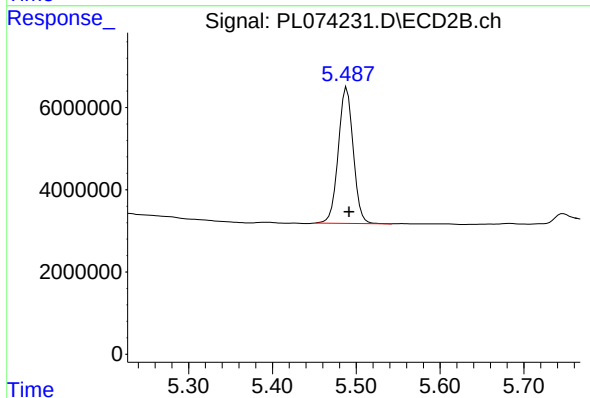


#1 Tetrachloro-m-xylene

R.T.: 5.489 min
Delta R.T.: -0.003 min
Response: 40812817
Conc: 22.89 ng/ml

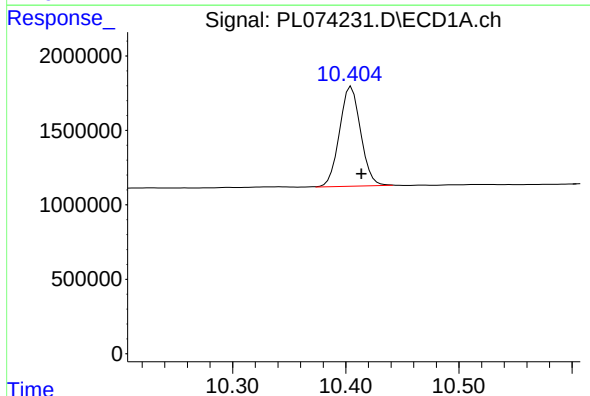

#28 Decachlorobiphenyl

R.T.: 10.404 min
Delta R.T.: -0.010 min
Response: 8689953
Conc: 16.71 ng/ml m

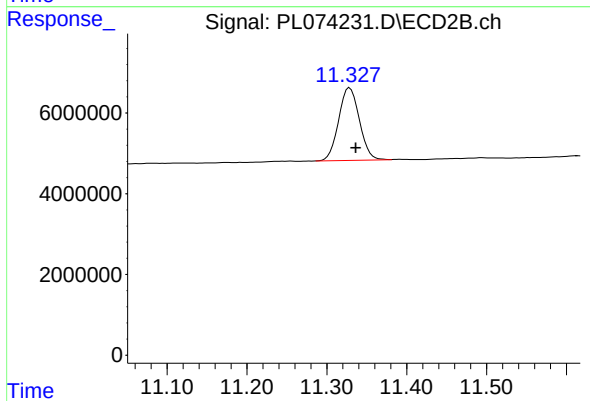

#28 Decachlorobiphenyl

R.T.: 11.329 min
Delta R.T.: -0.008 min
Response: 32497276
Conc: 18.40 ng/ml