

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042023\
 Data File : PL082218.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2023 19:55
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 01:46:09 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 21 01:44:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.323	2.647	124.3E6	137.9E6	50.000	50.000
28)	SA Decachlor...	8.741	7.760	88203674	104.5E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.466	3.633	56964756	45784457	500.000	500.000
24)	Chlordane-2	4.993	4.206	61771043	56510640	500.000	500.000
25)	Chlordane-3	5.698	4.833	222.3E6	147.7E6	500.000	500.000
26)	Chlordane-4	5.778	4.894	264.0E6	153.5E6	500.000	500.000
27)	Chlordane-5	6.619	5.787	46952955	51604631	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042023\
Data File : PL082218.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2023 19:55
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 01:46:09 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 01:44:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

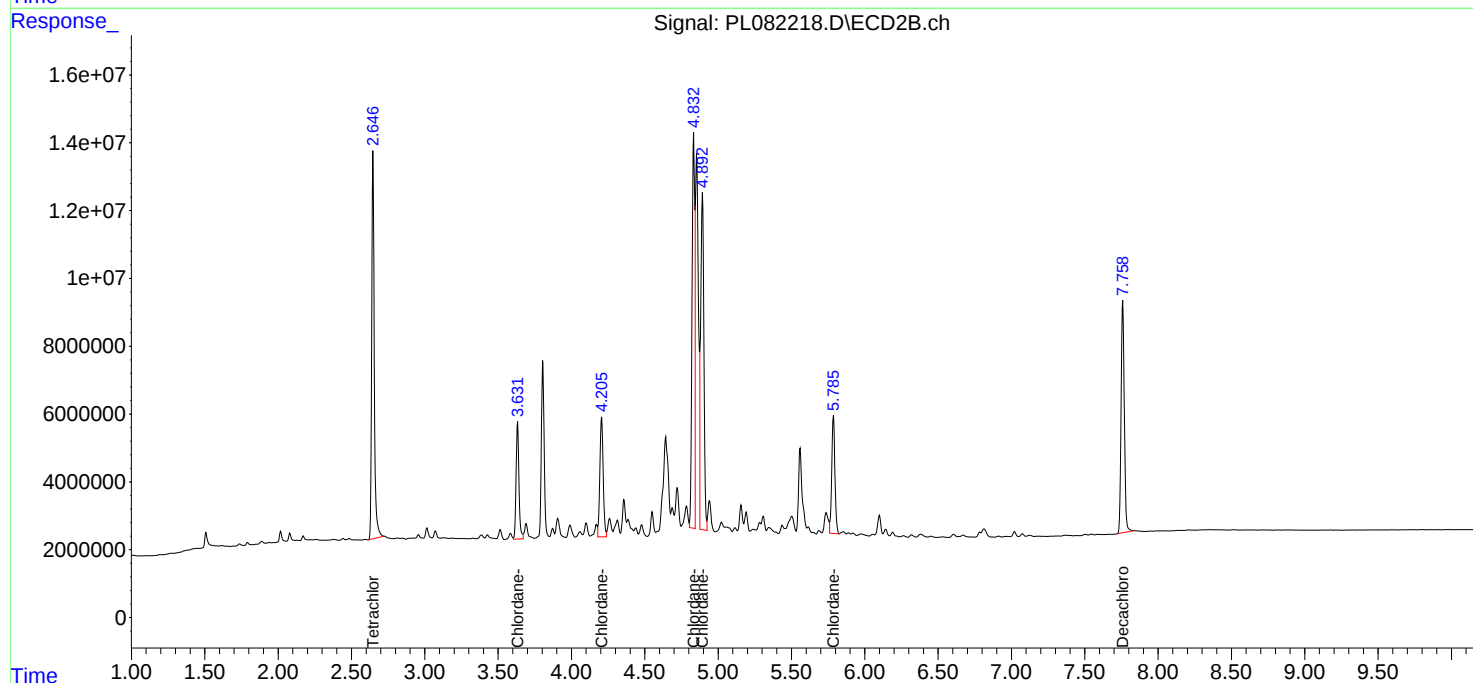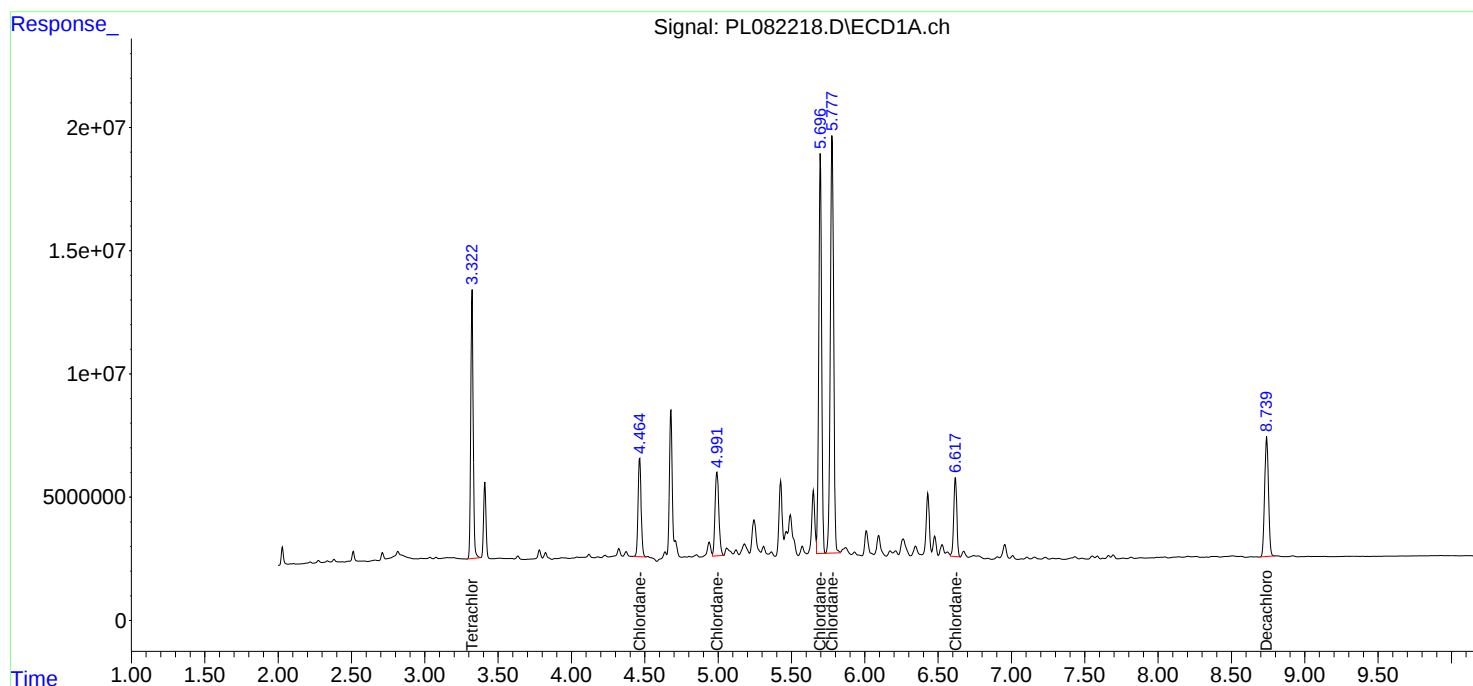


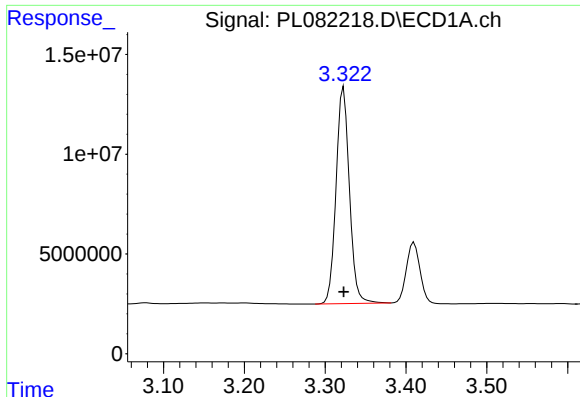

#1 Tetrachloro-m-xylene


R.T.: 3.323 min
Delta R.T.: 0.000 min
Response: 124336105
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

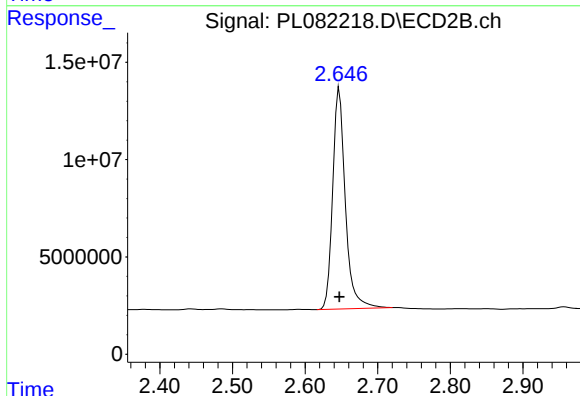


#1 Tetrachloro-m-xylene

R.T.: 2.647 min
Delta R.T.: 0.000 min
Response: 137914274
Conc: 50.00 ng/ml

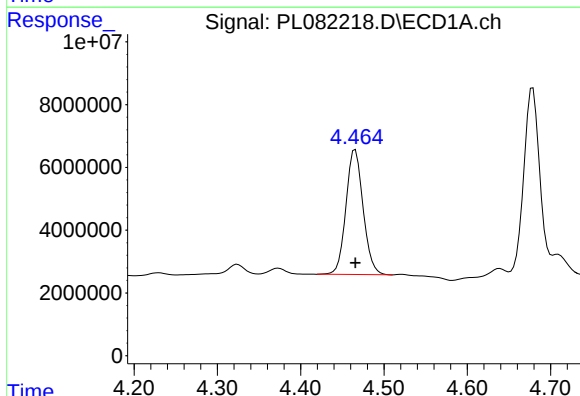


#23 Chlordane-1

R.T.: 4.466 min
Delta R.T.: 0.000 min
Response: 56964756
Conc: 500.00 ng/ml

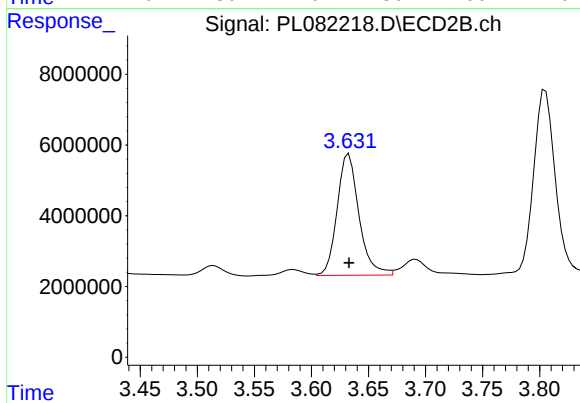

#23 Chlordane-1


R.T.: 3.633 min
Delta R.T.: 0.000 min
Response: 45784457
Conc: 500.00 ng/ml

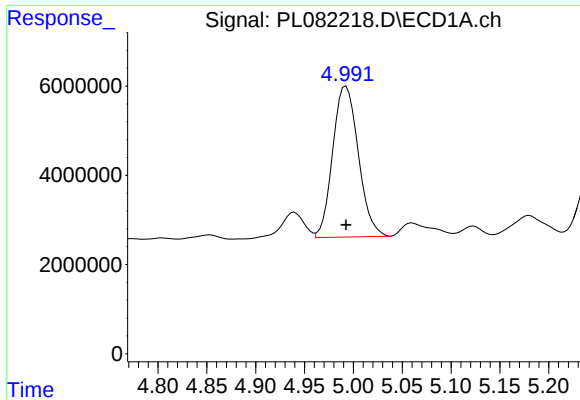

#24 Chlordane-2


R.T.: 4.993 min
Delta R.T.: 0.000 min
Response: 61771043
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

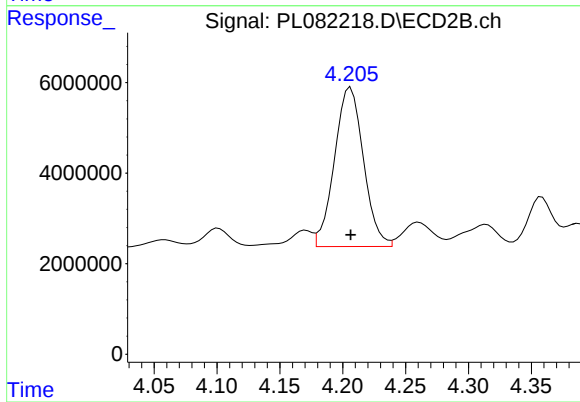


#24 Chlordane-2

R.T.: 4.206 min
Delta R.T.: 0.000 min
Response: 56510640
Conc: 500.00 ng/ml

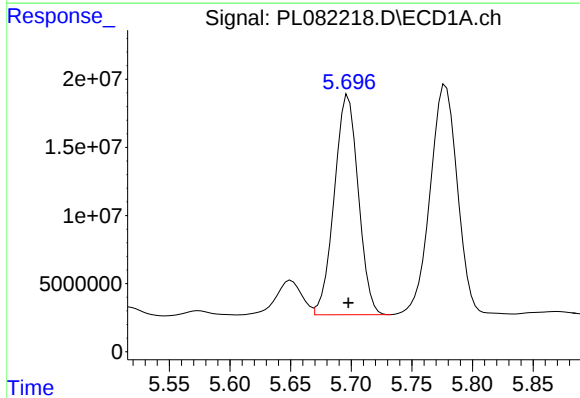


#25 Chlordane-3

R.T.: 5.698 min
Delta R.T.: 0.000 min
Response: 222301282
Conc: 500.00 ng/ml

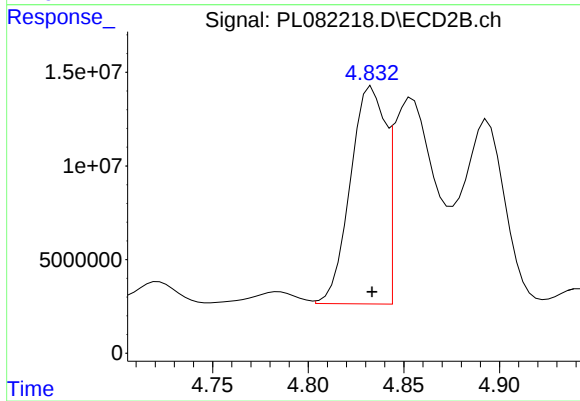

#25 Chlordane-3


R.T.: 4.833 min
Delta R.T.: 0.000 min
Response: 147689299
Conc: 500.00 ng/ml

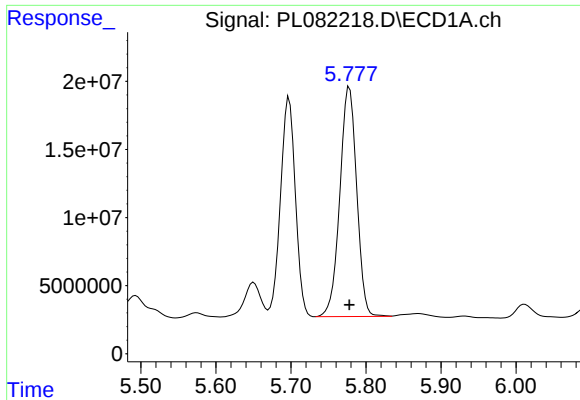

#26 Chlordane-4


R.T.: 5.778 min
Delta R.T.: 0.000 min
Response: 264040542
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

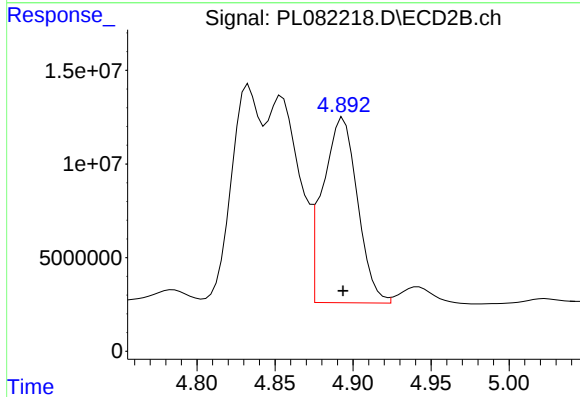


#26 Chlordane-4

R.T.: 4.894 min
Delta R.T.: 0.000 min
Response: 153485272
Conc: 500.00 ng/ml

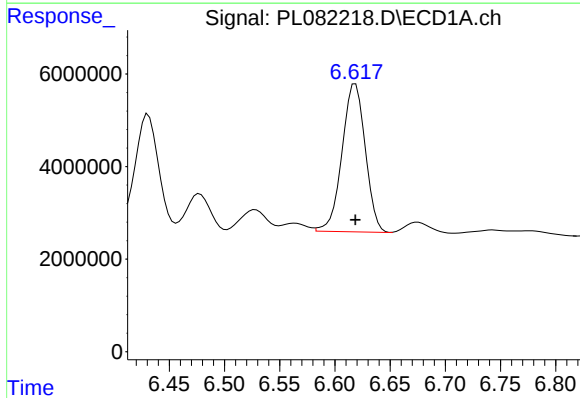


#27 Chlordane-5

R.T.: 6.619 min
Delta R.T.: 0.000 min
Response: 46952955
Conc: 500.00 ng/ml

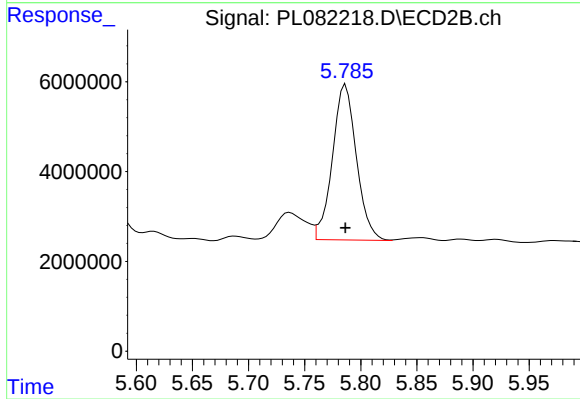

#27 Chlordane-5


R.T.: 5.787 min
Delta R.T.: 0.000 min
Response: 51604631
Conc: 500.00 ng/ml

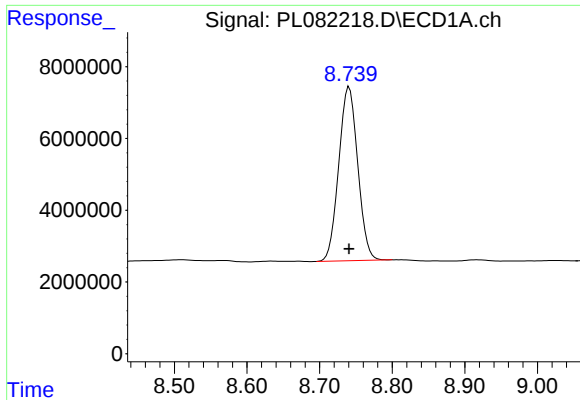

#28 Decachlorobiphenyl

R.T.: 8.741 min
Delta R.T.: 0.000 min
Response: 88203674
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

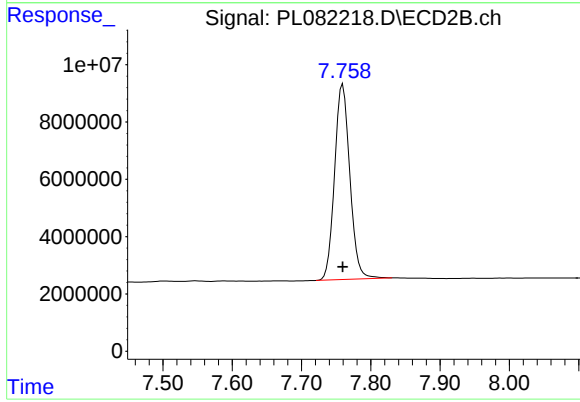

#28 Decachlorobiphenyl

R.T.: 7.760 min
Delta R.T.: 0.000 min
Response: 104515616
Conc: 50.00 ng/ml