

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042023\
 Data File : PL082216.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2023 19:27
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 01:48:32 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 21 01:44:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.323	2.647	244.4E6	273.1E6	99.124	99.505
28)	SA Decachlor...	8.741	7.760	162.7E6	195.5E6	95.953	96.664
Target Compounds							
23)	Chlordane-1	4.466	3.633	112.7E6	88591516	994.617	983.474
24)	Chlordane-2	4.992	4.207	115.3E6	105.9E6	965.656	967.591
25)	Chlordane-3	5.698	4.834	446.4E6	301.8E6	1002.014	1010.680
26)	Chlordane-4	5.778	4.894	523.0E6	311.0E6	995.192	1006.592
27)	Chlordane-5	6.619	5.786	92008396	102.6E6	989.794	996.877



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042023\
Data File : PL082216.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2023 19:27
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 01:48:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 01:44:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

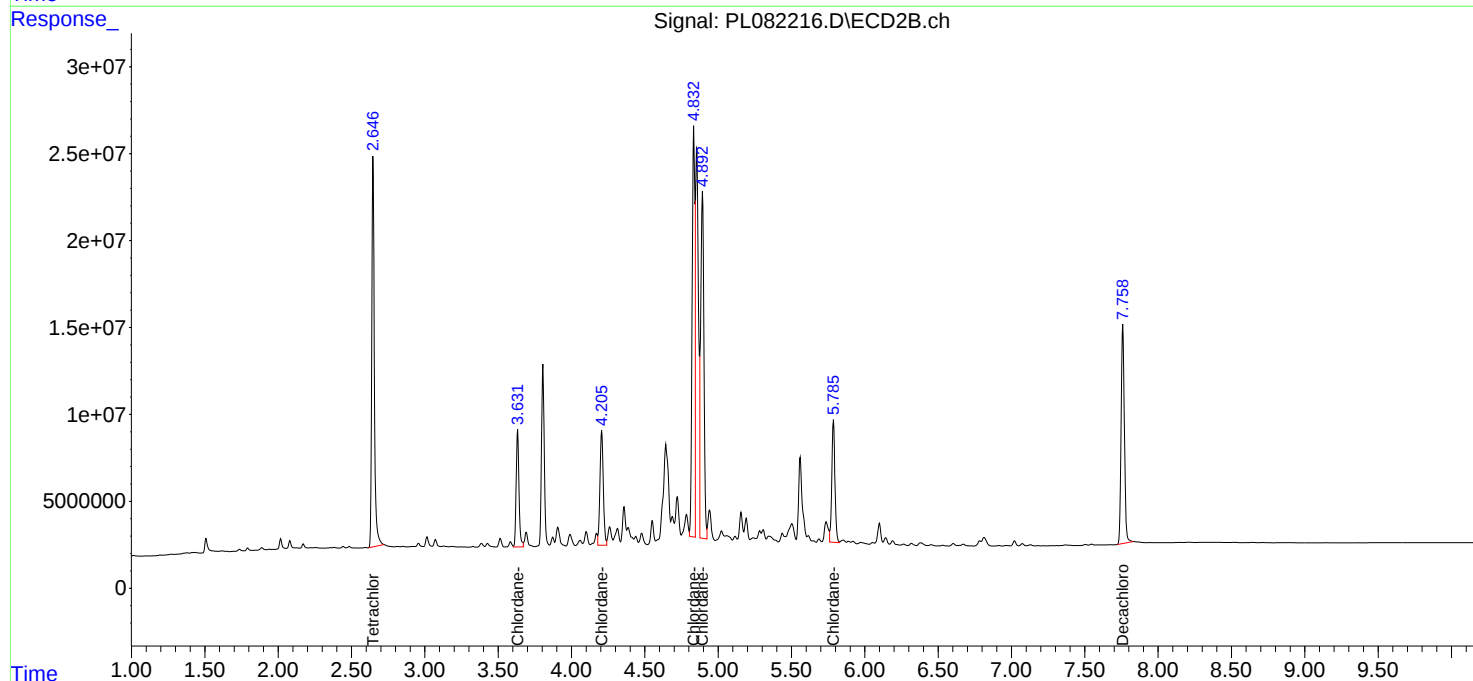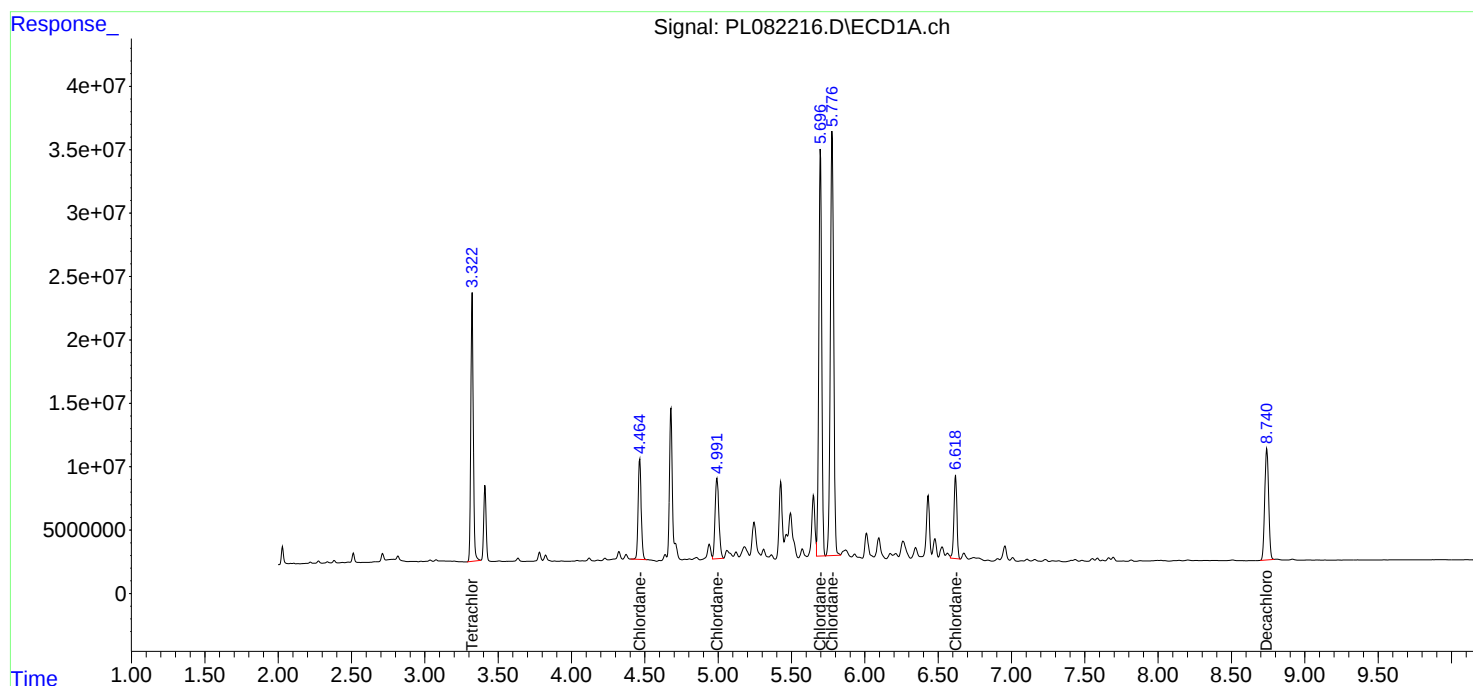


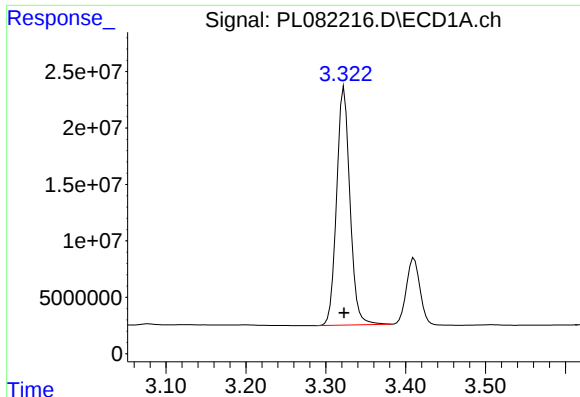

#1 Tetrachloro-m-xylene


R.T.: 3.323 min
Delta R.T.: 0.000 min
Response: 244351764
Conc: 99.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

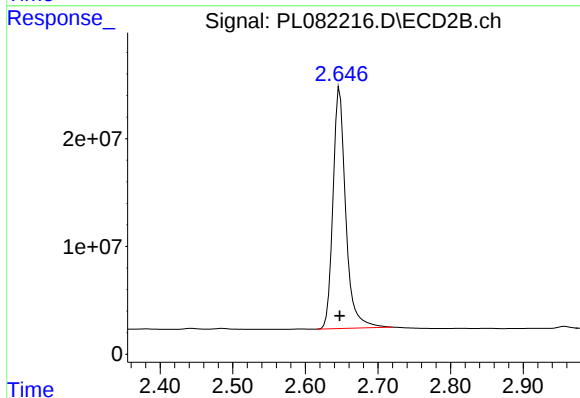


#1 Tetrachloro-m-xylene

R.T.: 2.647 min
Delta R.T.: 0.000 min
Response: 273112805
Conc: 99.51 ng/ml

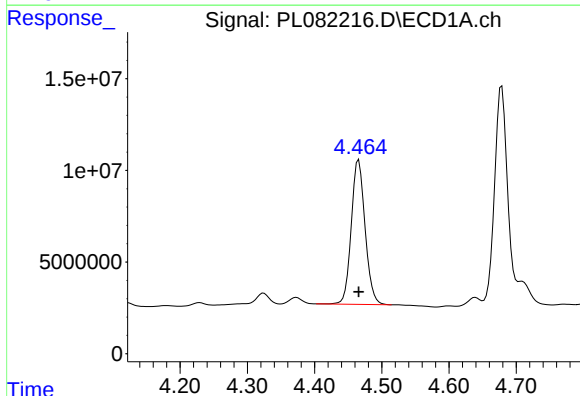


#23 Chlordane-1

R.T.: 4.466 min
Delta R.T.: 0.000 min
Response: 112709464
Conc: 994.62 ng/ml

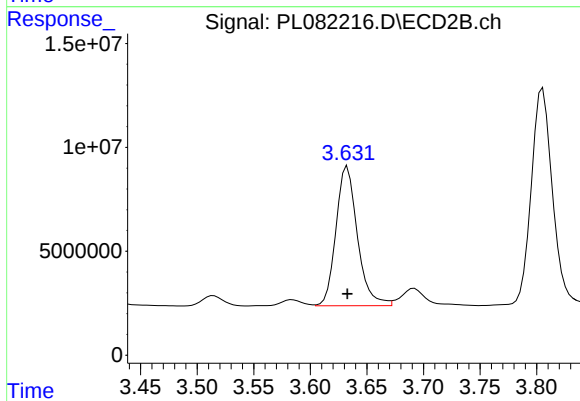

#23 Chlordane-1


R.T.: 3.633 min
Delta R.T.: 0.000 min
Response: 88591516
Conc: 983.47 ng/ml

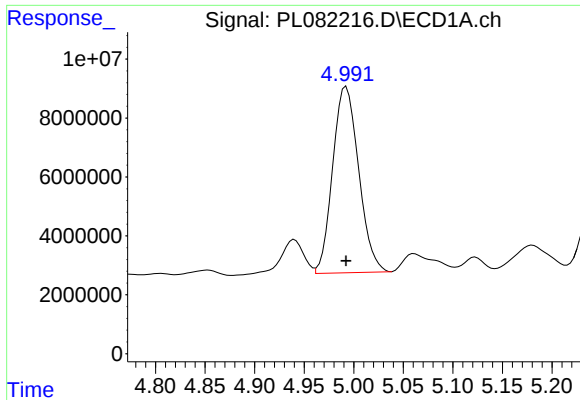

#24 Chlordane-2


R.T.: 4.992 min
Delta R.T.: 0.000 min
Response: 115337873
Conc: 965.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

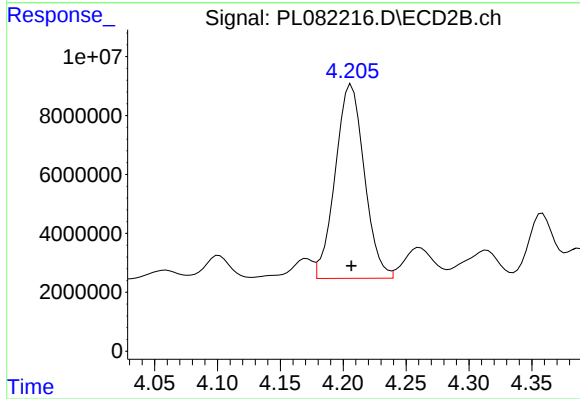


#24 Chlordane-2

R.T.: 4.207 min
Delta R.T.: 0.000 min
Response: 105925493
Conc: 967.59 ng/ml

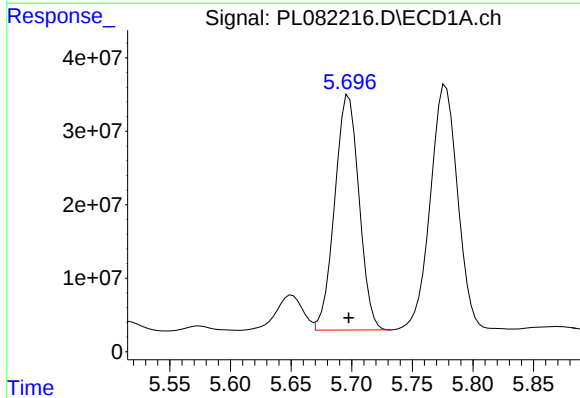


#25 Chlordane-3

R.T.: 5.698 min
Delta R.T.: 0.000 min
Response: 446397004
Conc: 1002.01 ng/ml

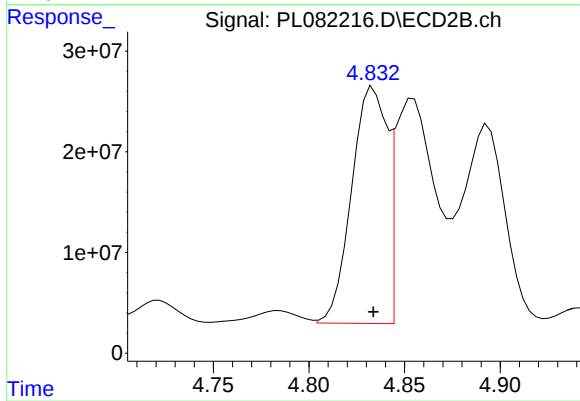

#25 Chlordane-3


R.T.: 4.834 min
Delta R.T.: 0.000 min
Response: 301756232
Conc: 1010.68 ng/ml

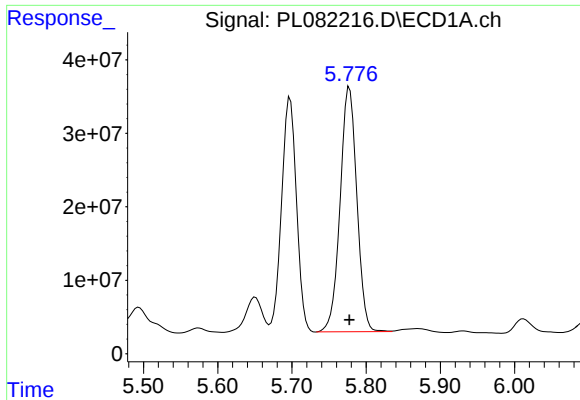

#26 Chlordane-4


R.T.: 5.778 min
Delta R.T.: 0.000 min
Response: 523027795
Conc: 995.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

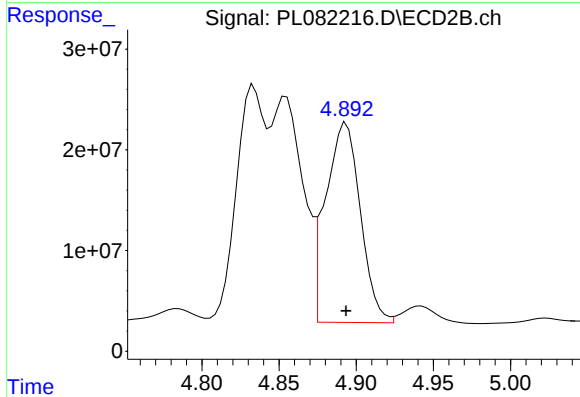


#26 Chlordane-4

R.T.: 4.894 min
Delta R.T.: 0.000 min
Response: 311044690
Conc: 1006.59 ng/ml

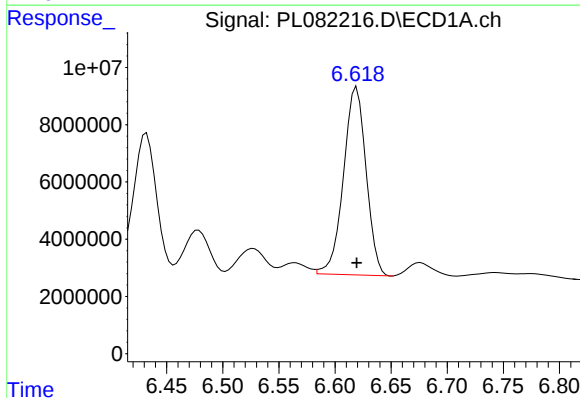


#27 Chlordane-5

R.T.: 6.619 min
Delta R.T.: 0.000 min
Response: 92008396
Conc: 989.79 ng/ml

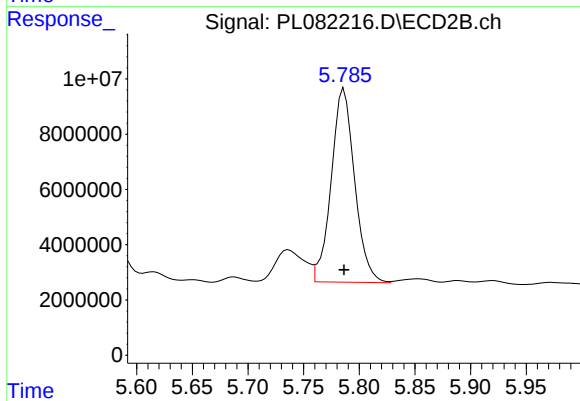

#27 Chlordane-5

R.T.: 5.786 min
Delta R.T.: 0.000 min
Response: 102566660
Conc: 996.88 ng/ml

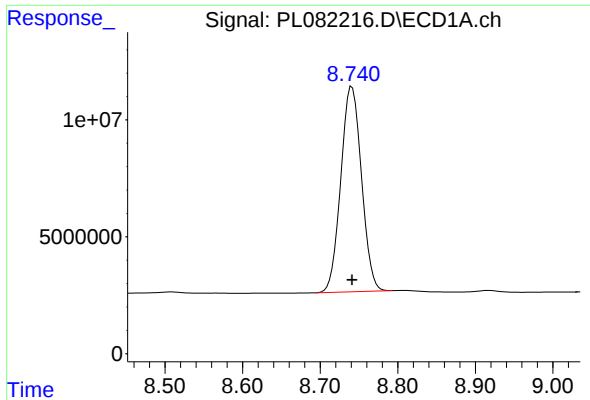

#28 Decachlorobiphenyl


R.T.: 8.741 min

Delta R.T.: 0.000 min

Response: 162683695

Conc: 95.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

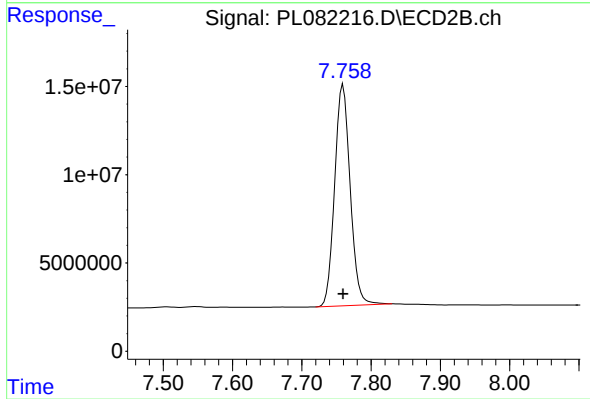

#28 Decachlorobiphenyl

R.T.: 7.760 min

Delta R.T.: 0.000 min

Response: 195533289

Conc: 96.66 ng/ml