

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042023\
 Data File : PL082217.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2023 19:41
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 01:51:03 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 21 01:44:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.323	2.647	180.3E6	199.7E6	73.750	73.488
28)	SA Decachlor...	8.742	7.760	123.6E6	147.0E6	73.580	73.420
Target Compounds							
23)	Chlordane-1	4.466	3.633	82231833	67309872	733.598	748.145
24)	Chlordane-2	4.993	4.206	87548387	79901535	738.574	736.460
25)	Chlordane-3	5.698	4.833	323.3E6	217.3E6	733.688	735.091
26)	Chlordane-4	5.779	4.894	388.5E6	227.4E6	742.721	740.493
27)	Chlordane-5	6.619	5.787	67074779	74482528	730.802	732.409



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042023\
Data File : PL082217.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2023 19:41
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 01:51:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 01:44:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

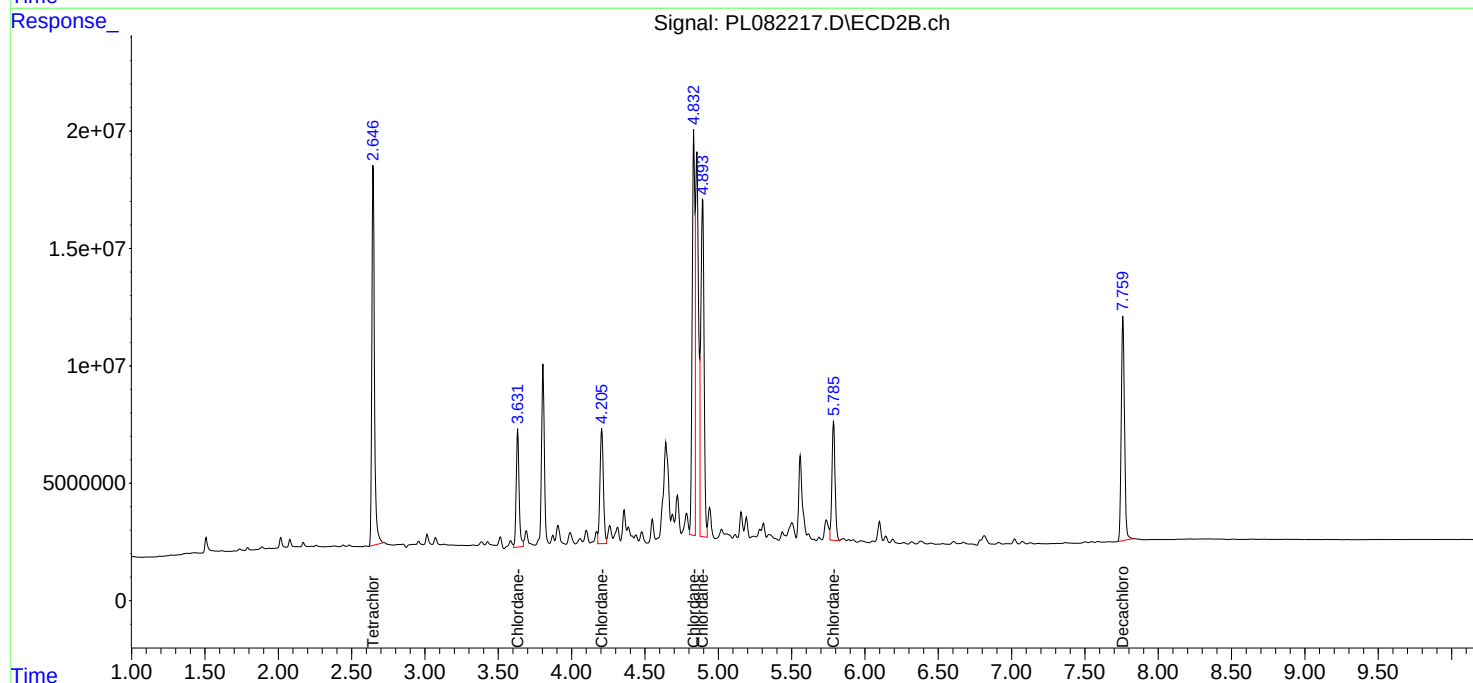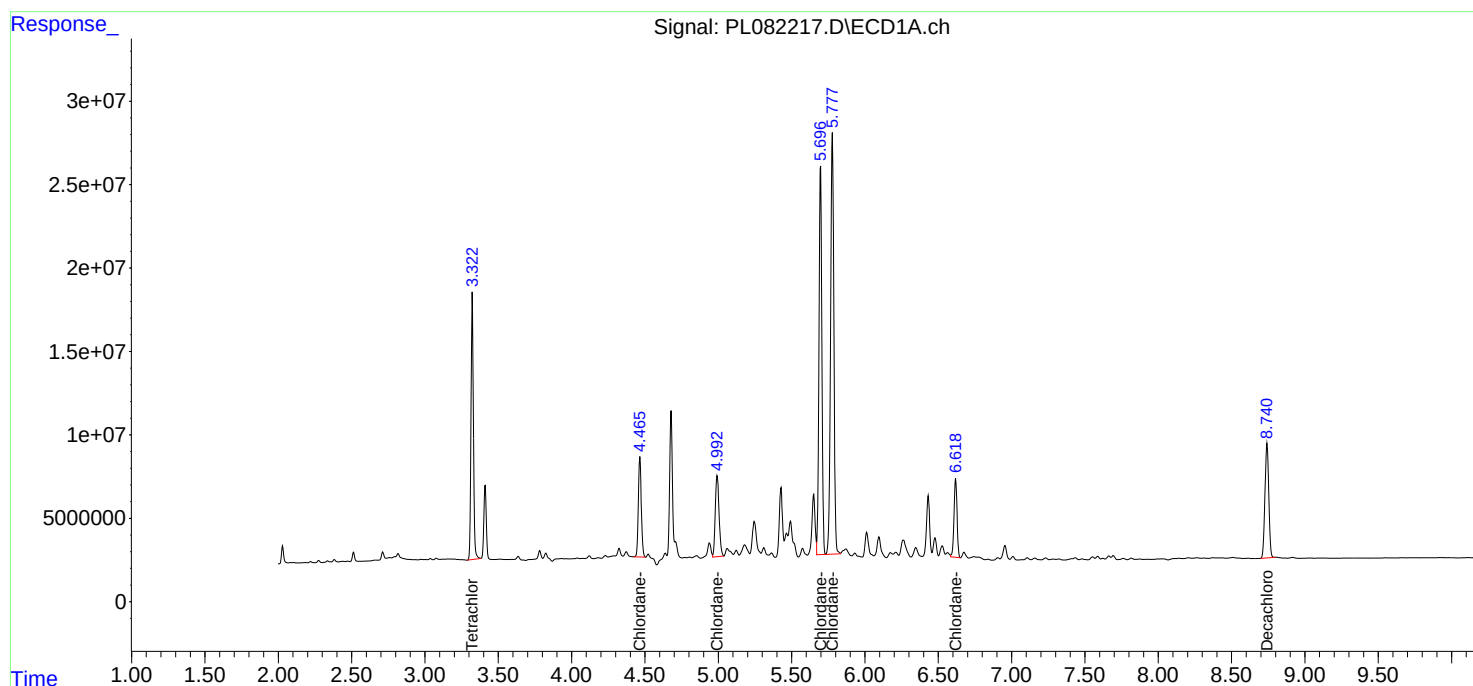


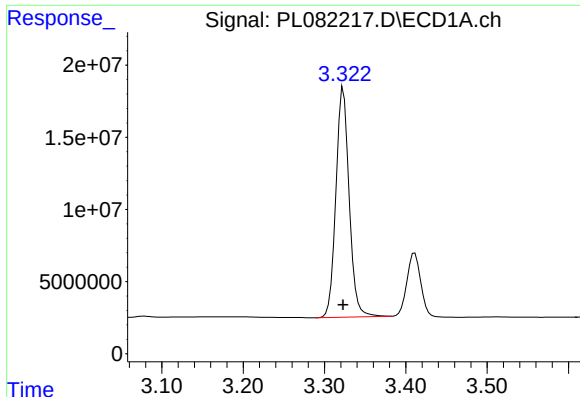

#1 Tetrachloro-m-xylene


R.T.: 3.323 min
Delta R.T.: 0.000 min
Response: 180300773
Conc: 73.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

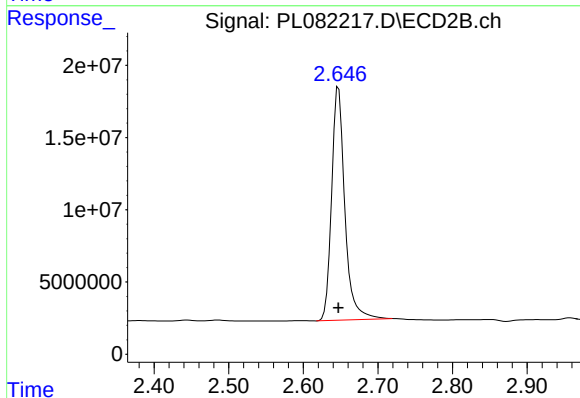


#1 Tetrachloro-m-xylene

R.T.: 2.647 min
Delta R.T.: 0.000 min
Response: 199689104
Conc: 73.49 ng/ml

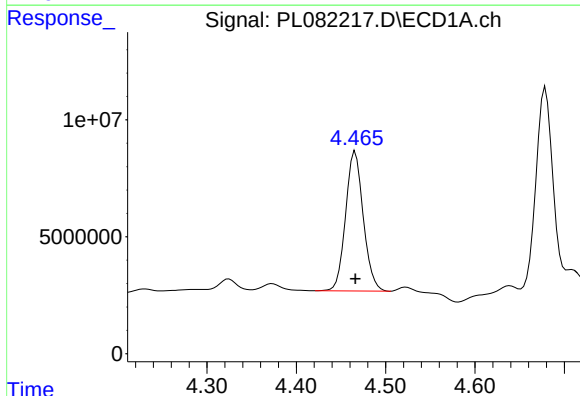


#23 Chlordane-1

R.T.: 4.466 min
Delta R.T.: 0.000 min
Response: 82231833
Conc: 733.60 ng/ml

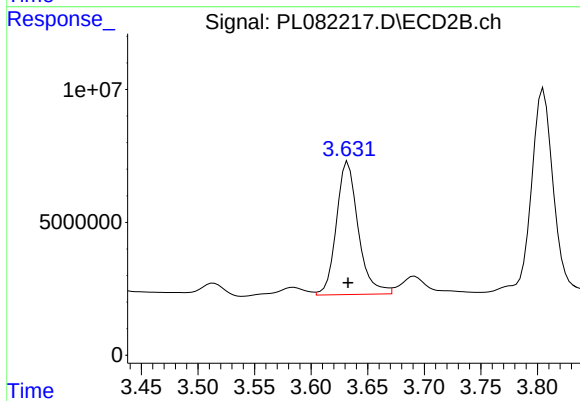

#23 Chlordane-1


R.T.: 3.633 min
Delta R.T.: 0.000 min
Response: 67309872
Conc: 748.15 ng/ml

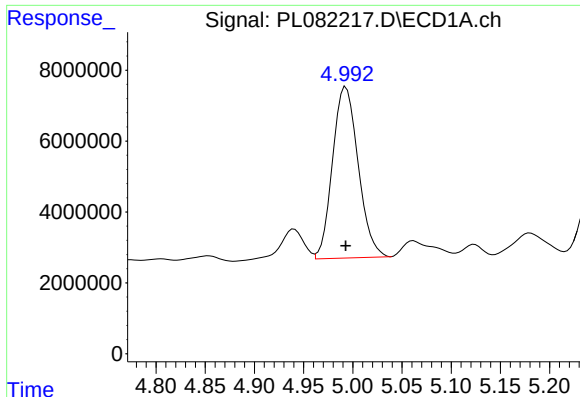

#24 Chlordane-2


R.T.: 4.993 min
Delta R.T.: 0.000 min
Response: 87548387
Conc: 738.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

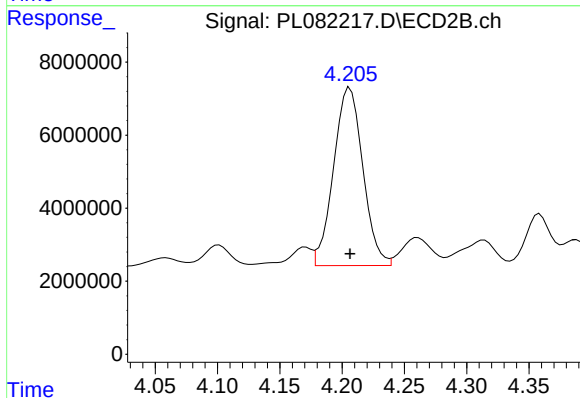


#24 Chlordane-2

R.T.: 4.206 min
Delta R.T.: 0.000 min
Response: 79901535
Conc: 736.46 ng/ml

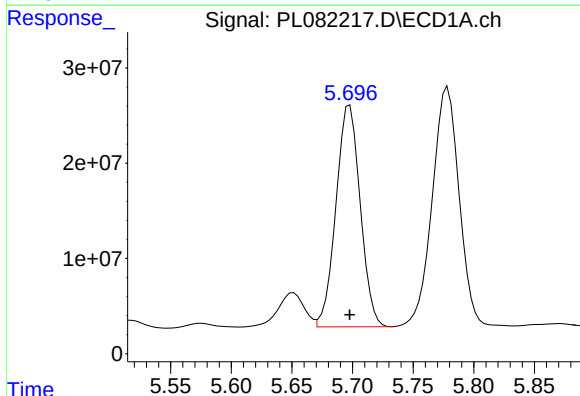


#25 Chlordane-3

R.T.: 5.698 min
Delta R.T.: 0.000 min
Response: 323341650
Conc: 733.69 ng/ml

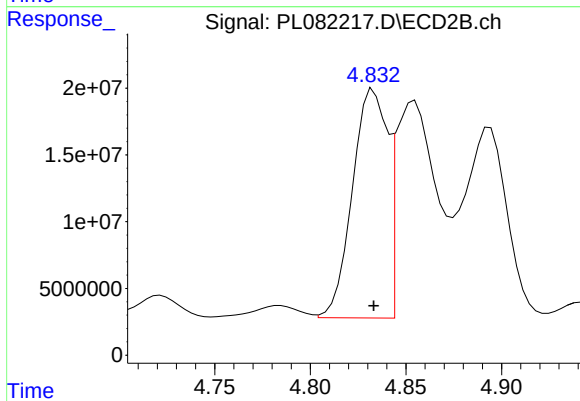

#25 Chlordane-3


R.T.: 4.833 min
Delta R.T.: 0.000 min
Response: 217314291
Conc: 735.09 ng/ml

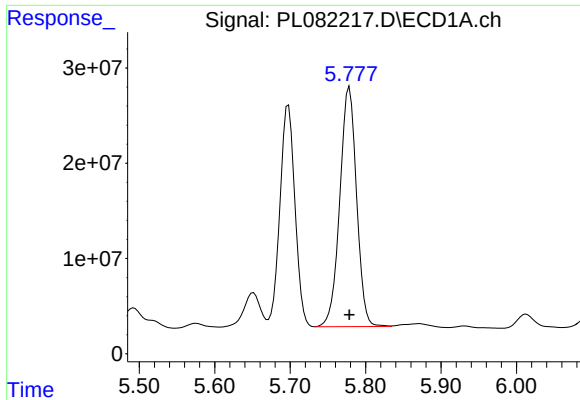

#26 Chlordane-4


R.T.: 5.779 min
Delta R.T.: 0.000 min
Response: 388455043
Conc: 742.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

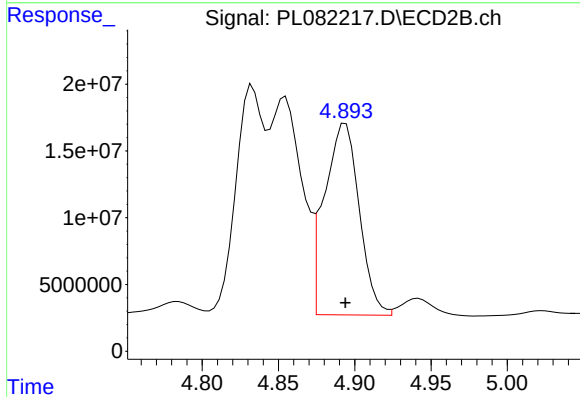


#26 Chlordane-4

R.T.: 4.894 min
Delta R.T.: 0.000 min
Response: 227376717
Conc: 740.49 ng/ml

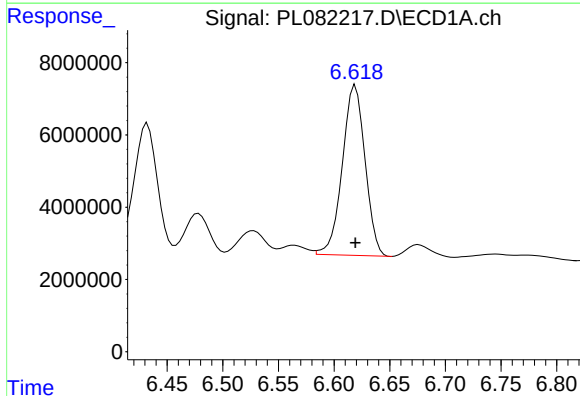


#27 Chlordane-5

R.T.: 6.619 min
Delta R.T.: 0.000 min
Response: 67074779
Conc: 730.80 ng/ml

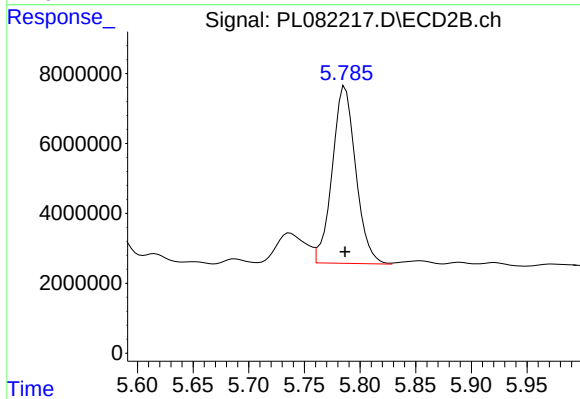

#27 Chlordane-5


R.T.: 5.787 min
Delta R.T.: 0.000 min
Response: 74482528
Conc: 732.41 ng/ml

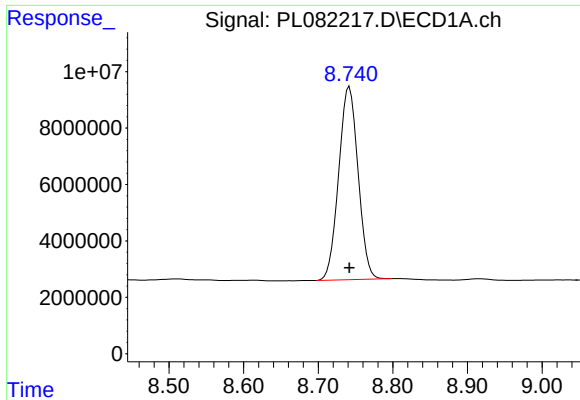

#28 Decachlorobiphenyl

R.T.: 8.742 min
Delta R.T.: 0.000 min
Response: 123582876
Conc: 73.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

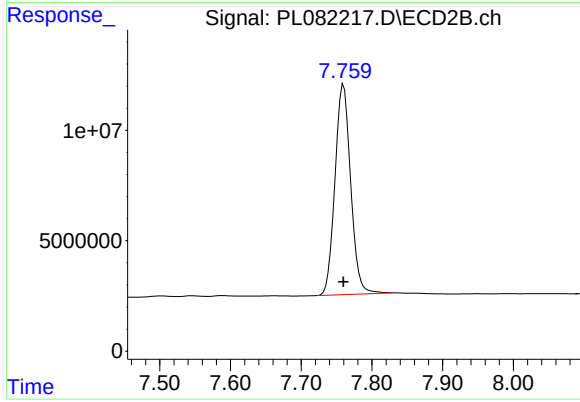

#28 Decachlorobiphenyl

R.T.: 7.760 min
Delta R.T.: 0.000 min
Response: 146968896
Conc: 73.42 ng/ml