

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042023\
 Data File : PL082219.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2023 20:09
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 01:53:43 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 21 01:44:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.323	2.647	61062684	65615618	24.983	24.355
28)	SA Decachlor...	8.742	7.760	44794150	53540410	26.232	26.288
Target Compounds							
23)	Chlordane-1	4.465	3.633	27870722	22450930	248.977	249.655
24)	Chlordane-2	4.992	4.206	30827430	28516459	257.474	259.507
25)	Chlordane-3	5.697	4.833	105.7E6	68822995	242.323	236.876
26)	Chlordane-4	5.778	4.894	129.1E6	73491897	247.588	241.918
27)	Chlordane-5	6.619	5.786	23538491	24574155	254.814	243.681



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042023\
Data File : PL082219.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2023 20:09
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 01:53:43 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 01:44:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

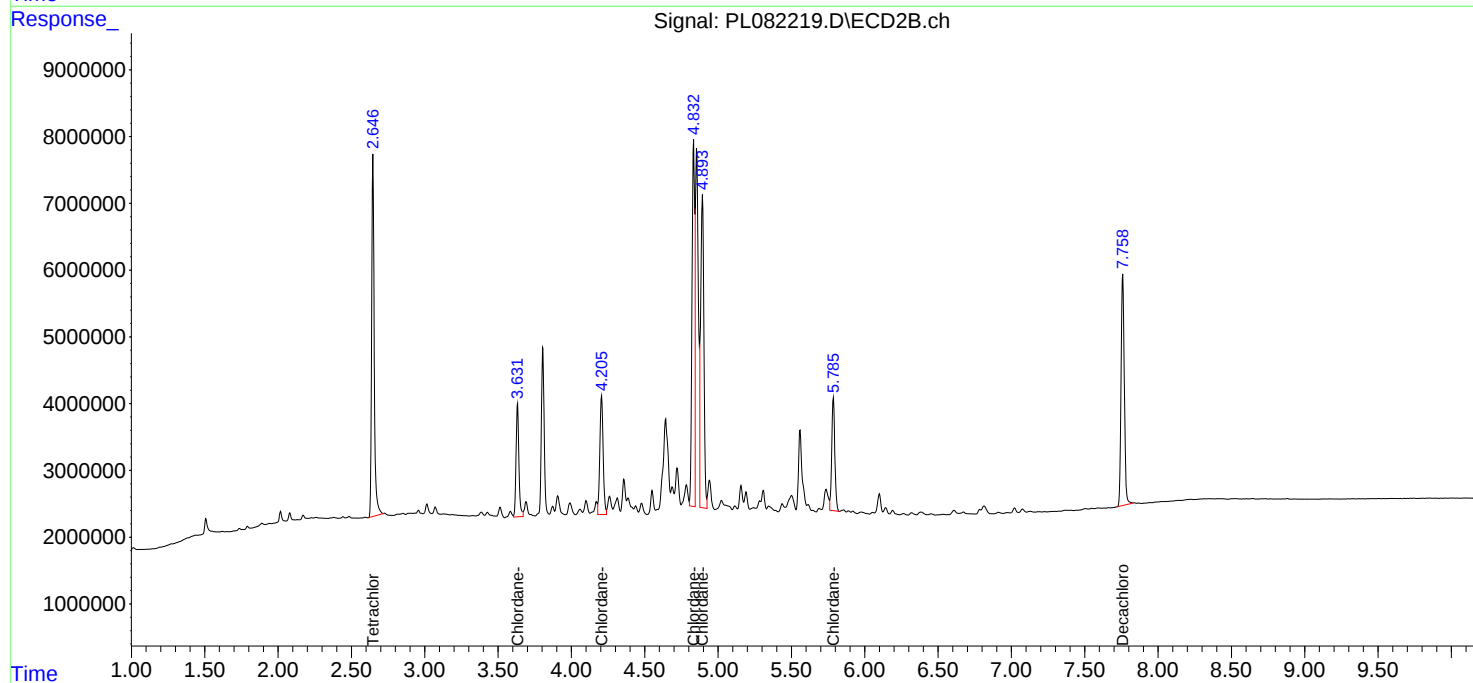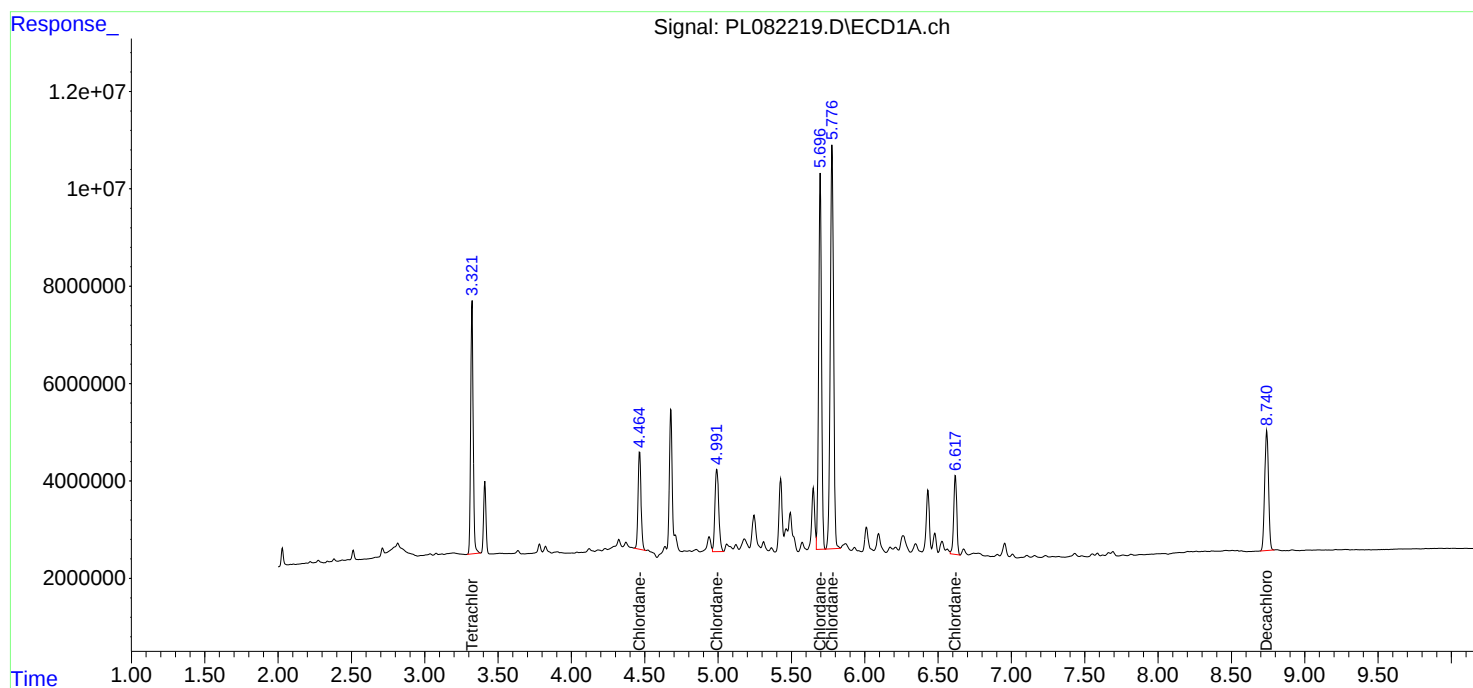


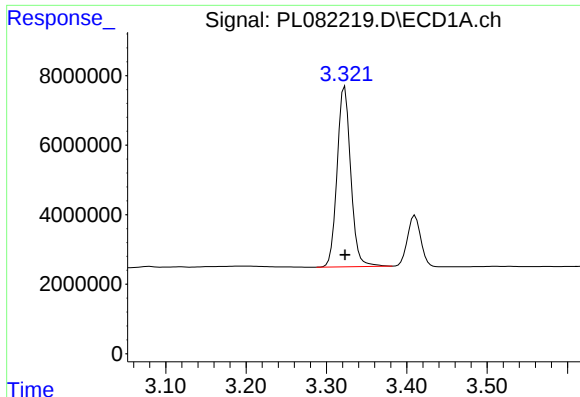

#1 Tetrachloro-m-xylene


R.T.: 3.323 min
Delta R.T.: 0.000 min
Response: 61062684
Conc: 24.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

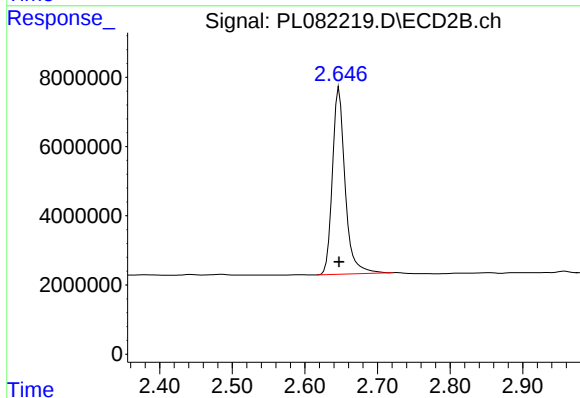


#1 Tetrachloro-m-xylene

R.T.: 2.647 min
Delta R.T.: 0.000 min
Response: 65615618
Conc: 24.35 ng/ml

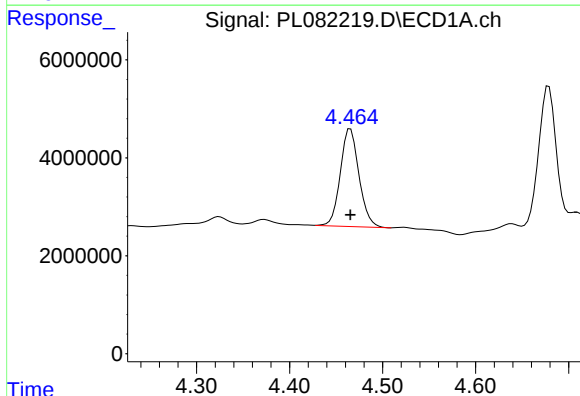


#23 Chlordane-1

R.T.: 4.465 min
Delta R.T.: 0.000 min
Response: 27870722
Conc: 248.98 ng/ml

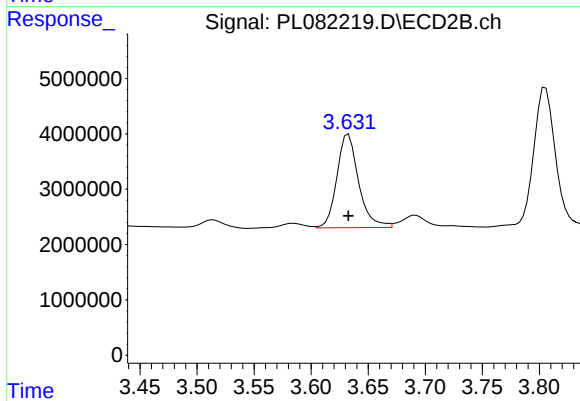

#23 Chlordane-1


R.T.: 3.633 min
Delta R.T.: 0.000 min
Response: 22450930
Conc: 249.66 ng/ml

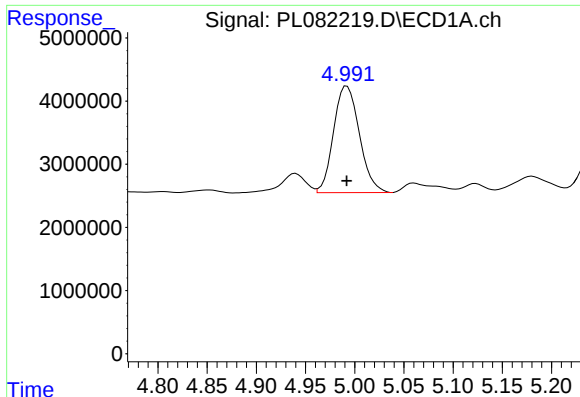

#24 Chlordane-2


R.T.: 4.992 min
Delta R.T.: 0.000 min
Response: 30827430
Conc: 257.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

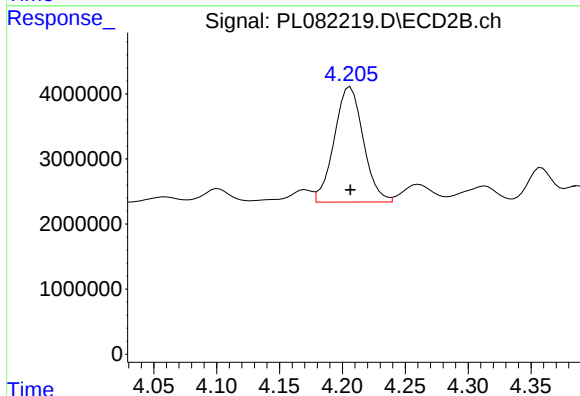


#24 Chlordane-2

R.T.: 4.206 min
Delta R.T.: 0.000 min
Response: 28516459
Conc: 259.51 ng/ml

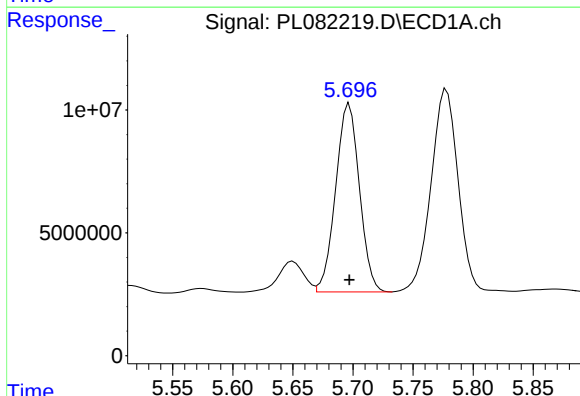


#25 Chlordane-3

R.T.: 5.697 min
Delta R.T.: 0.000 min
Response: 105711471
Conc: 242.32 ng/ml

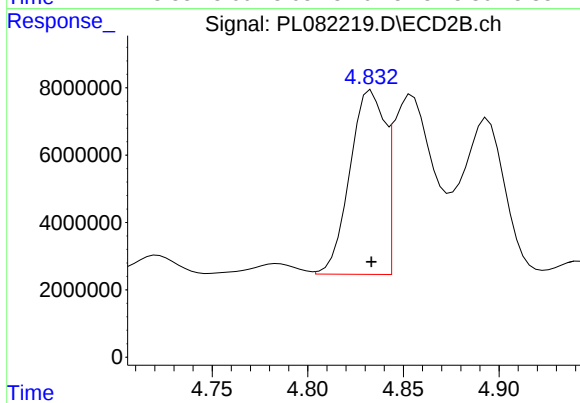

#25 Chlordane-3


R.T.: 4.833 min
Delta R.T.: 0.000 min
Response: 68822995
Conc: 236.88 ng/ml

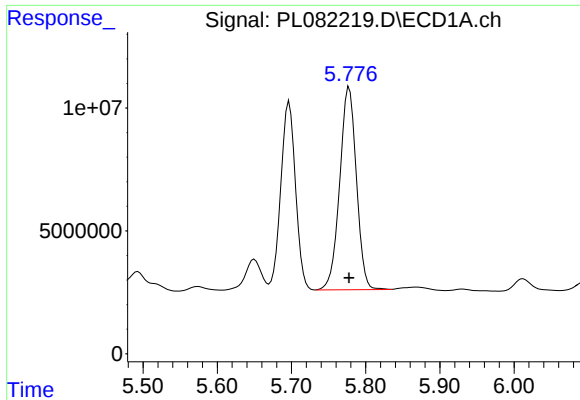

#26 Chlordane-4


R.T.: 5.778 min
Delta R.T.: 0.000 min
Response: 129077477
Conc: 247.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

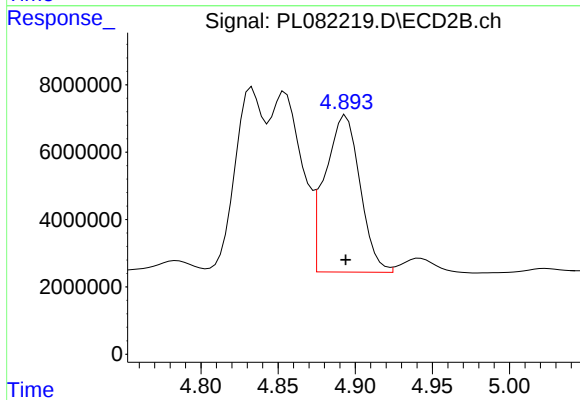


#26 Chlordane-4

R.T.: 4.894 min
Delta R.T.: 0.000 min
Response: 73491897
Conc: 241.92 ng/ml

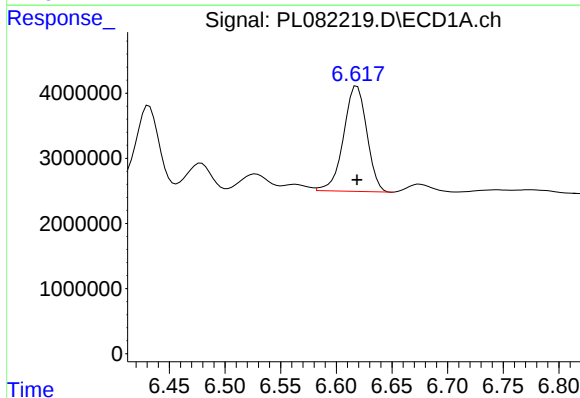


#27 Chlordane-5

R.T.: 6.619 min
Delta R.T.: 0.000 min
Response: 23538491
Conc: 254.81 ng/ml

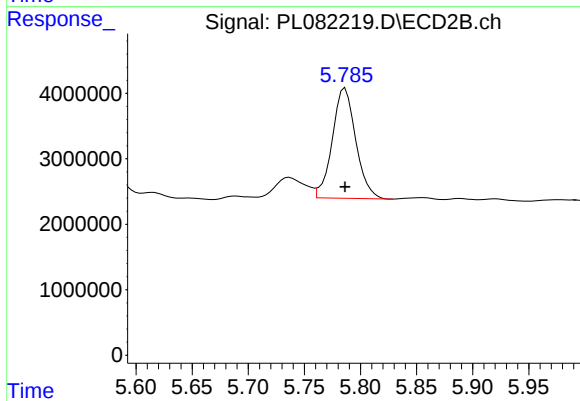

#27 Chlordane-5


R.T.: 5.786 min
Delta R.T.: 0.000 min
Response: 24574155
Conc: 243.68 ng/ml

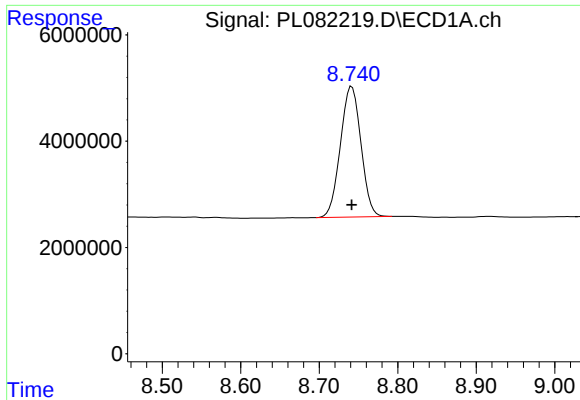

#28 Decachlorobiphenyl

R.T.: 8.742 min
Delta R.T.: 0.000 min
Response: 44794150
Conc: 26.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

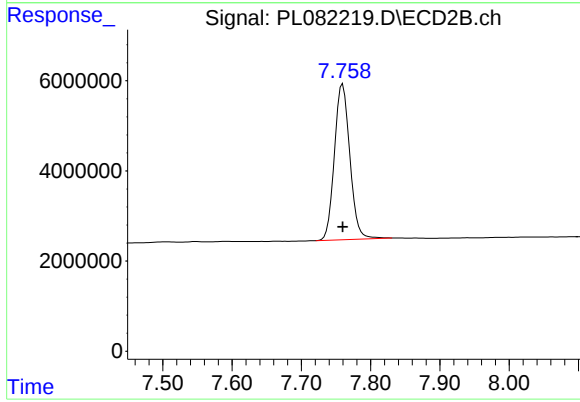

#28 Decachlorobiphenyl

R.T.: 7.760 min
Delta R.T.: 0.000 min
Response: 53540410
Conc: 26.29 ng/ml