

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042023\
 Data File : PL082227.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2023 22:01
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL042023CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 01:58:15 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 21 01:57:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.323	2.647	125.1E6	134.9E6	52.129	50.946
28)	SA Decachlor...	8.741	7.760	87912099	103.0E6	50.848	49.794
Target Compounds							
23)	Chlordane-1	4.466	3.633	56807489	44764894	513.901	504.762
24)	Chlordane-2	4.992	4.206	62251714	55608461	522.893	495.872
25)	Chlordane-3	5.697	4.833	222.4E6	142.4E6	515.132	501.229
26)	Chlordane-4	5.778	4.894	268.4E6	153.1E6	516.170	512.900
27)	Chlordane-5	6.619	5.786	47867779	50573726	509.787	512.334



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042023\
Data File : PL082227.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2023 22:01
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL042023CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 01:58:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 01:57:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

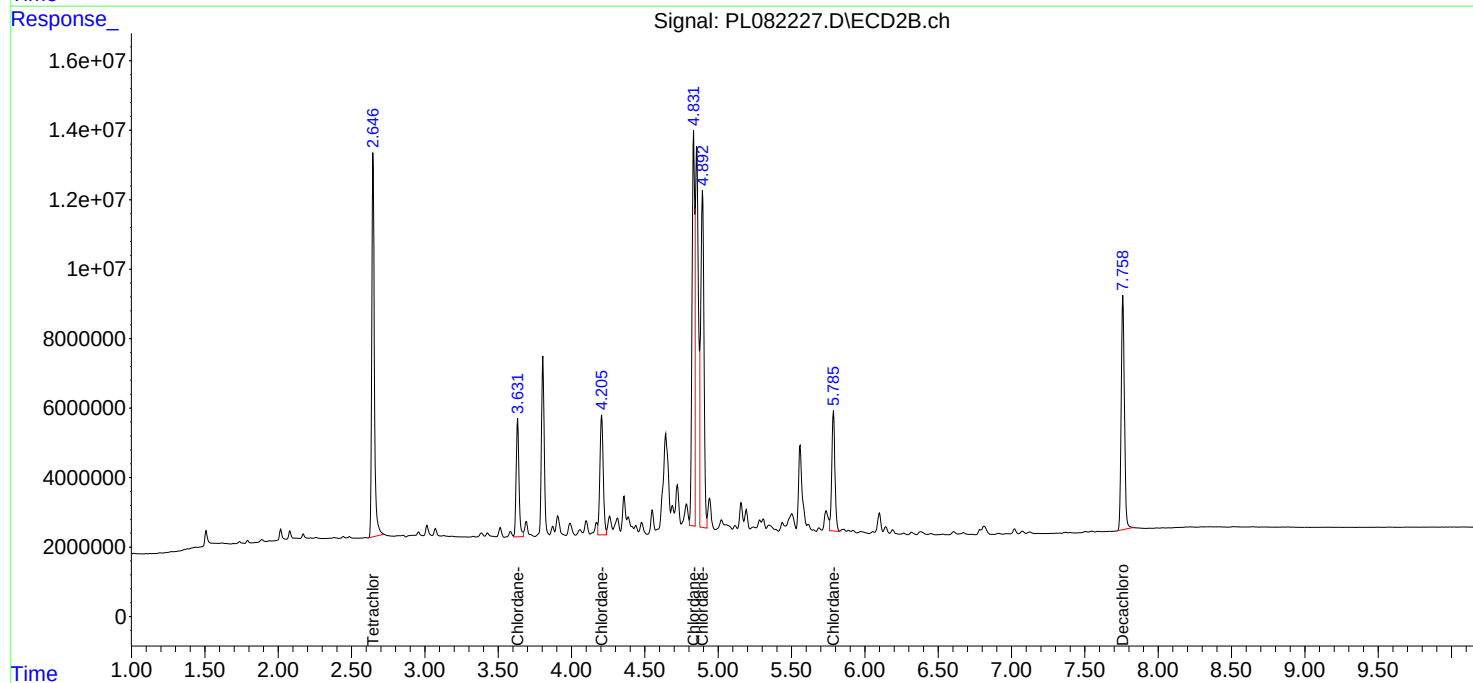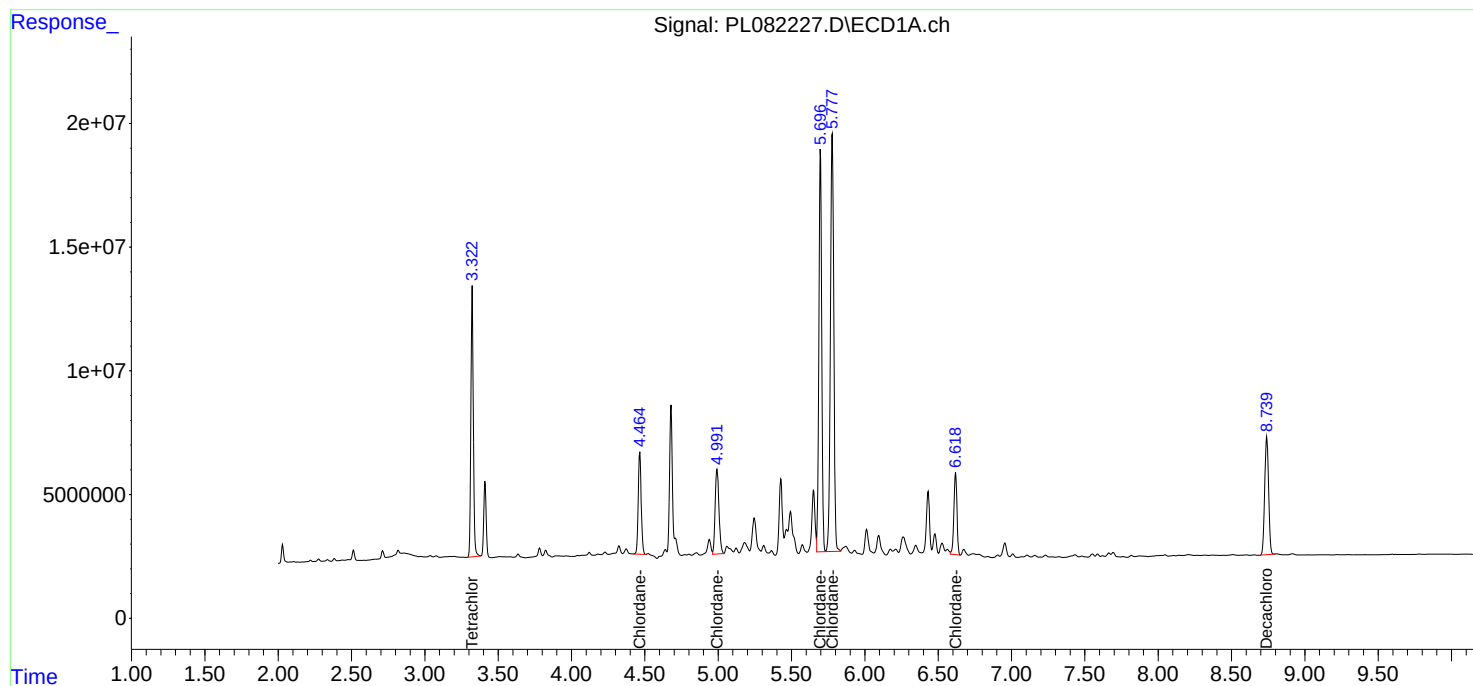


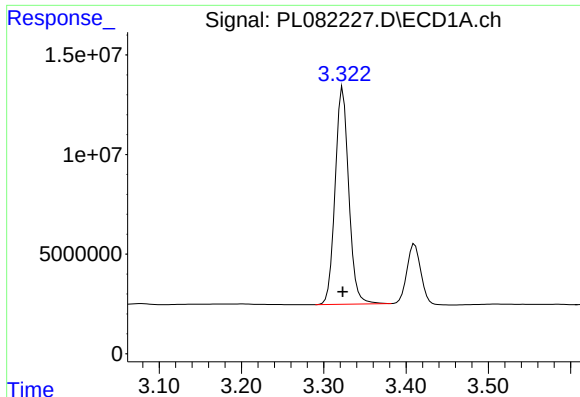

#1 Tetrachloro-m-xylene


R.T.: 3.323 min
Delta R.T.: 0.000 min
Response: 125127344
Conc: 52.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL042023CHLOR

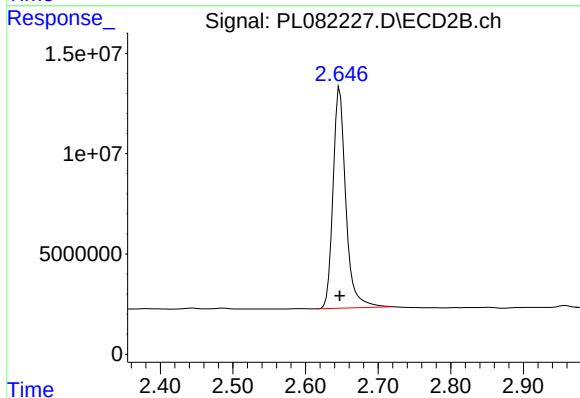


#1 Tetrachloro-m-xylene

R.T.: 2.647 min
Delta R.T.: 0.000 min
Response: 134898117
Conc: 50.95 ng/ml

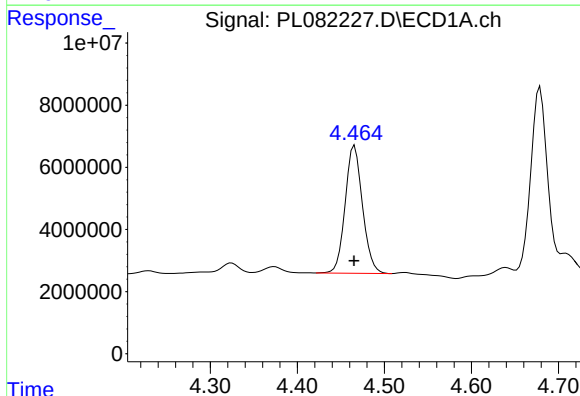


#23 Chlordane-1

R.T.: 4.466 min
Delta R.T.: 0.000 min
Response: 56807489
Conc: 513.90 ng/ml

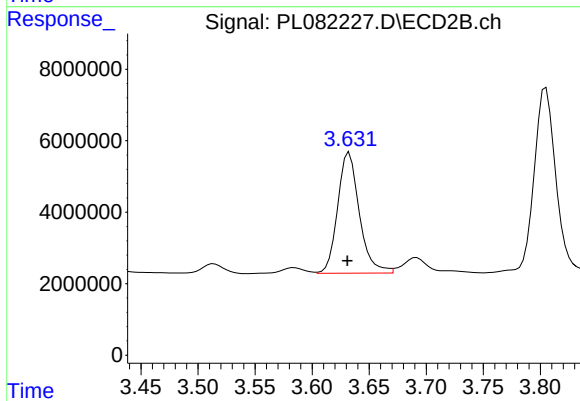

#23 Chlordane-1


R.T.: 3.633 min
Delta R.T.: 0.002 min
Response: 44764894
Conc: 504.76 ng/ml

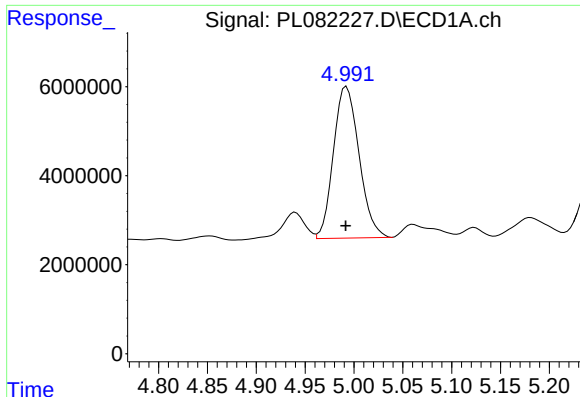

#24 Chlordane-2


R.T.: 4.992 min
Delta R.T.: 0.000 min
Response: 62251714
Conc: 522.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL042023CHLOR

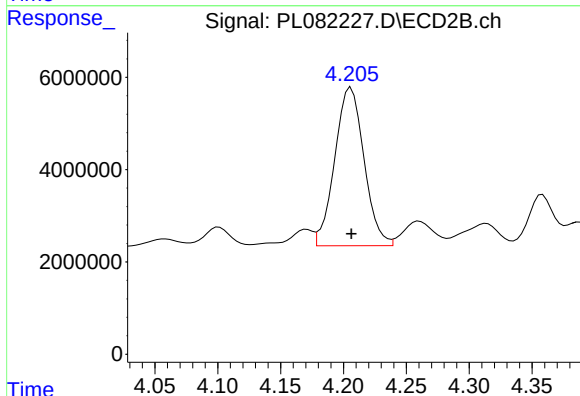


#24 Chlordane-2

R.T.: 4.206 min
Delta R.T.: 0.000 min
Response: 55608461
Conc: 495.87 ng/ml

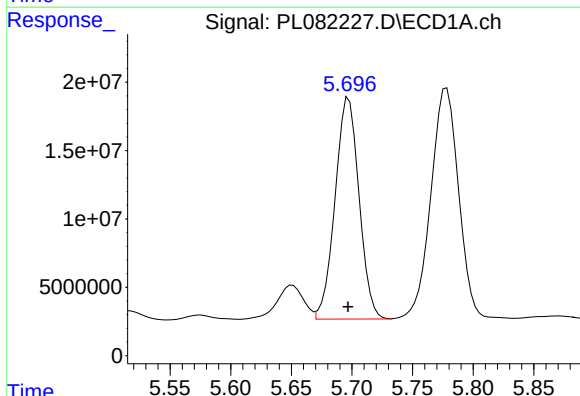


#25 Chlordane-3

R.T.: 5.697 min
Delta R.T.: 0.000 min
Response: 222384246
Conc: 515.13 ng/ml

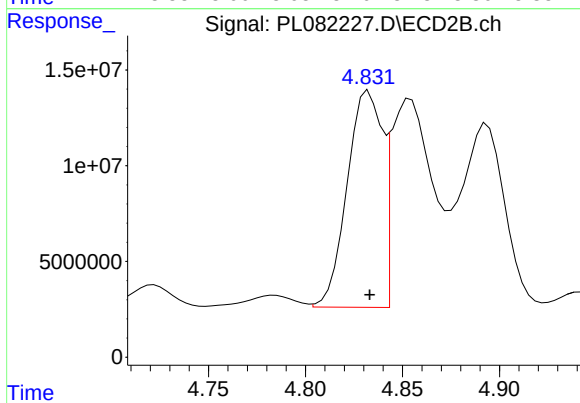

#25 Chlordane-3


R.T.: 4.833 min
Delta R.T.: 0.000 min
Response: 142404177
Conc: 501.23 ng/ml

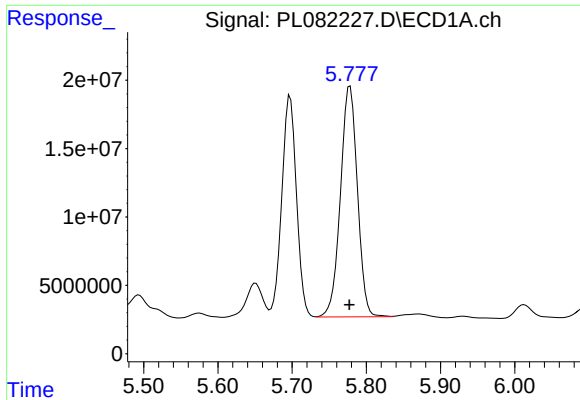

#26 Chlordane-4


R.T.: 5.778 min
Delta R.T.: 0.000 min
Response: 268364509
Conc: 516.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL042023CHLOR

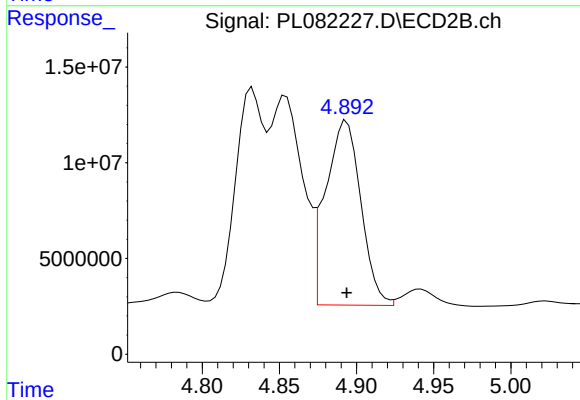


#26 Chlordane-4

R.T.: 4.894 min
Delta R.T.: 0.000 min
Response: 153052898
Conc: 512.90 ng/ml

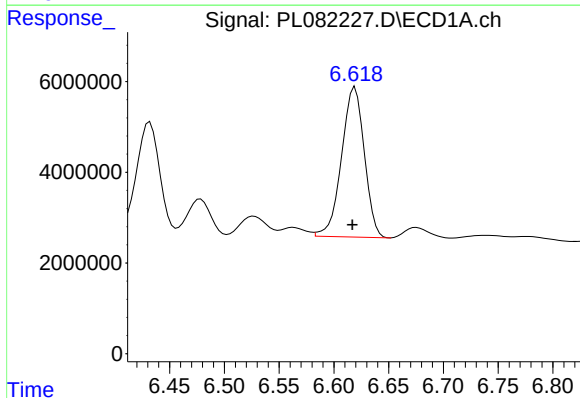


#27 Chlordane-5

R.T.: 6.619 min
Delta R.T.: 0.002 min
Response: 47867779
Conc: 509.79 ng/ml

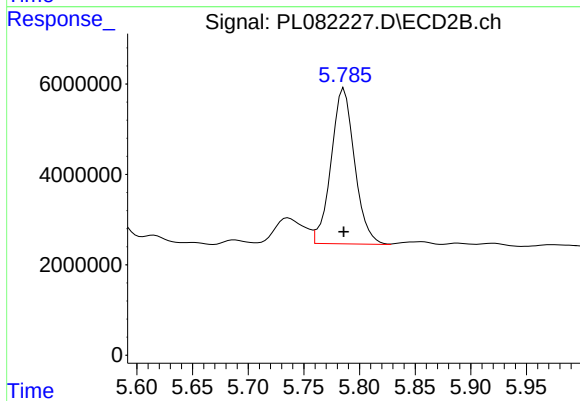

#27 Chlordane-5


R.T.: 5.786 min
Delta R.T.: 0.000 min
Response: 50573726
Conc: 512.33 ng/ml

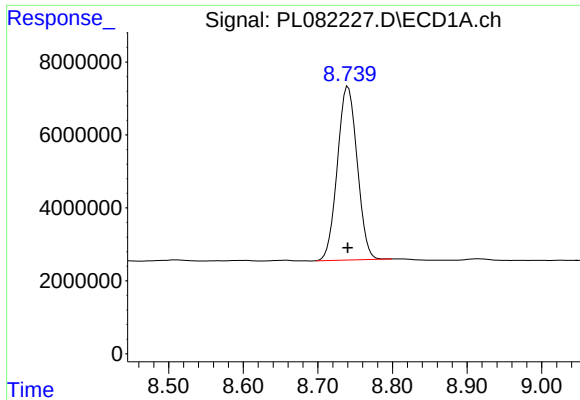

#28 Decachlorobiphenyl

R.T.: 8.741 min
Delta R.T.: 0.000 min
Response: 87912099
Conc: 50.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL042023CHLOR

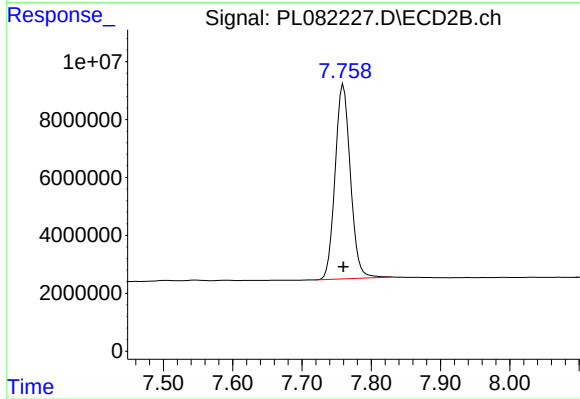

#28 Decachlorobiphenyl

R.T.: 7.760 min
Delta R.T.: 0.000 min
Response: 103046766
Conc: 49.79 ng/ml