

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042120\
 Data File : PL058244.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Apr 2020 17:45
 Operator : AJ\MA
 Sample : PB128355BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB128355BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 00:58:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.456	3.955	219.8E6	44569327	21.808	20.537
28)	SA Decachlor...	8.205	8.979	211.2E6	45418282	20.486	20.333
Target Compounds							
2)	A alpha-BHC	3.897	0.000	4840883	0	0.279	N.D. #
4)	MA Heptachlor	0.000	5.134	0	4860475	N.D.	1.448 #
7)	B delta-BHC	0.000	4.987f	0	5147495	N.D.	4.001 #
11)	B alpha-Chl...	5.467	0.000	1653586	0	0.124	N.D. #
13)	MA Dieldrin	5.764	0.000	394549	0	0.030	N.D. #
15)	B Endosulfa...	0.000	6.869f	0	601088	N.D.	0.232 #
16)	A 4,4'-DDD	6.109f	0.000	374124	0	0.037	N.D. #
18)	B Endrin al...	6.434f	0.000	3325265	0	0.356	N.D. #
23)	Chlordane-1	4.352f	0.000	10577468	0	28.599	N.D. #
26)	Chlordane-4	5.467	0.000	1653586	0	1.590	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042120\
Data File : PL058244.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Apr 2020 17:45
Operator : AJ\MA
Sample : PB128355BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleID :
PB128355BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 00:58:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

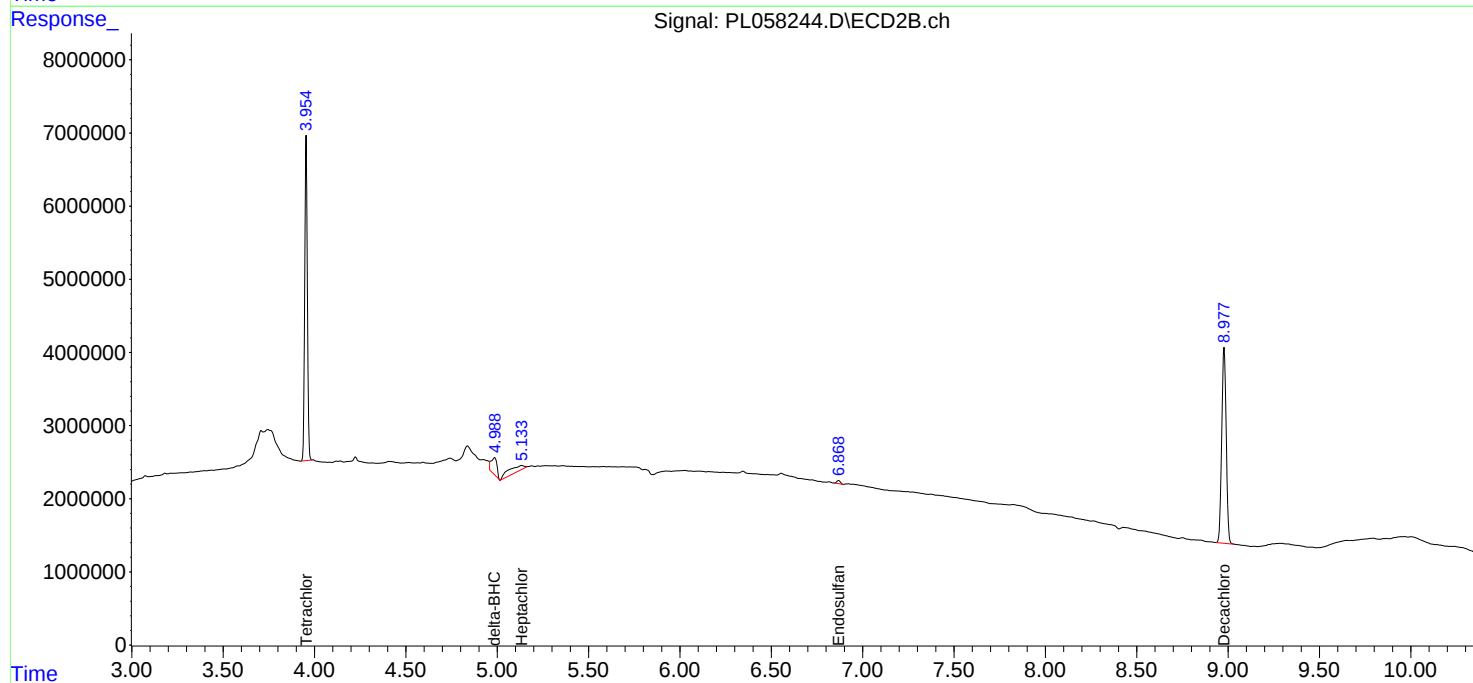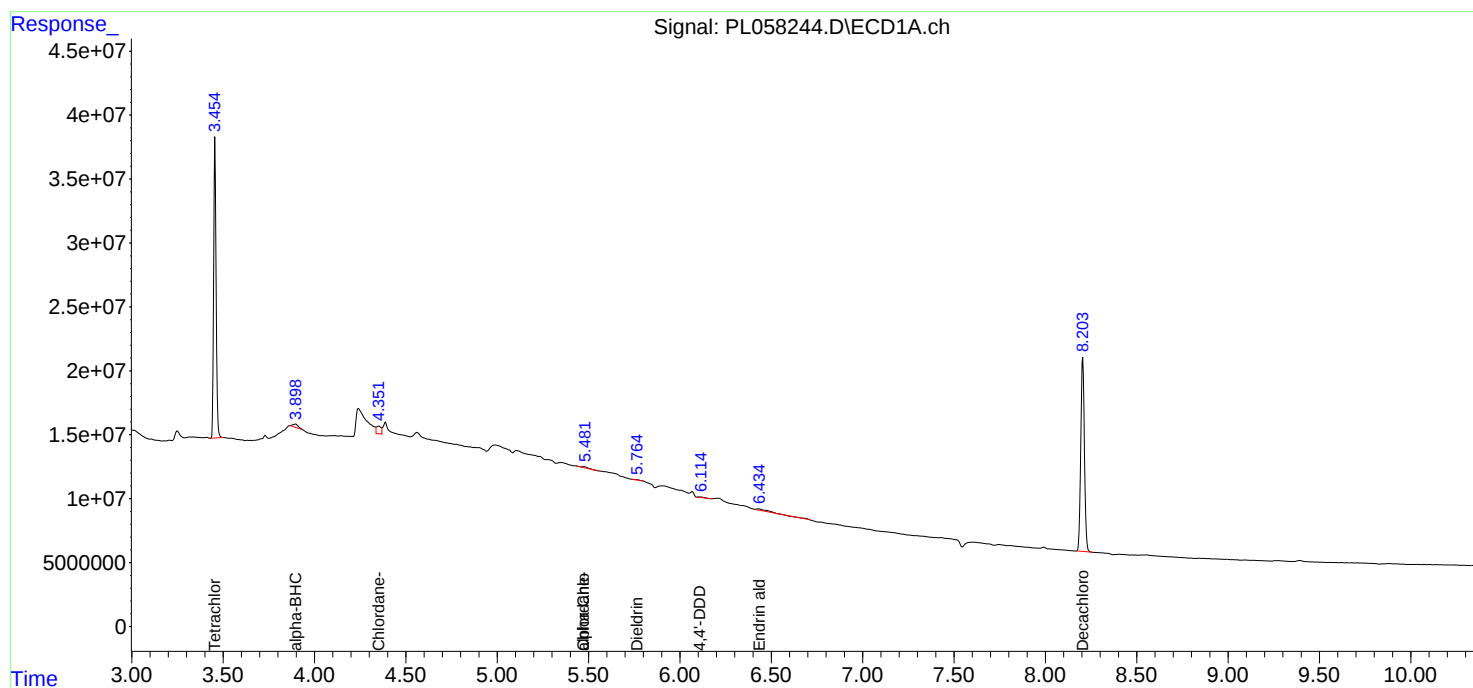


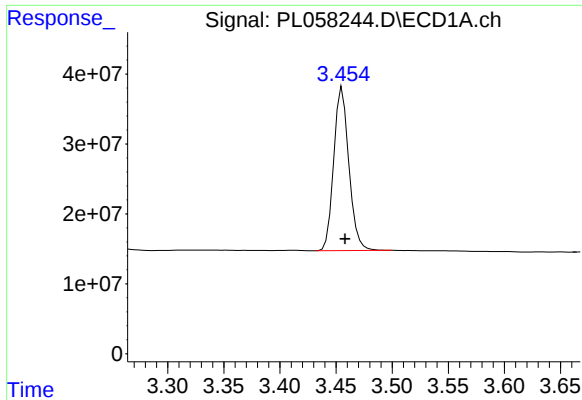

#1 Tetrachloro-m-xylene


R.T.: 3.456 min
Delta R.T.: -0.002 min
Response: 219844221
Conc: 21.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB128355BL

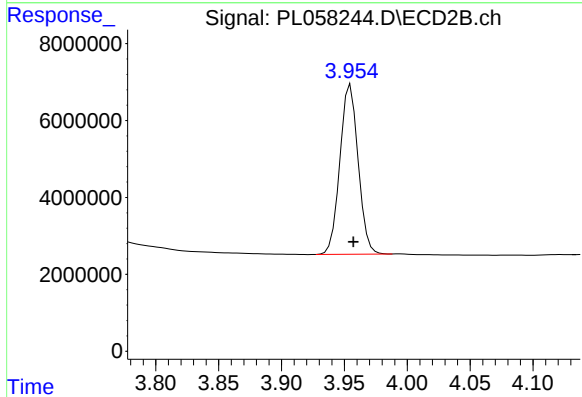


#1 Tetrachloro-m-xylene

R.T.: 3.955 min
Delta R.T.: -0.002 min
Response: 44569327
Conc: 20.54 ng/ml

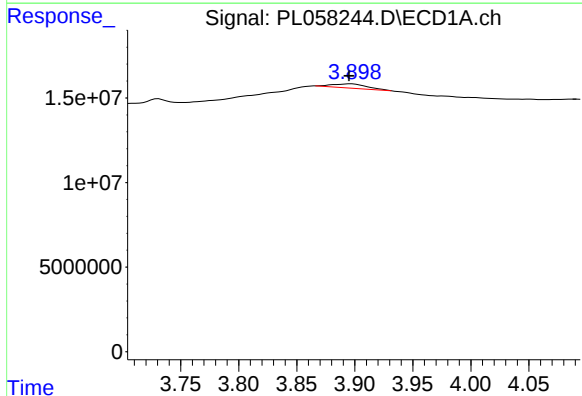


#2 alpha-BHC

R.T.: 3.897 min
Delta R.T.: 0.002 min
Response: 4840883
Conc: 0.28 ng/ml

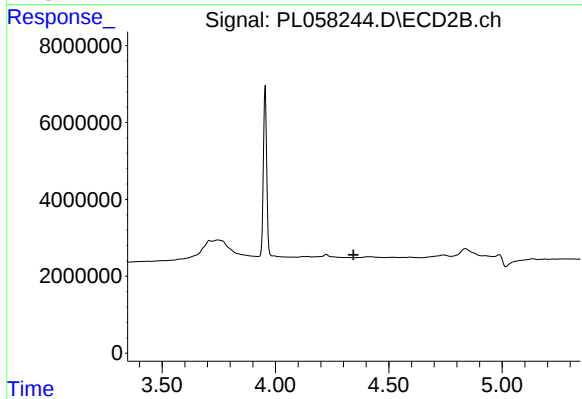

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.345 min
Response: 0
Conc: N.D.

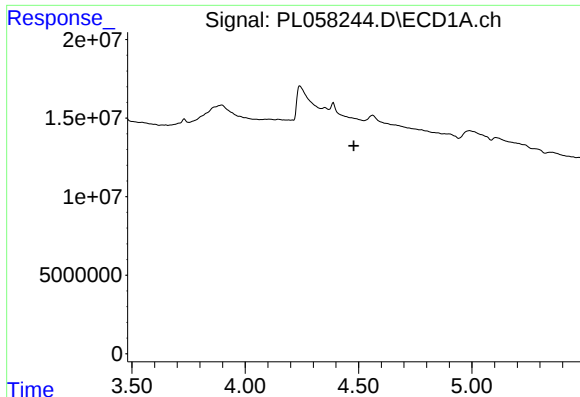

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB128355BL

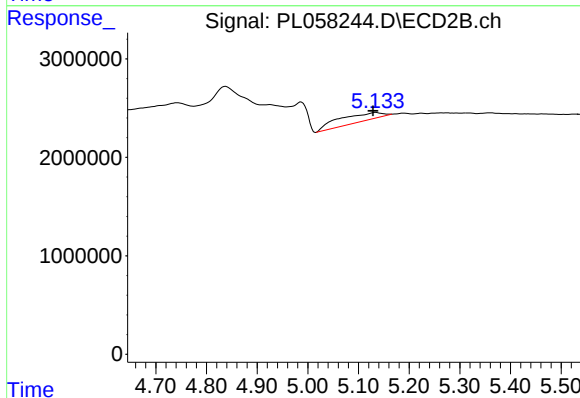


#4 Heptachlor

R.T.: 5.134 min
Delta R.T.: 0.005 min
Response: 4860475
Conc: 1.45 ng/ml

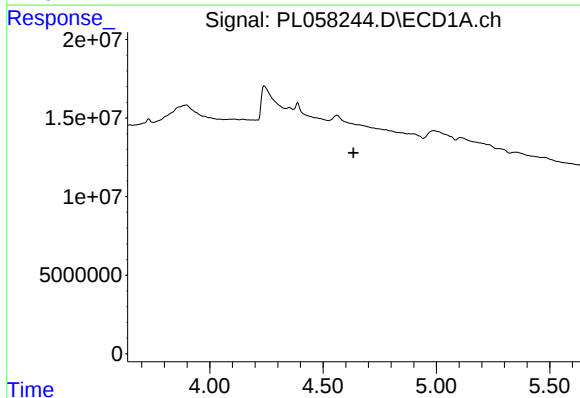


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.634 min
Response: 0
Conc: N.D.

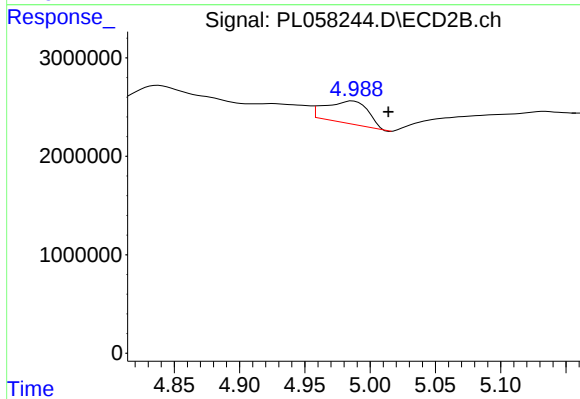

#7 delta-BHC


R.T.: 4.987 min
Delta R.T.: -0.027 min
Response: 5147495
Conc: 4.00 ng/ml

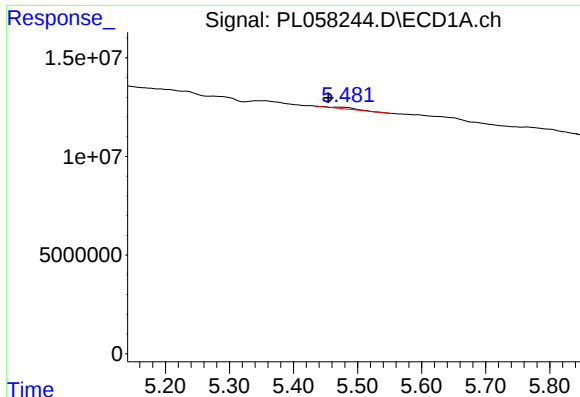

#11 alpha-Chlordane


R.T.: 5.467 min
Delta R.T.: 0.013 min
Response: 1653586
Conc: 0.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB128355BL

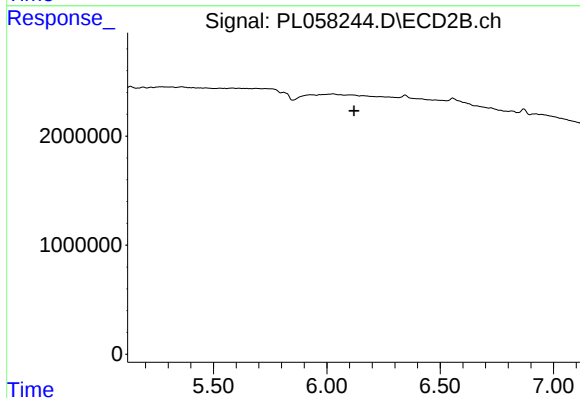


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.120 min
Response: 0
Conc: N.D.

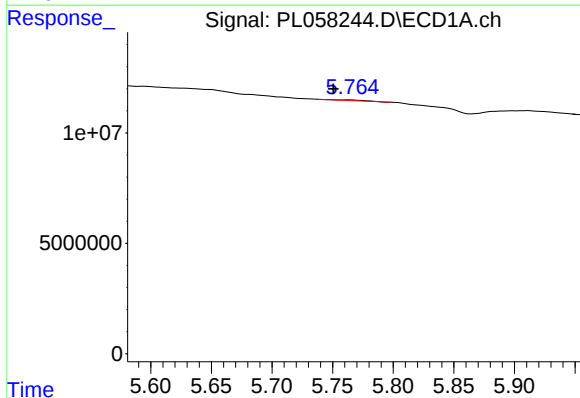


#13 Dieldrin

R.T.: 5.764 min
Delta R.T.: 0.014 min
Response: 394549
Conc: 0.03 ng/ml

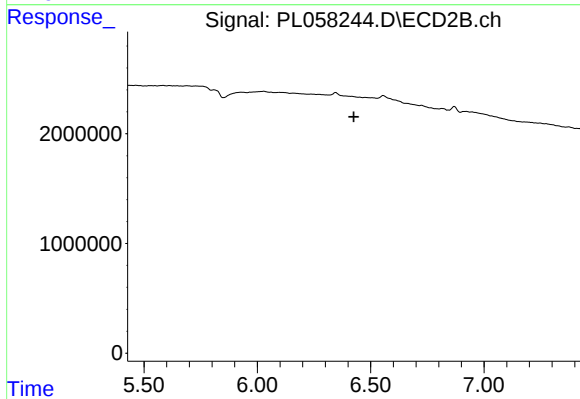

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.425 min
Response: 0
Conc: N.D.

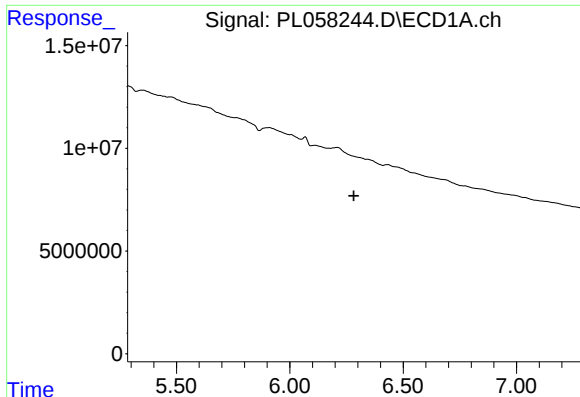

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.282 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB128355BL

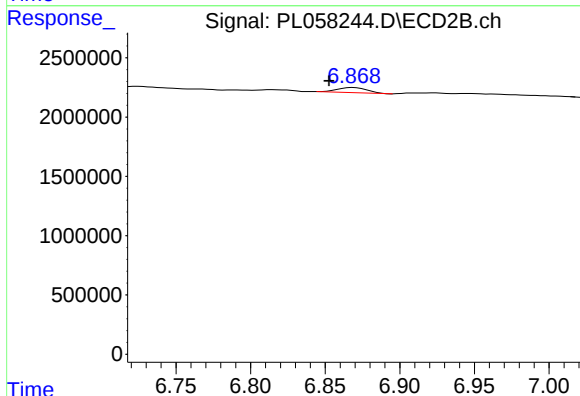


#15 Endosulfan II

R.T.: 6.869 min
Delta R.T.: 0.016 min
Response: 601088
Conc: 0.23 ng/ml

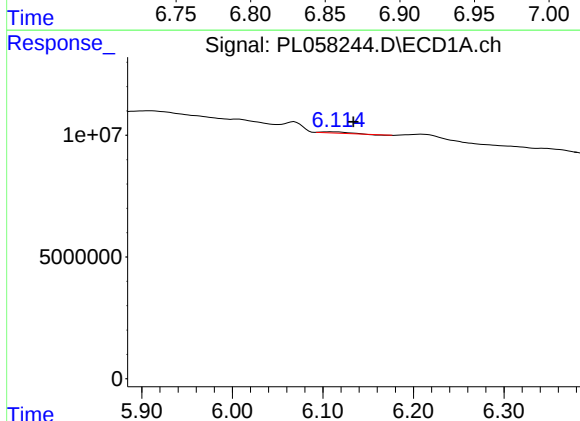


#16 4,4'-DDD

R.T.: 6.109 min
Delta R.T.: -0.025 min
Response: 374124
Conc: 0.04 ng/ml

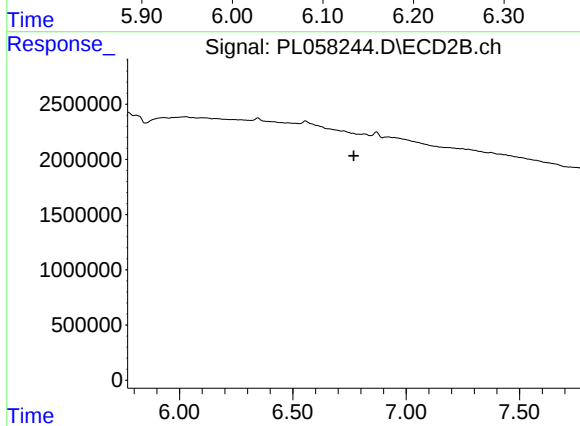

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.769 min
Response: 0
Conc: N.D.

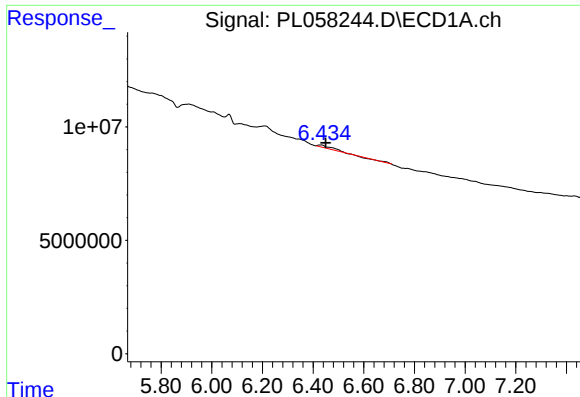

#18 Endrin aldehyde


R.T.: 6.434 min
Delta R.T.: -0.016 min
Response: 3325265
Conc: 0.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB128355BL

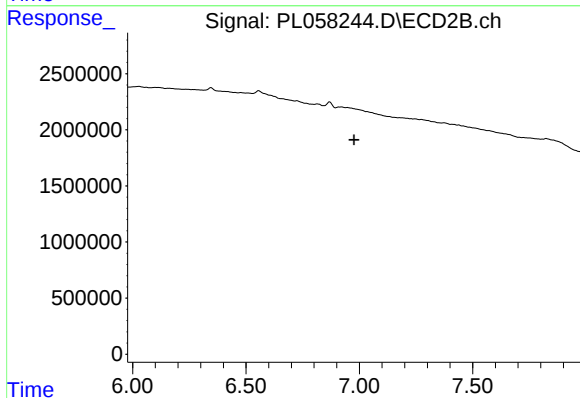


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.976 min
Response: 0
Conc: N.D.

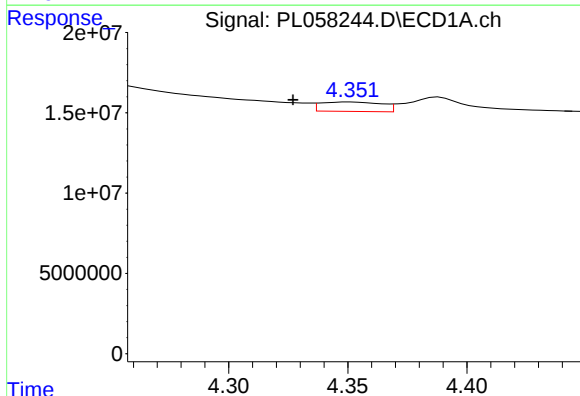


#23 Chlordane-1

R.T.: 4.352 min
Delta R.T.: 0.025 min
Response: 10577468
Conc: 28.60 ng/ml

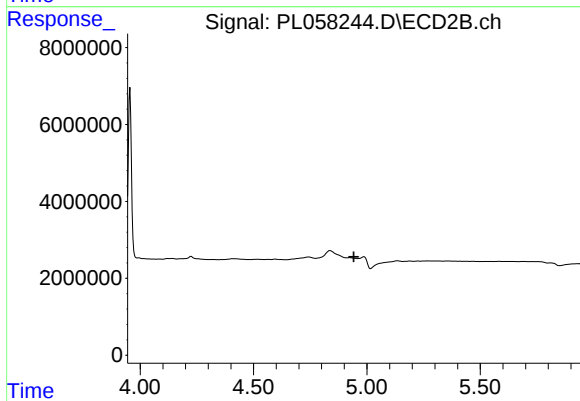

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

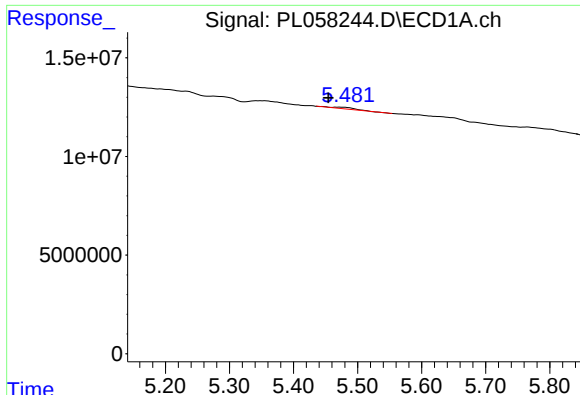

#26 Chlordane-4


R.T.: 5.467 min
Delta R.T.: 0.013 min
Response: 1653586
Conc: 1.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB128355BL

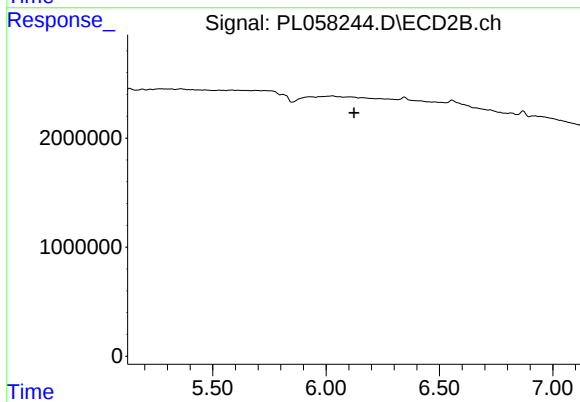


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.123 min
Response: 0
Conc: N.D.

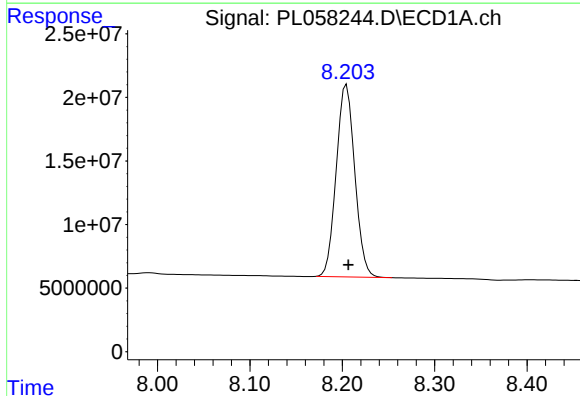

#28 Decachlorobiphenyl

R.T.: 8.205 min
Delta R.T.: -0.002 min
Response: 211177151
Conc: 20.49 ng/ml

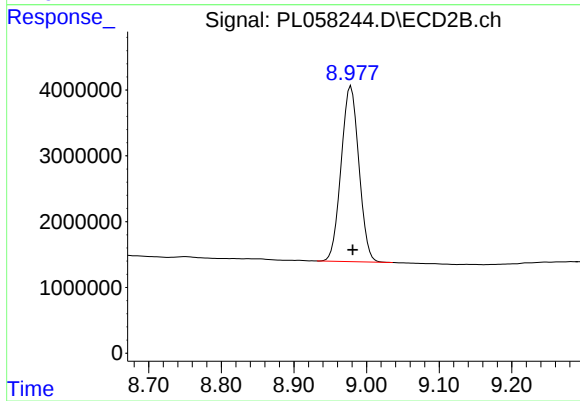

#28 Decachlorobiphenyl

R.T.: 8.979 min
Delta R.T.: -0.002 min
Response: 45418282
Conc: 20.33 ng/ml