

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042120\
 Data File : PL058263.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Apr 2020 22:14
 Operator : AJ\MA
 Sample : L2327-33
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-6-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 01:04:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.455	3.955	96666618	20407945	9.589	9.404
28)	SA Decachlor...	8.203	8.978	115.7E6	24875558	11.225	11.136
Target Compounds							
2)	A alpha-BHC	3.899	0.000	3277419	0	0.189	N.D. #
3)	MA gamma-BHC...	4.183	0.000	91308	0	0.006	N.D. #
4)	MA Heptachlor	4.484	5.135	490439	3836484	0.031	1.143 #
7)	B delta-BHC	0.000	4.985f	0	4196912	N.D.	3.636 #
8)	B Heptachlo...	0.000	5.815	0	680998	N.D.	0.252 #
9)	A Endosulfan I	5.493f	0.000	621745	0	0.051	N.D. #
11)	B alpha-Chl...	5.446	0.000	3815663	0	0.287	N.D. #
15)	B Endosulfa...	0.000	6.869f	0	441157	N.D.	0.170 #
16)	A 4,4'-DDD	6.107f	0.000	1544752	0	0.155	N.D. #
18)	B Endrin al...	6.462	0.000	1077581	0	0.115	N.D. #
24)	Chlordane-2	4.858f	0.000	1011783	0	2.506	N.D. #
26)	Chlordane-4	5.446	0.000	3815663	0	3.668	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042120\
Data File : PL058263.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Apr 2020 22:14
Operator : AJ\MA
Sample : L2327-33
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
TP-6-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 01:04:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

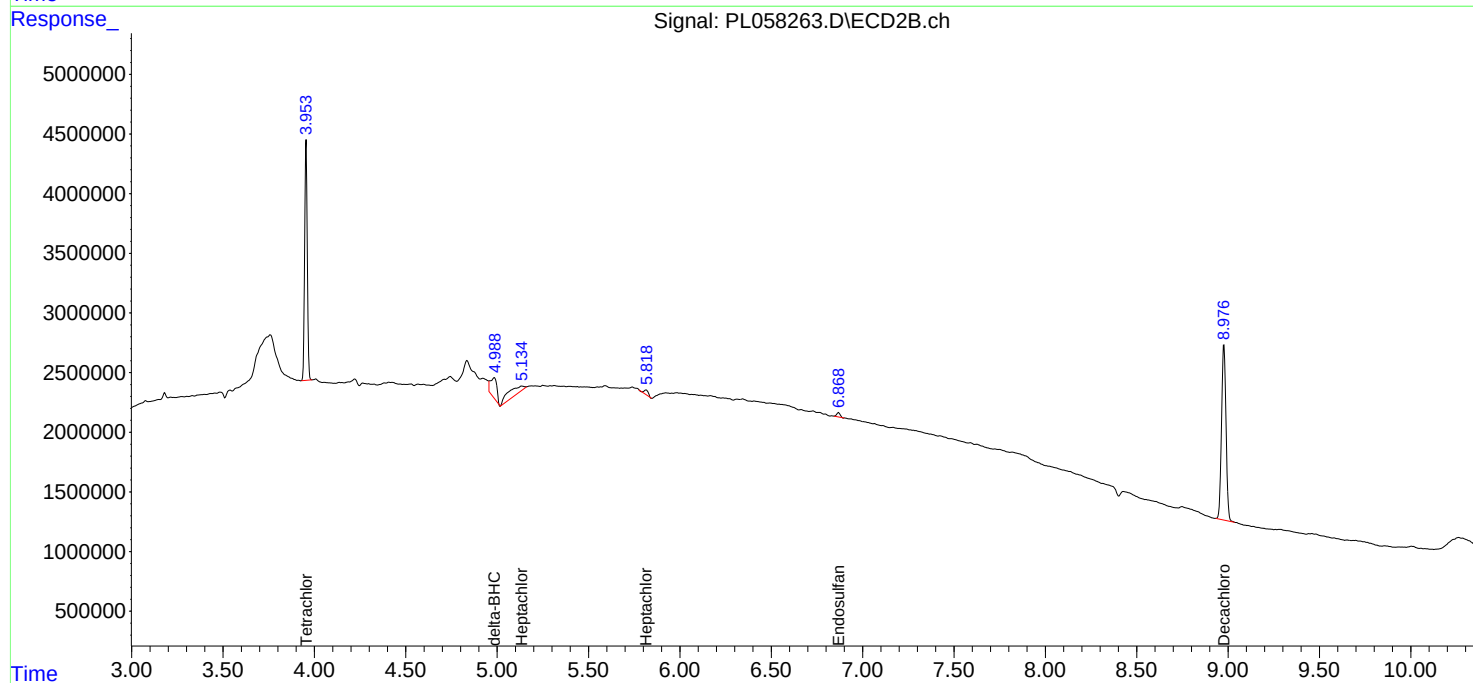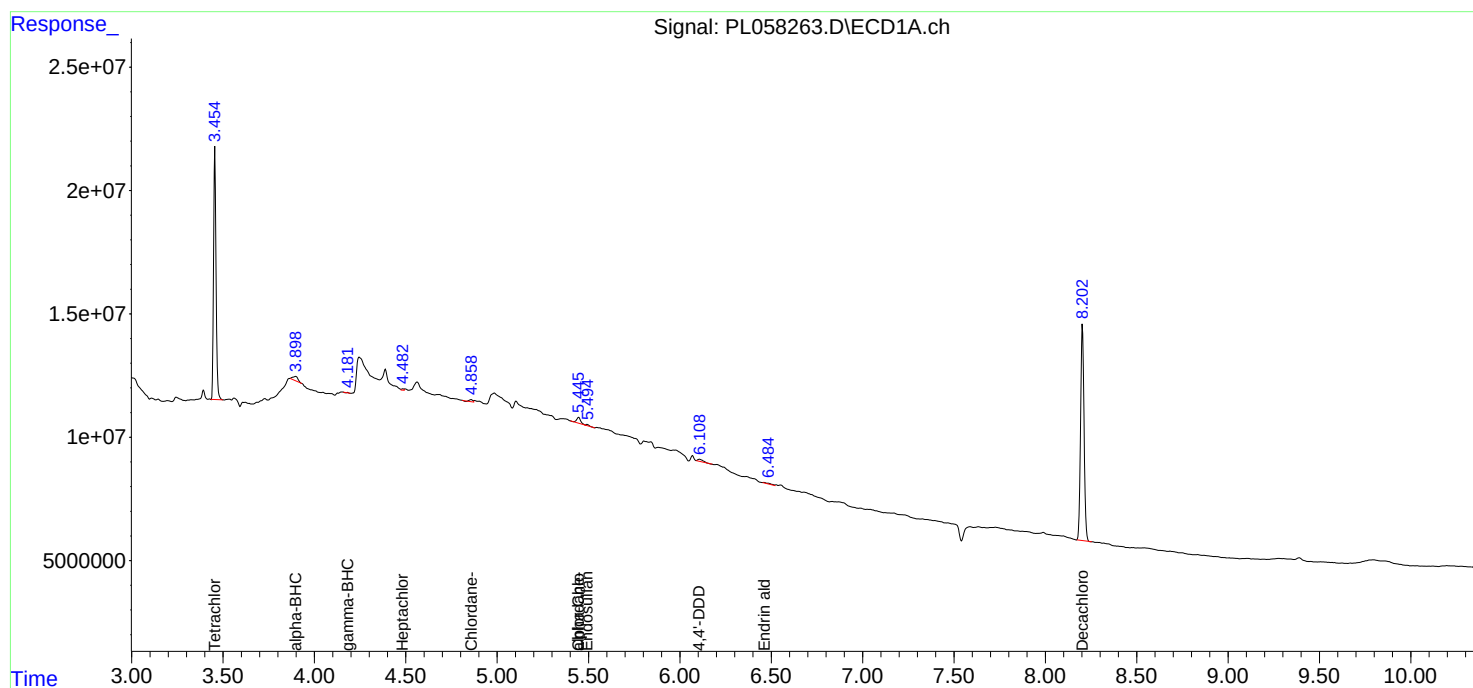


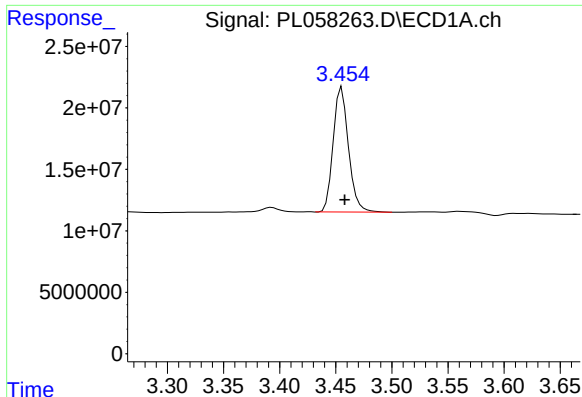

#1 Tetrachloro-m-xylene


R.T.: 3.455 min
Delta R.T.: -0.003 min
Response: 96666618
Conc: 9.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6-S

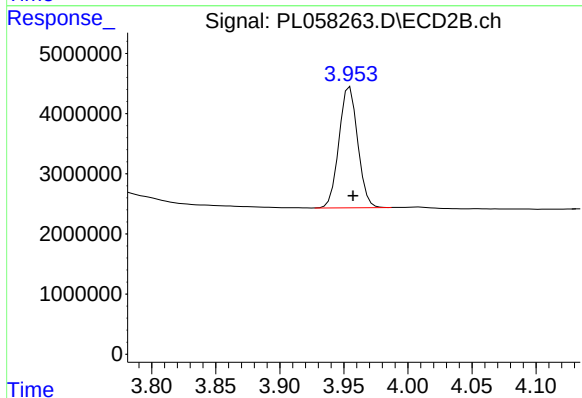


#1 Tetrachloro-m-xylene

R.T.: 3.955 min
Delta R.T.: -0.003 min
Response: 20407945
Conc: 9.40 ng/ml

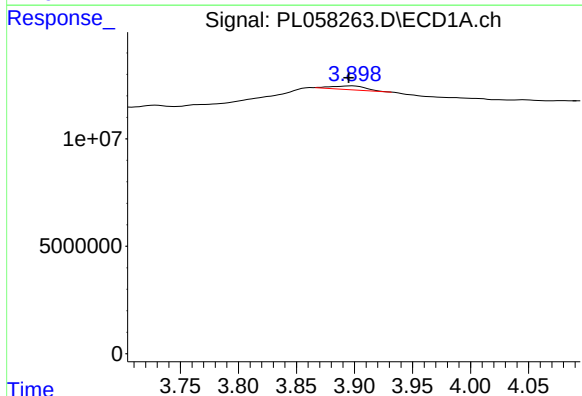


#2 alpha-BHC

R.T.: 3.899 min
Delta R.T.: 0.004 min
Response: 3277419
Conc: 0.19 ng/ml

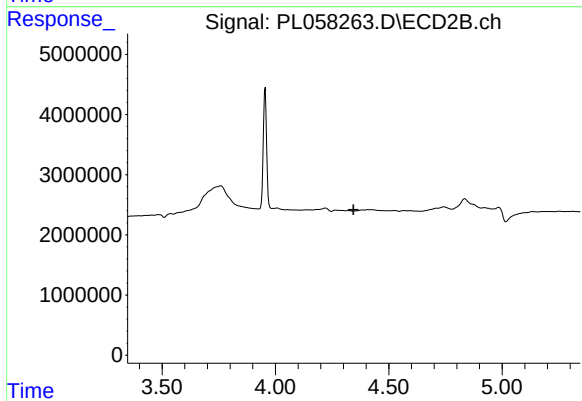

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.345 min
Response: 0
Conc: N.D.

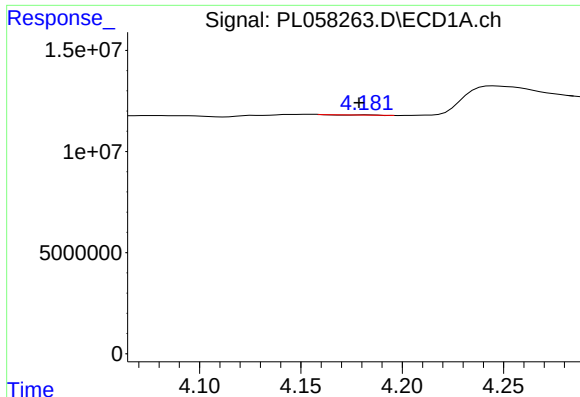

#3 gamma-BHC (Lindane)


R.T.: 4.183 min
Delta R.T.: 0.004 min
Response: 91308
Conc: 0.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6-S

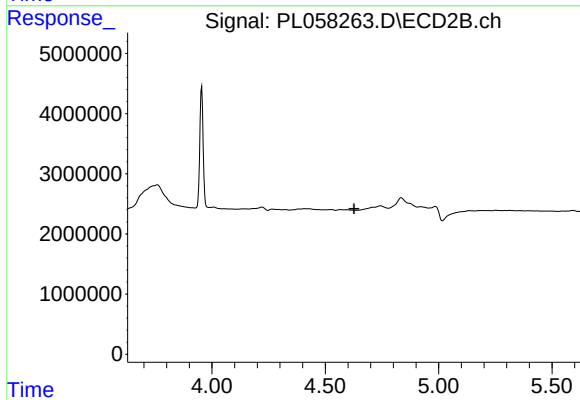


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.627 min
Response: 0
Conc: N.D.

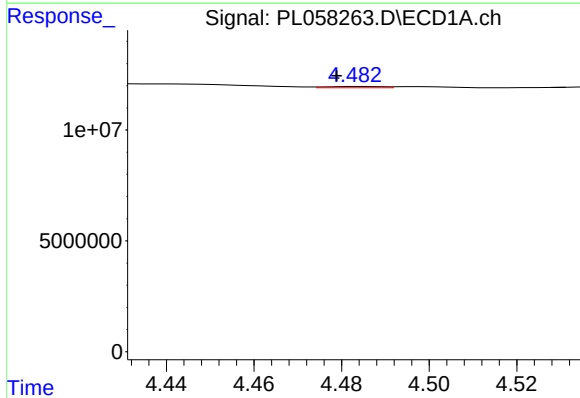


#4 Heptachlor

R.T.: 4.484 min
Delta R.T.: 0.005 min
Response: 490439
Conc: 0.03 ng/ml

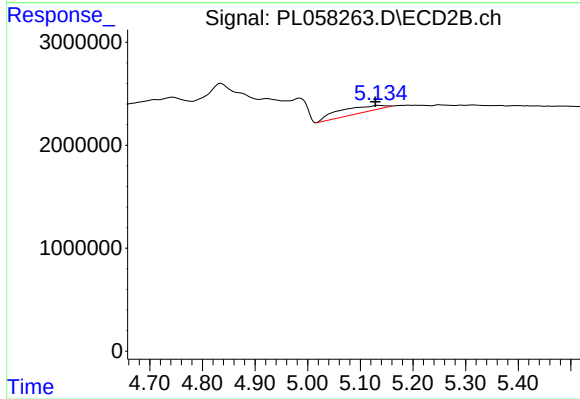

#4 Heptachlor


R.T.: 5.135 min
Delta R.T.: 0.006 min
Response: 3836484
Conc: 1.14 ng/ml

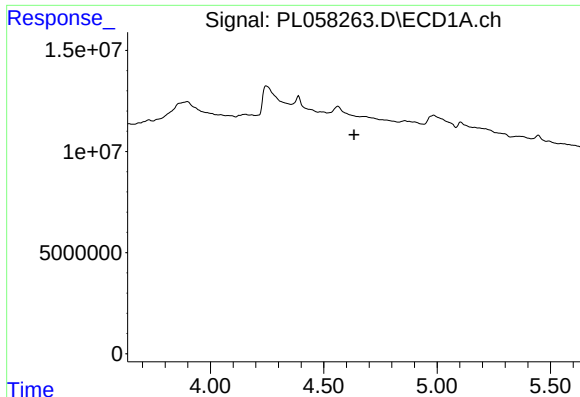

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.634 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-6-S

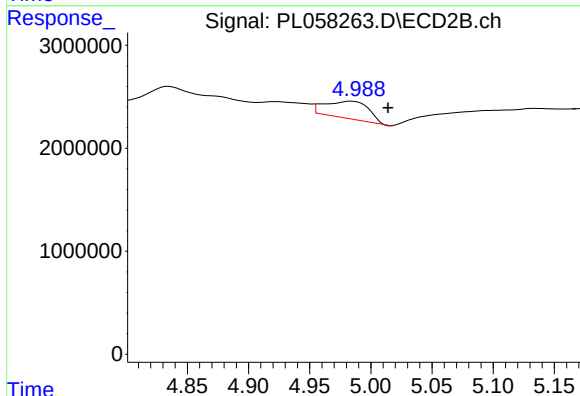


#7 delta-BHC

R.T.: 4.985 min
Delta R.T.: -0.029 min
Response: 4196912
Conc: 3.64 ng/ml

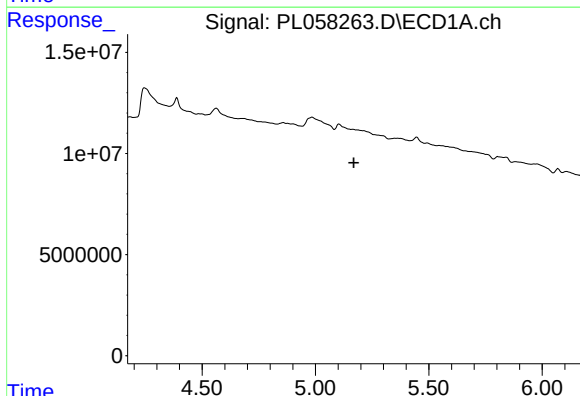


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.169 min
Response: 0
Conc: N.D.

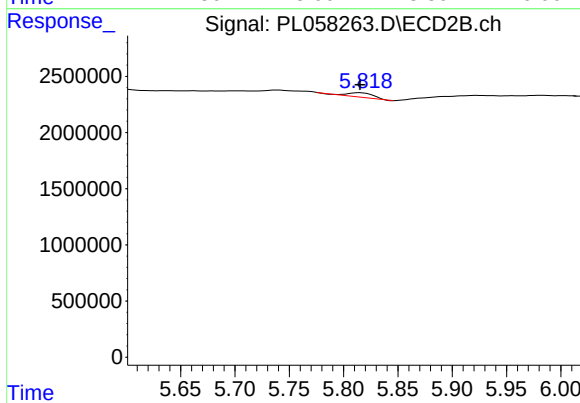

#8 Heptachlor epoxide


R.T.: 5.815 min
Delta R.T.: 0.000 min
Response: 680998
Conc: 0.25 ng/ml

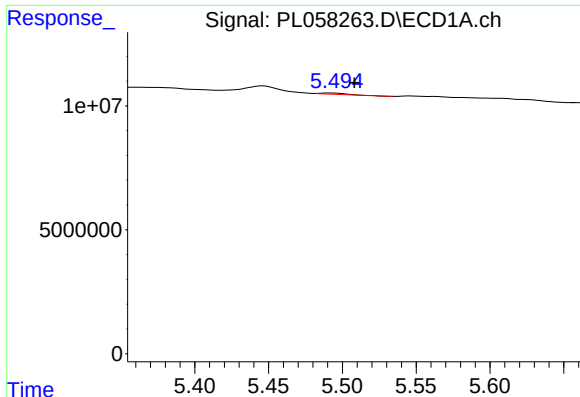

#9 Endosulfan I


R.T.: 5.493 min
Delta R.T.: -0.015 min
Response: 621745
Conc: 0.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6-S

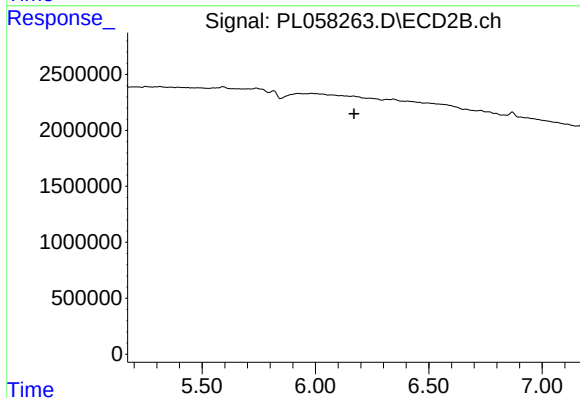


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.170 min
Response: 0
Conc: N.D.

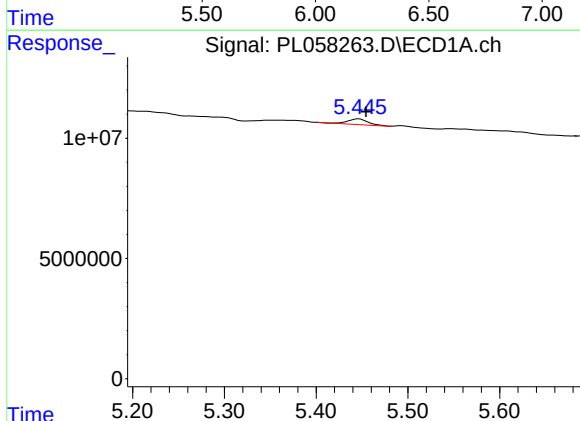


#11 alpha-Chlordane

R.T.: 5.446 min
Delta R.T.: -0.008 min
Response: 3815663
Conc: 0.29 ng/ml

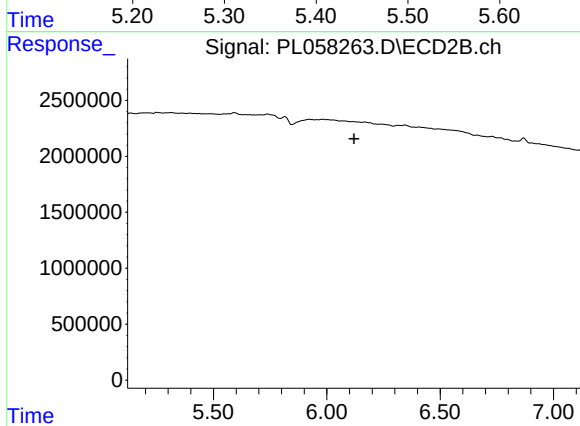

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.120 min
Response: 0
Conc: N.D.

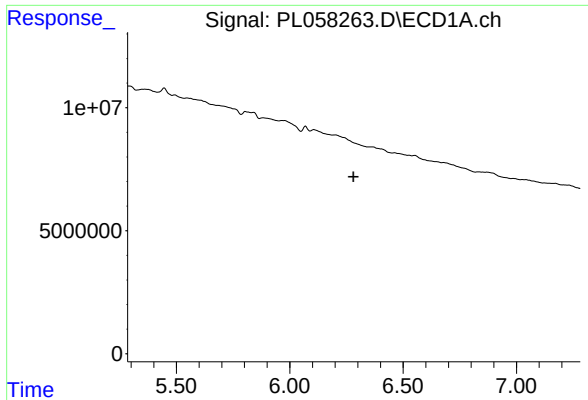

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.282 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-6-S

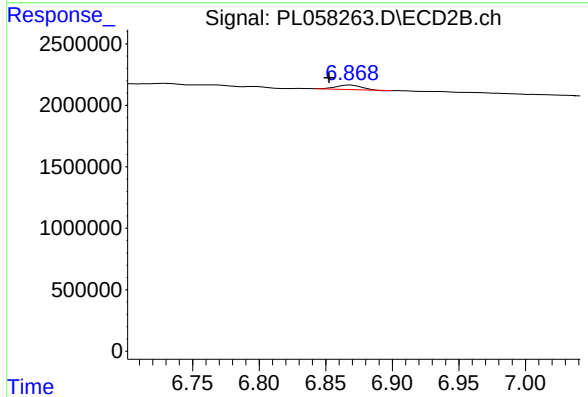


#15 Endosulfan II

R.T.: 6.869 min
Delta R.T.: 0.016 min
Response: 441157
Conc: 0.17 ng/ml

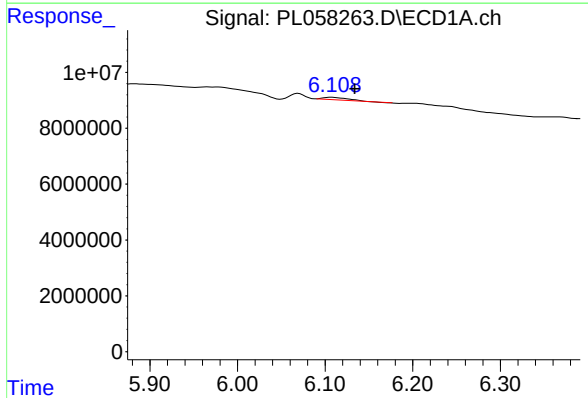


#16 4,4'-DDD

R.T.: 6.107 min
Delta R.T.: -0.027 min
Response: 1544752
Conc: 0.15 ng/ml

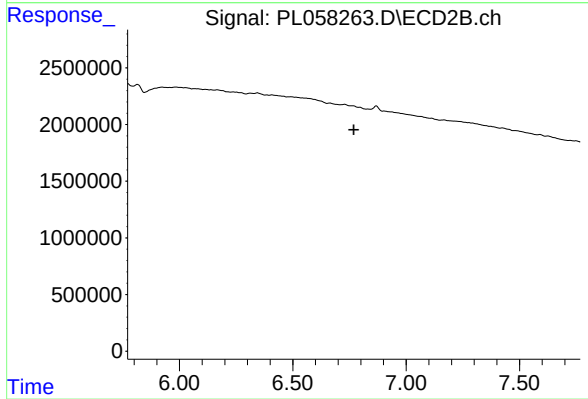

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.769 min
Response: 0
Conc: N.D.

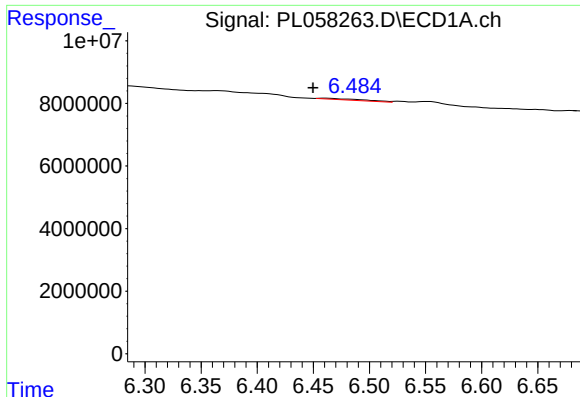

#18 Endrin aldehyde


R.T.: 6.462 min
Delta R.T.: 0.012 min
Response: 1077581
Conc: 0.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6-S

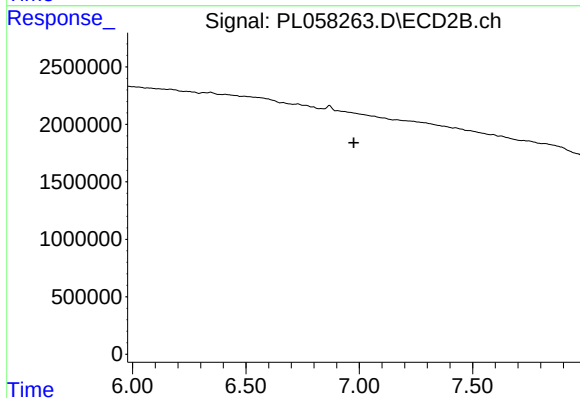


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.976 min
Response: 0
Conc: N.D.

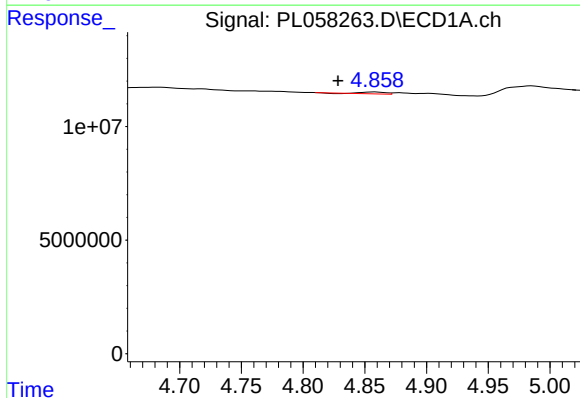


#24 Chlordane-2

R.T.: 4.858 min
Delta R.T.: 0.030 min
Response: 1011783
Conc: 2.51 ng/ml

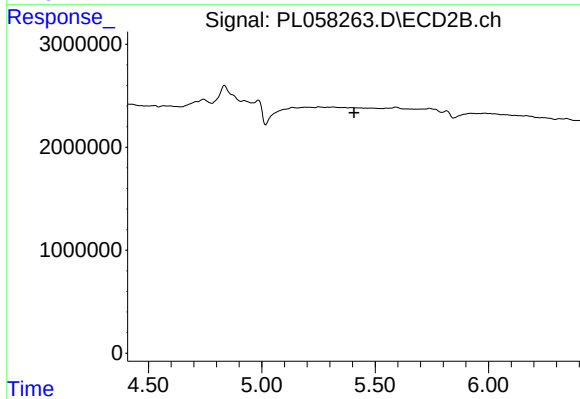

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.407 min
Response: 0
Conc: N.D.

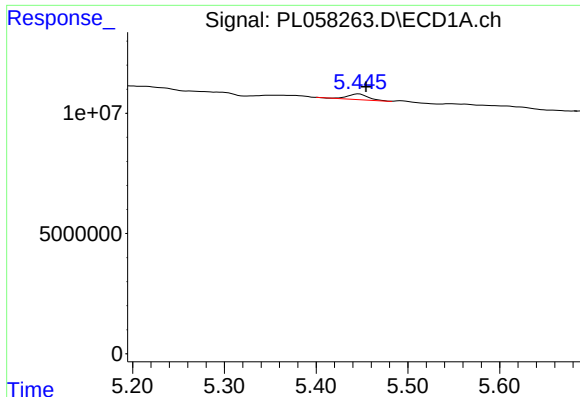

#26 Chlordane-4


R.T.: 5.446 min
Delta R.T.: -0.008 min
Response: 3815663
Conc: 3.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6-S

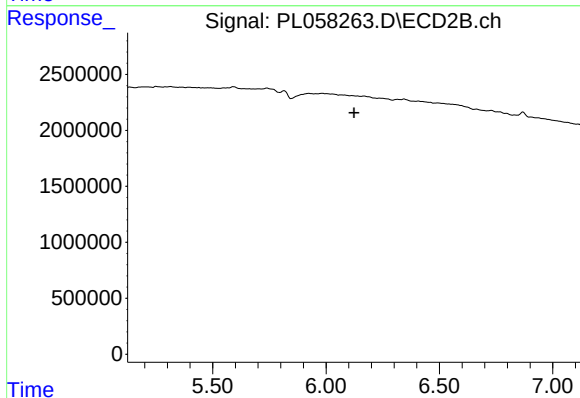


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.123 min
Response: 0
Conc: N.D.

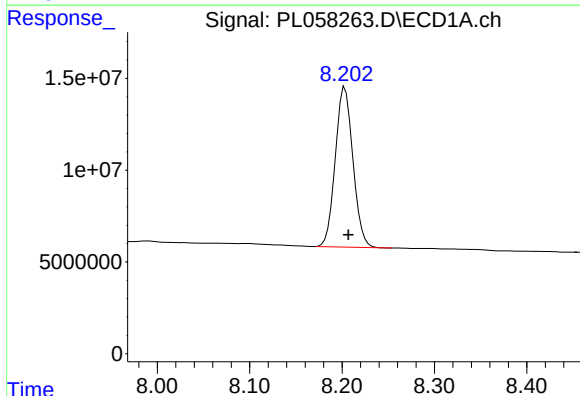

#28 Decachlorobiphenyl

R.T.: 8.203 min
Delta R.T.: -0.004 min
Response: 115708862
Conc: 11.22 ng/ml

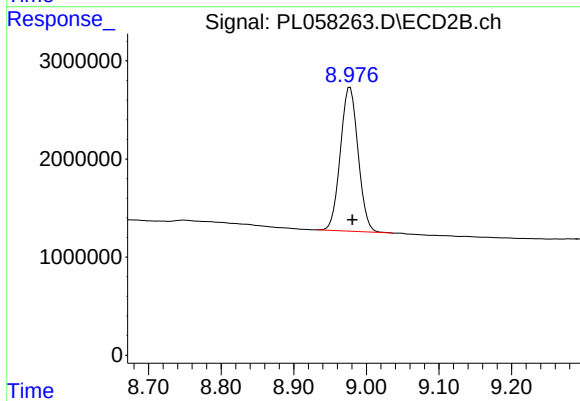

#28 Decachlorobiphenyl

R.T.: 8.978 min
Delta R.T.: -0.003 min
Response: 24875558
Conc: 11.14 ng/ml