

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042120\
 Data File : PL058283.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2020 02:58
 Operator : AJ\MA
 Sample : L2347-06
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-4-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 04:33:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.456	3.955	214.5E6	45344883	21.276	20.895
28)	SA Decachlor...	8.203	8.977	204.0E6	42032737	19.789	18.817
Target Compounds							
4)	MA Heptachlor	4.505f	5.135	75234	3101625	0.005	0.924 #
5)	MB Aldrin	4.713	0.000	231936	0	0.016	N.D. #
7)	B delta-BHC	0.000	4.987f	0	10562239	N.D.	6.079 #
9)	A Endosulfan I	5.510	0.000	690528	0	0.056	N.D. #
15)	B Endosulfa...	0.000	6.869f	0	541669	N.D.	0.209 #
19)	B Endosulfa...	6.673	0.000	31077	0	0.003	N.D. #
23)	Chlordane-1	4.356f	0.000	5956937	0	16.106	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042120\
Data File : PL058283.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2020 02:58
Operator : AJ\MA
Sample : L2347-06
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-4-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 04:33:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

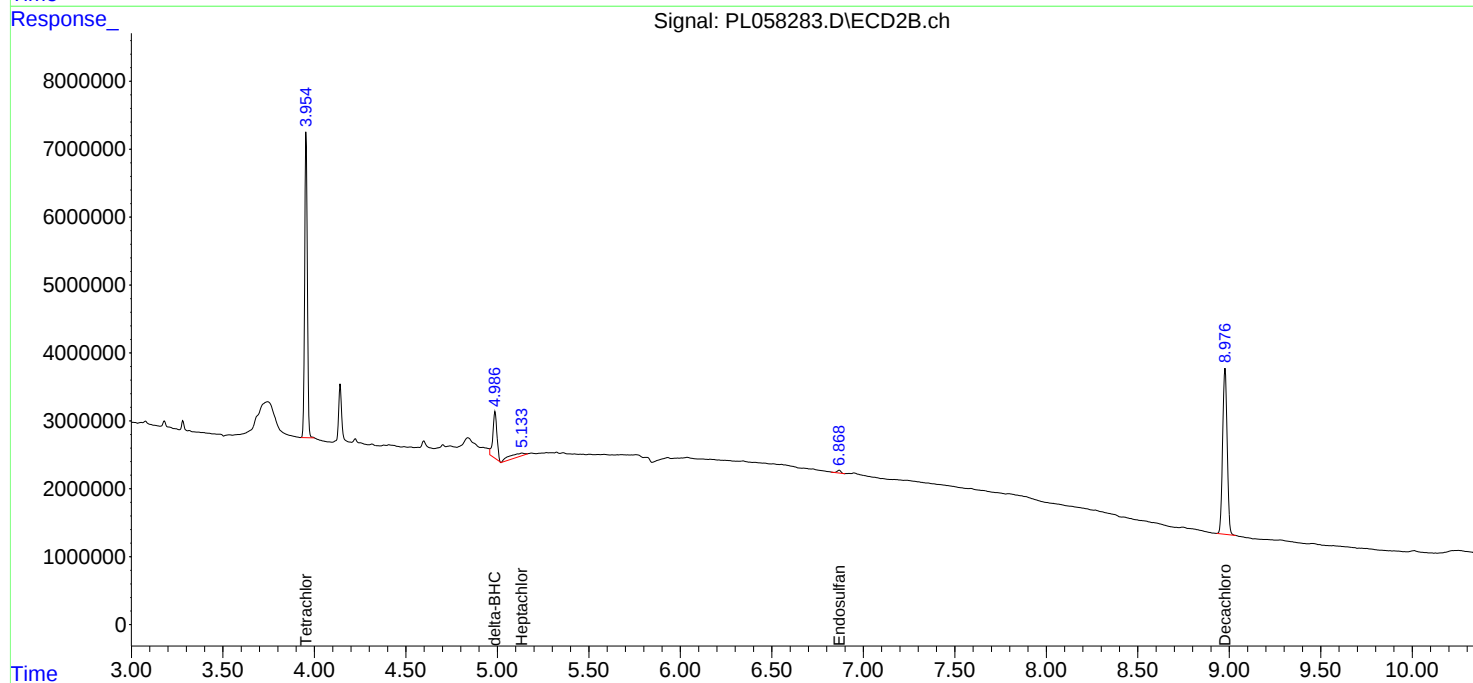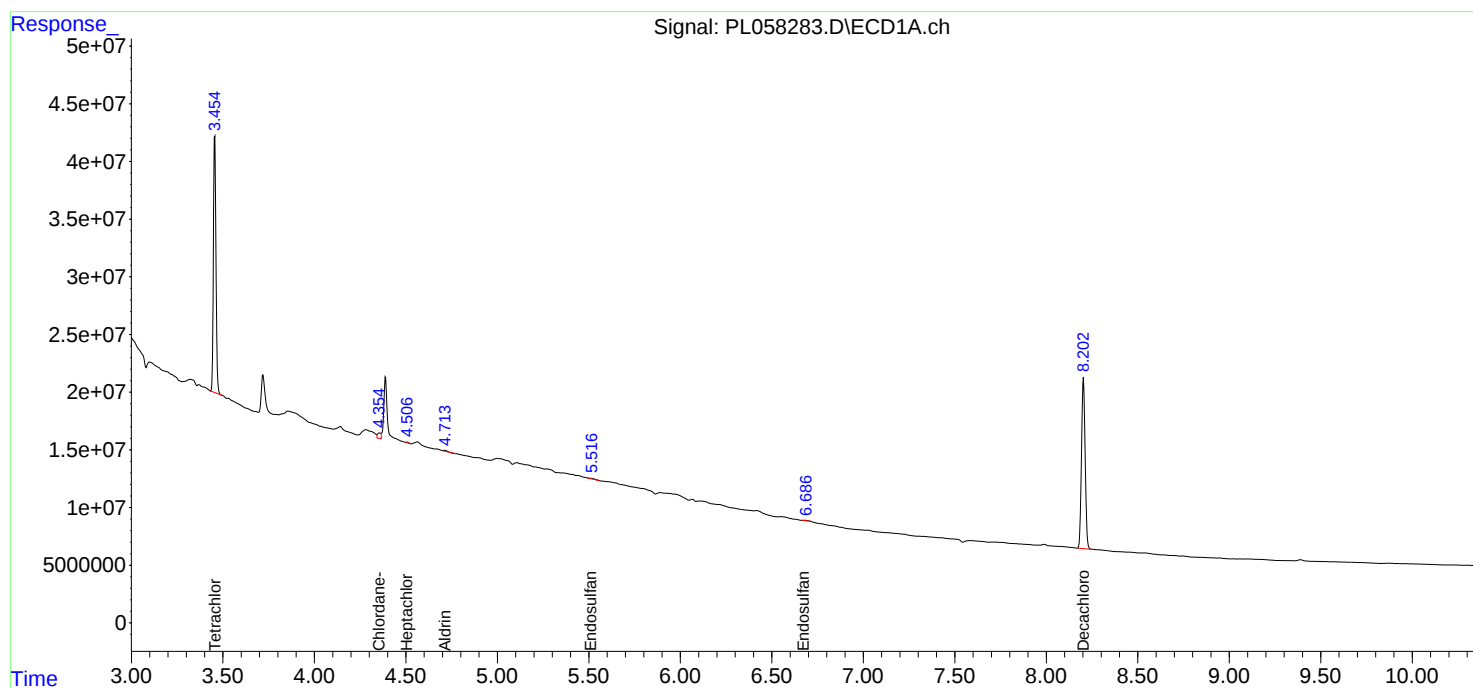


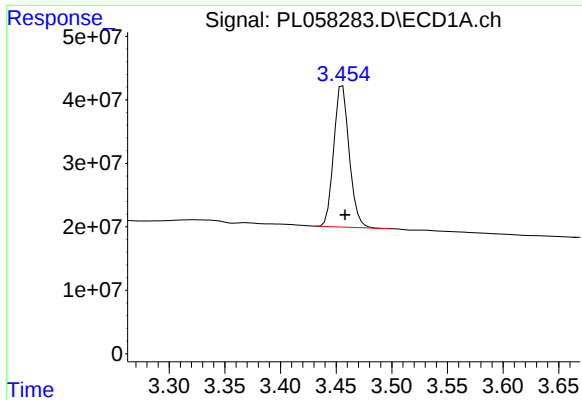

#1 Tetrachloro-m-xylene


R.T.: 3.456 min
Delta R.T.: -0.002 min
Response: 214480718
Conc: 21.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-4-COMP

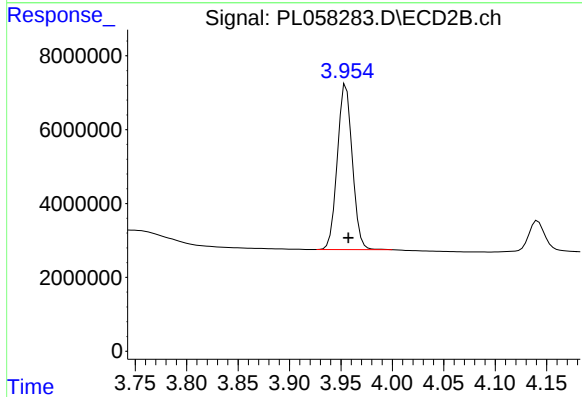


#1 Tetrachloro-m-xylene

R.T.: 3.955 min
Delta R.T.: -0.002 min
Response: 45344883
Conc: 20.89 ng/ml

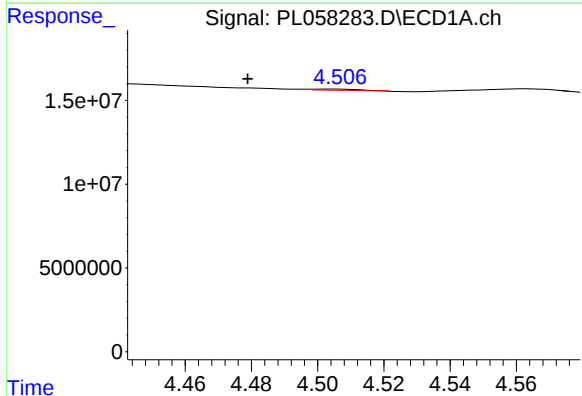


#4 Heptachlor

R.T.: 4.505 min
Delta R.T.: 0.026 min
Response: 75234
Conc: 0.00 ng/ml

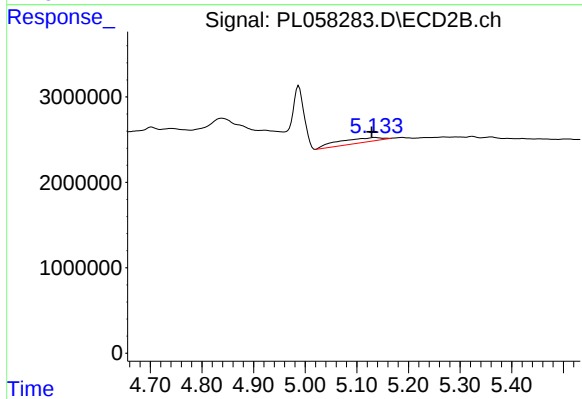

#4 Heptachlor


R.T.: 5.135 min
Delta R.T.: 0.006 min
Response: 3101625
Conc: 0.92 ng/ml

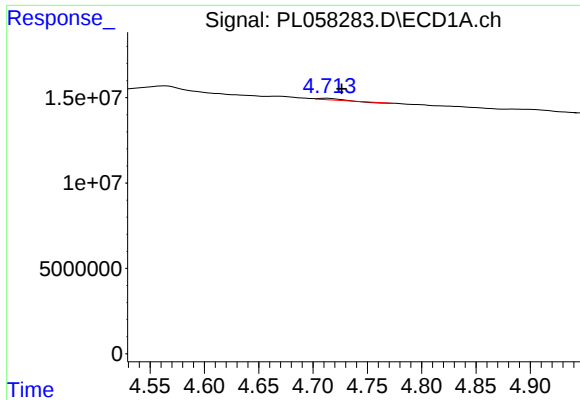

#5 Aldrin


R.T.: 4.713 min
Delta R.T.: -0.014 min
Response: 231936
Conc: 0.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-4-COMP

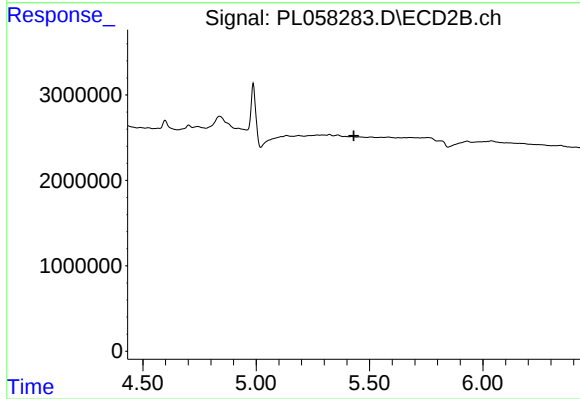


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.431 min
Response: 0
Conc: N.D.

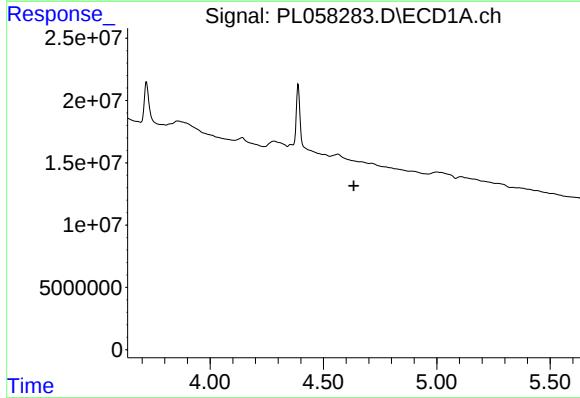


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.634 min
Response: 0
Conc: N.D.

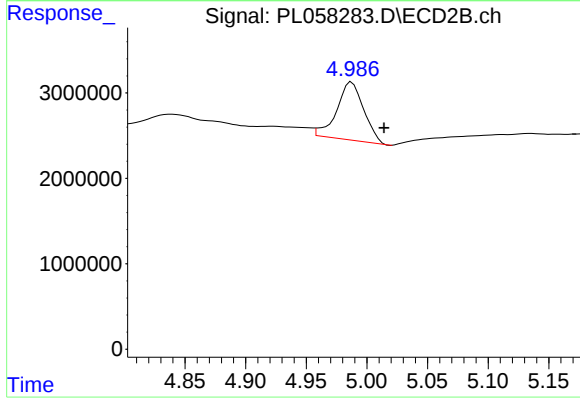

#7 delta-BHC


R.T.: 4.987 min
Delta R.T.: -0.027 min
Response: 10562239
Conc: 6.08 ng/ml

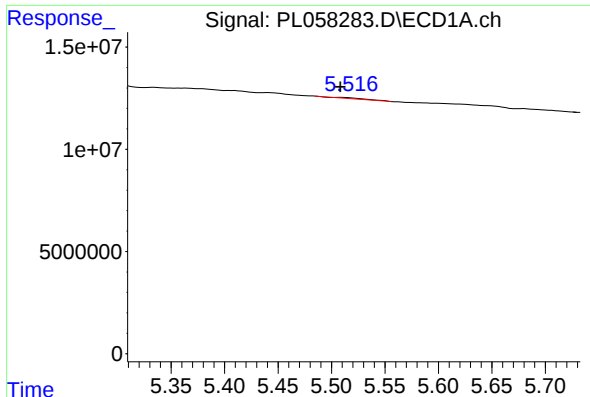

#9 Endosulfan I


R.T.: 5.510 min
Delta R.T.: 0.002 min
Response: 690528
Conc: 0.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-4-COMP

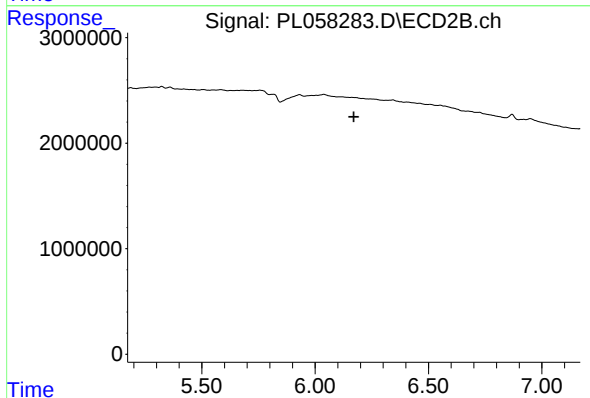


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.170 min
Response: 0
Conc: N.D.

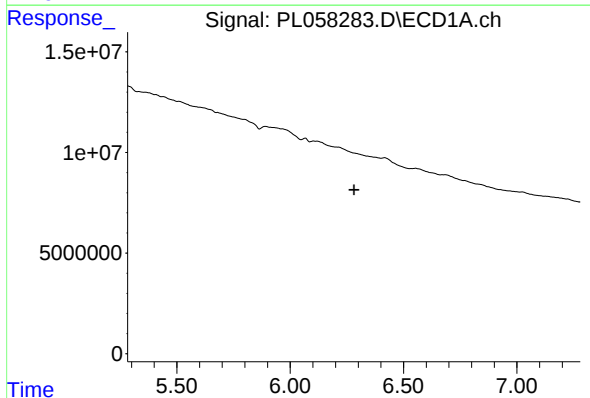


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.282 min
Response: 0
Conc: N.D.

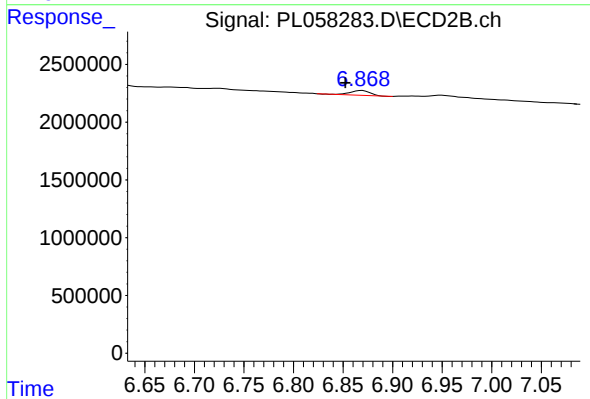

#15 Endosulfan II

R.T.: 6.869 min
Delta R.T.: 0.017 min
Response: 541669
Conc: 0.21 ng/ml

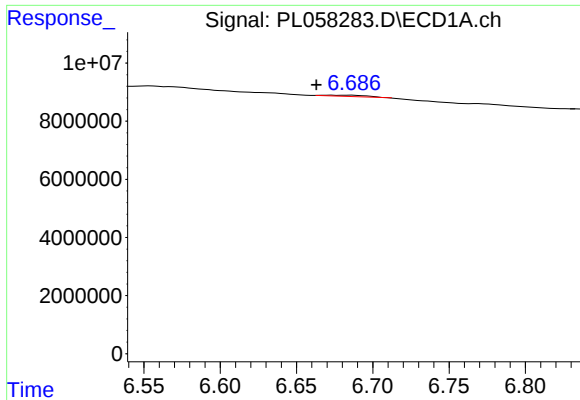

#19 Endosulfan Sulfate


R.T.: 6.673 min

Delta R.T.: 0.010 min

Response: 31077

Conc: 0.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-4-COMP

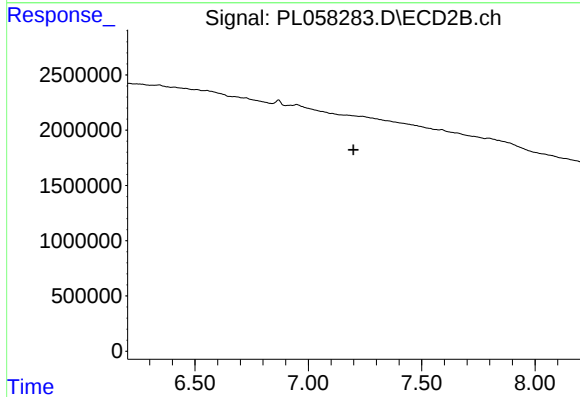


#19 Endosulfan Sulfate

R.T.: 0.000 min

Exp R.T. : 7.199 min

Response: 0

Conc: N.D.

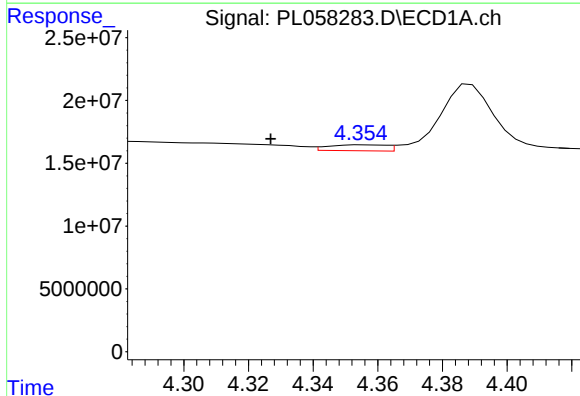


#23 Chlordane-1

R.T.: 4.356 min

Delta R.T.: 0.029 min

Response: 5956937

Conc: 16.11 ng/ml

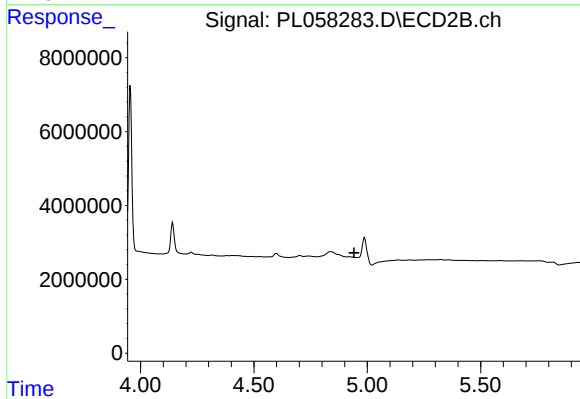


#23 Chlordane-1

R.T.: 0.000 min

Exp R.T. : 4.942 min

Response: 0


Conc: N.D.

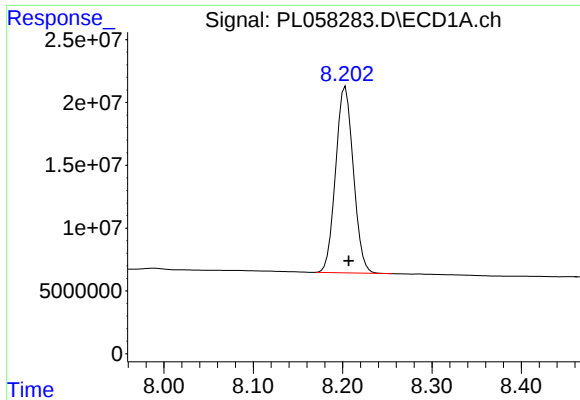

#28 Decachlorobiphenyl

R.T.: 8.203 min
Delta R.T.: -0.003 min
Response: 203996347
Conc: 19.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-4-COMP

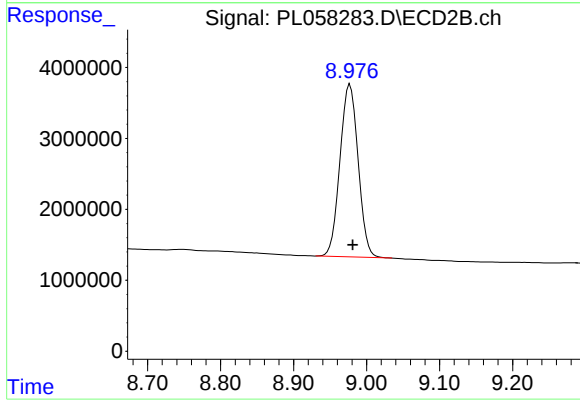

#28 Decachlorobiphenyl

R.T.: 8.977 min
Delta R.T.: -0.004 min
Response: 42032737
Conc: 18.82 ng/ml