

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042120\
 Data File : PL058243.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Apr 2020 17:31
 Operator : AJ\MA
 Sample : L2346-09DL 25X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 S-6DL

Manual Integrations
 APPROVED

mohammad
 4/23/2020 12:37:43 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 00:57:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.455	3.953	11180217	1669020	1.109m	0.769m#
28) SA Decachlor...	8.204	8.978	8958874	1748341	0.869m	0.783m
Target Compounds						
16) A 4,4'-DDD	6.132	6.768	14271677	2746356	1.428	1.203
17) MA 4,4'-DDT	6.371	7.064	763.8E6	150.3E6	75.252m	67.495

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042120\
Data File : PL058243.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Apr 2020 17:31
Operator : AJ\MA
Sample : L2346-09DL 25X
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
S-6DL


Manual Integrations
APPROVED

mohammad
4/23/2020 12:37:43 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 00:57:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

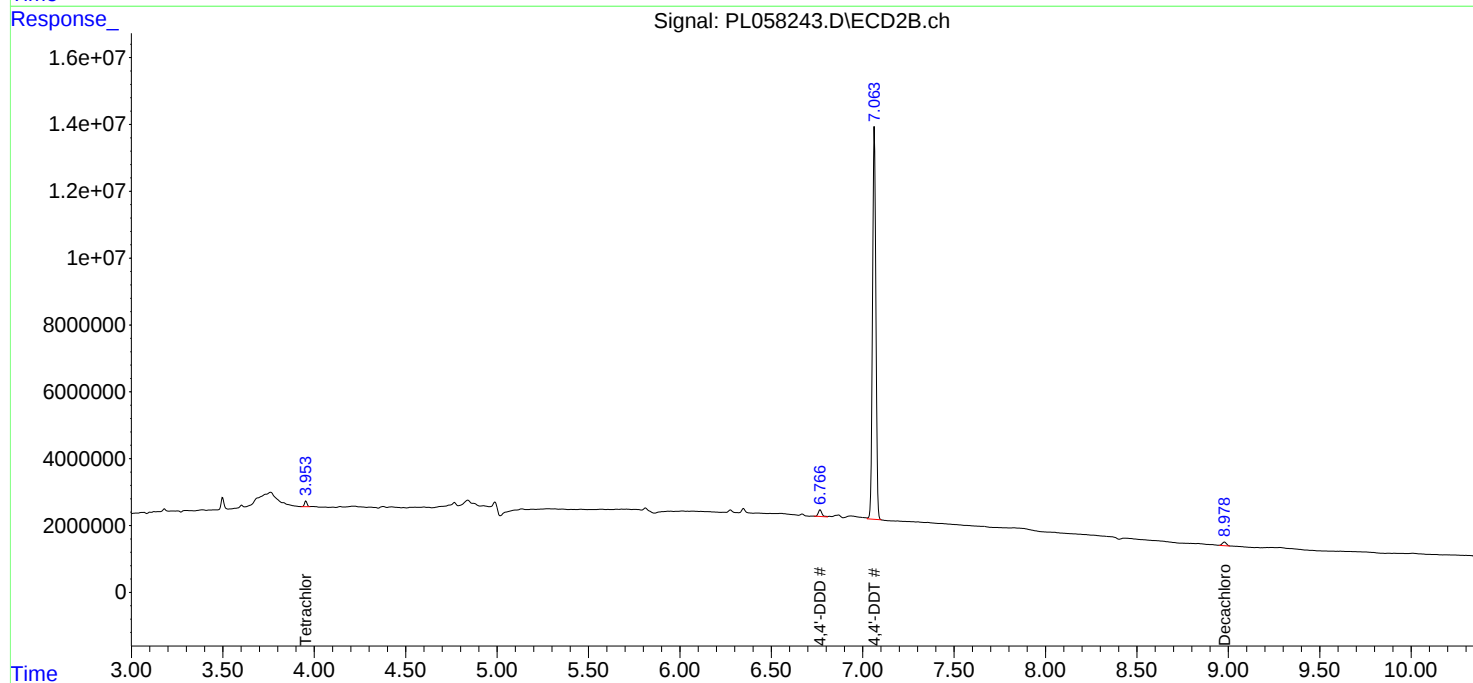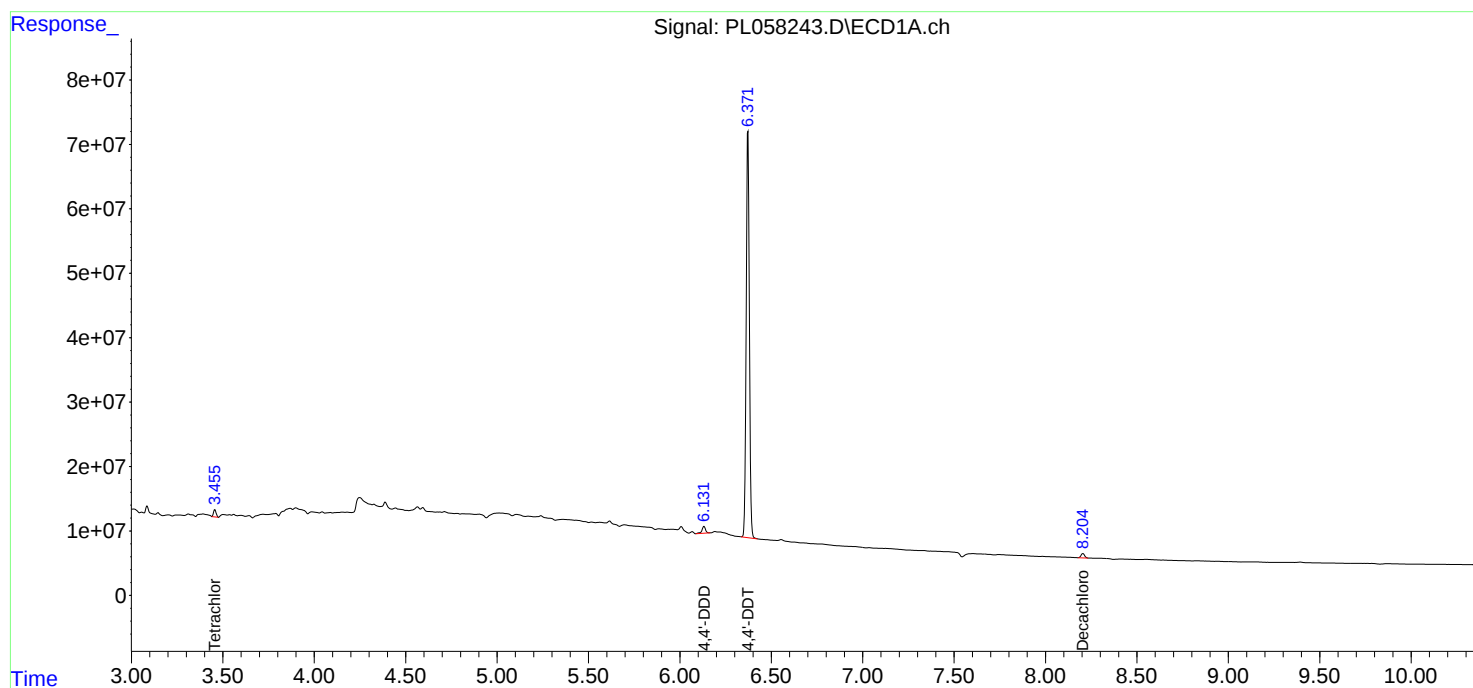

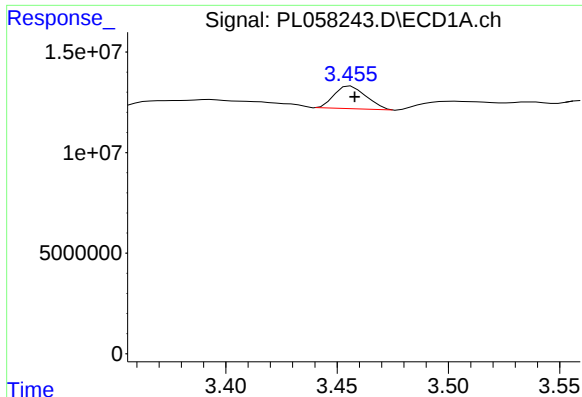


#1 Tetrachloro-m-xylene

R.T.: 3.455 min
Delta R.T.: -0.003 min
Response: 11180217
Conc: 1.11 ng/ml m

Instrument :
ECD_L
ClientSampleId :
S-6DL


Manual Integrations
APPROVED

mohammad
4/23/2020 12:37:43 PM

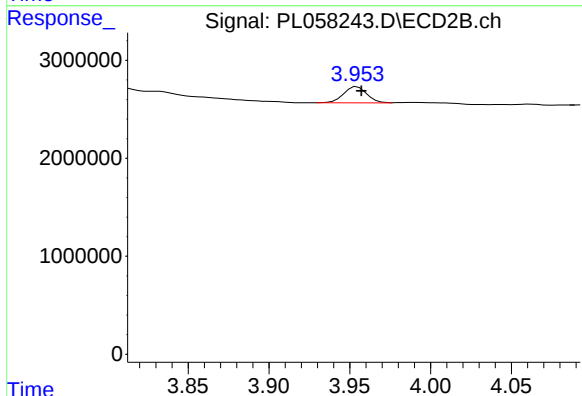


#1 Tetrachloro-m-xylene

R.T.: 3.953 min
Delta R.T.: -0.004 min
Response: 1669020
Conc: 0.77 ng/ml m

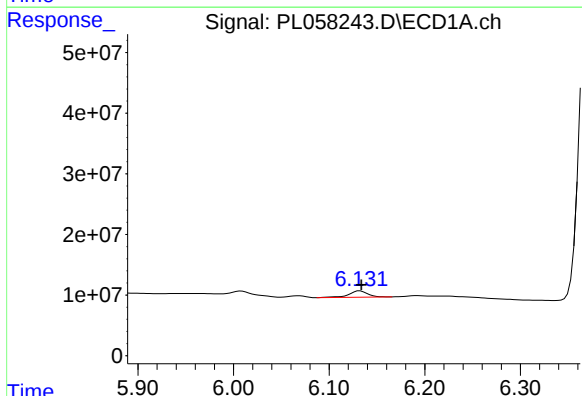


#16 4,4'-DDD

R.T.: 6.132 min
Delta R.T.: -0.002 min
Response: 14271677
Conc: 1.43 ng/ml

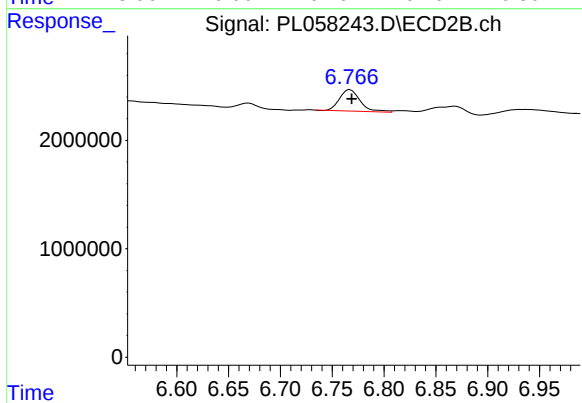

#16 4,4'-DDD

R.T.: 6.768 min
Delta R.T.: -0.001 min
Response: 2746356
Conc: 1.20 ng/ml

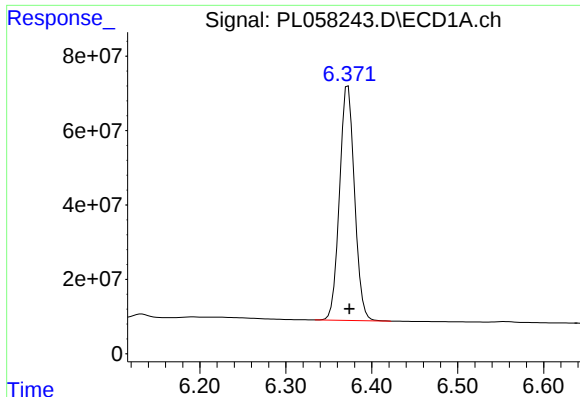


#17 4,4'-DDT

R.T.: 6.371 min
Delta R.T.: -0.003 min
Response: 763764543
Conc: 75.25 ng/ml m

Instrument :
ECD_L
ClientSampleId :
S-6DL


Manual Integrations
APPROVED

mohammad
4/23/2020 12:37:43 PM

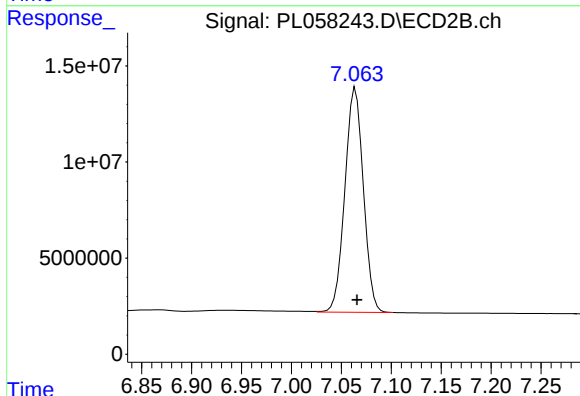


#17 4,4'-DDT

R.T.: 7.064 min
Delta R.T.: -0.001 min
Response: 150337901
Conc: 67.50 ng/ml

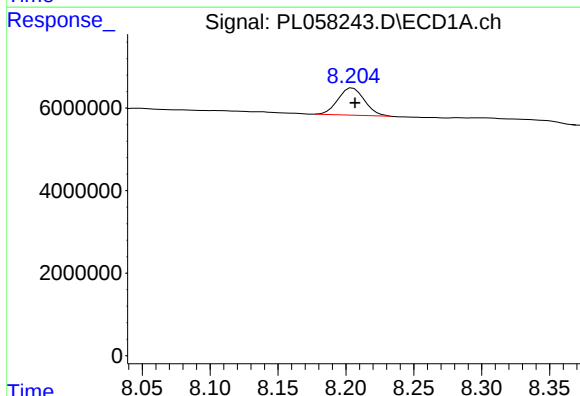

#28 Decachlorobiphenyl

R.T.: 8.204 min
Delta R.T.: -0.003 min
Response: 8958874
Conc: 0.87 ng/ml m

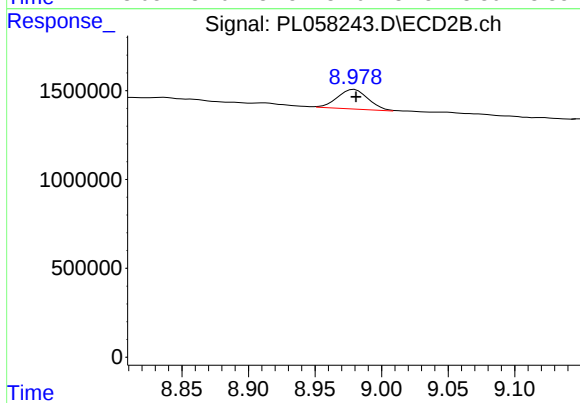

#28 Decachlorobiphenyl

R.T.: 8.978 min
Delta R.T.: -0.003 min
Response: 1748341
Conc: 0.78 ng/ml m