

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042122\
 Data File : PL074270.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Apr 2022 16:22
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 03:24:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 14 09:29:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.637	5.489	8250090	40201904	25.533	22.548
28)	SA Decachlor...	10.407	11.331	8956105	30247052	17.222	17.125
Target Compounds							
2)	A alpha-BHC	5.344	0.000	46107	0	0.110	N.D. #
6)	B beta-BHC	0.000	6.675	0	397345	N.D.	0.353 #
7)	B delta-BHC	0.000	6.957	0	1070872	N.D.	0.438 #
10)	B gamma-Chl...	0.000	8.193	0	89814	N.D.	0.040 #
13)	MA Dieldrin	7.767	0.000	131624	0	0.306	N.D. #
14)	MA Endrin	8.083f	0.000	292907	0	0.721	N.D. #
15)	B Endosulfa...	0.000	9.058	0	51200	N.D.	0.029 #
16)	A 4,4'-DDD	0.000	8.975	0	140114	N.D.	0.091 #
18)	B Endrin al...	8.560	9.209	45051	48510	0.139	0.038 #
20)	A Methoxychlor	0.000	9.786	0	99395	N.D.	0.103 #
23)	Chlordane-1	0.000	6.846f	0	558300	N.D.	6.996 #
25)	Chlordane-3	0.000	8.193	0	89814	N.D.	0.265 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042122\
Data File : PL074270.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Apr 2022 16:22
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 03:24:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
Quant Title : GC Extractables
QLast Update : Thu Apr 14 09:29:23 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

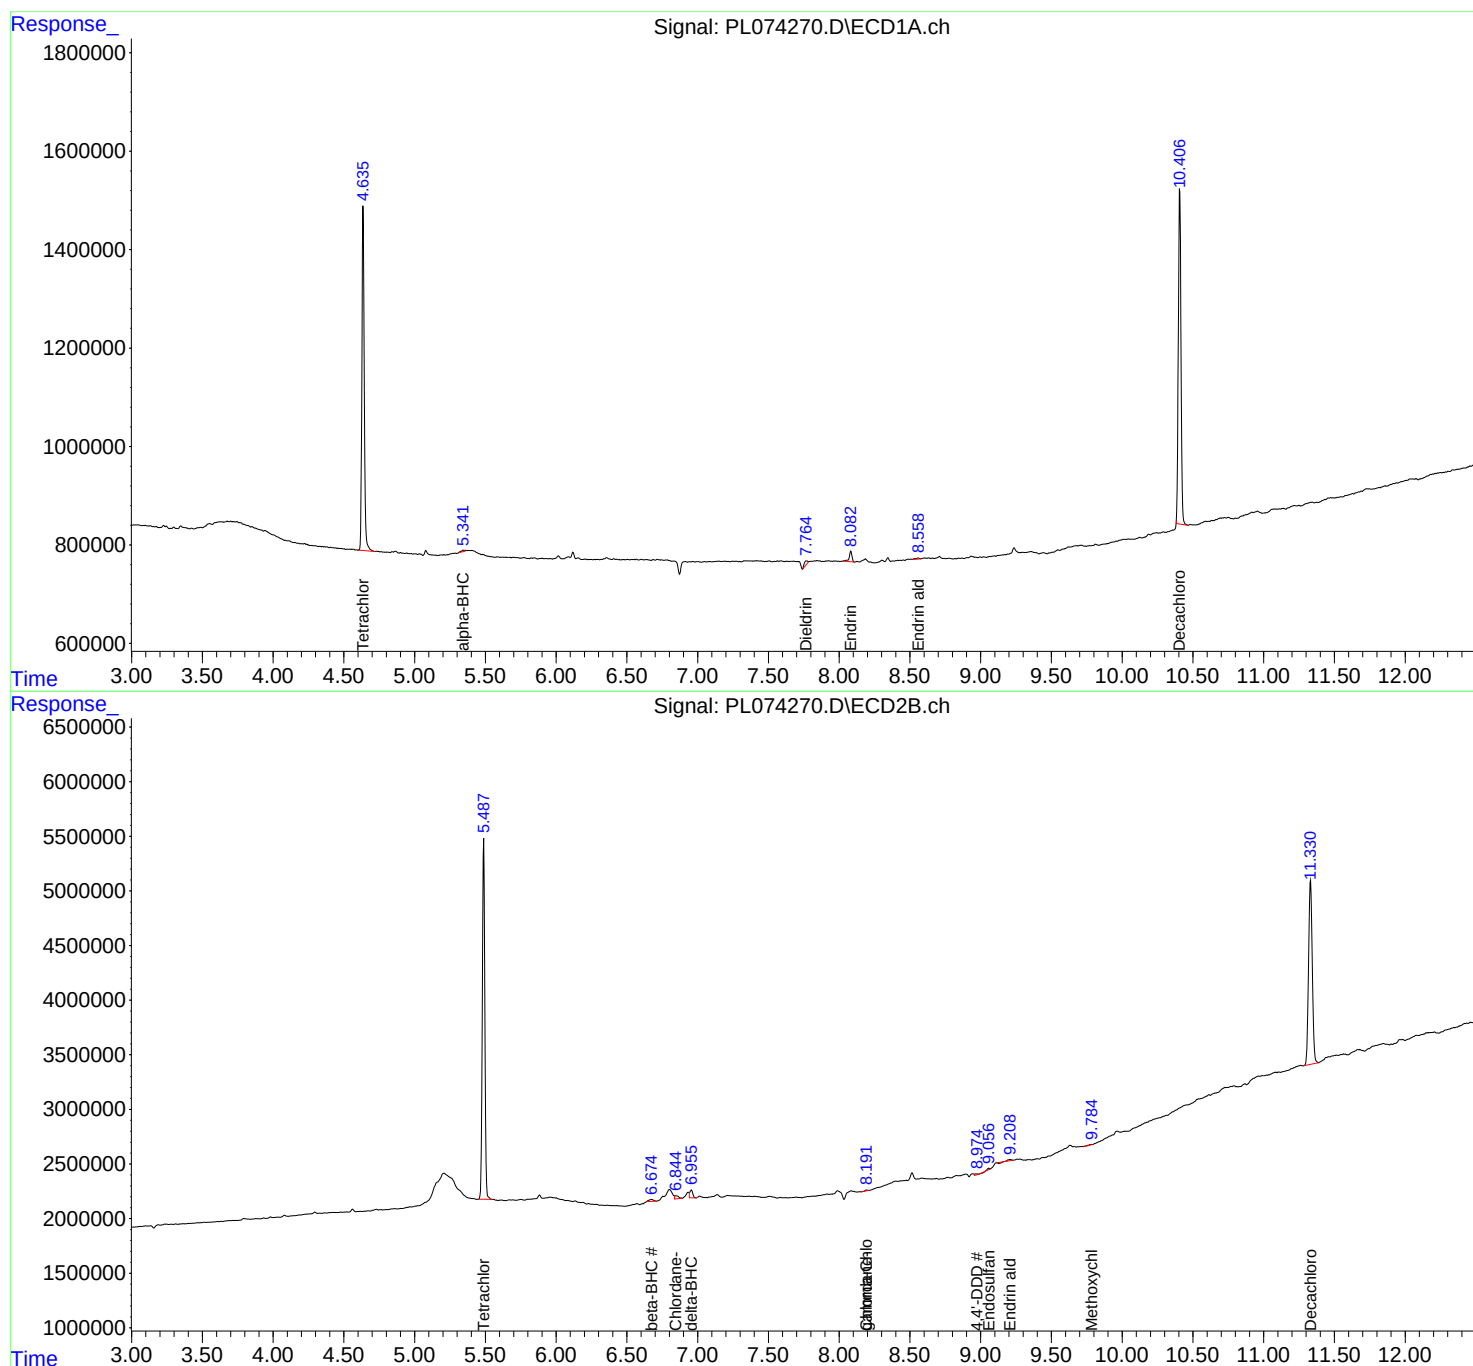


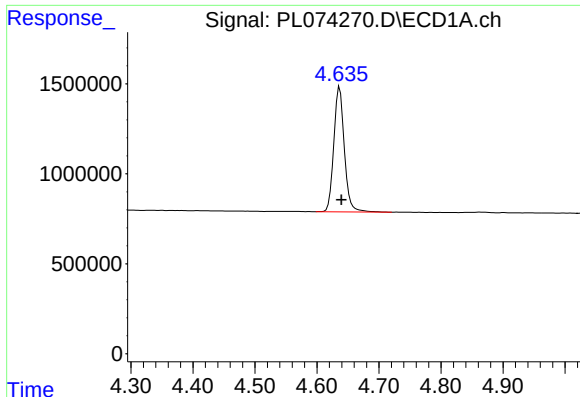

#1 Tetrachloro-m-xylene


R.T.: 4.637 min
Delta R.T.: -0.002 min
Response: 8250090
Conc: 25.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

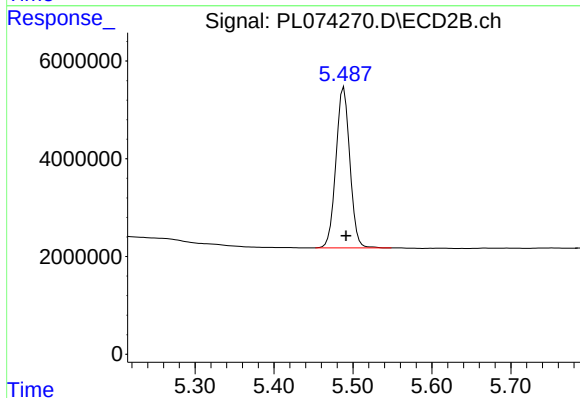


#1 Tetrachloro-m-xylene

R.T.: 5.489 min
Delta R.T.: -0.003 min
Response: 40201904
Conc: 22.55 ng/ml

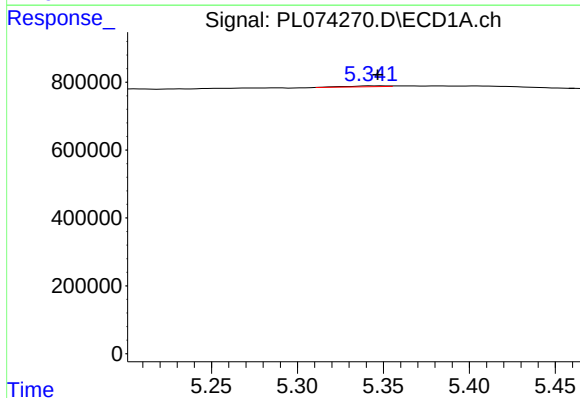


#2 alpha-BHC

R.T.: 5.344 min
Delta R.T.: -0.003 min
Response: 46107
Conc: 0.11 ng/ml

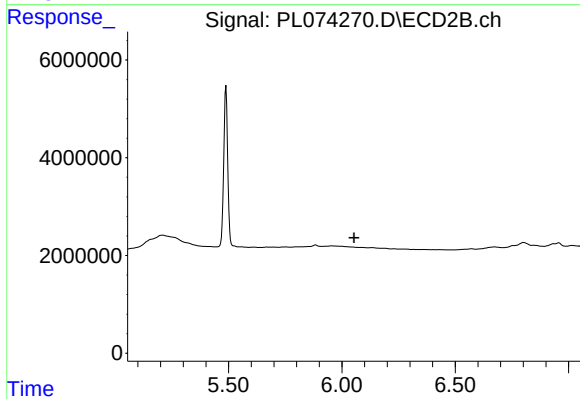

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 6.054 min
Response: 0
Conc: N.D.

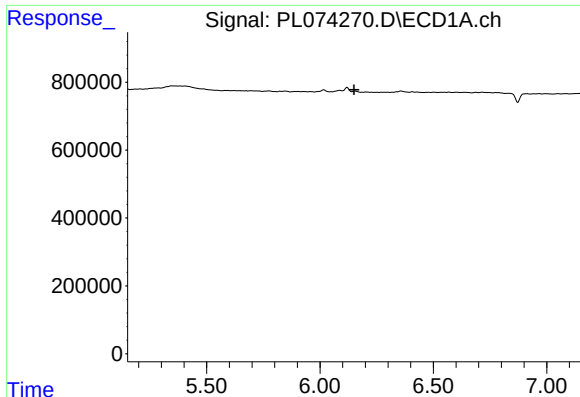

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.151 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

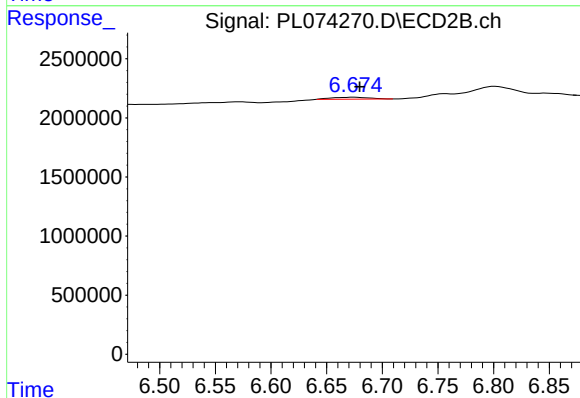


#6 beta-BHC

R.T.: 6.675 min
Delta R.T.: -0.005 min
Response: 397345
Conc: 0.35 ng/ml

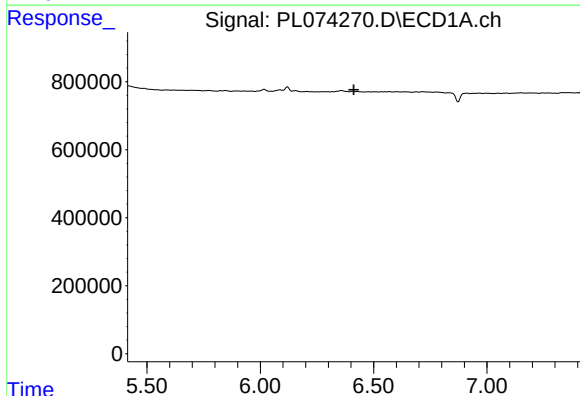


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 6.412 min
Response: 0
Conc: N.D.

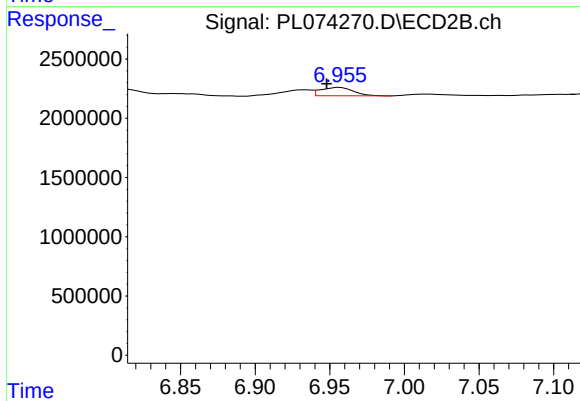

#7 delta-BHC


R.T.: 6.957 min
Delta R.T.: 0.009 min
Response: 1070872
Conc: 0.44 ng/ml

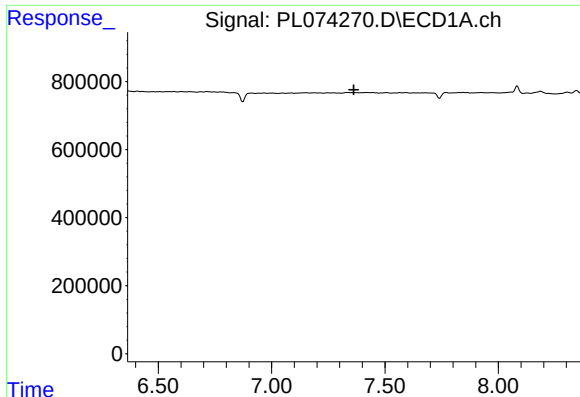

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

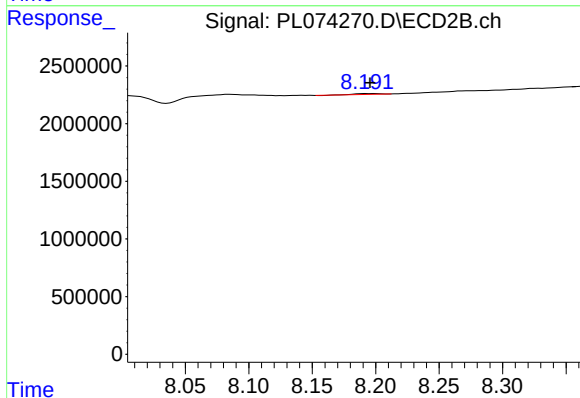


#10 gamma-Chlordane

R.T.: 8.193 min
Delta R.T.: -0.003 min
Response: 89814
Conc: 0.04 ng/ml

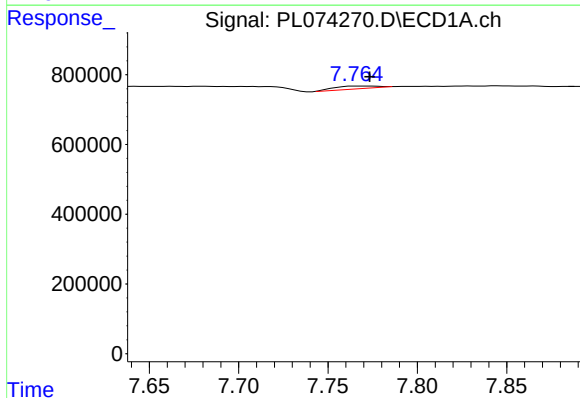


#13 Dieldrin

R.T.: 7.767 min
Delta R.T.: -0.007 min
Response: 131624
Conc: 0.31 ng/ml

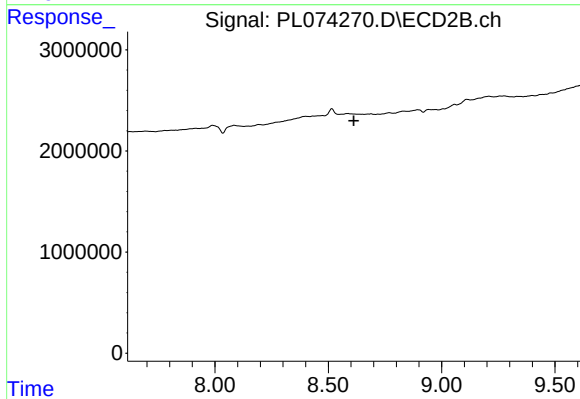

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 8.613 min
Response: 0
Conc: N.D.

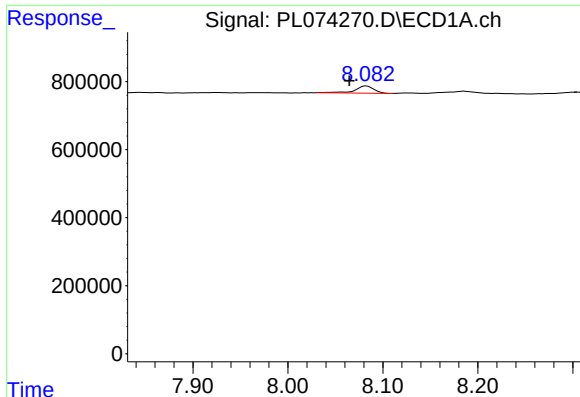

#14 Endrin


R.T.: 8.083 min
Delta R.T.: 0.018 min
Response: 292907
Conc: 0.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

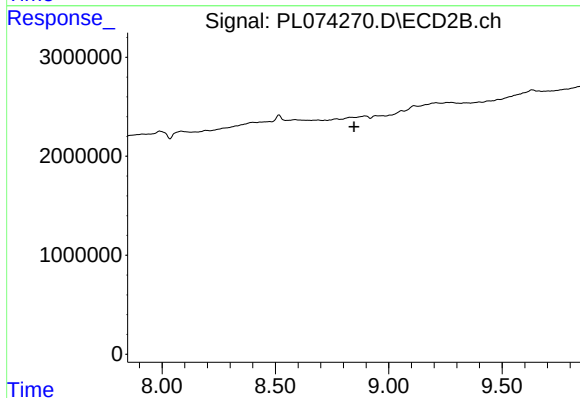


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.847 min
Response: 0
Conc: N.D.

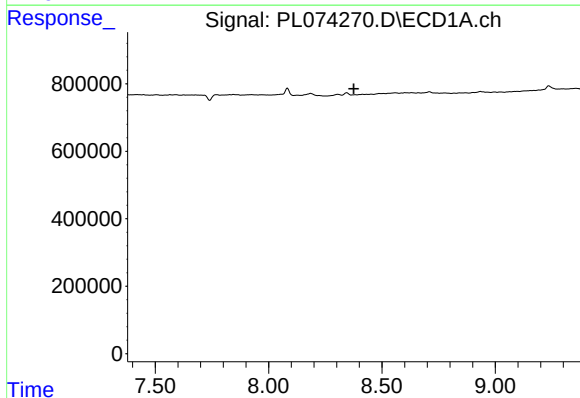


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.375 min
Response: 0
Conc: N.D.

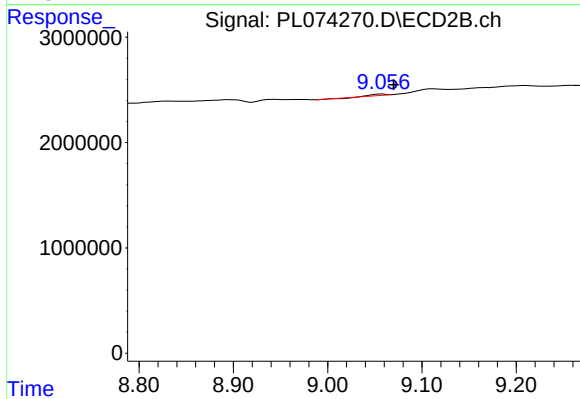

#15 Endosulfan II


R.T.: 9.058 min
Delta R.T.: -0.013 min
Response: 51200
Conc: 0.03 ng/ml

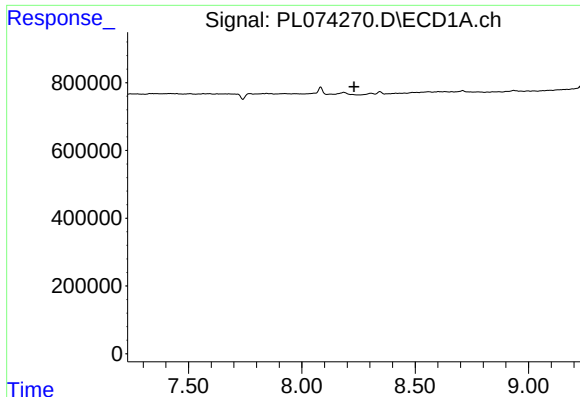

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.231 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

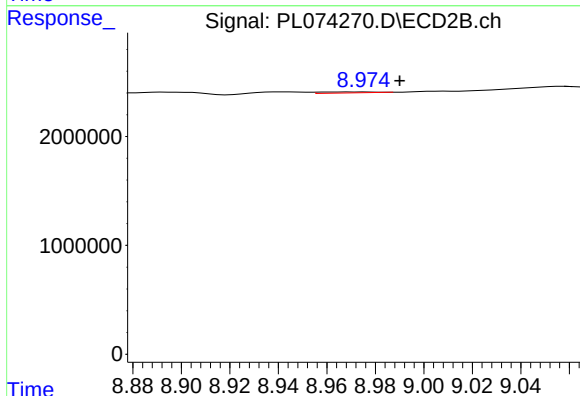


#16 4,4'-DDD

R.T.: 8.975 min
Delta R.T.: -0.015 min
Response: 140114
Conc: 0.09 ng/ml

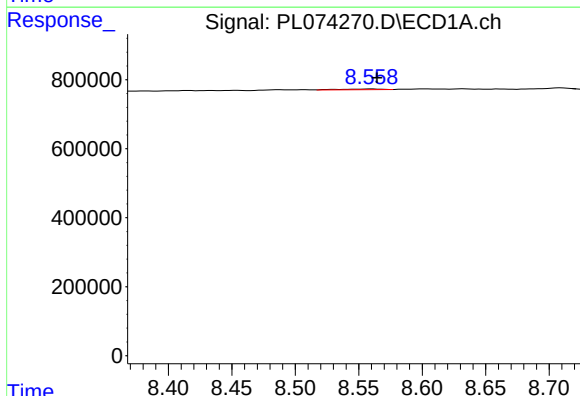


#18 Endrin aldehyde

R.T.: 8.560 min
Delta R.T.: -0.004 min
Response: 45051
Conc: 0.14 ng/ml

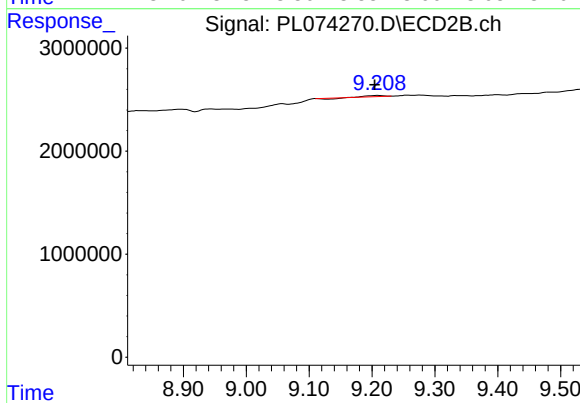

#18 Endrin aldehyde


R.T.: 9.209 min
Delta R.T.: 0.005 min
Response: 48510
Conc: 0.04 ng/ml

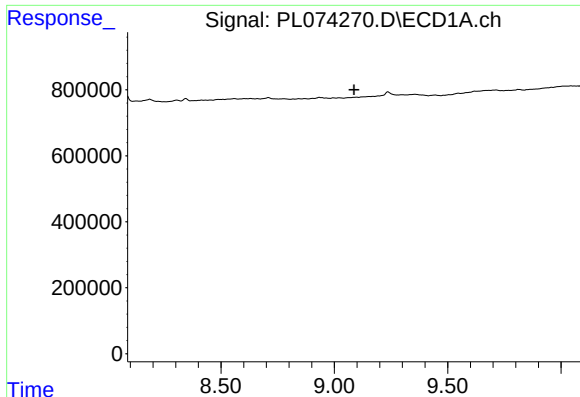

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 9.087 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

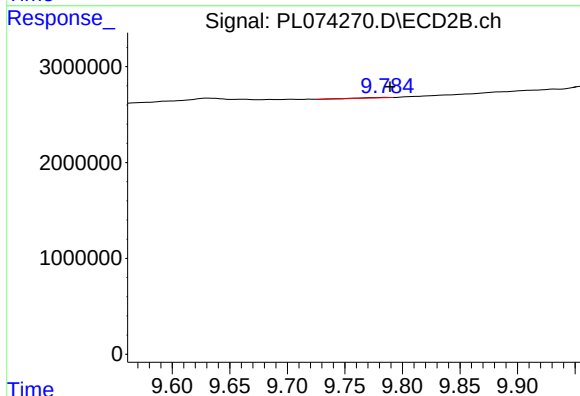


#20 Methoxychlor

R.T.: 9.786 min
Delta R.T.: -0.003 min
Response: 99395
Conc: 0.10 ng/ml

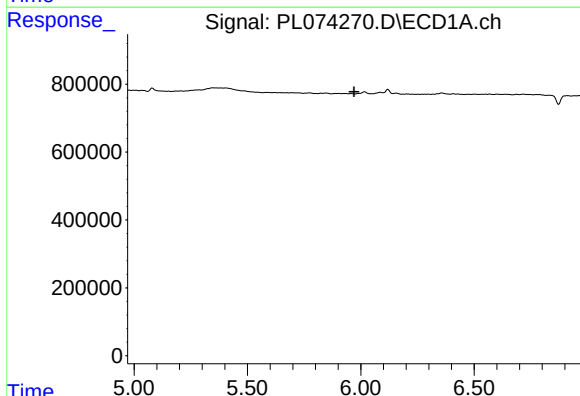


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.970 min
Response: 0
Conc: N.D.

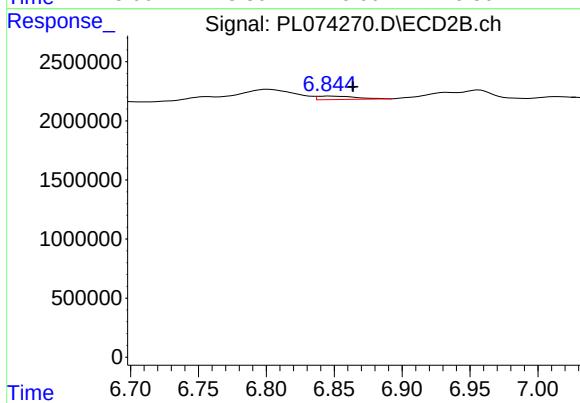

#23 Chlordane-1


R.T.: 6.846 min
Delta R.T.: -0.018 min
Response: 558300
Conc: 7.00 ng/ml

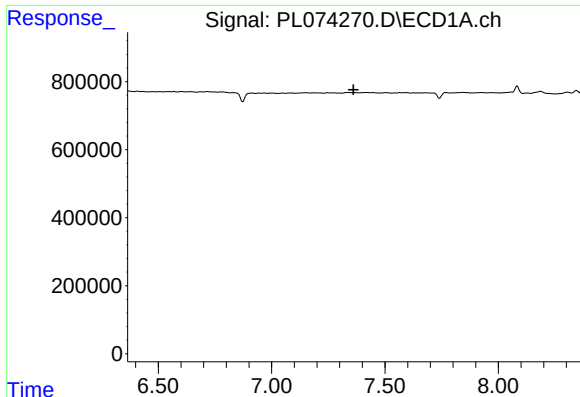

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

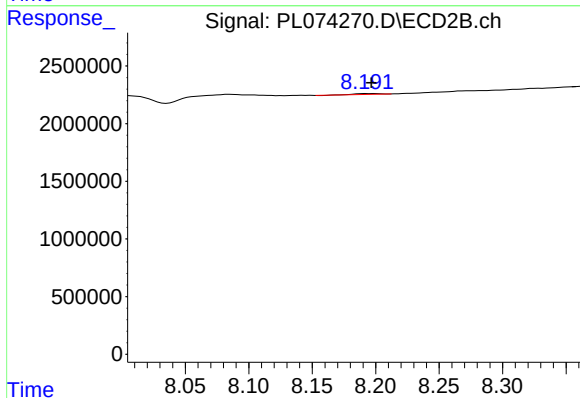


#25 Chlordane-3

R.T.: 8.193 min
Delta R.T.: -0.004 min
Response: 89814
Conc: 0.27 ng/ml

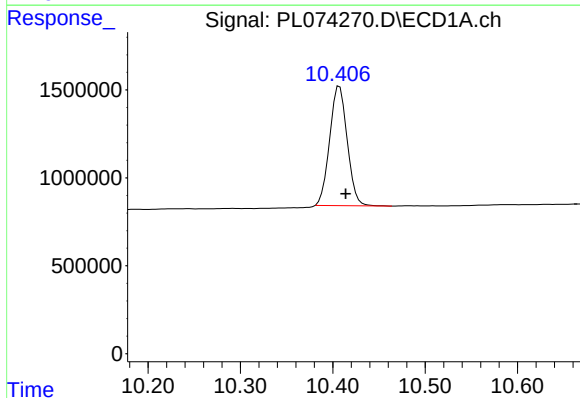

#28 Decachlorobiphenyl

R.T.: 10.407 min
Delta R.T.: -0.007 min
Response: 8956105
Conc: 17.22 ng/ml

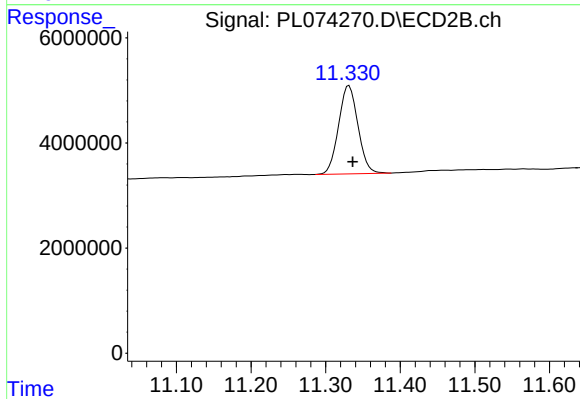

#28 Decachlorobiphenyl

R.T.: 11.331 min
Delta R.T.: -0.005 min
Response: 30247052
Conc: 17.12 ng/ml