

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042123\
 Data File : PL082241.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Apr 2023 13:47
 Operator : AR\AJ
 Sample : 02427-08
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20230349-COMP-27

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 04/24/2023
 Supervised By : Ankita Jodhani 04/24/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 21:38:57 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 21 03:12:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.323	2.649	40674395	34243239	15.227m	14.781
28) SA Decachlor...	8.747	7.764	25946904	29487044	13.591	12.919

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042123\
Data File : PL082241.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Apr 2023 13:47
Operator : AR\AJ
Sample : 02427-08
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
20230349-COMP-27


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 04/24/2023
Supervised By : Ankita Jodhani 04/24/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 21:38:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 03:12:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

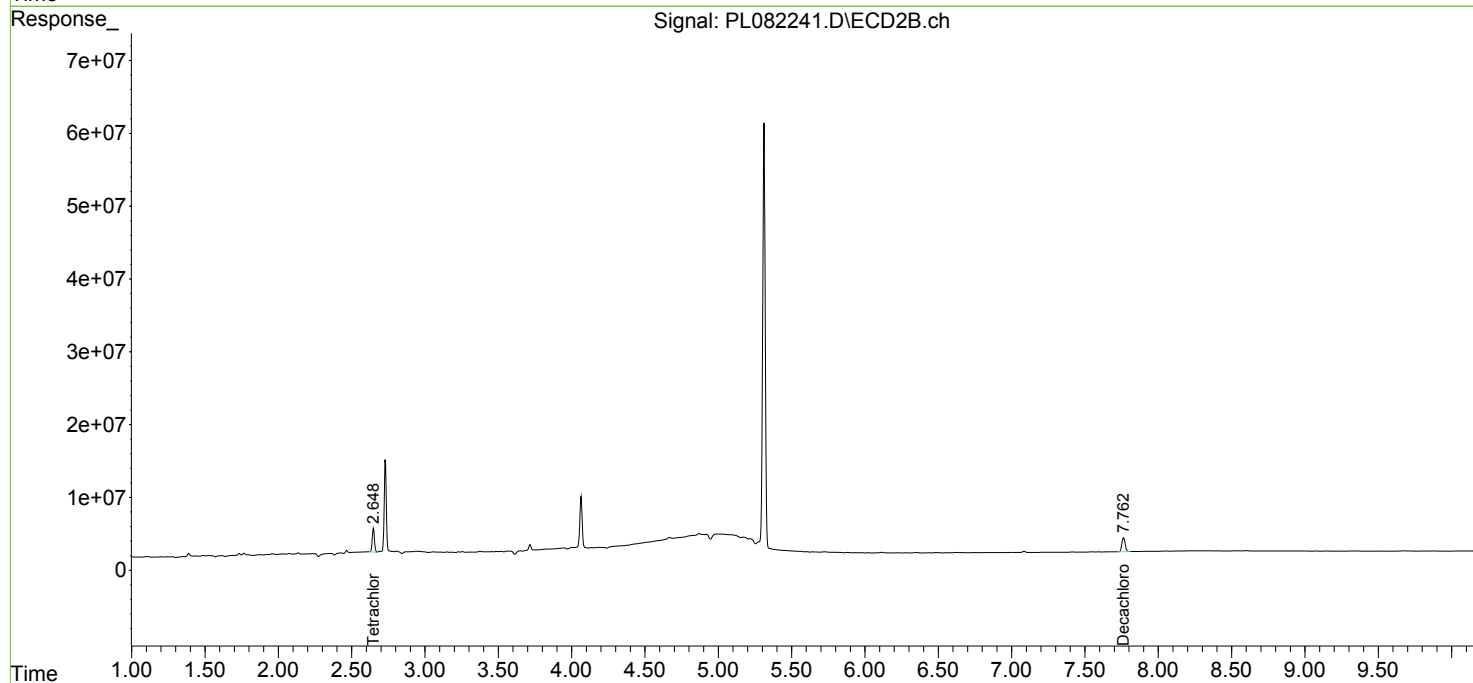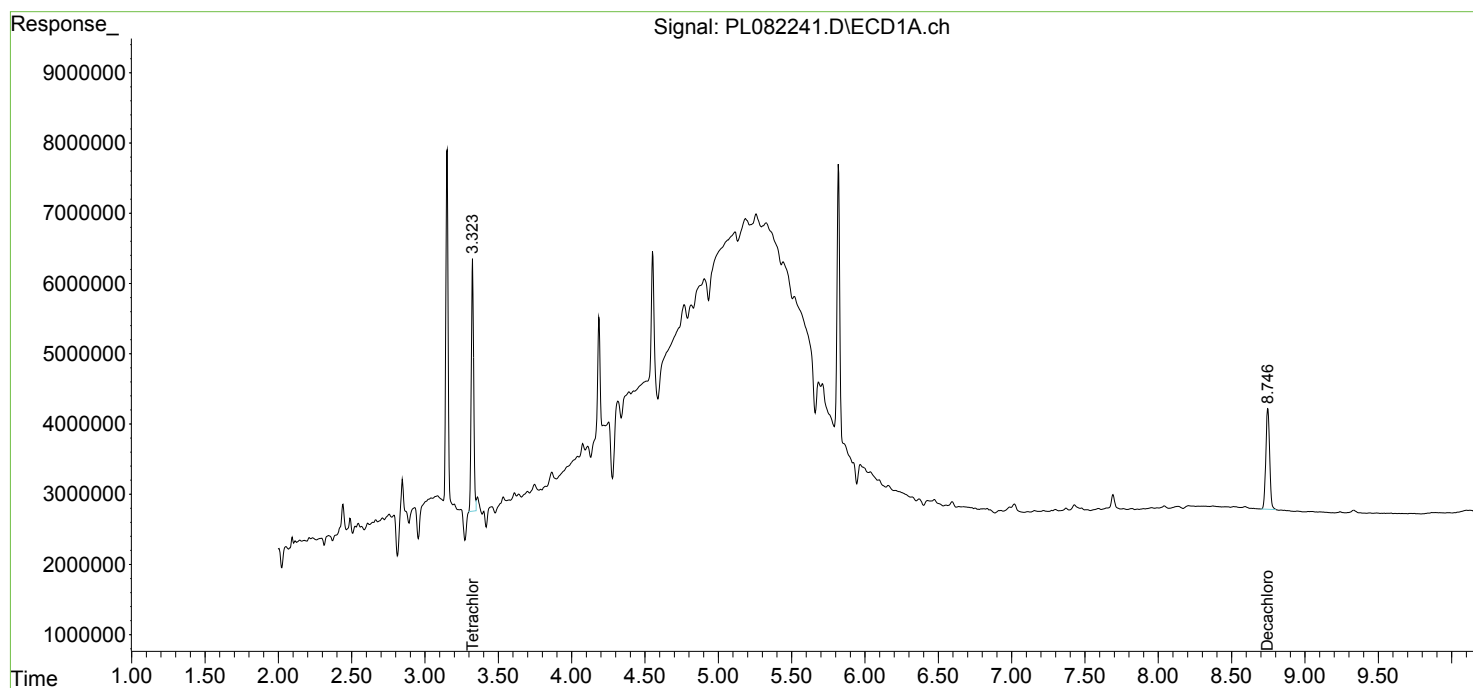

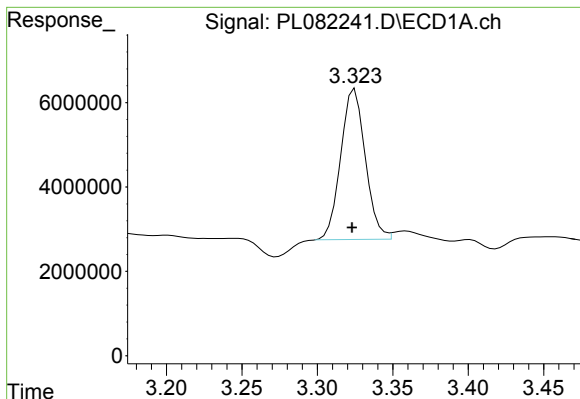


#1 Tetrachloro-m-xylene

R.T.: 3.323 min
Delta R.T.: 0.000 min
Response: 40674395
Conc: 15.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
20230349-COMP-27


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/24/2023
Supervised By :Ankita Jodhani 04/24/2023

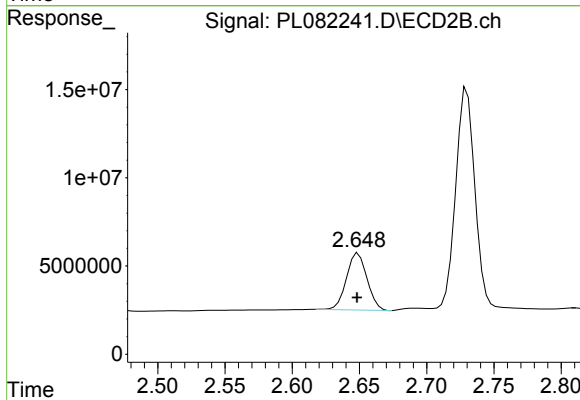


#1 Tetrachloro-m-xylene

R.T.: 2.649 min
Delta R.T.: 0.000 min
Response: 34243239
Conc: 14.78 ng/ml

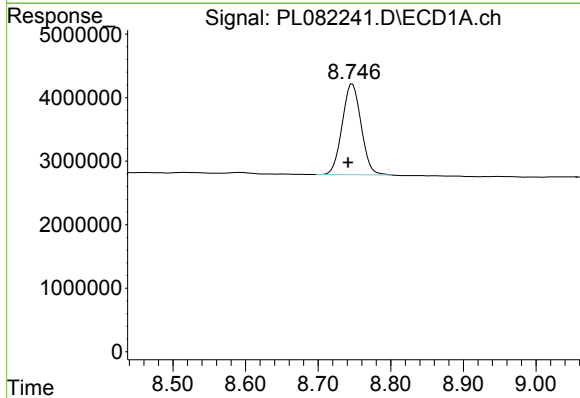

#28 Decachlorobiphenyl

R.T.: 8.747 min
Delta R.T.: 0.006 min
Response: 25946904
Conc: 13.59 ng/ml

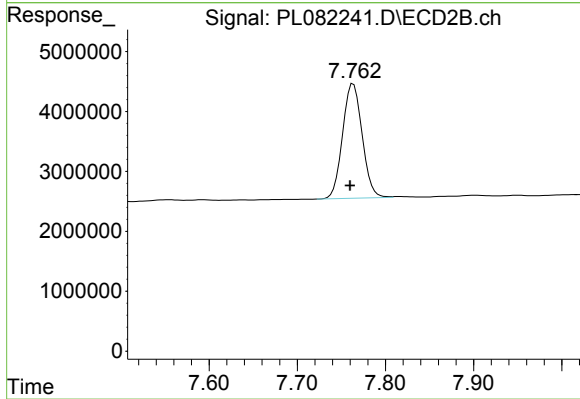

#28 Decachlorobiphenyl

R.T.: 7.764 min
Delta R.T.: 0.004 min
Response: 29487044
Conc: 12.92 ng/ml