

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042123\
 Data File : PL082263.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Apr 2023 18:54
 Operator : AR\AJ
 Sample : 02403-01
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-1

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 04/24/2023
 Supervised By :Ankita Jodhani 04/24/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 22:09:55 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 21 03:12:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.321	2.648	41492784	36403325	15.533m	15.713
2) SA Decachlor...	8.739	7.759	29439322	35238656	15.421m	15.439

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042123\
Data File : PL082263.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Apr 2023 18:54
Operator : AR\AJ
Sample : 02403-01
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
COMP-1


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 04/24/2023
Supervised By : Ankita Jodhani 04/24/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 22:09:55 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 03:12:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

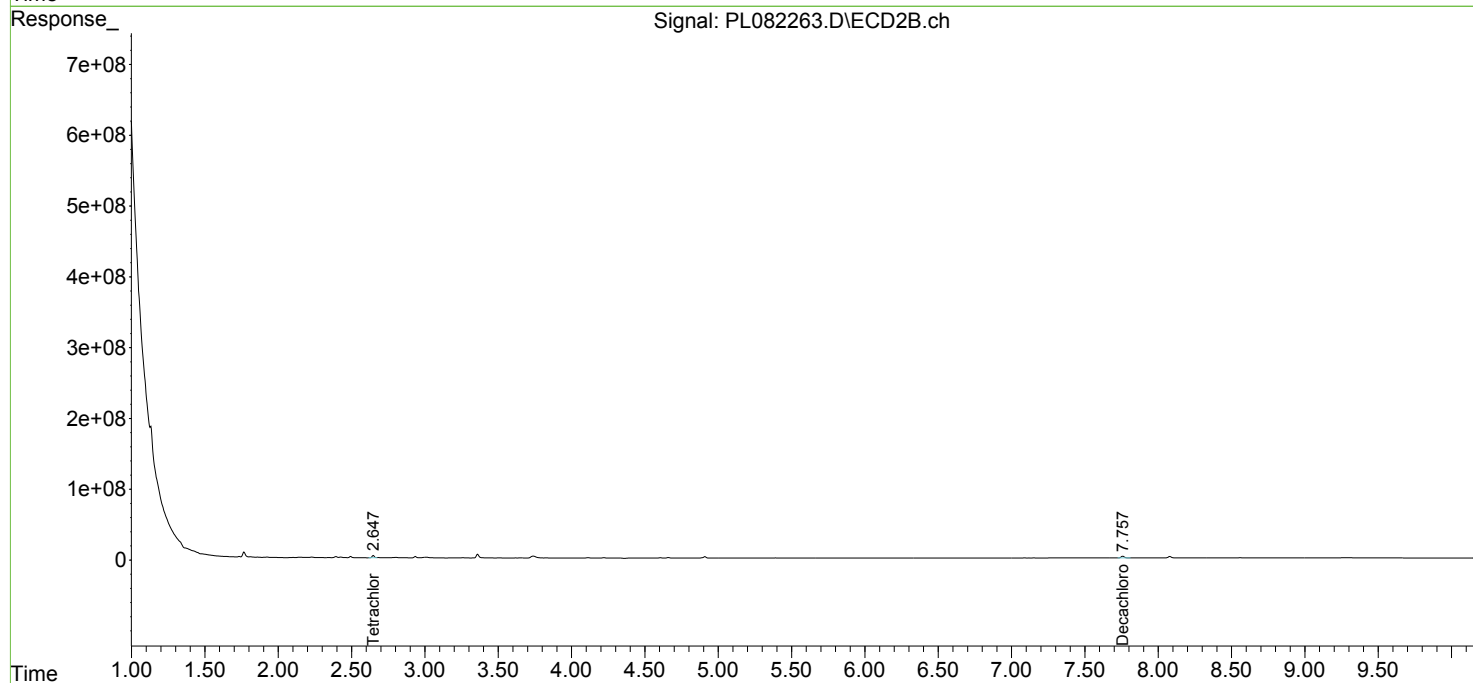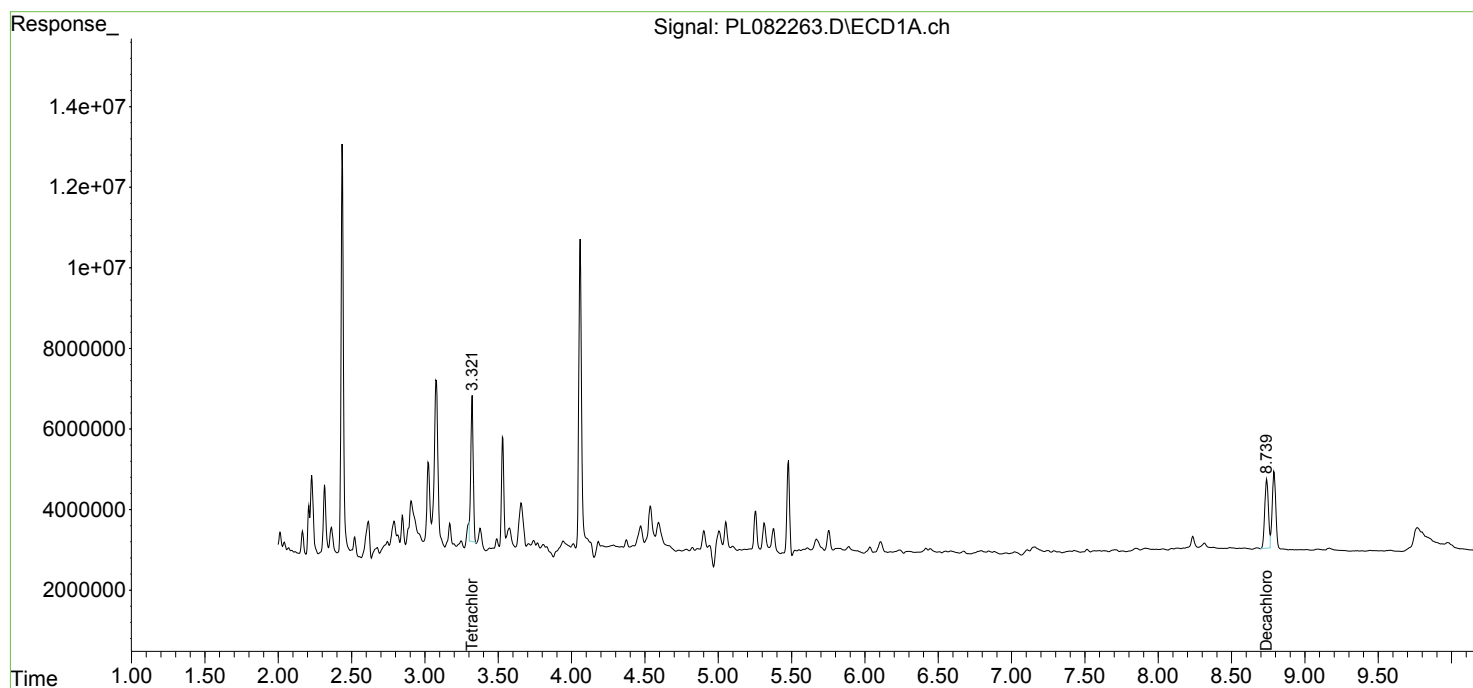

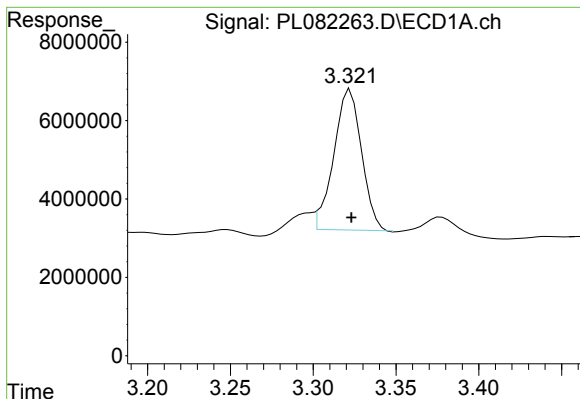


#1 Tetrachloro-m-xylene

R.T.: 3.321 min
Delta R.T.: -0.002 min
Response: 41492784
Conc: 15.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-1


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/24/2023
Supervised By :Ankita Jodhani 04/24/2023

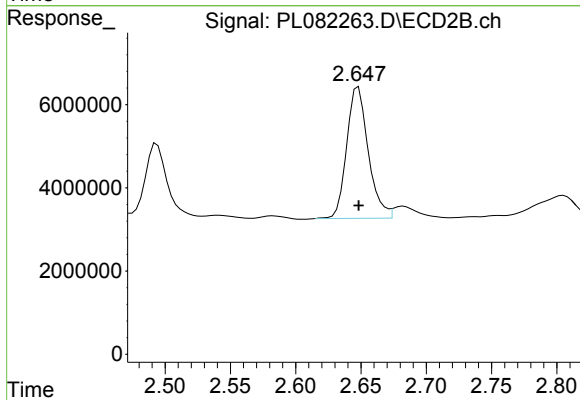


#1 Tetrachloro-m-xylene

R.T.: 2.648 min
Delta R.T.: 0.000 min
Response: 36403325
Conc: 15.71 ng/ml

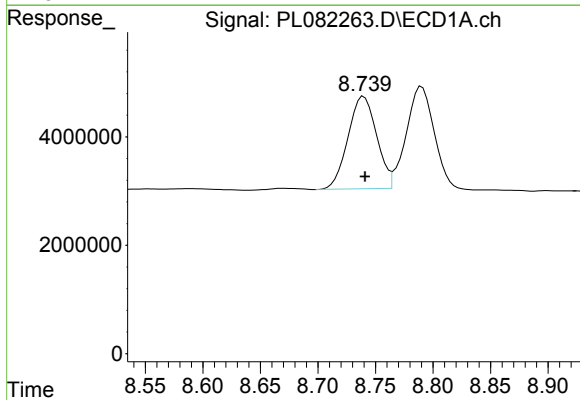

#28 Decachlorobiphenyl

R.T.: 8.739 min
Delta R.T.: -0.002 min
Response: 29439322
Conc: 15.42 ng/ml m

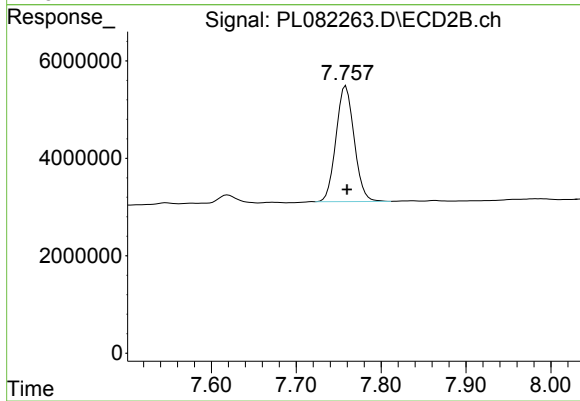

#28 Decachlorobiphenyl

R.T.: 7.759 min
Delta R.T.: -0.001 min
Response: 35238656
Conc: 15.44 ng/ml