

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042123\
 Data File : PL082264.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Apr 2023 19:08
 Operator : AR\AJ
 Sample : 02403-07
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-2

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 04/24/2023
 Supervised By :Ankita Jodhani 04/24/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 22:11:01 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 21 03:12:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.323	2.648	40575392	35547615	15.190	15.344
28) SA Decachlor...	8.738	7.758	27892408	32325782	14.610m	14.162

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042123\
Data File : PL082264.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Apr 2023 19:08
Operator : AR\AJ
Sample : 02403-07
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
COMP-2


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 04/24/2023
Supervised By : Ankita Jodhani 04/24/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 22:11:01 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 03:12:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

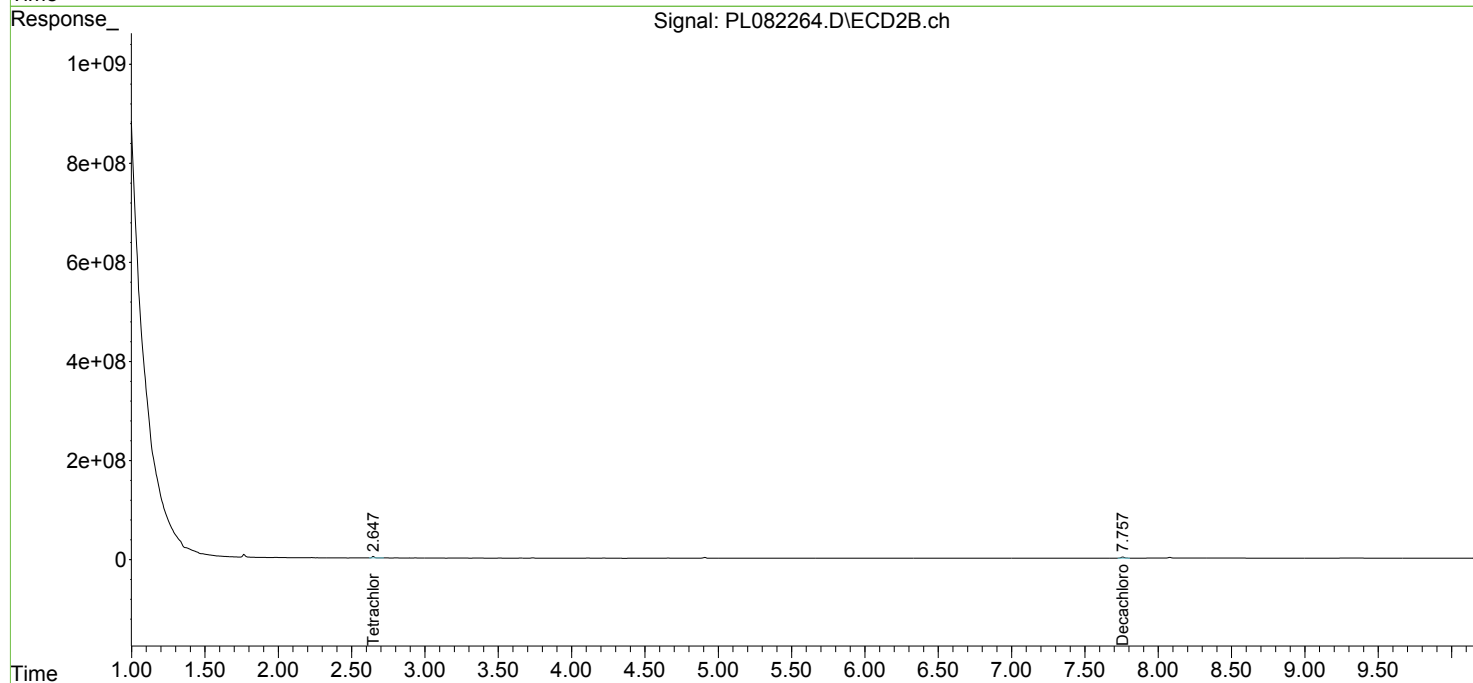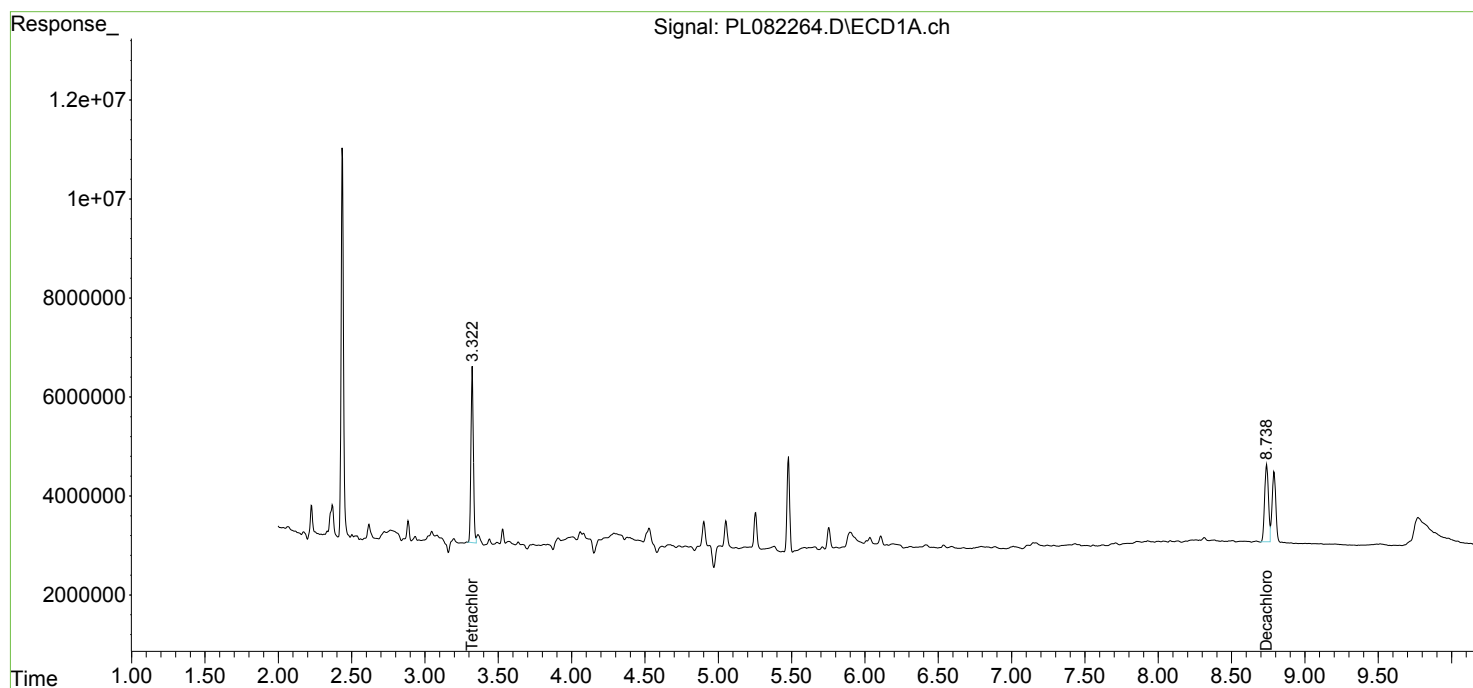

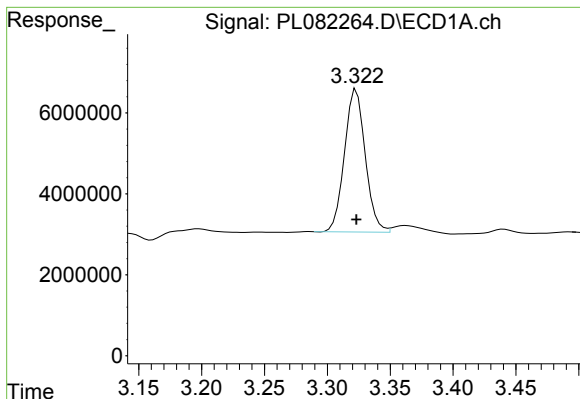


#1 Tetrachloro-m-xylene

R.T.: 3.323 min
Delta R.T.: 0.000 min
Response: 40575392
Conc: 15.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-2


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/24/2023
Supervised By :Ankita Jodhani 04/24/2023

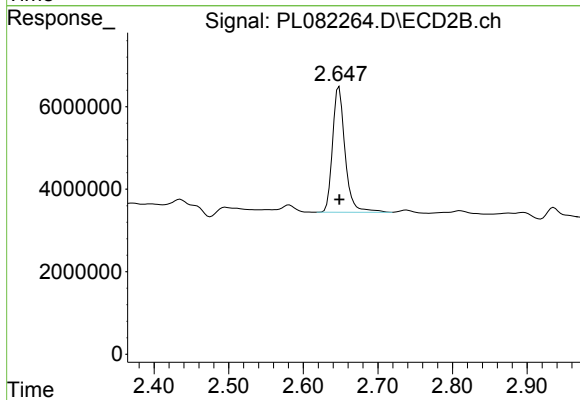


#1 Tetrachloro-m-xylene

R.T.: 2.648 min
Delta R.T.: 0.000 min
Response: 35547615
Conc: 15.34 ng/ml

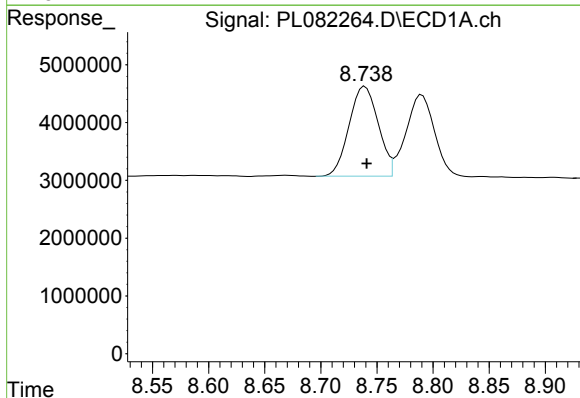

#28 Decachlorobiphenyl

R.T.: 8.738 min
Delta R.T.: -0.003 min
Response: 27892408
Conc: 14.61 ng/ml m

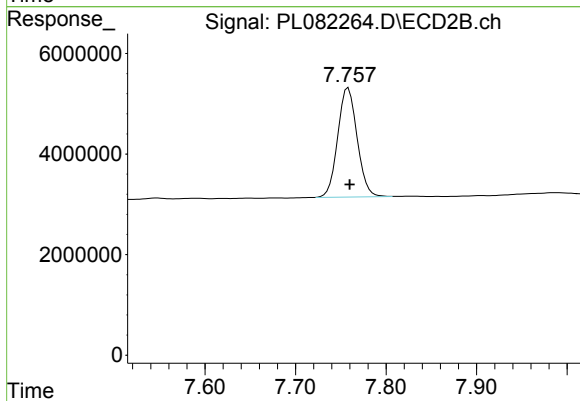

#28 Decachlorobiphenyl

R.T.: 7.758 min
Delta R.T.: -0.002 min
Response: 32325782
Conc: 14.16 ng/ml