

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042219\
 Data File : PL047622.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2019 17:23
 Operator : AJ\SJ
 Sample : K2515-03
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-15

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 01:07:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041919.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 19 16:51:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.330	3.940	44329537	13022831	4.996	4.878
28)	SA Decachlor...	8.003	8.973	79437773	25637766	7.864	8.446
Target Compounds							
10)	B gamma-Chl...	5.240f	0.000	8439386	0	0.690	N.D. #
11)	B alpha-Chl...	0.000	6.111	0	2696289	N.D.	0.842 #
25)	Chlordane-3	5.240f	0.000	8439386	0	6.155	N.D. #
26)	Chlordane-4	0.000	6.111	0	2696289	N.D.	5.707 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042219\
Data File : PL047622.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2019 17:23
Operator : AJ\SJ
Sample : K2515-03
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-15

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 01:07:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041919.M
Quant Title : GC Extractables
QLast Update : Fri Apr 19 16:51:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

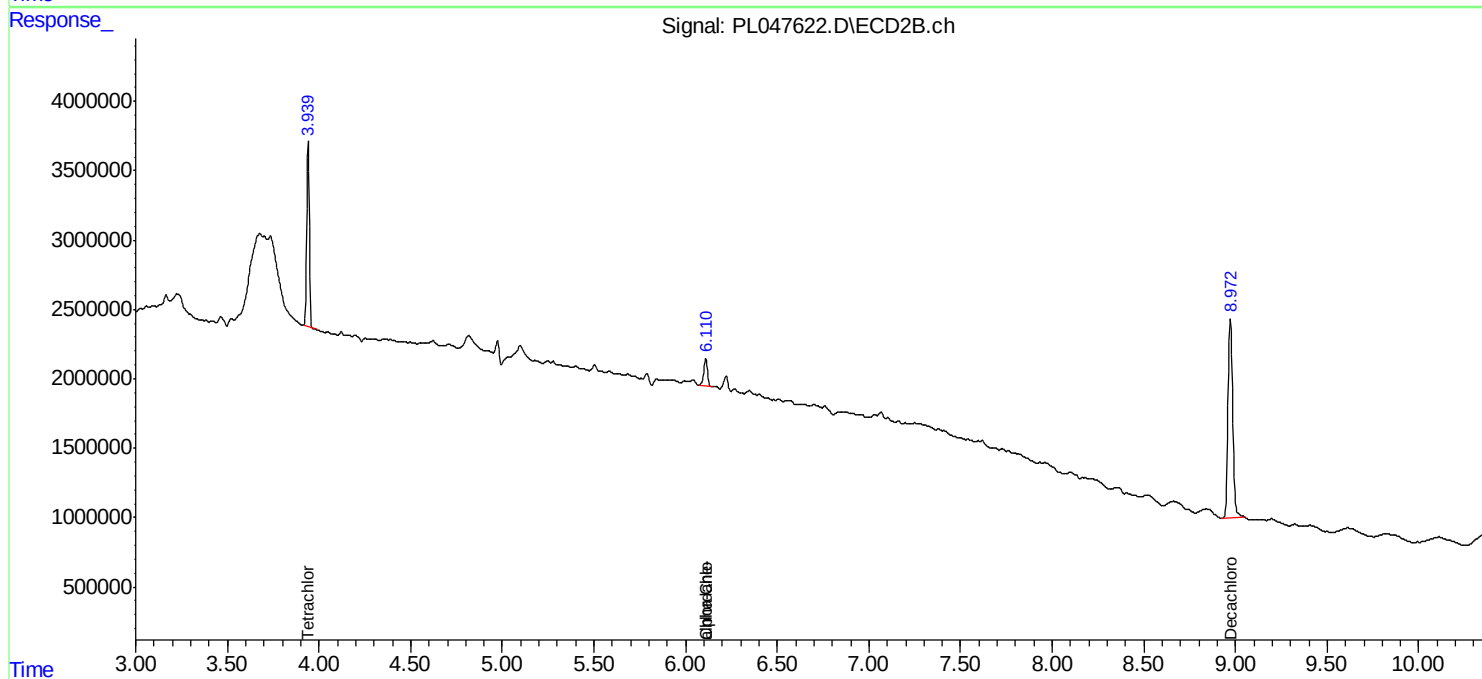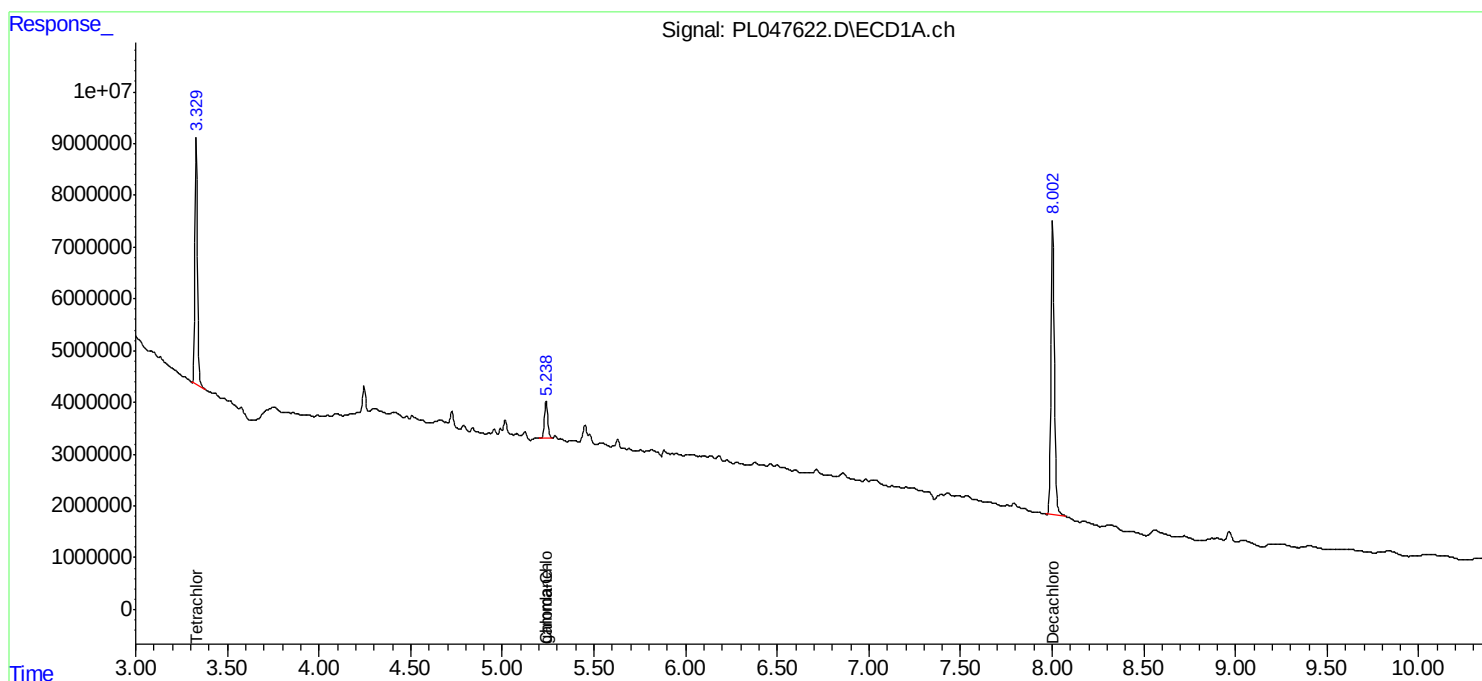


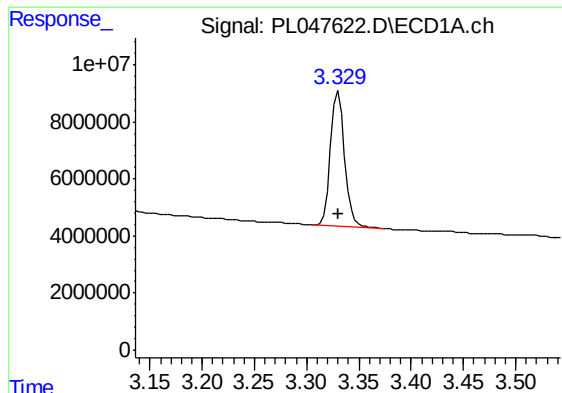

#1 Tetrachloro-m-xylene


R.T.: 3.330 min
Delta R.T.: 0.000 min
Response: 44329537
Conc: 5.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-15

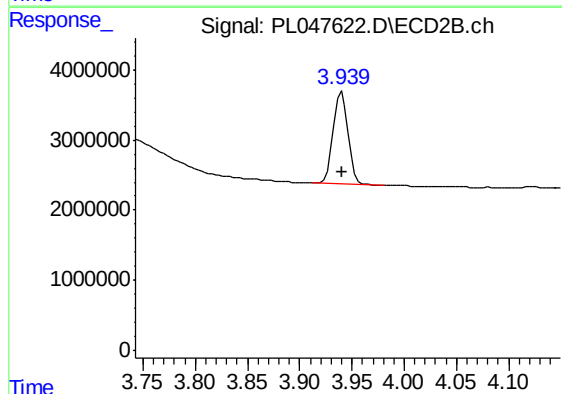


#1 Tetrachloro-m-xylene

R.T.: 3.940 min
Delta R.T.: 0.000 min
Response: 13022831
Conc: 4.88 ng/ml

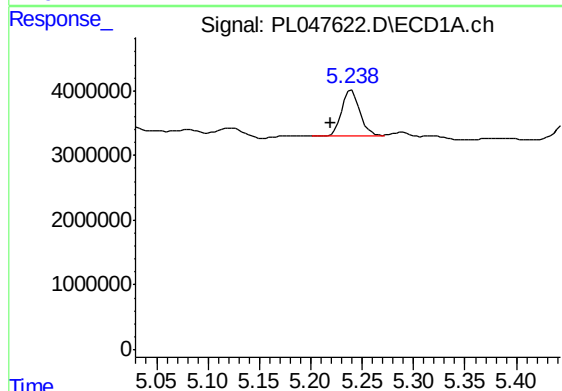


#10 gamma-Chlordane

R.T.: 5.240 min
Delta R.T.: 0.020 min
Response: 8439386
Conc: 0.69 ng/ml

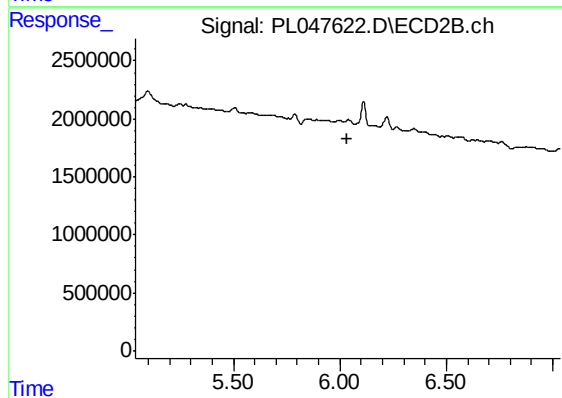

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.037 min
Response: 0
Conc: N.D.

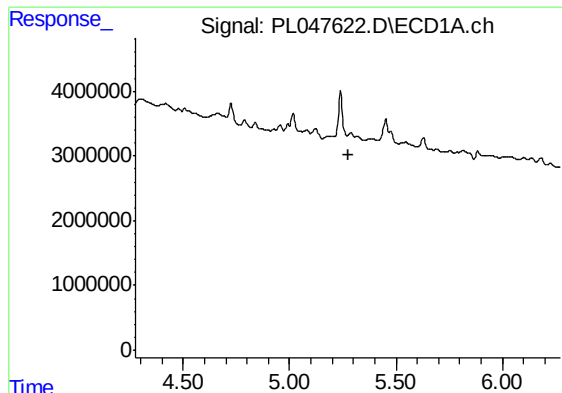

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.276 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-15

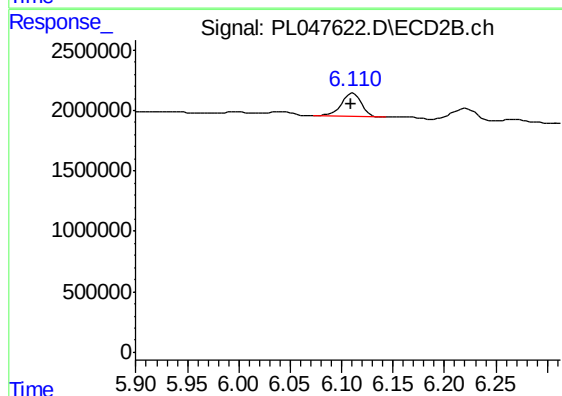


#11 alpha-Chlordane

R.T.: 6.111 min
Delta R.T.: 0.002 min
Response: 2696289
Conc: 0.84 ng/ml

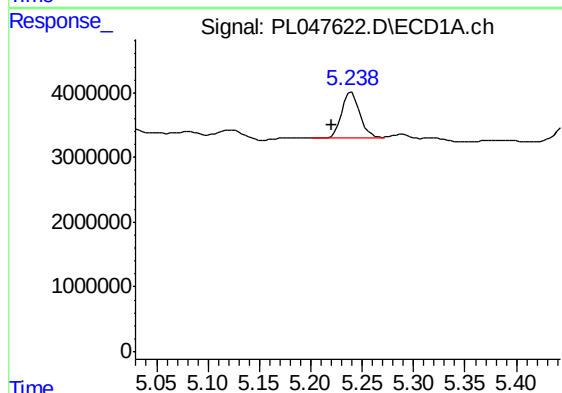


#25 Chlordane-3

R.T.: 5.240 min
Delta R.T.: 0.019 min
Response: 8439386
Conc: 6.16 ng/ml

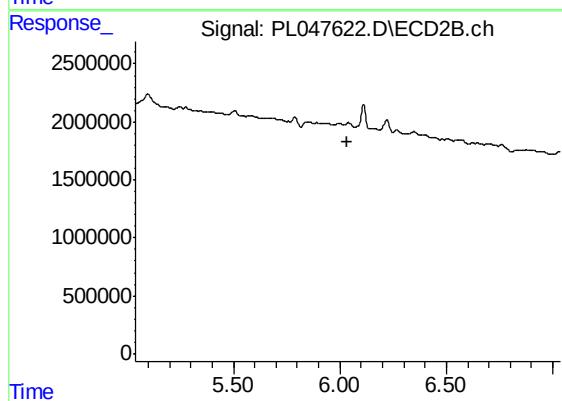

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 6.037 min
Response: 0
Conc: N.D.

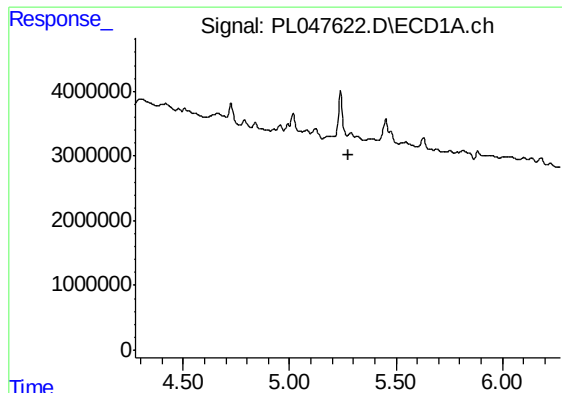

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.276 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-15

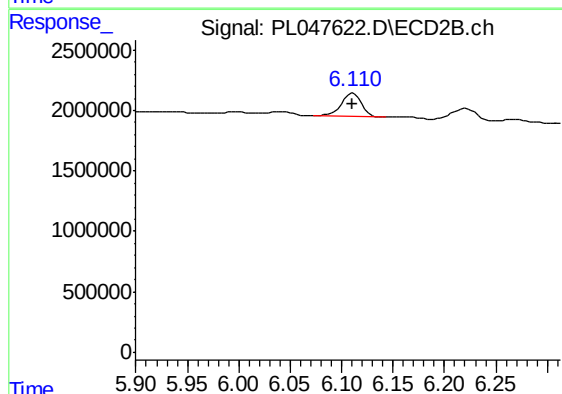


#26 Chlordane-4

R.T.: 6.111 min
Delta R.T.: 0.001 min
Response: 2696289
Conc: 5.71 ng/ml

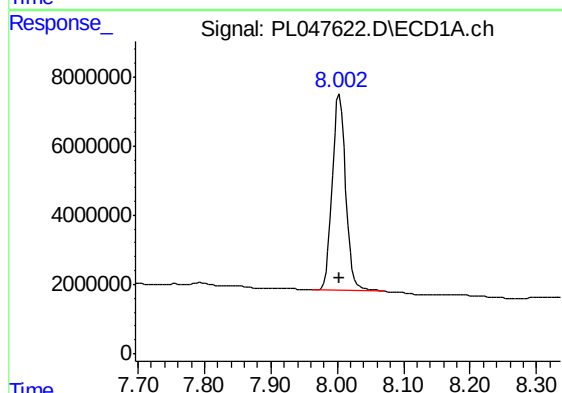

#28 Decachlorobiphenyl

R.T.: 8.003 min
Delta R.T.: 0.000 min
Response: 79437773
Conc: 7.86 ng/ml

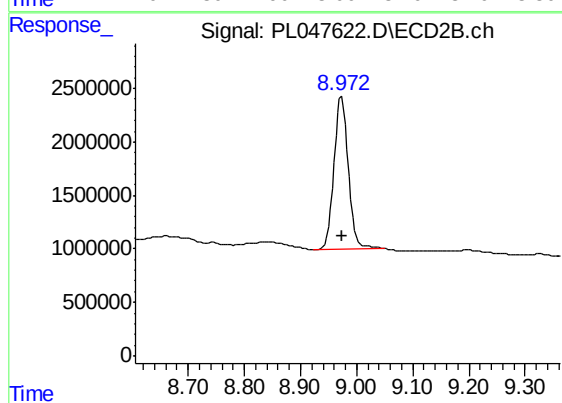

#28 Decachlorobiphenyl

R.T.: 8.973 min
Delta R.T.: -0.001 min
Response: 25637766
Conc: 8.45 ng/ml